

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN027004.D
 Acq On : 21 Aug 2023 22:45
 Operator : MA/JU
 Sample : 03967-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A48M6

Quant Time: Aug 22 01:40:35 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 18 13:11:26 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.101	152	9365	0.400	ng/ul	0.00
4) Naphthalene-d8	10.927	136	30639	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.726	164	17585	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.472	188	40290	0.400	ng/ul	0.00
17) Chrysene-d12	21.641	240	32982	0.400	ng/ul	# 0.00
23) Perylene-d12	24.182	264	31481	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.439	96	39124	3.519	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.500	152	9251	0.205	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	23321	0.224	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.977	128	9878	0.114	ng/ul	96
7) 2-Methylnaphthalene	12.572	142	4573	0.087	ng/ul	100
8) 1-Methylnaphthalene	12.791	142	3543	0.065	ng/ul	100
10) Acenaphthylene	14.458	152	28186	0.286	ng/ul	100
11) Acenaphthene	14.791	153	5535	0.081	ng/ul	98
12) Fluorene	15.771	166	9979	0.129	ng/ul	99
15) Phenanthrene	17.515	178	276495	2.089	ng/ul	100
16) Anthracene	17.607	178	41845	0.350	ng/ul	99
19) Fluoranthene	19.520	202	578044	4.219	ng/ul	100
20) Pyrene	19.882	202	640242	4.380	ng/ul	100
21) Benzo(a)anthracene	21.624	228	264790	2.019	ng/ul	99
22) Chrysene	21.679	228	348166	2.689	ng/ul	98
24) Benzo(b)fluoranthene	23.395	252	612546	5.144	ng/ul	90
26) Benzo(a)pyrene	24.070	252	271183	2.524	ng/ul	98
27) Indeno(1,2,3-cd)pyrene	26.864	276	190741	1.357	ng/ul#	90
28) Dibenzo(a,h)anthracene	26.881	278	43115	0.385	ng/ul#	89
29) Benzo(g,h,i)perylene	27.706	276	206136	1.761	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN027004.D
Acq On : 21 Aug 2023 22:45
Operator : MA/JU
Sample : 03967-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A48M6

Quant Time: Aug 22 01:40:35 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 18 13:11:26 2023
Response via : Initial Calibration

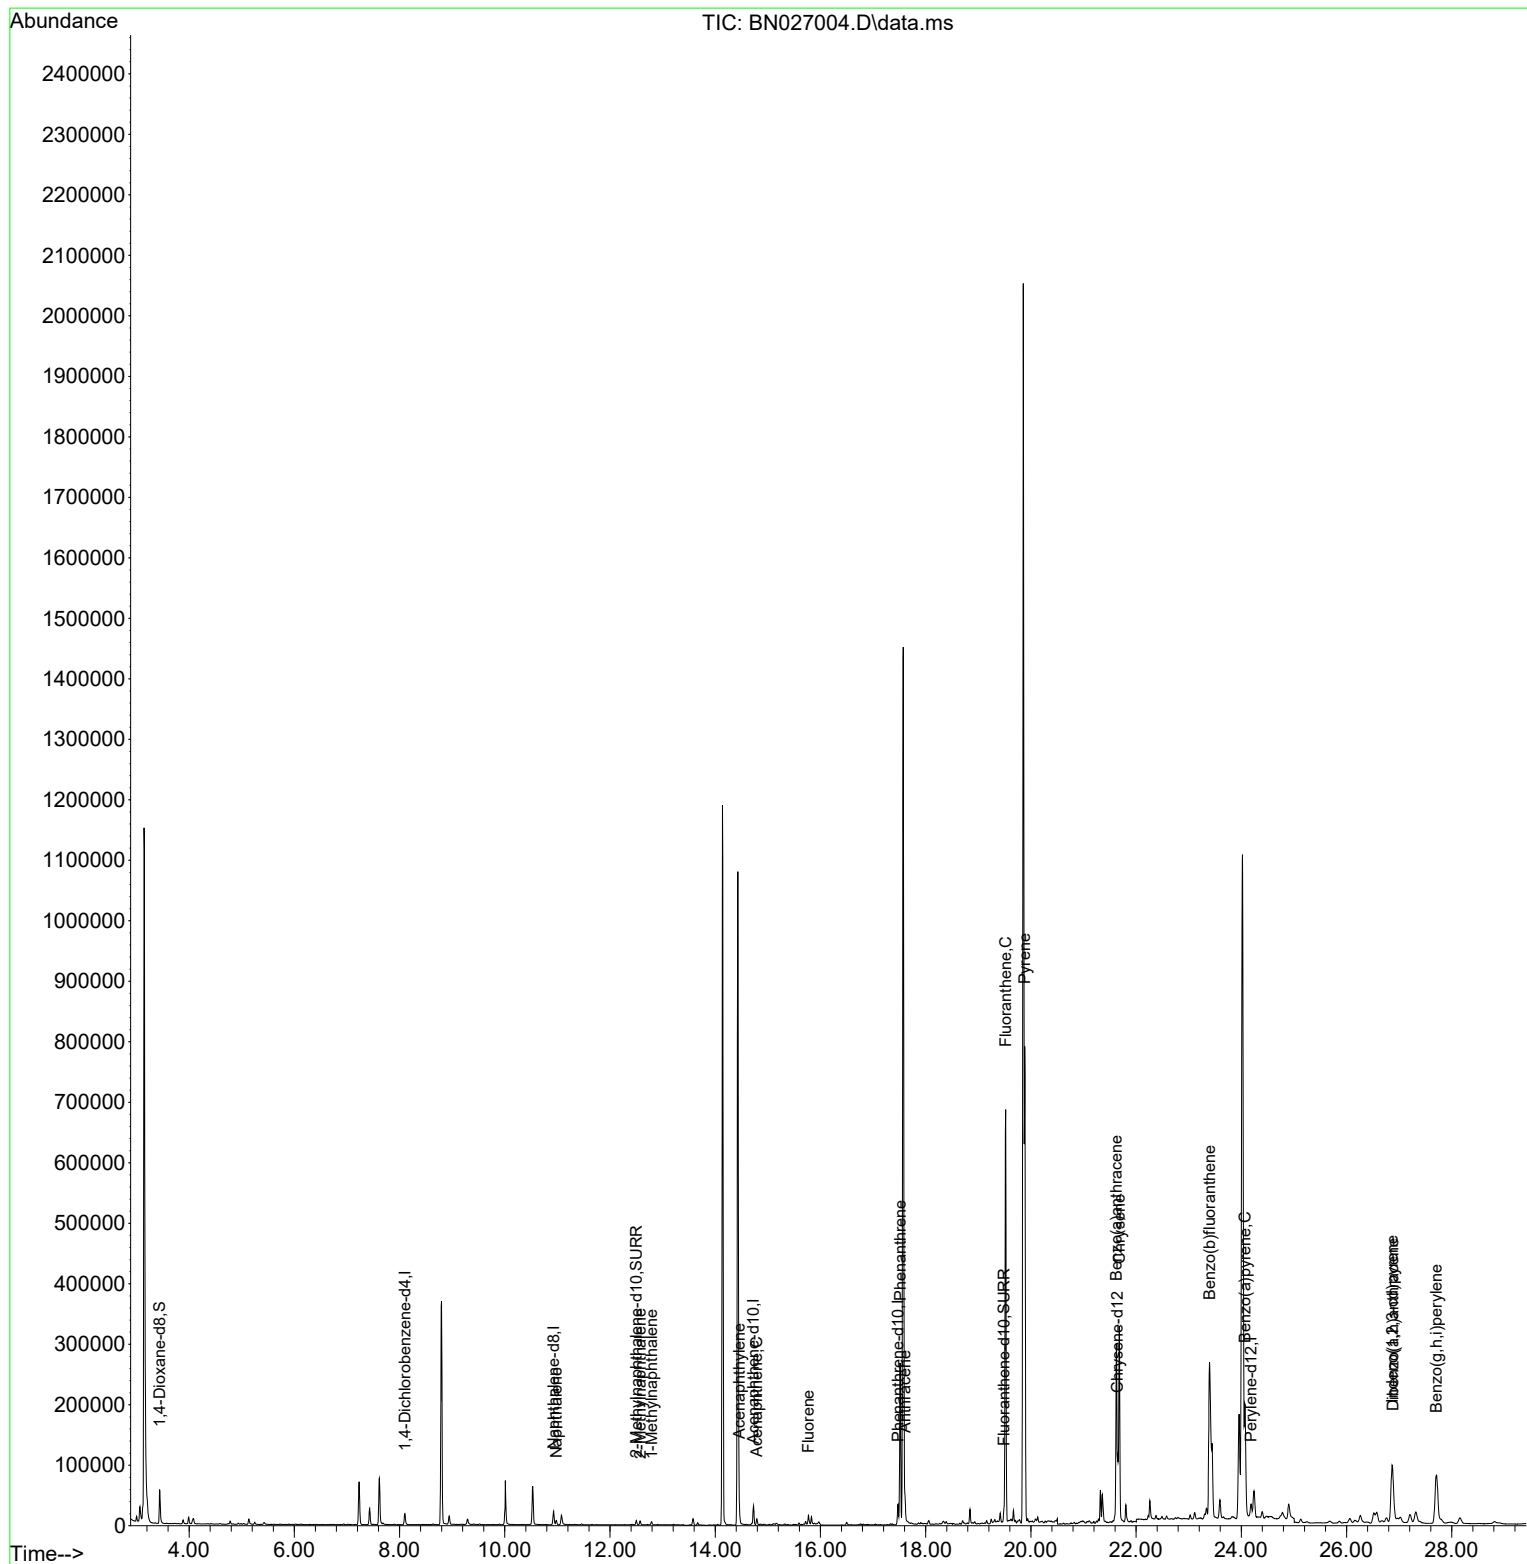



#5

Naphthalene

Concen: 0.114 ng/ul

RT: 10.977 min Scan# 1868

Delta R.T. -0.006 min

Lab File: BN027004.D

Acq: 21 Aug 2023 22:45

Instrument :

BNA_N

ClientSampleId :

A48M6





Tgt Ion:128 Resp: 9878

Ion Ratio Lower Upper

128 100

129 13.6 9.2 13.8

127 14.1 10.5 15.7

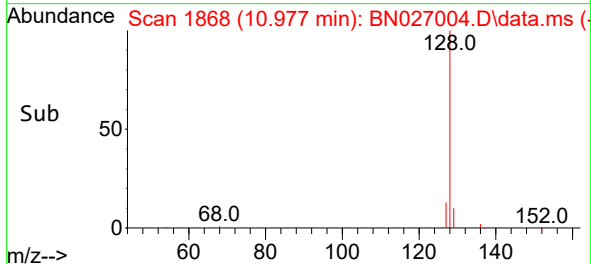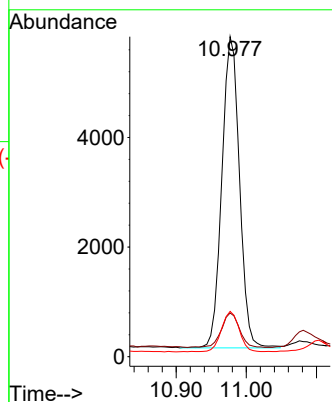

#7

2-Methylnaphthalene

Concen: 0.087 ng/ul

RT: 12.572 min Scan# 2158

Delta R.T. -0.006 min

Lab File: BN027004.D




Acq: 21 Aug 2023 22:45


Tgt Ion:142 Resp: 4573

Ion Ratio Lower Upper

142 100

141 89.0 70.9 106.3


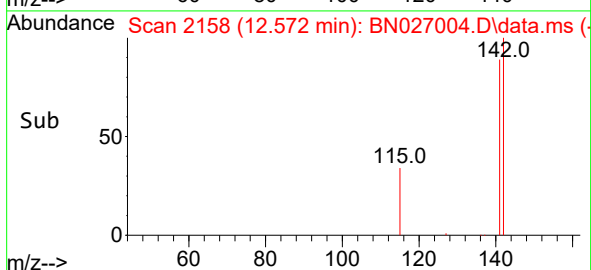






#8
1-Methylnaphthalene
Concen: 0.065 ng/ul
RT: 12.791 min Scan# 2197
Delta R.T. -0.000 min
Lab File: BN027004.D
Acq: 21 Aug 2023 22:45




Instrument :
BNA_N
ClientSampleId :
A48M6


Tgt Ion:142 Resp: 3543
Ion Ratio Lower Upper
142 100
141 92.0 73.2 109.8

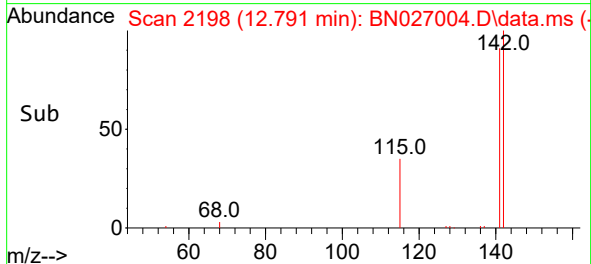

#10
Acenaphthylene
Concen: 0.286 ng/ul
RT: 14.458 min Scan# 2537
Delta R.T. -0.000 min
Lab File: BN027004.D
Acq: 21 Aug 2023 22:45

Tgt Ion:152 Resp: 28186
Ion Ratio Lower Upper
152 100
151 19.7 15.9 23.9
153 13.7 11.0 16.6


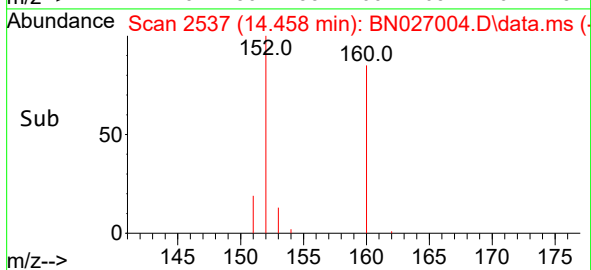

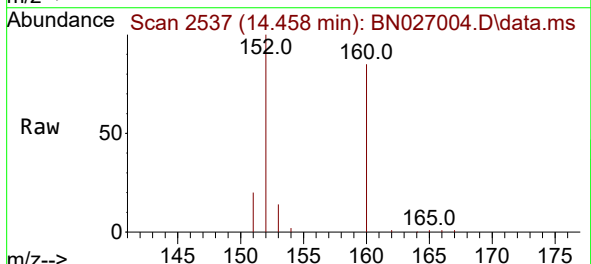




#11
Acenaphthene
Concen: 0.081 ng/ul
RT: 14.791 min Scan# 2609
Delta R.T. -0.000 min
Lab File: BN027004.D
Acq: 21 Aug 2023 22:45




Instrument :
BNA_N
ClientSampleId :
A48M6


Tgt Ion:153 Resp: 5535
Ion Ratio Lower Upper
153 100
152 52.8 41.1 61.7
154 86.9 71.6 107.4

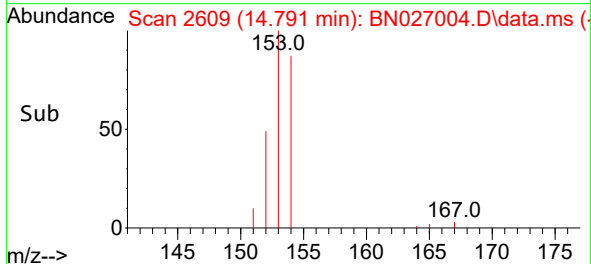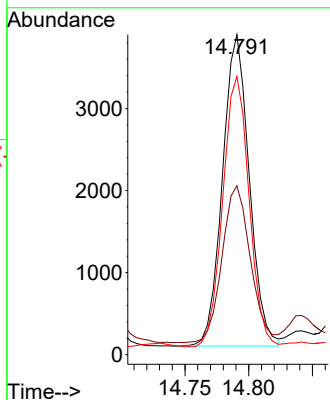

#12
Fluorene
Concen: 0.129 ng/ul
RT: 15.771 min Scan# 2821
Delta R.T. -0.000 min
Lab File: BN027004.D
Acq: 21 Aug 2023 22:45

Tgt Ion:166 Resp: 9979
Ion Ratio Lower Upper
166 100
165 98.7 79.1 118.7
167 16.5 11.4 17.0

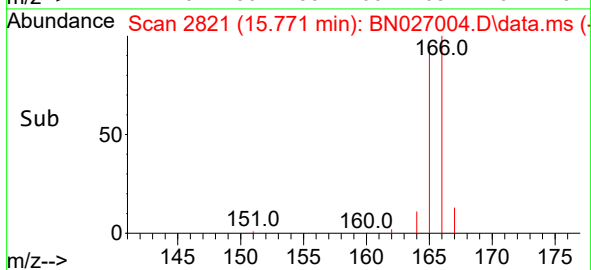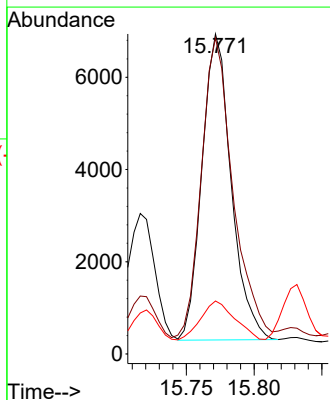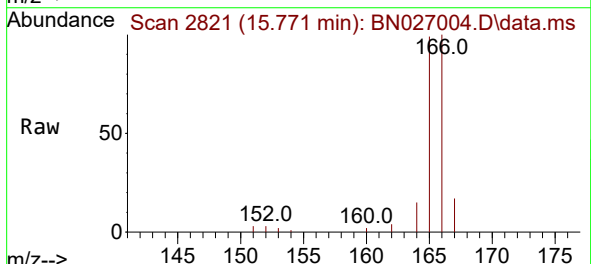



#15

Phenanthrene

Concen: 2.089 ng/ul

RT: 17.515 min Scan# 31

Delta R.T. -0.004 min

Lab File: BN027004.D

Acq: 21 Aug 2023 22:45

Instrument :

BNA_N

ClientSampleId :

A48M6





Tgt Ion:178 Resp: 276495

Ion Ratio Lower Upper

178 100

179 15.3 12.6 18.8

176 19.3 15.4 23.2

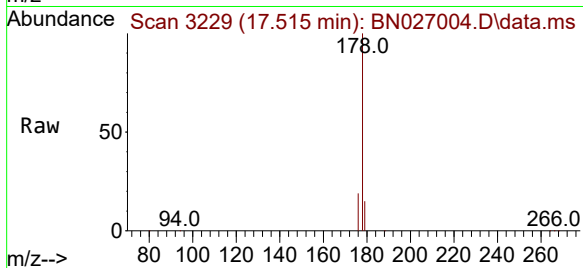

#16

Anthracene

Concen: 0.350 ng/ul

RT: 17.607 min Scan# 3251

Delta R.T. -0.000 min

Lab File: BN027004.D

Acq: 21 Aug 2023 22:45




Tgt Ion:178 Resp: 41845


Ion Ratio Lower Upper

178 100

179 16.3 12.6 19.0

176 19.0 15.0 22.6


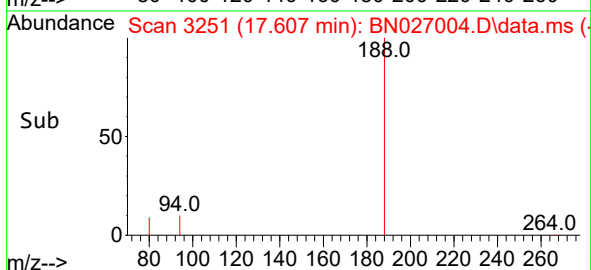

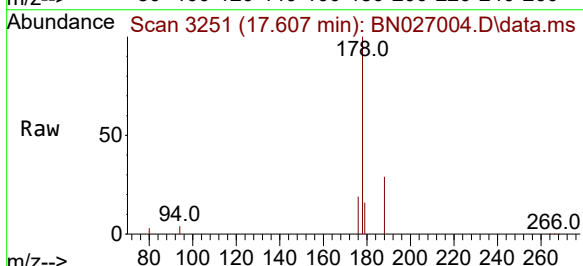




#19
Fluoranthene
Concen: 4.219 ng/ul
RT: 19.520 min Scan# 3682
Delta R.T. -0.005 min
Lab File: BN027004.D
Acq: 21 Aug 2023 22:45




Instrument :
BNA_N
ClientSampleId :
A48M6


Tgt Ion:202 Resp: 578044
Ion Ratio Lower Upper
202 100
101 10.5 8.3 12.5
100 7.6 6.2 9.2

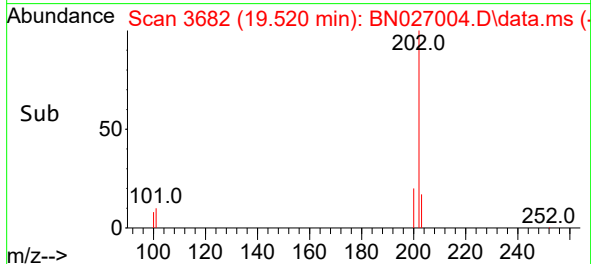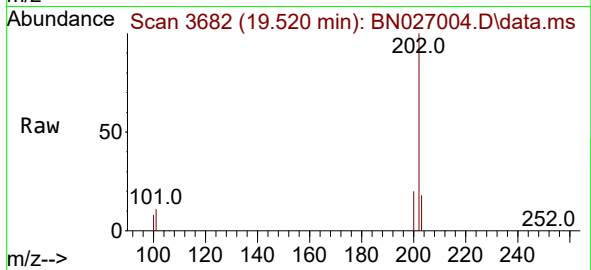

#20
Pyrene
Concen: 4.380 ng/ul
RT: 19.882 min Scan# 3760
Delta R.T. -0.005 min
Lab File: BN027004.D
Acq: 21 Aug 2023 22:45


Tgt Ion:202 Resp: 640242
Ion Ratio Lower Upper
202 100
101 13.2 10.7 16.1
100 10.6 8.5 12.7

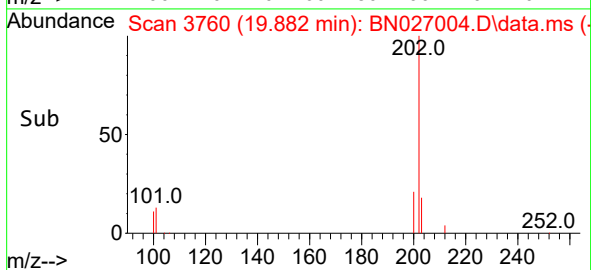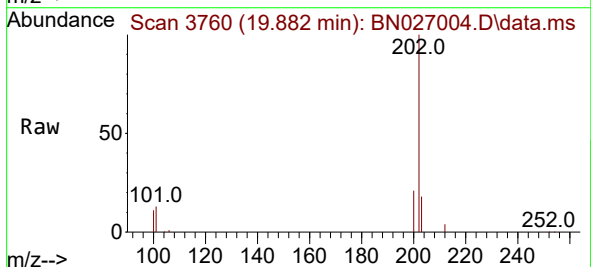






#21
Benzo(a)anthracene
Concen: 2.019 ng/ul
RT: 21.624 min Scan# 41
Delta R.T. -0.009 min
Lab File: BN027004.D
Acq: 21 Aug 2023 22:45

Instrument :
BNA_N
ClientSampleId :
A48M6







Tgt Ion:228 Resp: 264790
Ion Ratio Lower Upper
228 100
229 20.8 16.0 24.0
226 28.2 22.2 33.2

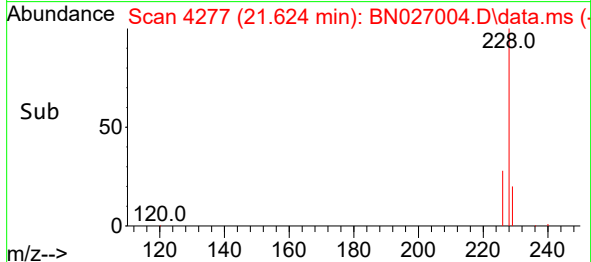

#22
Chrysene
Concen: 2.689 ng/ul
RT: 21.679 min Scan# 4296
Delta R.T. -0.012 min
Lab File: BN027004.D
Acq: 21 Aug 2023 22:45


Tgt Ion:228 Resp: 348166
Ion Ratio Lower Upper
228 100
226 30.8 24.6 36.8
229 21.7 15.8 23.6

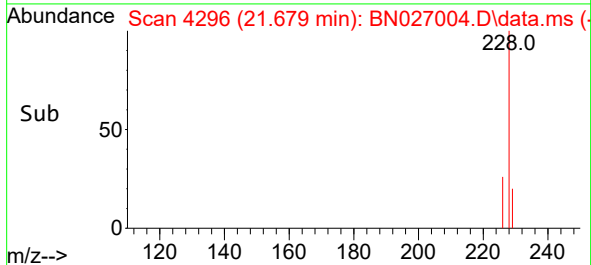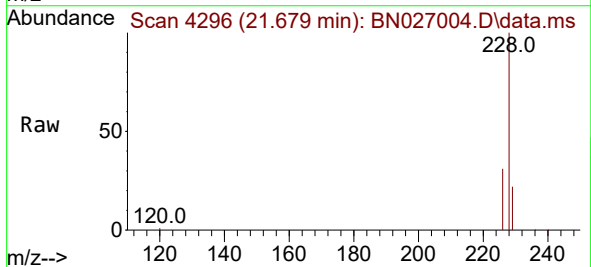






#24
Benzo(b)fluoranthene
Concen: 5.144 ng/ul
RT: 23.395 min Scan# 4883
Delta R.T. -0.012 min
Lab File: BN027004.D
Acq: 21 Aug 2023 22:45

Instrument :
BNA_N
ClientSampleId :
A48M6







Tgt Ion:252 Resp: 612546
Ion Ratio Lower Upper
252 100
253 22.9 0.0 46.8
125 23.1 0.0 25.2

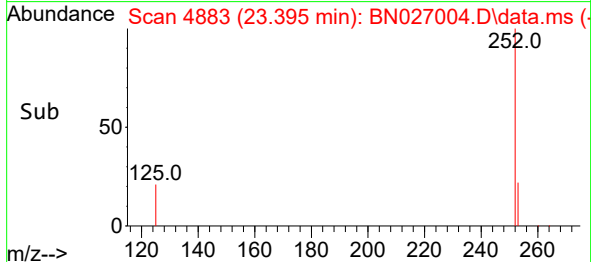

#26
Benzo(a)pyrene
Concen: 2.524 ng/ul
RT: 24.070 min Scan# 5114
Delta R.T. -0.015 min
Lab File: BN027004.D
Acq: 21 Aug 2023 22:45

Tgt Ion:252 Resp: 271183
Ion Ratio Lower Upper
252 100
253 22.9 19.0 28.6
125 13.6 11.4 17.0


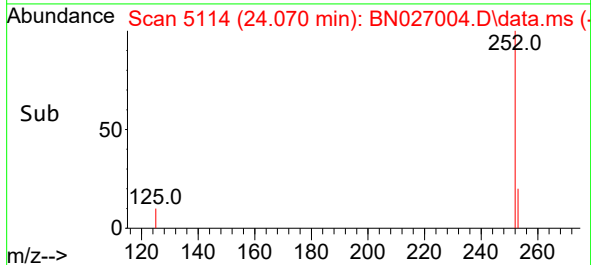

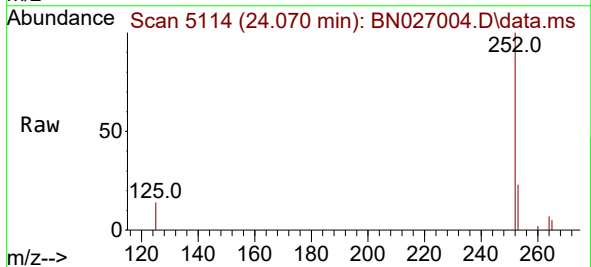




#27
 Indeno(1,2,3-cd)pyrene
 Concen: 1.357 ng/ul
 RT: 26.864 min Scan# 5988
 Delta R.T. -0.021 min
 Lab File: BN027004.D
 Acq: 21 Aug 2023 22:45




Instrument :
 BNA_N
 ClientSampleId :
 A48M6


Tgt Ion:276 Resp: 190741
 Ion Ratio Lower Upper
 276 100
 138 22.0 21.6 32.4
 227 0.1 0.0 0.0#

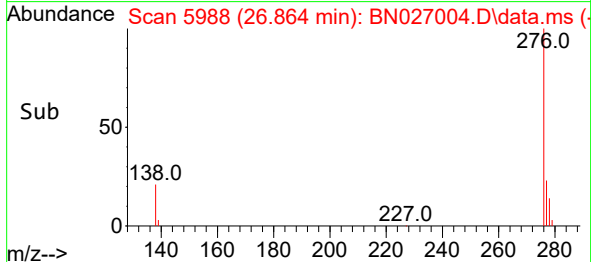

#28
 Dibenzo(a,h)anthracene
 Concen: 0.385 ng/ul
 RT: 26.881 min Scan# 5993
 Delta R.T. -0.041 min
 Lab File: BN027004.D
 Acq: 21 Aug 2023 22:45


Tgt Ion:278 Resp: 43115
 Ion Ratio Lower Upper
 278 100
 139 25.8 15.7 23.5#
 279 29.7 20.2 30.4

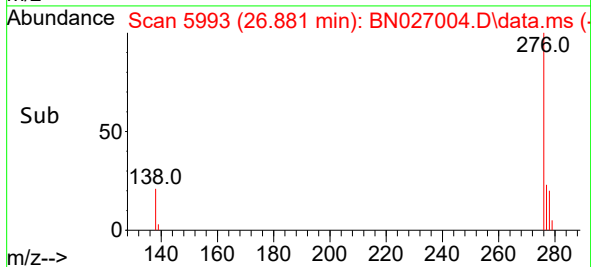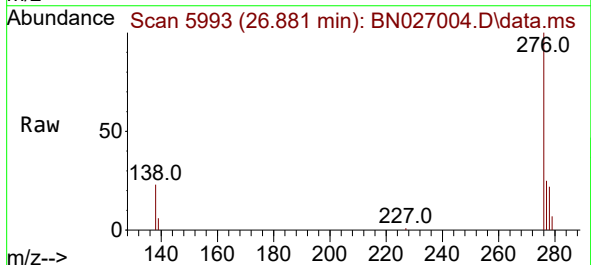

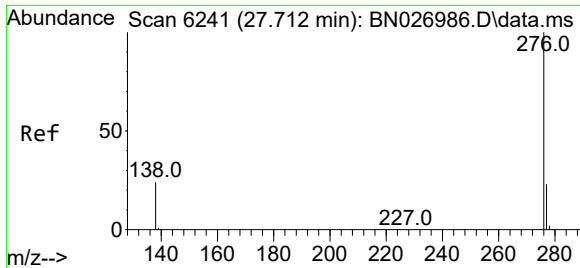

#29
 Benzo(g,h,i)perylene
 Concen: 1.761 ng/ul
 RT: 27.706 min Scan# 61
 Delta R.T. -0.017 min
 Lab File: BN027004.D
 Acq: 21 Aug 2023 22:45

Instrument :
 BNA_N
 ClientSampleId :
 A48M6

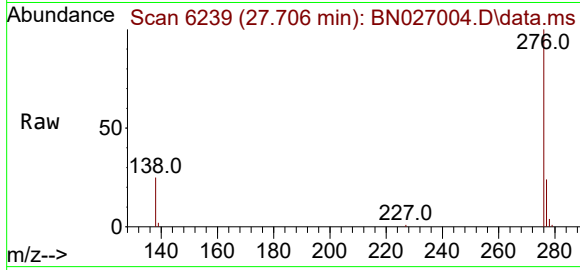

Tgt Ion:	276	Resp:	206136
Ion Ratio	Lower	Upper	
276	100		
138	24.7	19.3	28.9
277	24.2	19.8	29.8

