

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN027027.D
 Acq On : 22 Aug 2023 15:18
 Operator : MA/JU
 Sample : PB154935BL
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK935

Quant Time: Aug 23 01:43:00 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 18 13:11:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.089	152	6510	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.916	136	22507	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.721	164	13601	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.468	188	28916	0.400	ng/ul	0.00
17) Chrysene-d12	21.647	240	21705	0.400	ng/ul	0.00
23) Perylene-d12	24.190	264	21806	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.431	96	52352	6.774	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.489	152	13694	0.413	ng/ul	-0.01
18) Fluoranthene-d10	19.487	212	32057	0.468	ng/ul	0.00
Target Compounds						
					Qvalue	
19) Fluoranthene	19.515	202	2464	0.027	ng/ul#	87
20) Pyrene	19.859	202	4277	0.044	ng/ul#	1
26) Benzo(a)pyrene	24.024	252	8226	0.111	ng/ul#	43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN027027.D
Acq On : 22 Aug 2023 15:18
Operator : MA/JU
Sample : PB154935BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK935

Quant Time: Aug 23 01:43:00 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 18 13:11:26 2023
Response via : Initial Calibration




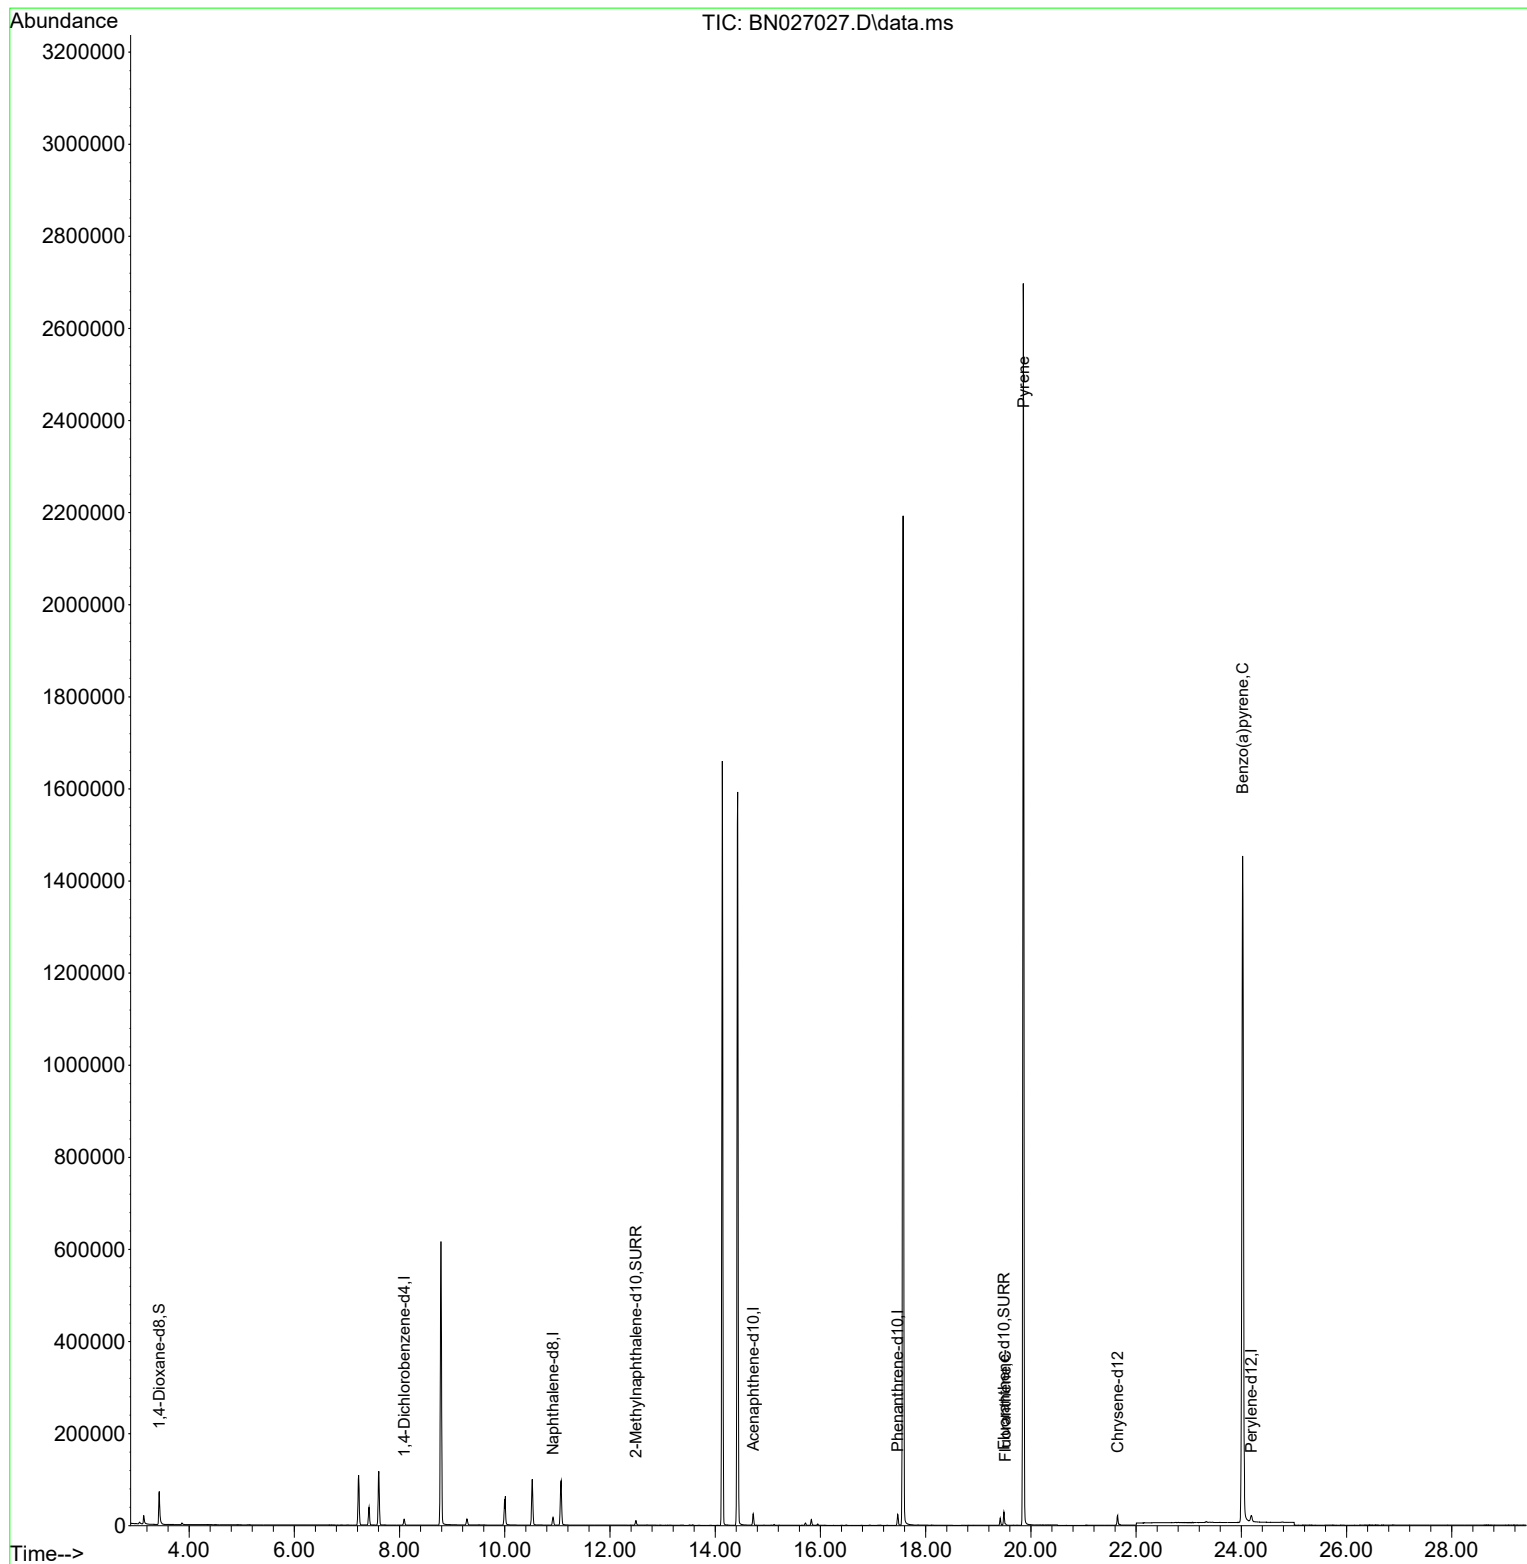


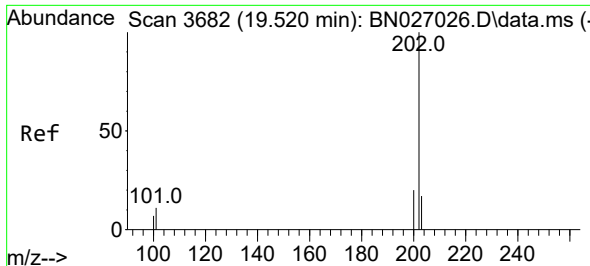

#19
Fluoranthene
Concen: 0.027 ng/ul
RT: 19.515 min Scan# 3075
Delta R.T. -0.009 min
Lab File: BN027027.D
Acq: 22 Aug 2023 15:18




Instrument :
BNA_N
ClientSampleId :
SBLK935


Tgt Ion:202 Resp: 2464
Ion Ratio Lower Upper
202 100
101 15.8 8.3 12.5#
100 11.9 6.2 9.2#

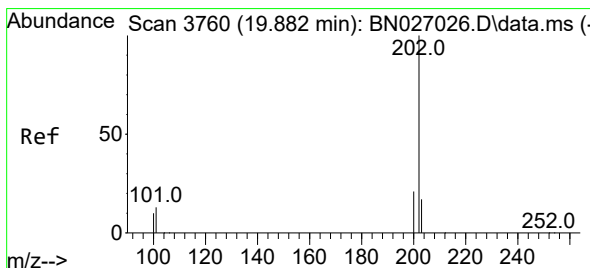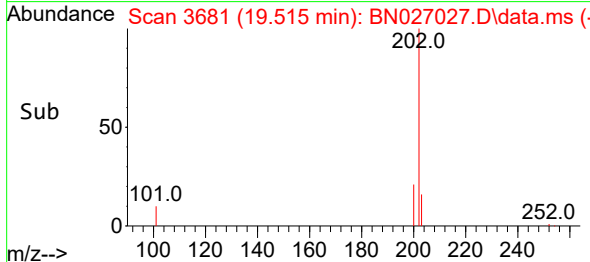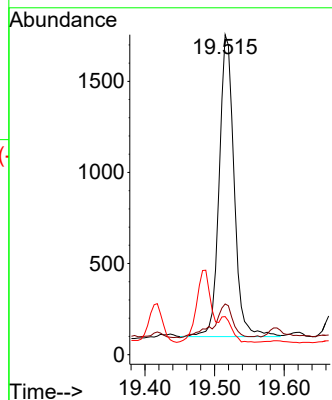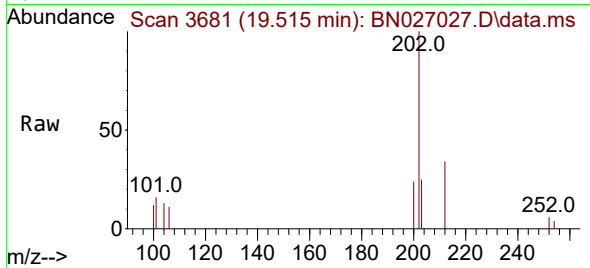

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.859 min Scan# 3755
Delta R.T. -0.028 min
Lab File: BN027027.D
Acq: 22 Aug 2023 15:18


Tgt Ion:202 Resp: 4277
Ion Ratio Lower Upper
202 100
101 143.4 10.7 16.1#
100 1012.8 8.5 12.7#

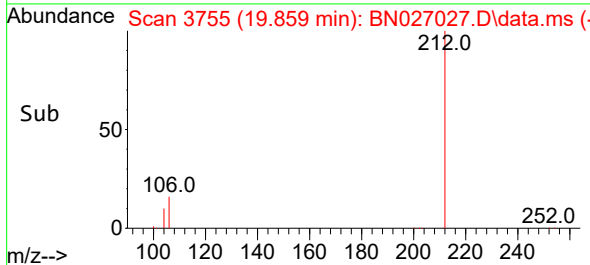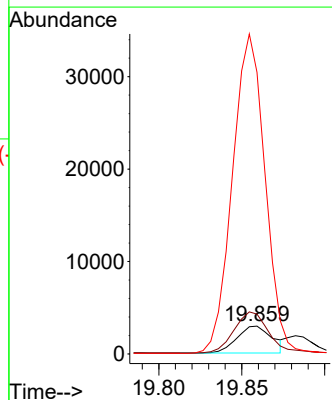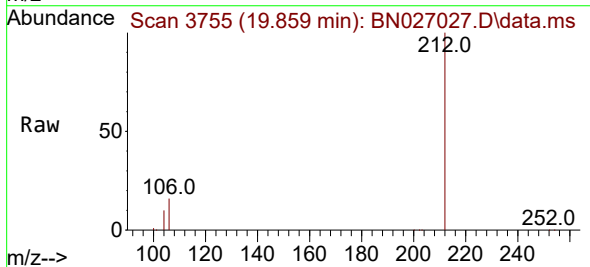

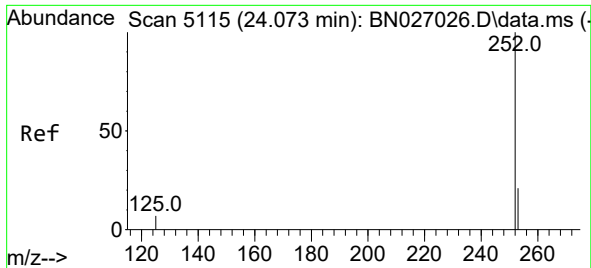

#26
Benzo(a)pyrene
Concen: 0.111 ng/ul
RT: 24.024 min Scan# 5098
Delta R.T. -0.061 min
Lab File: BN027027.D
Acq: 22 Aug 2023 15:18

Instrument :
BNA_N
ClientSampleId :
SBLK935

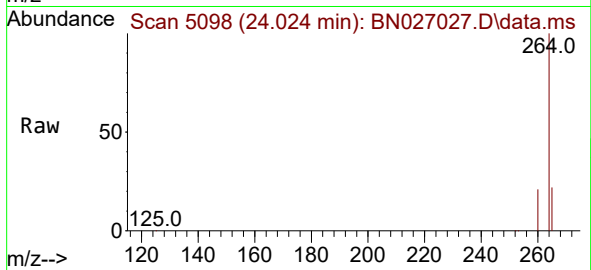

Tgt Ion:252 Resp: 8226
Ion Ratio Lower Upper
252 100
253 45.8 19.0 28.6#
125 46.0 11.4 17.0#

