

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN027039.D
 Acq On : 22 Aug 2023 23:15
 Operator : MA/JU
 Sample : PB154877BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK877

Quant Time: Aug 23 02:29:46 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 23 02:28:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.097	152	7656	0.400	ng/ul	0.00
4) Naphthalene-d8	10.922	136	26269	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.721	164	15209	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.468	188	32451	0.400	ng/ul	0.00
17) Chrysene-d12	21.641	240	21710	0.400	ng/ul	0.00
23) Perylene-d12	24.176	264	21384	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.435	96	54459	5.992	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.495	152	13860	0.359	ng/ul	0.00
18) Fluoranthene-d10	19.483	212	30797	0.449	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.850	202	4688	0.049	ng/ul#	1
26) Benzo(a)pyrene	24.012	252	7050	0.097	ng/ul#	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN027039.D
Acq On : 22 Aug 2023 23:15
Operator : MA/JU
Sample : PB154877BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK877

Quant Time: Aug 23 02:29:46 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 23 02:28:27 2023
Response via : Initial Calibration




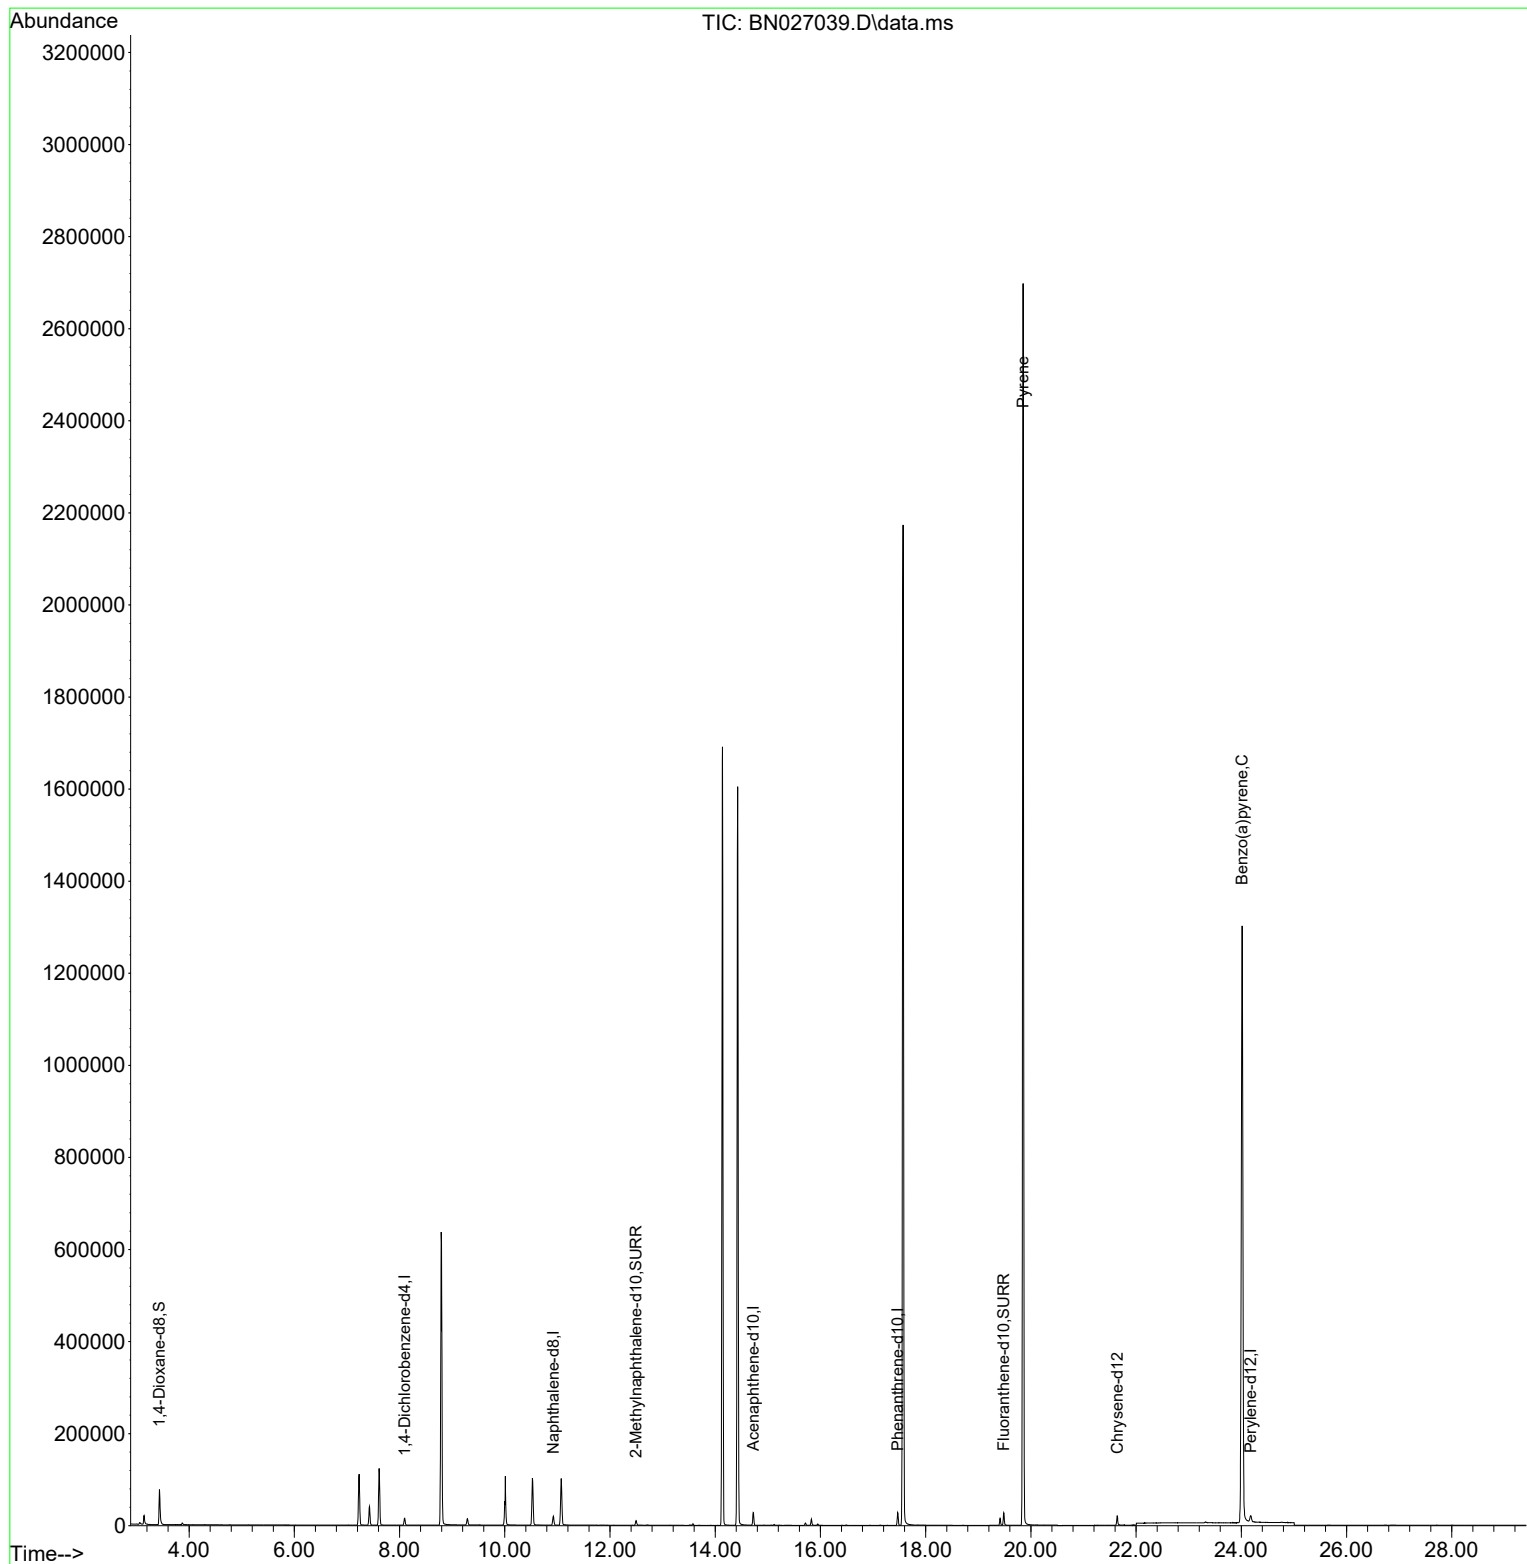


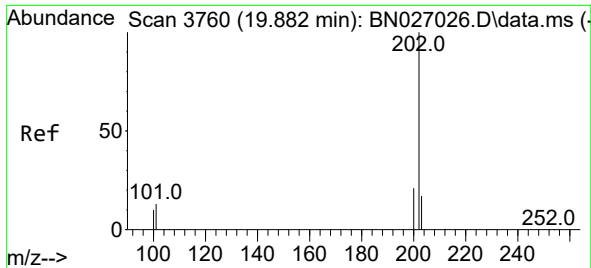

#20
Pyrene
Concen: 0.049 ng/ul
RT: 19.850 min Scan# 31
Delta R.T. -0.033 min
Lab File: BN027039.D
Acq: 22 Aug 2023 23:15

Instrument :
BNA_N
ClientSampleId :
SBLK877

Tgt Ion:202 Resp: 4688
Ion Ratio Lower Upper
202 100
101 151.1 10.7 16.1#
100 1142.1 8.5 12.7#

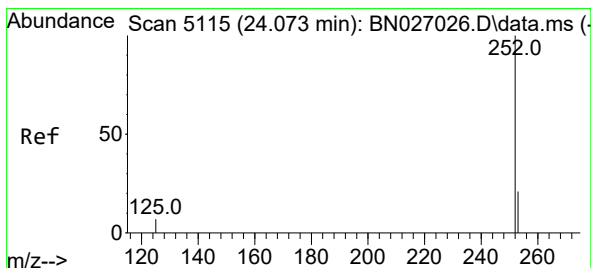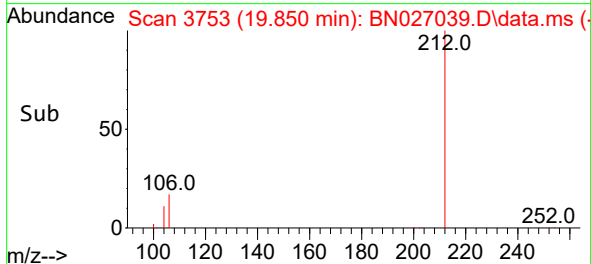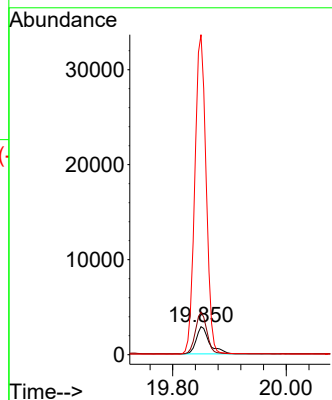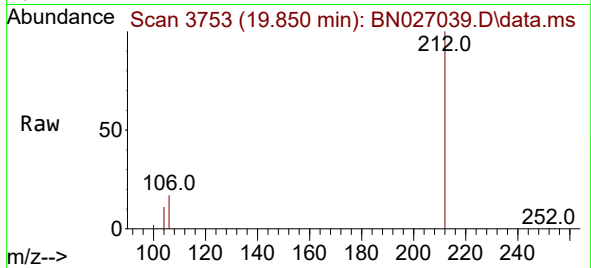

#26
Benzo(a)pyrene
Concen: 0.097 ng/ul
RT: 24.012 min Scan# 5094
Delta R.T. -0.050 min
Lab File: BN027039.D
Acq: 22 Aug 2023 23:15

Tgt Ion:252 Resp: 7050
Ion Ratio Lower Upper
252 100
253 44.1 19.0 28.6#
125 45.6 11.4 17.0#

