

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN027042.D
 Acq On : 23 Aug 2023 01:04
 Operator : MA/JU
 Sample : 04049-02
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH8T5

Quant Time: Aug 23 02:30:07 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 23 02:28:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.093	152	9173	0.400	ng/ul	0.00
4) Naphthalene-d8	10.922	136	31157	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.721	164	18429	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.468	188	39623	0.400	ng/ul	0.00
17) Chrysene-d12	21.638	240	26849	0.400	ng/ul	0.00
23) Perylene-d12	24.179	264	25894	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.439	96	35475	3.258	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.495	152	15280	0.333	ng/ul	0.00
18) Fluoranthene-d10	19.483	212	39665	0.468	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.473	88	30053	2.703	ng/ul#	91
20) Pyrene	19.855	202	6015	0.051	ng/ul#	1
26) Benzo(a)pyrene	24.015	252	9399	0.106	ng/ul#	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN027042.D
Acq On : 23 Aug 2023 01:04
Operator : MA/JU
Sample : 04049-02
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH8T5

Quant Time: Aug 23 02:30:07 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 23 02:28:27 2023
Response via : Initial Calibration




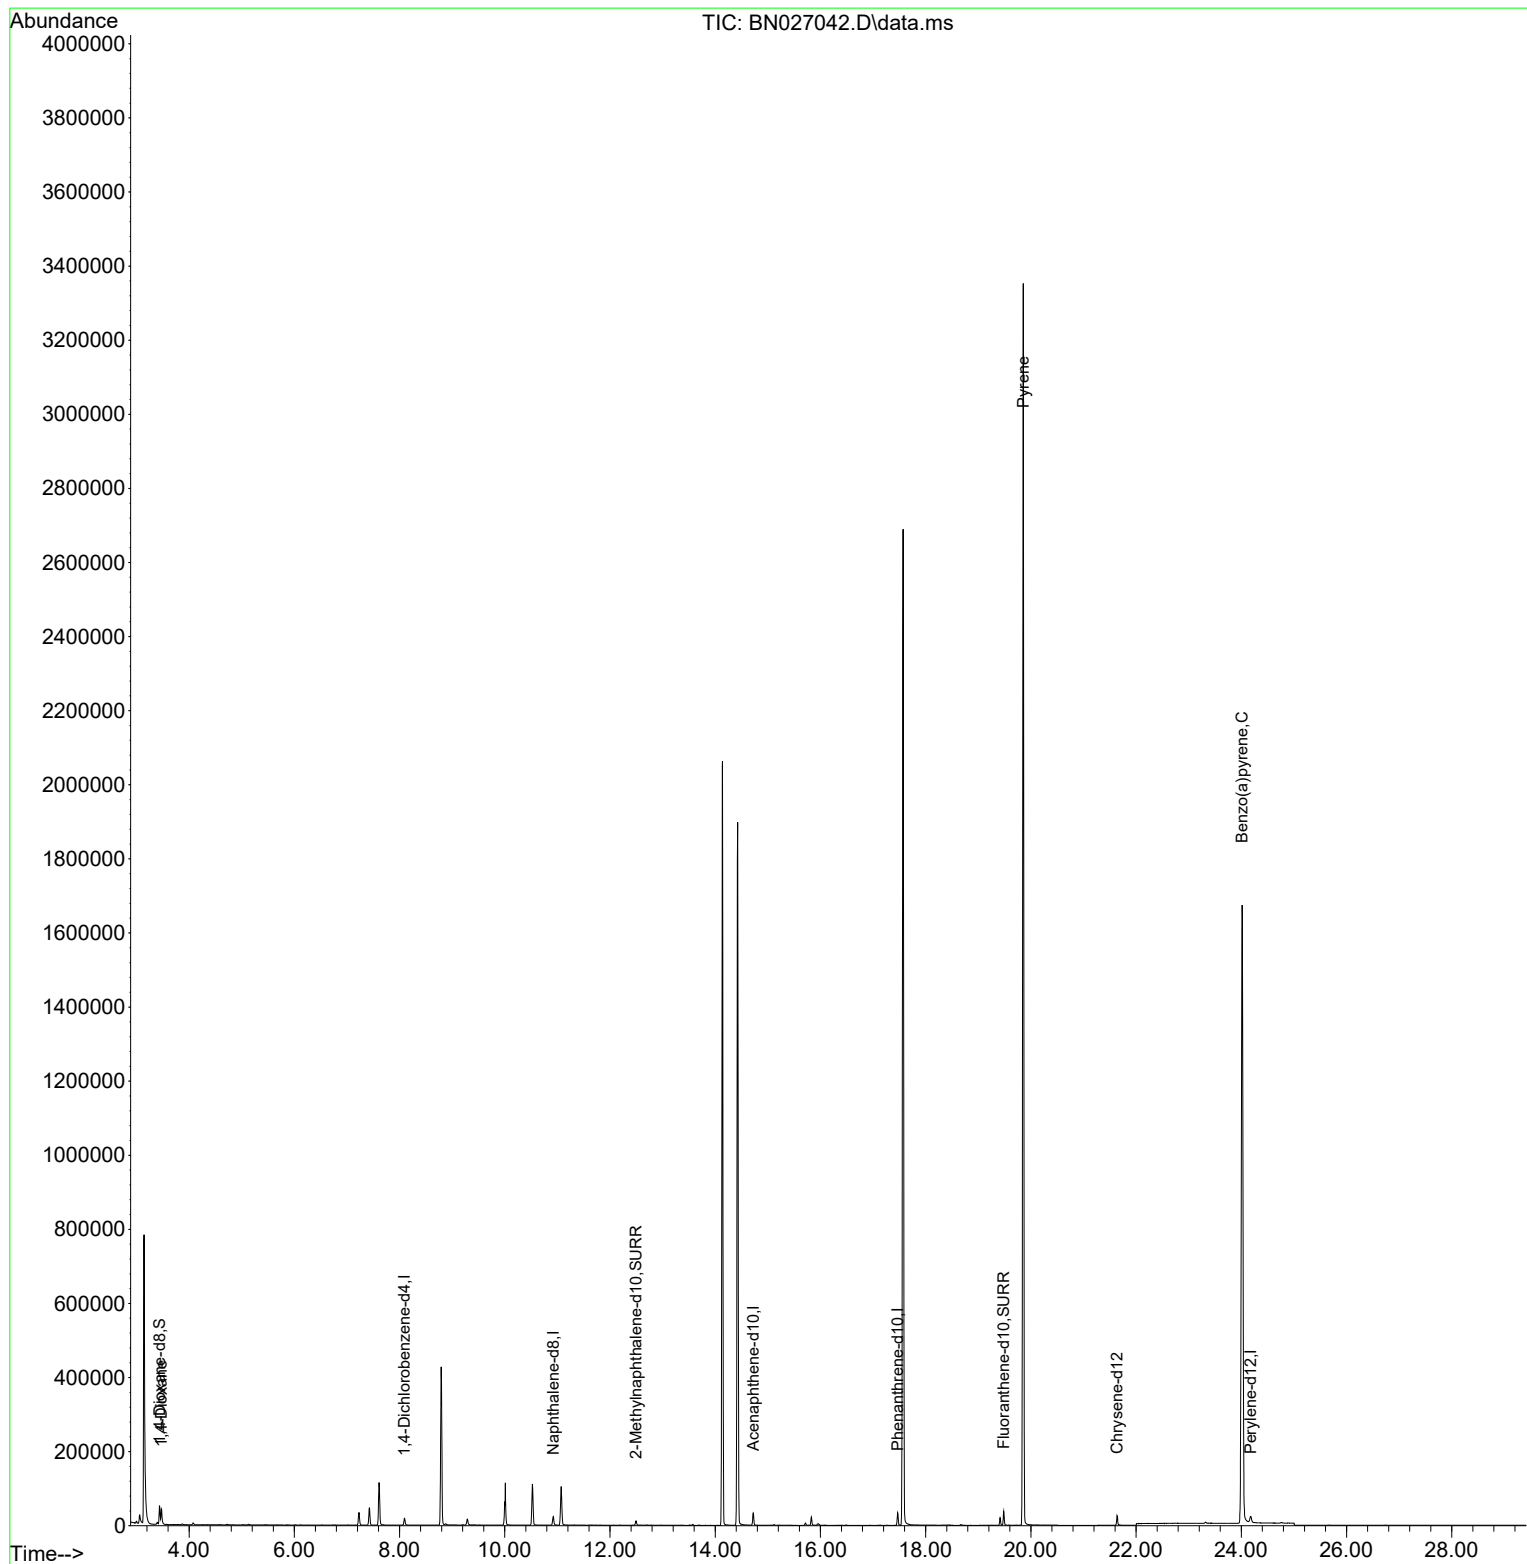


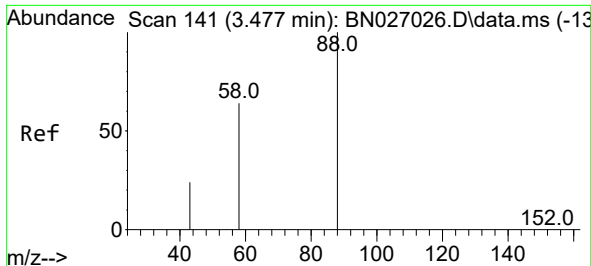

#2
1,4-Dioxane
Concen: 2.703 ng/ul
RT: 3.473 min Scan# 141
Delta R.T. -0.004 min
Lab File: BN027042.D
Acq: 23 Aug 2023 01:04




Instrument :
BNA_N
ClientSampleId :
BH8T5


Tgt Ion: 88 Resp: 30053
Ion Ratio Lower Upper
88 100
43 26.9 28.0 42.0#
58 61.6 46.0 69.0

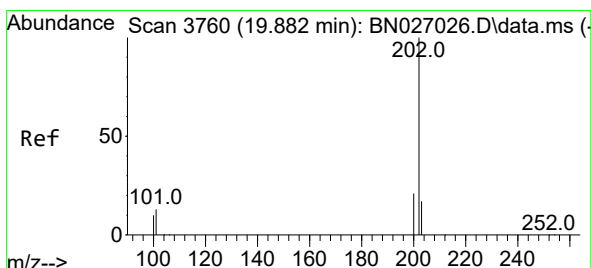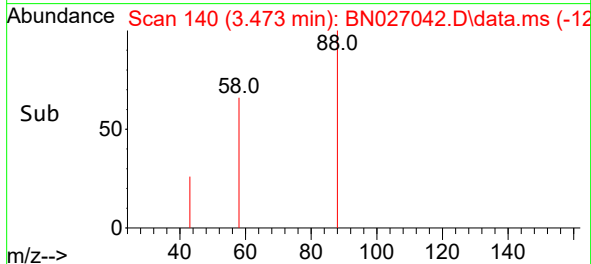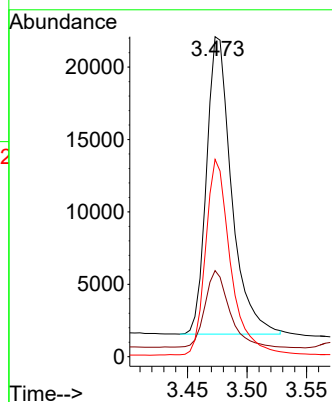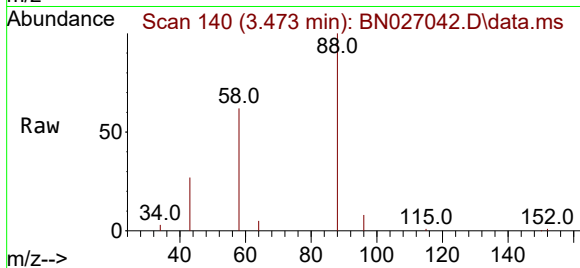

#20
Pyrene
Concen: 0.051 ng/ul
RT: 19.855 min Scan# 3754
Delta R.T. -0.028 min
Lab File: BN027042.D
Acq: 23 Aug 2023 01:04


Tgt Ion: 202 Resp: 6015
Ion Ratio Lower Upper
202 100
101 148.1 10.7 16.1#
100 1081.5 8.5 12.7#

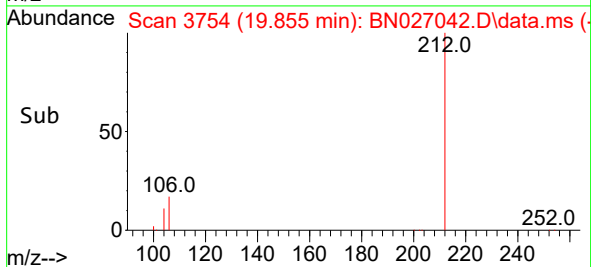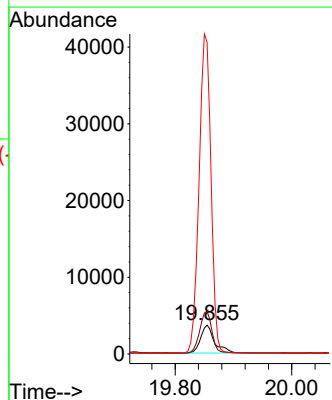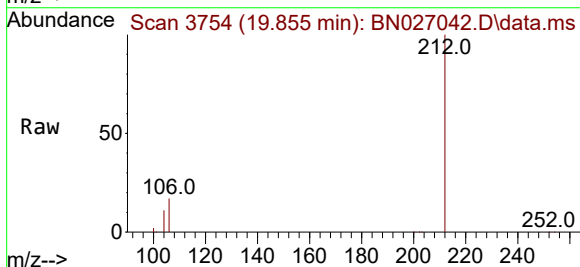

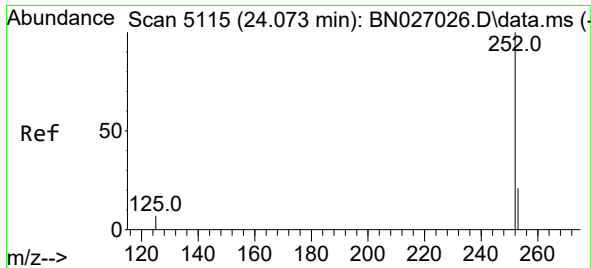

#26
Benzo(a)pyrene
Concen: 0.106 ng/ul
RT: 24.015 min Scan# 5095
Delta R.T. -0.047 min
Lab File: BN027042.D
Acq: 23 Aug 2023 01:04

Instrument :
BNA_N
ClientSampleId :
BH8T5

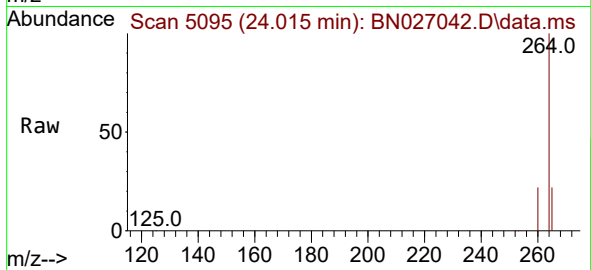

Tgt Ion:252 Resp: 9399
Ion Ratio Lower Upper
252 100
253 42.8 19.0 28.6#
125 42.7 11.4 17.0#

