

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN027058.D
 Acq On : 23 Aug 2023 11:17
 Operator : MA/JU
 Sample : 04034-03
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EZYX2

Quant Time: Aug 24 01:37:51 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 23 02:28:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.093	152	7505	0.400	ng/ul	0.00
4) Naphthalene-d8	10.916	136	25938	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.721	164	15512	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.468	188	33455	0.400	ng/ul	0.00
17) Chrysene-d12	21.638	240	22541	0.400	ng/ul	0.00
23) Perylene-d12	24.175	264	21986	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.435	96	37927	4.257	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.489	152	14280	0.374	ng/ul	0.00
18) Fluoranthene-d10	19.482	212	35550	0.499	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.850	202	4928	0.049	ng/ul#	1
26) Benzo(a)pyrene	24.012	252	7792	0.104	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN027058.D
Acq On : 23 Aug 2023 11:17
Operator : MA/JU
Sample : 04034-03
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EZYX2

Quant Time: Aug 24 01:37:51 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 23 02:28:27 2023
Response via : Initial Calibration

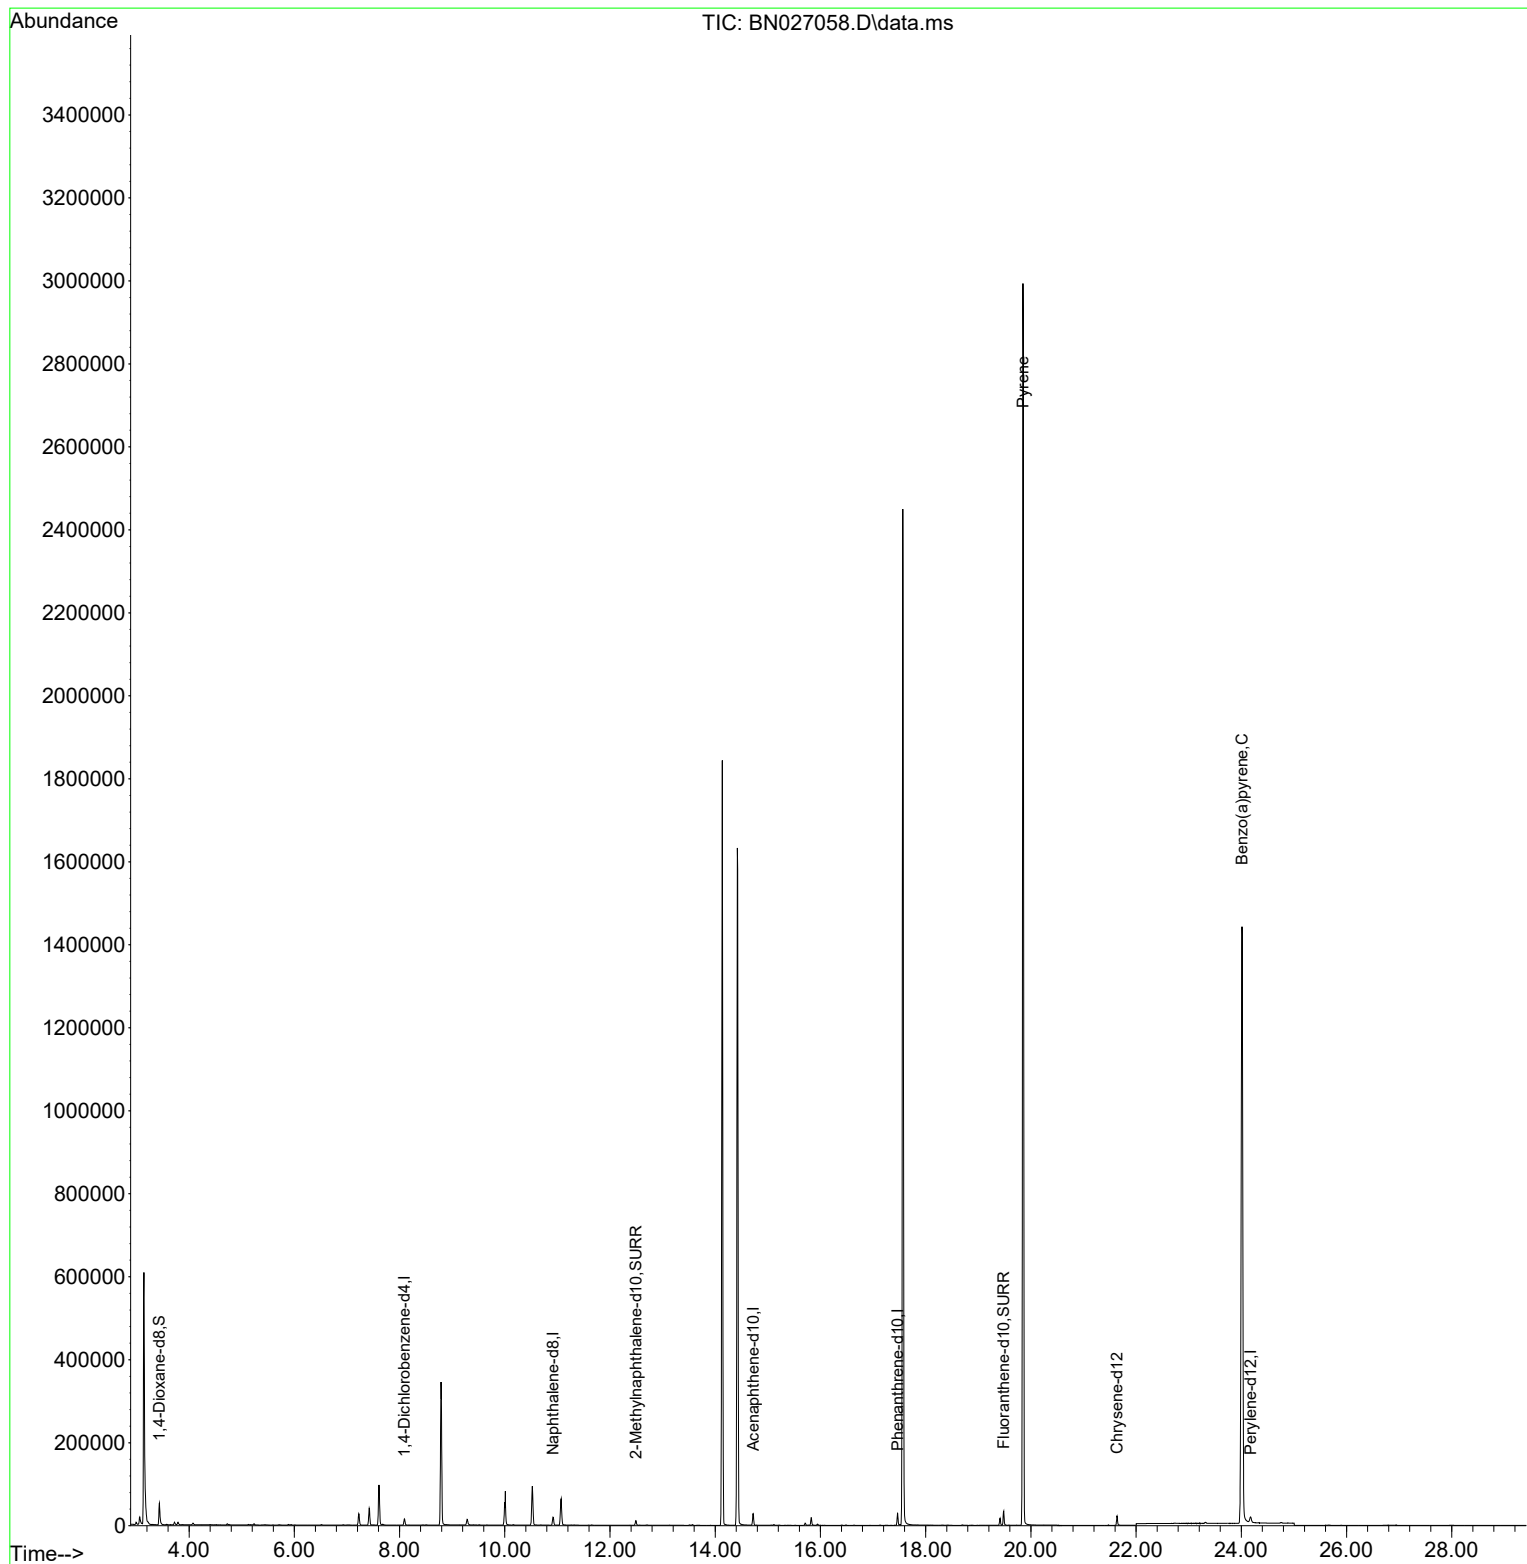

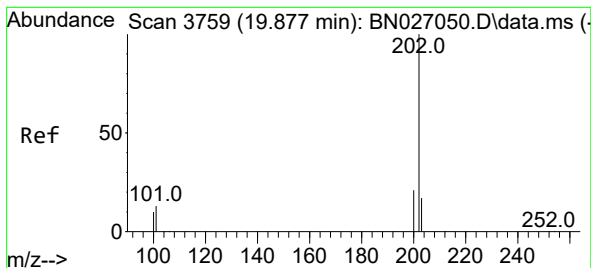

#20

Pyrene

Concen: 0.049 ng/ul

RT: 19.850 min Scan# 31

Delta R.T. -0.033 min

Lab File: BN027058.D

Acq: 23 Aug 2023 11:17

Instrument :

BNA_N

ClientSampleId :

EZYX2





Tgt Ion:202 Resp: 4928

Ion Ratio Lower Upper

202 100

101 151.7 10.7 16.1#

100 1157.0 8.5 12.7#

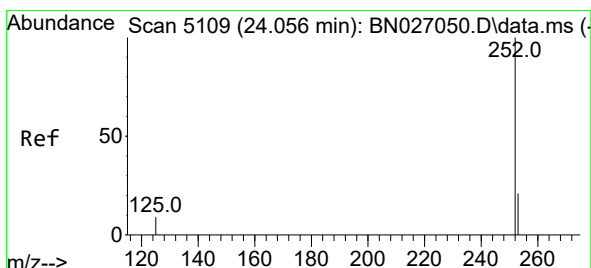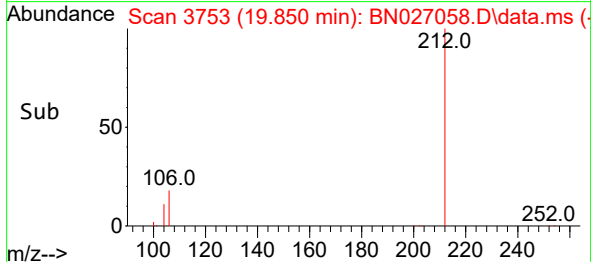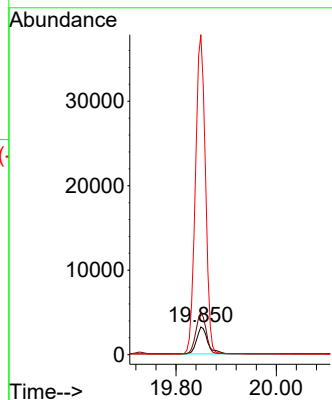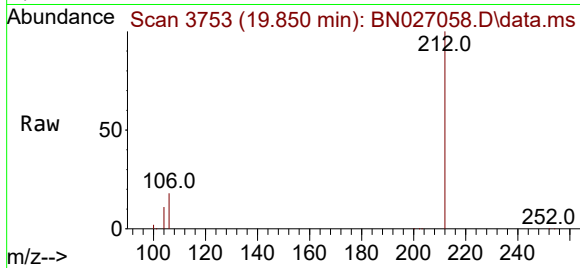

#26

Benzo(a)pyrene

Concen: 0.104 ng/ul

RT: 24.012 min Scan# 5094

Delta R.T. -0.050 min

Lab File: BN027058.D

Acq: 23 Aug 2023 11:17

Tgt Ion:252 Resp: 7792

Ion Ratio Lower Upper

252 100

253 42.8 19.0 28.6#

125 44.0 11.4 17.0#

