

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN027059.D
 Acq On : 23 Aug 2023 11:54
 Operator : MA/JU
 Sample : 04034-06
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EZYN6

Quant Time: Aug 24 01:37:57 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 23 02:28:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.093	152	6993	0.400	ng/ul	0.00
4) Naphthalene-d8	10.916	136	25609	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.721	164	14938	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.464	188	31392	0.400	ng/ul	0.00
17) Chrysene-d12	21.638	240	19780	0.400	ng/ul	0.00
23) Perylene-d12	24.176	264	19112	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.435	96	34323	4.134	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.489	152	12629	0.335	ng/ul	0.00
18) Fluoranthene-d10	19.483	212	29313	0.469	ng/ul	0.00
Target Compounds						
					Qvalue	
11) Acenaphthene	14.777	153	1367	0.024	ng/ul#	34
20) Pyrene	19.850	202	4335	0.049	ng/ul#	1
26) Benzo(a)pyrene	24.009	252	6405	0.098	ng/ul#	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN027059.D
Acq On : 23 Aug 2023 11:54
Operator : MA/JU
Sample : 04034-06
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EZY6

Quant Time: Aug 24 01:37:57 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 23 02:28:27 2023
Response via : Initial Calibration




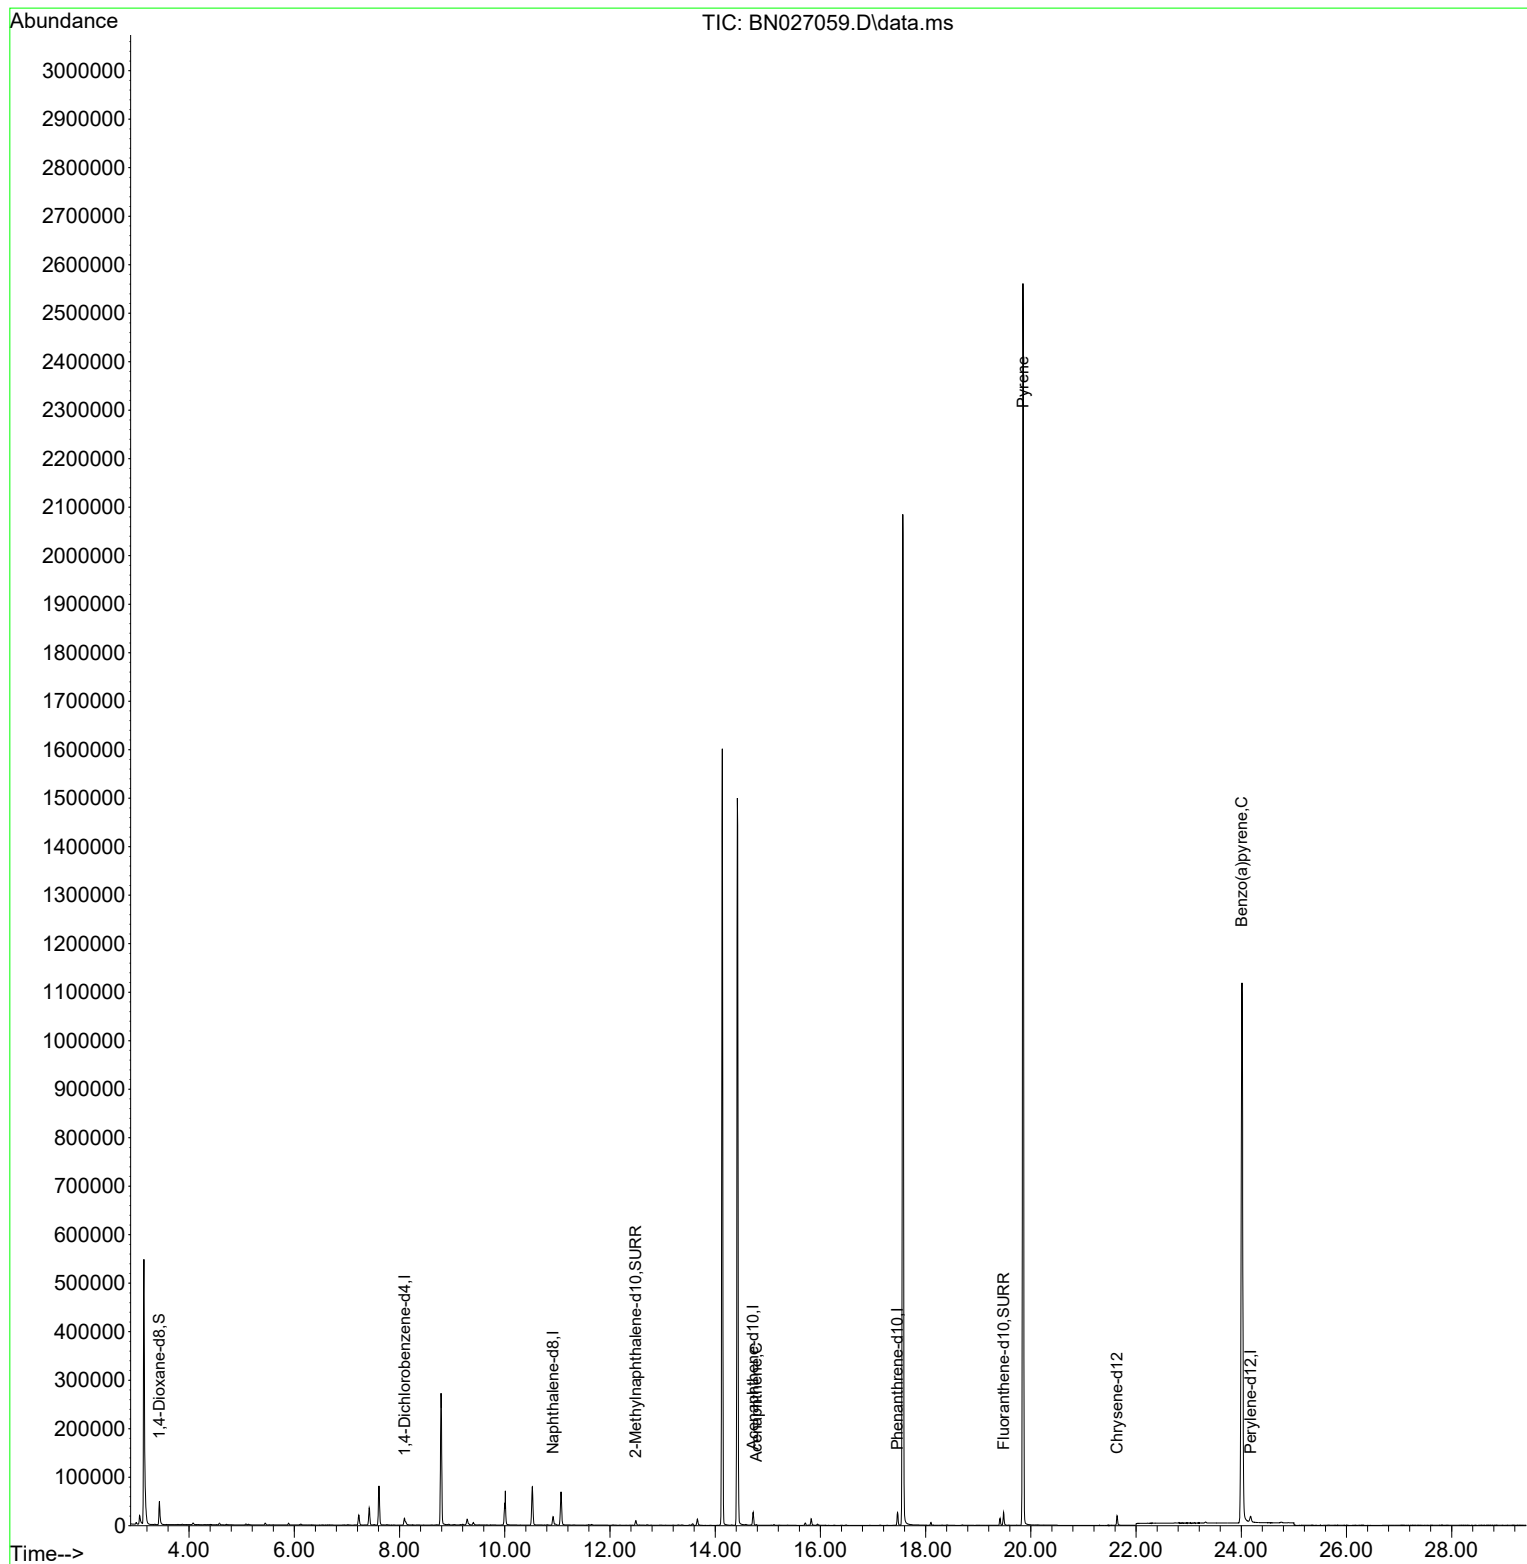


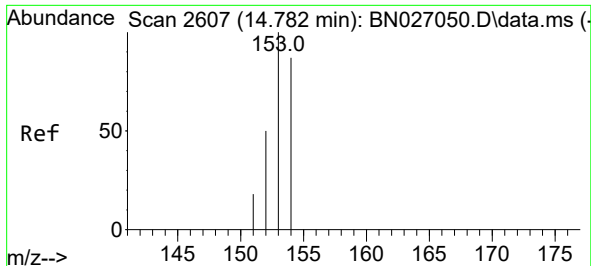

#11
Acenaphthene
Concen: 0.024 ng/ul
RT: 14.777 min Scan# 2606
Delta R.T. -0.009 min
Lab File: BN027059.D
Acq: 23 Aug 2023 11:54




Instrument :
BNA_N
ClientSampleId :
EZYN6


Tgt Ion:153 Resp: 1367
Ion Ratio Lower Upper
153 100
152 12.7 41.1 61.7#
154 21.4 71.6 107.4#

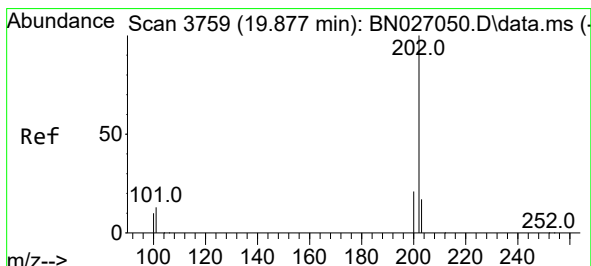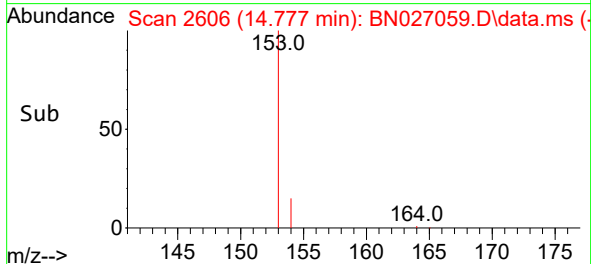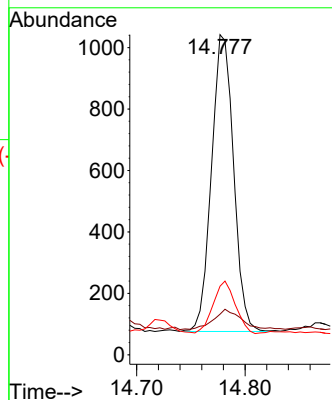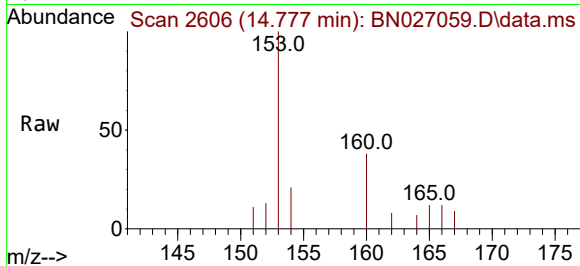

#20
Pyrene
Concen: 0.049 ng/ul
RT: 19.850 min Scan# 3753
Delta R.T. -0.033 min
Lab File: BN027059.D
Acq: 23 Aug 2023 11:54


Tgt Ion:202 Resp: 4335
Ion Ratio Lower Upper
202 100
101 156.8 10.7 16.1#
100 1177.4 8.5 12.7#

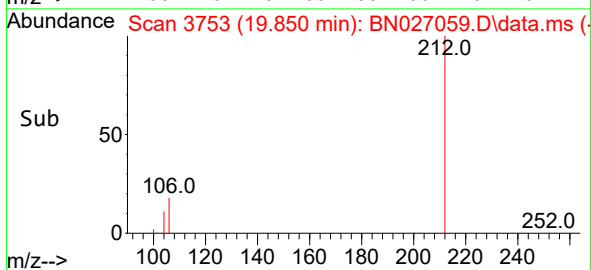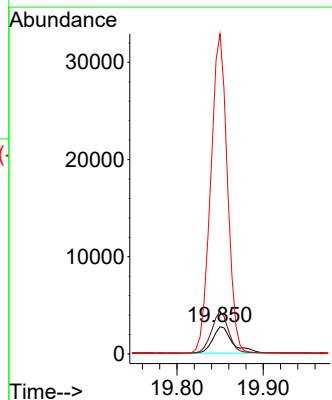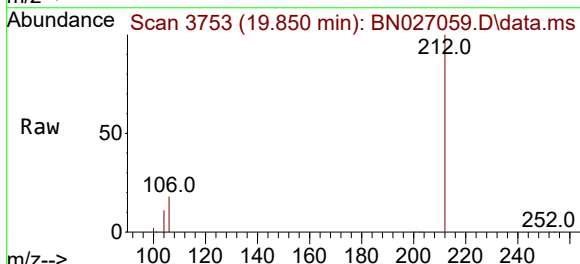

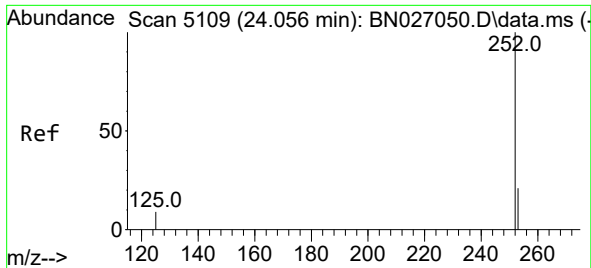

#26
Benzo(a)pyrene
Concen: 0.098 ng/ul
RT: 24.009 min Scan# 5093
Delta R.T. -0.053 min
Lab File: BN027059.D
Acq: 23 Aug 2023 11:54

Instrument :
BNA_N
ClientSampleId :
EZYN6

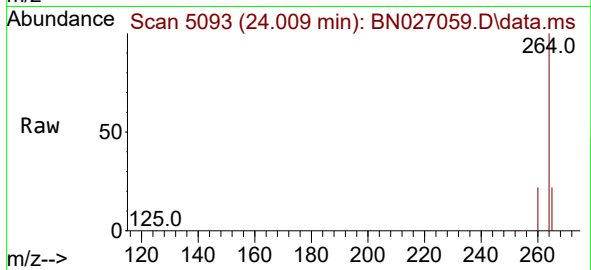

Tgt Ion:252 Resp: 6405
Ion Ratio Lower Upper
252 100
253 45.5 19.0 28.6#
125 51.6 11.4 17.0#

