

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN027070.D
 Acq On : 23 Aug 2023 20:19
 Operator : MA/JU
 Sample : 03902-01
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH315

Quant Time: Aug 24 01:39:41 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 23 02:28:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.093	152	8091	0.400	ng/ul	0.00
4) Naphthalene-d8	10.916	136	26093	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.721	164	15783	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.464	188	35164	0.400	ng/ul	0.00
17) Chrysene-d12	21.638	240	26398	0.400	ng/ul	0.00
23) Perylene-d12	24.176	264	28534	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.435	96	46310	4.821	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.489	152	11888	0.310	ng/ul	0.00
18) Fluoranthene-d10	19.483	212	32393	0.389	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.473	88	7075	0.721	ng/ul	92
20) Pyrene	19.850	202	5153	0.044	ng/ul#	1
26) Benzo(a)pyrene	24.015	252	9915	0.102	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN027070.D
Acq On : 23 Aug 2023 20:19
Operator : MA/JU
Sample : 03902-01
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH315

Quant Time: Aug 24 01:39:41 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 23 02:28:27 2023
Response via : Initial Calibration




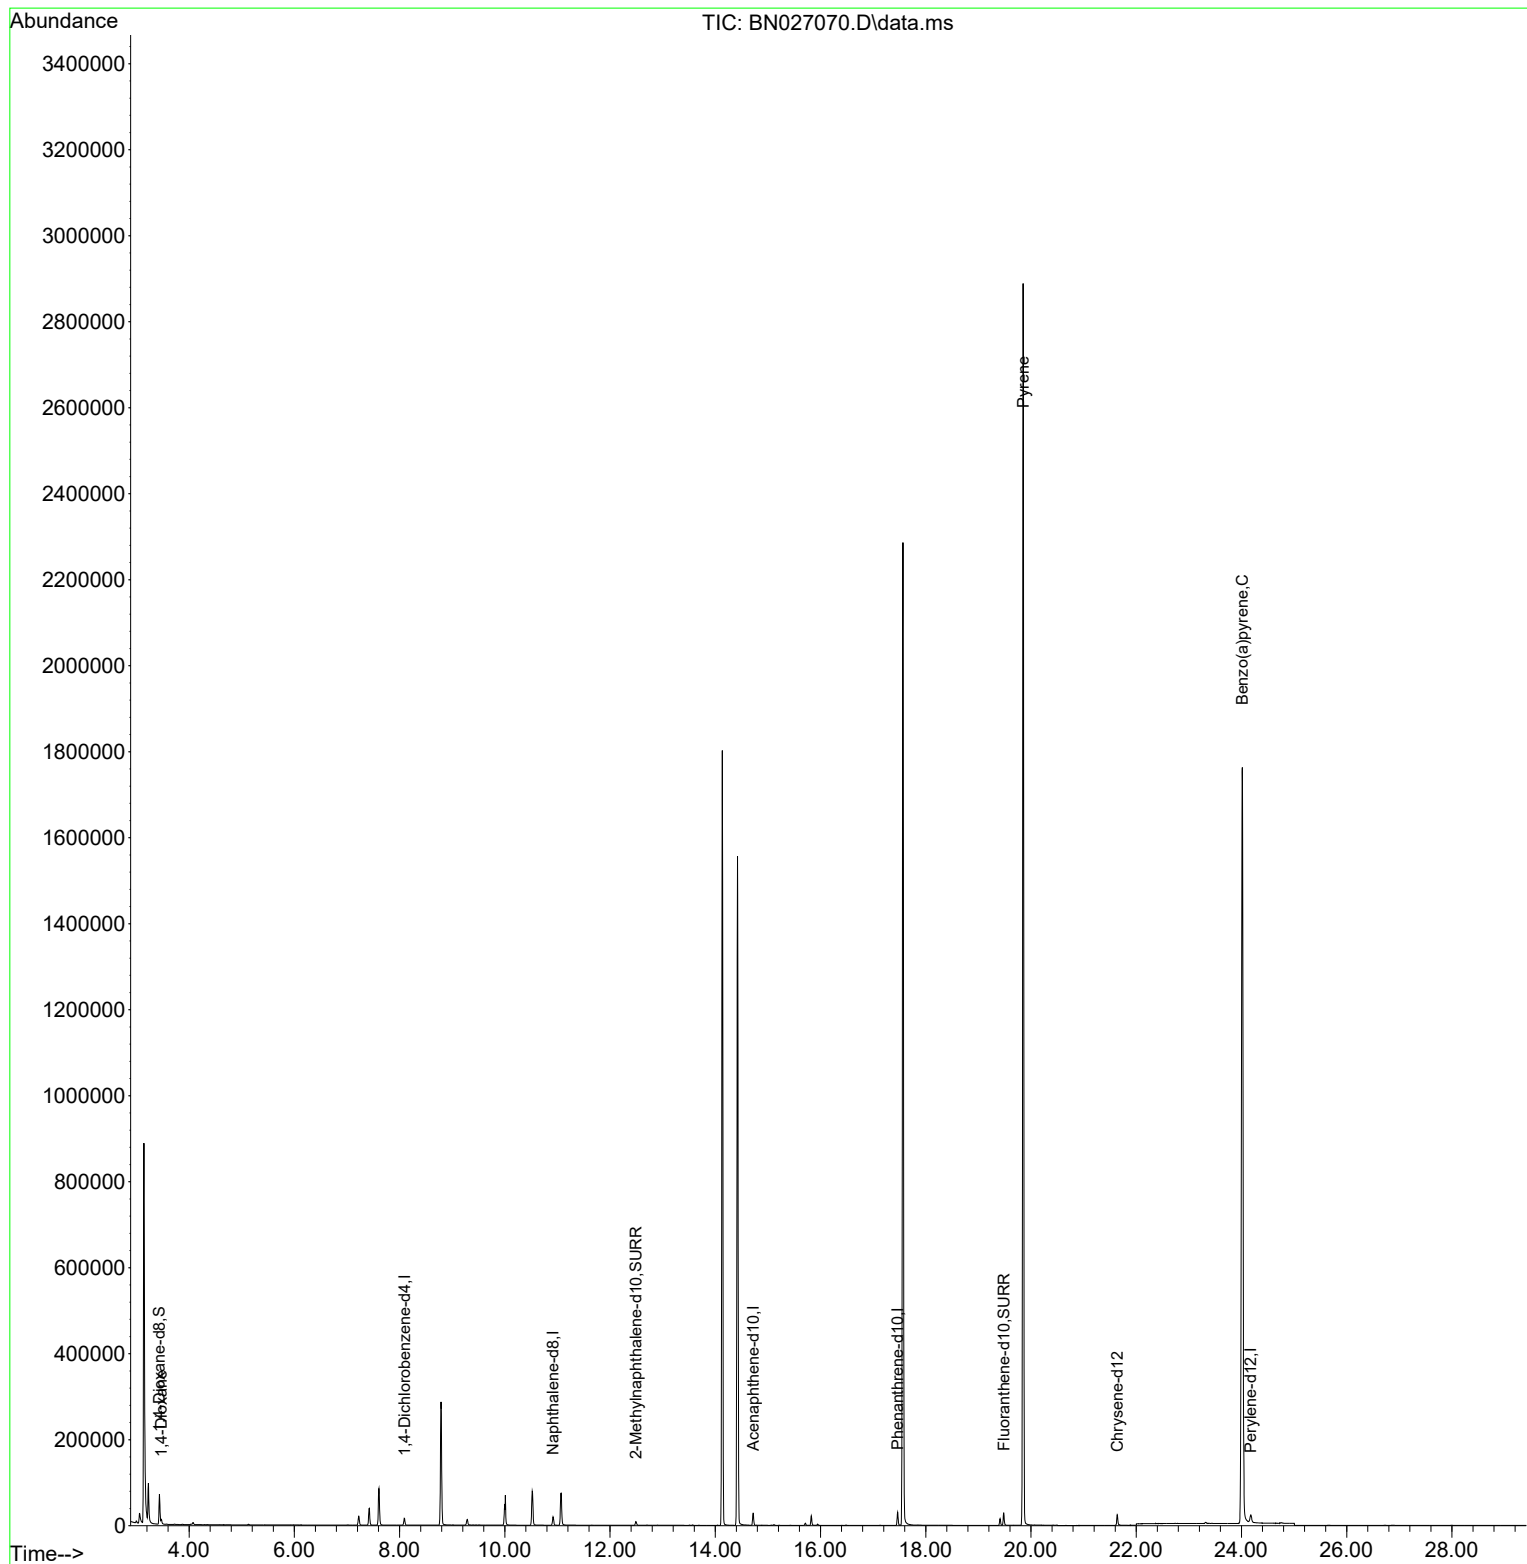


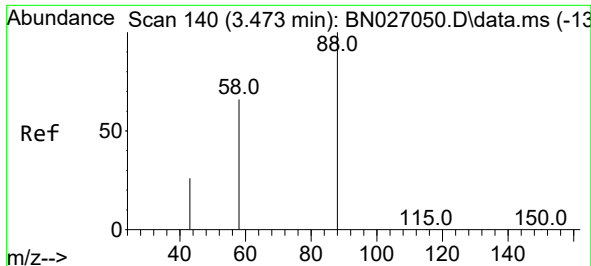

#2
1,4-Dioxane
Concen: 0.721 ng/ul
RT: 3.473 min Scan# 140
Delta R.T. -0.004 min
Lab File: BN027070.D
Acq: 23 Aug 2023 20:19




Instrument :
BNA_N
ClientSampleId :
BH315


Tgt Ion: 88 Resp: 7075
Ion Ratio Lower Upper
88 100
43 31.4 28.0 42.0
58 51.1 46.0 69.0

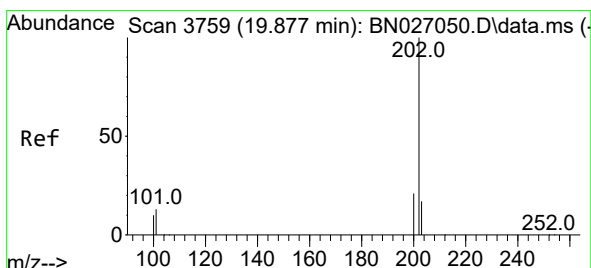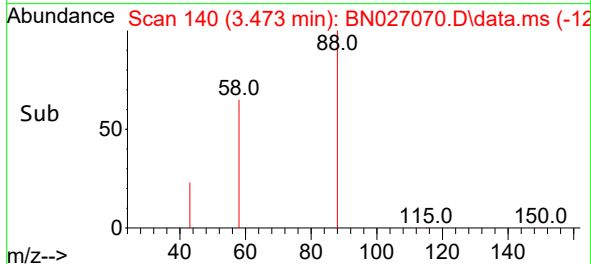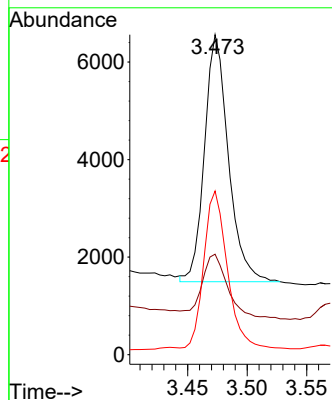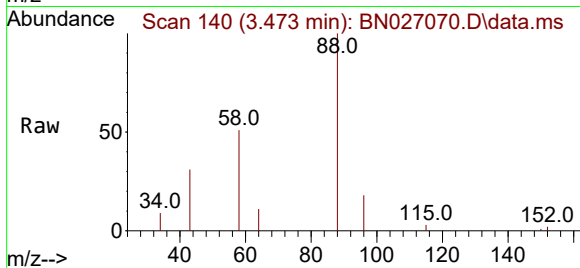

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.850 min Scan# 3753
Delta R.T. -0.033 min
Lab File: BN027070.D
Acq: 23 Aug 2023 20:19


Tgt Ion: 202 Resp: 5153
Ion Ratio Lower Upper
202 100
101 154.3 10.7 16.1#
100 1161.4 8.5 12.7#

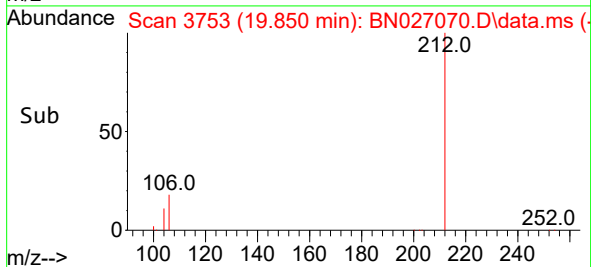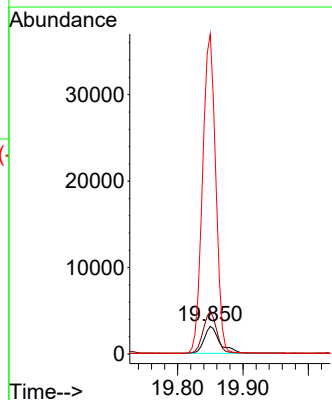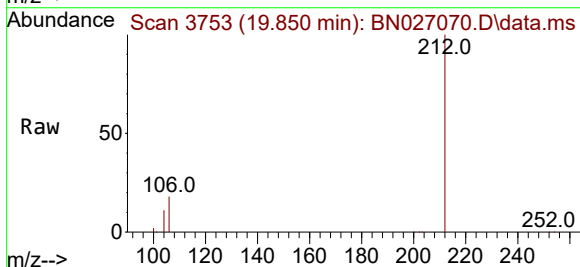

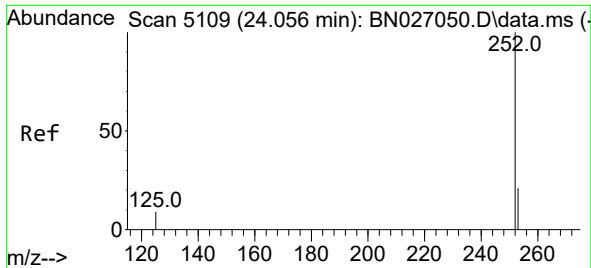

#26
Benzo(a)pyrene
Concen: 0.102 ng/ul
RT: 24.015 min Scan# 5095
Delta R.T. -0.047 min
Lab File: BN027070.D
Acq: 23 Aug 2023 20:19

Instrument :
BNA_N
ClientSampleId :
BH315

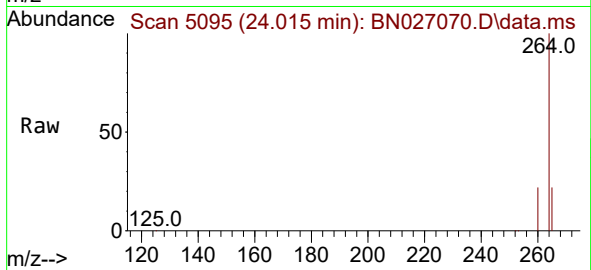

Tgt Ion:252 Resp: 9915
Ion Ratio Lower Upper
252 100
253 40.4 19.0 28.6#
125 37.5 11.4 17.0#

