

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN026995.D
 Acq On : 21 Aug 2023 16:32
 Operator : MA/JU
 Sample : 03967-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A48K5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/22/2023
 Supervised By :mohammad ahmed 08/22/2023

Quant Time: Aug 22 01:39:12 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 18 13:11:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.101	152	7391	0.400	ng/ul	0.00
4) Naphthalene-d8	10.927	136	24634	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.731	164	13985	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.472	188	31716	0.400	ng/ul	0.00
17) Chrysene-d12	21.650	240	26544	0.400	ng/ul	0.00
23) Perylene-d12	24.193	264	27530	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.439	96	24868	2.834	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.500	152	5130	0.142	ng/ul	0.00
18) Fluoranthene-d10	19.492	212	12138	0.145	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.982	128	1981	0.028	ng/ul#	84
10) Acenaphthylene	14.458	152	3149	0.040	ng/ul#	93
15) Phenanthrene	17.515	178	23136	0.222	ng/ul	99
16) Anthracene	17.607	178	3953m	0.042	ng/ul	
19) Fluoranthene	19.520	202	70597	0.640	ng/ul	97
20) Pyrene	19.887	202	62230m	0.529	ng/ul	
21) Benzo(a)anthracene	21.635	228	28161	0.267	ng/ul	97
22) Chrysene	21.691	228	38589	0.370	ng/ul	97
24) Benzo(b)fluoranthene	23.404	252	55640m	0.534	ng/ul	
25) Benzo(k)fluoranthene	23.454	252	19193m	0.187	ng/ul	
26) Benzo(a)pyrene	24.082	252	30888	0.329	ng/ul#	92
27) Indeno(1,2,3-cd)pyrene	26.884	276	23696	0.193	ng/ul#	86
28) Dibenzo(a,h)anthracene	26.908	278	5199	0.053	ng/ul#	60
29) Benzo(g,h,i)perylene	27.723	276	24307	0.238	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN026995.D
Acq On : 21 Aug 2023 16:32
Operator : MA/JU
Sample : 03967-05
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A48K5

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/22/2023
Supervised By :mohammad ahmed 08/22/2023


Quant Time: Aug 22 01:39:12 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 18 13:11:26 2023
Response via : Initial Calibration

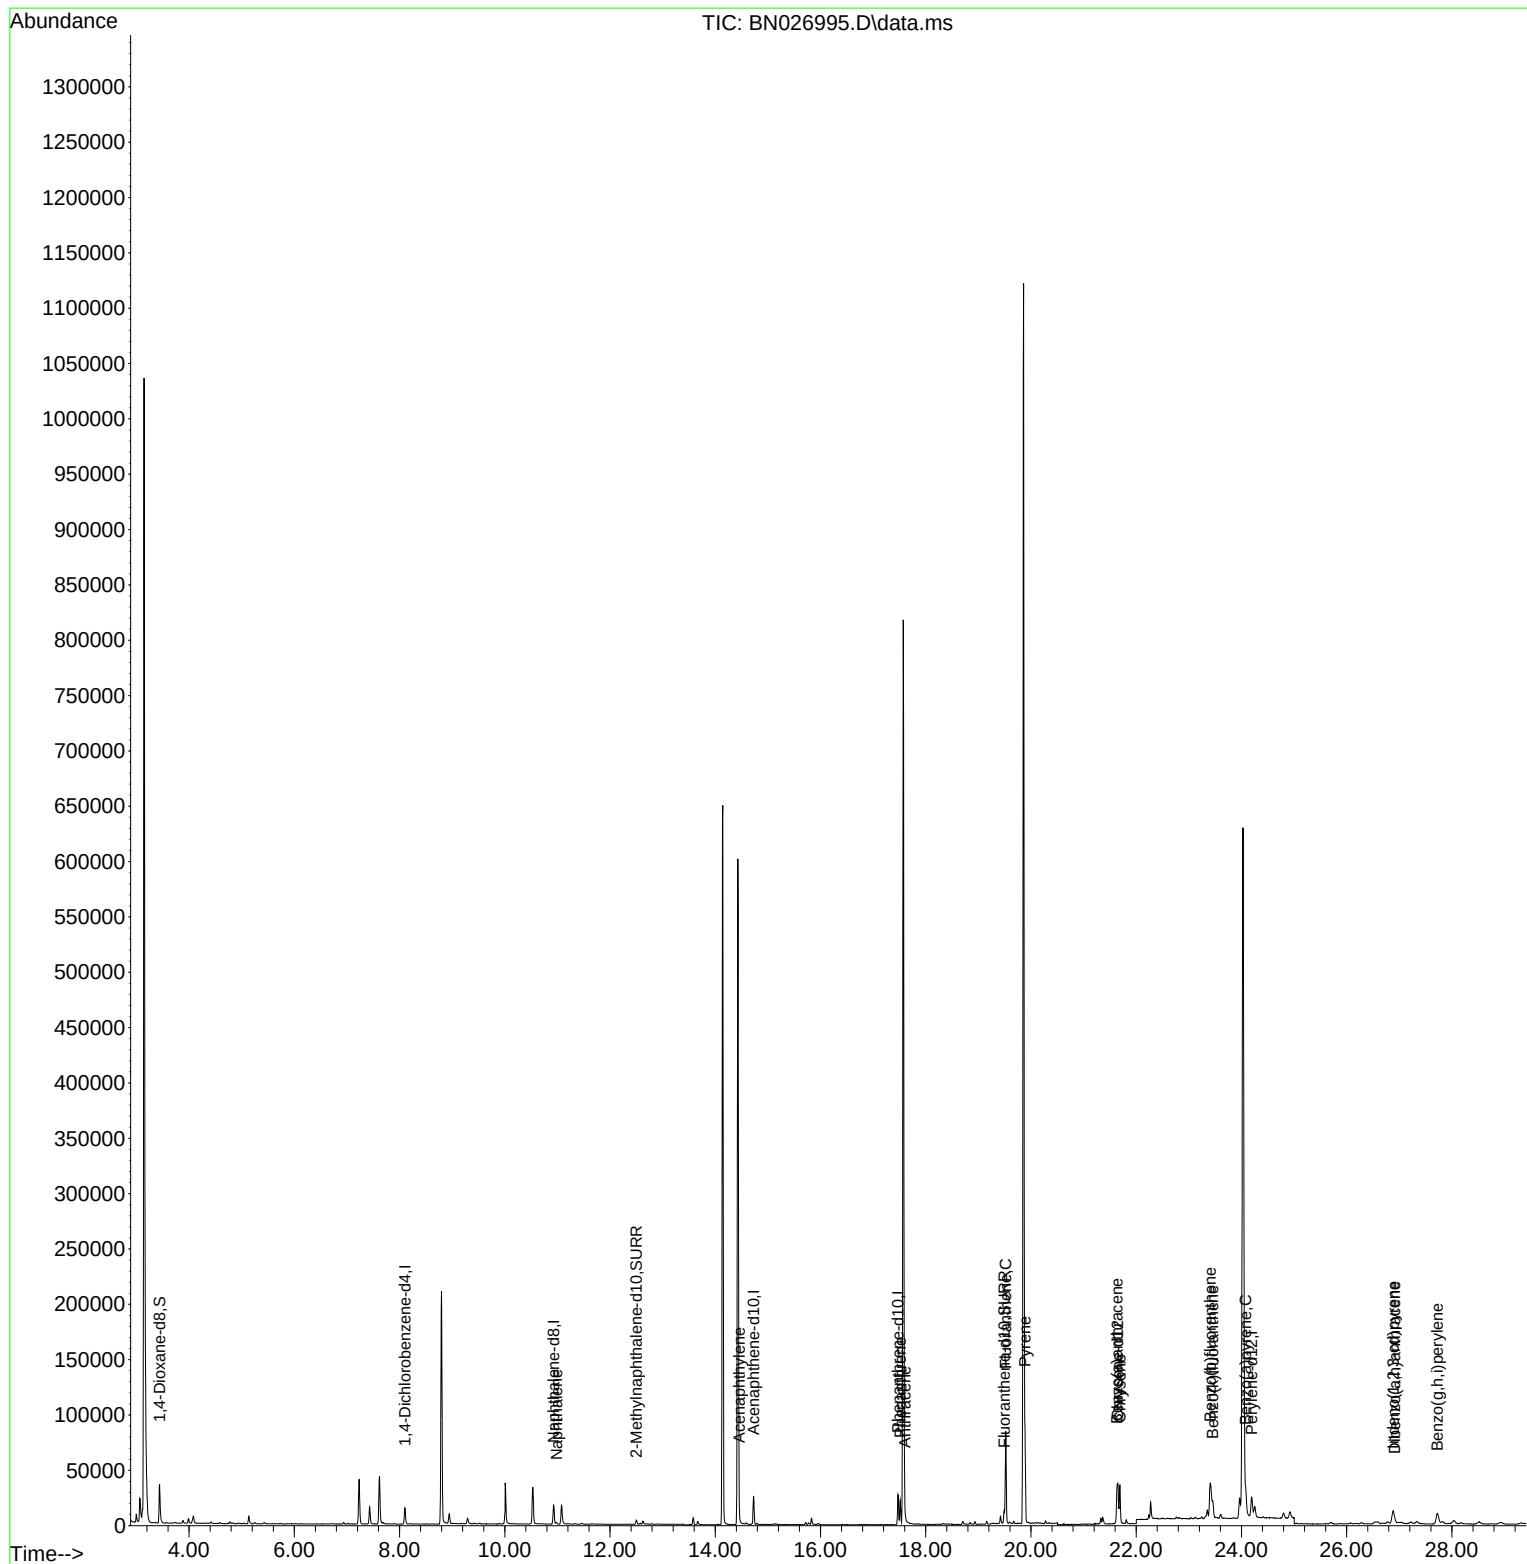

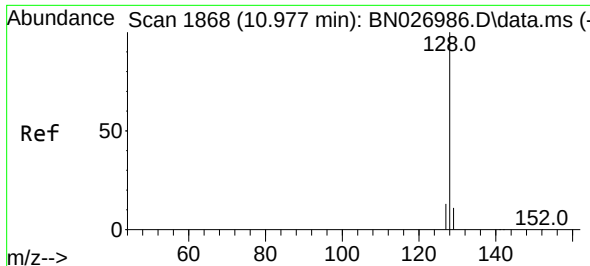

#5
Naphthalene
Concen: 0.028 ng/ul
RT: 10.982 min Scan# 1869
Delta R.T. -0.000 min
Lab File: BN026995.D
Acq: 21 Aug 2023 16:32




Instrument :
BNA_N
ClientSampleId :
A48K5

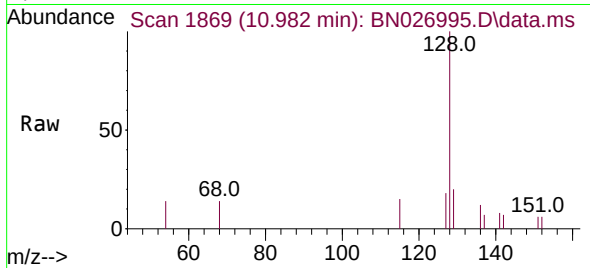

Tgt Ion:128 Resp: 1981
Ion Ratio Lower Upper
128 100
129 20.0 9.2 13.8
127 17.7 10.5 15.7




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/22/2023
Supervised By :mohammad ahmed 08/22/2023

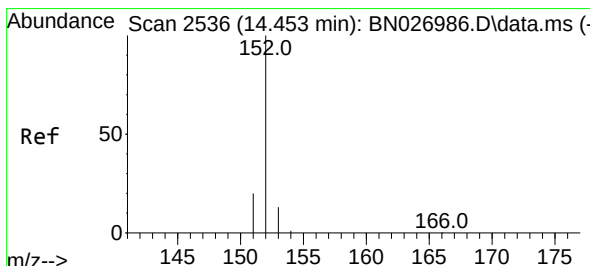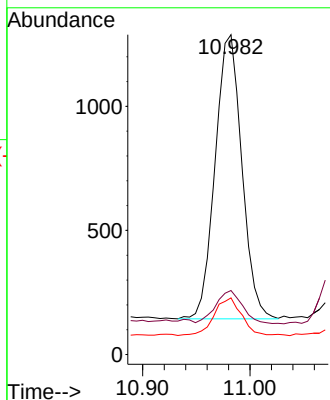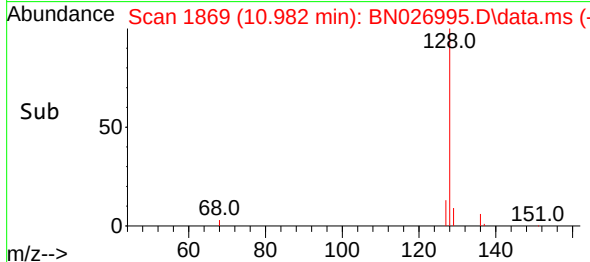

#10
Acenaphthylene
Concen: 0.040 ng/ul
RT: 14.458 min Scan# 2537
Delta R.T. -0.000 min
Lab File: BN026995.D
Acq: 21 Aug 2023 16:32


Tgt Ion:152 Resp: 3149
Ion Ratio Lower Upper
152 100
151 22.9 15.9 23.9
153 17.2 11.0 16.6

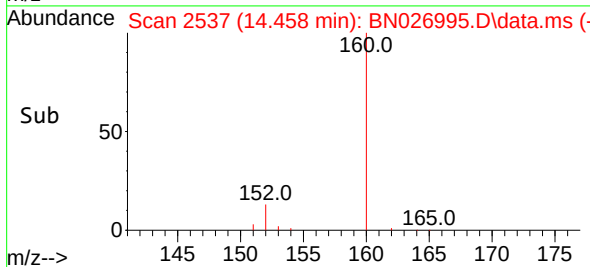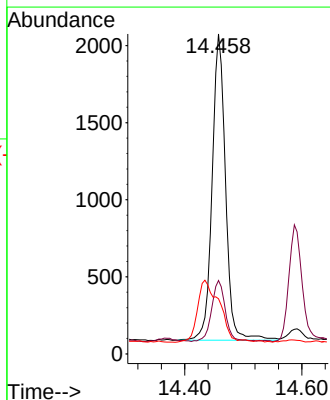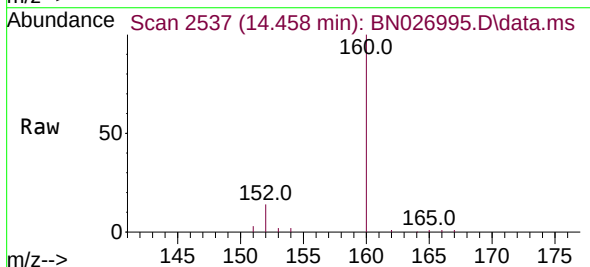

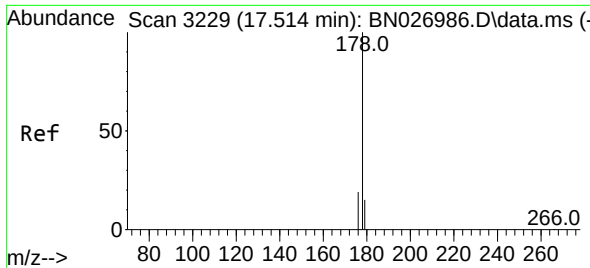

#15
Phenanthrene
Concen: 0.222 ng/ul
RT: 17.515 min Scan# 3229
Delta R.T. -0.004 min
Lab File: BN026995.D
Acq: 21 Aug 2023 16:32




Instrument :
BNA_N
ClientSampleId :
A48K5

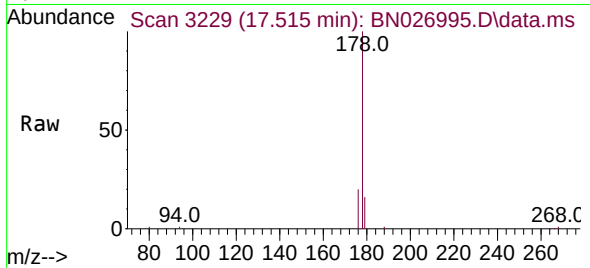

Tgt Ion:178 Resp: 23136
Ion Ratio Lower Upper
178 100
179 15.9 12.6 18.8
176 19.7 15.4 23.2




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/22/2023
Supervised By :mohammad ahmed 08/22/2023

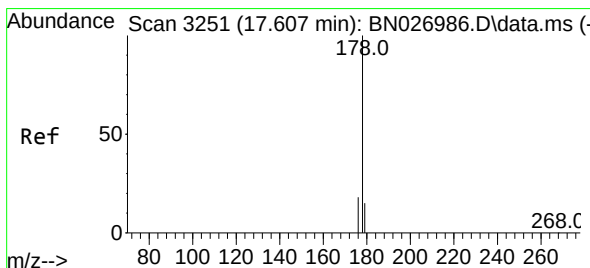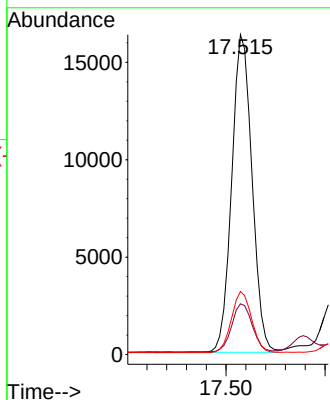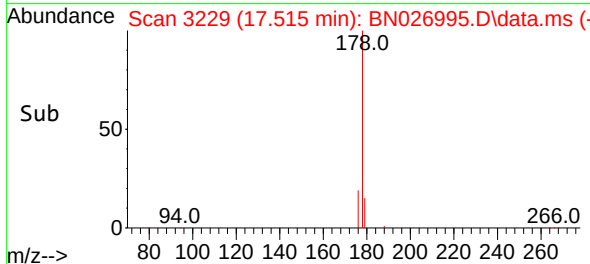

#16
Anthracene
Concen: 0.042 ng/ul m
RT: 17.607 min Scan# 3251
Delta R.T. -0.000 min
Lab File: BN026995.D
Acq: 21 Aug 2023 16:32


Tgt Ion:178 Resp: 3953
Ion Ratio Lower Upper
178 100
179 20.5 12.6 19.0#
176 21.3 15.0 22.6

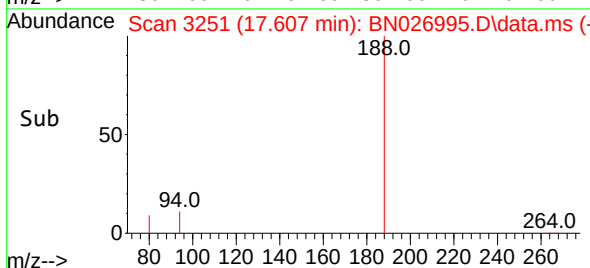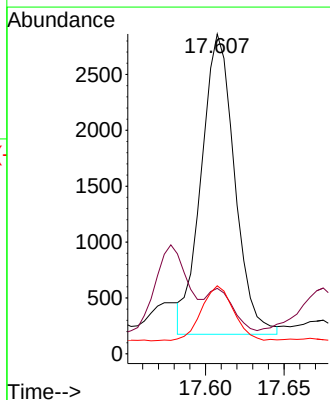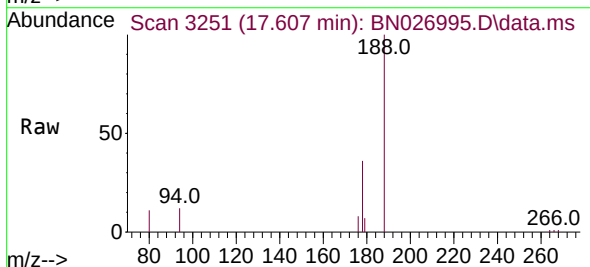

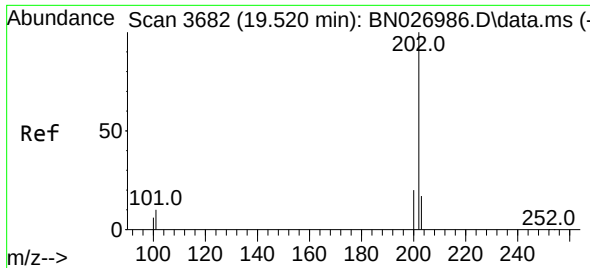

#19
Fluoranthene
Concen: 0.640 ng/ul
RT: 19.520 min Scan# 3682
Delta R.T. -0.005 min
Lab File: BN026995.D
Acq: 21 Aug 2023 16:32




Instrument :
BNA_N
ClientSampleId :
A48K5

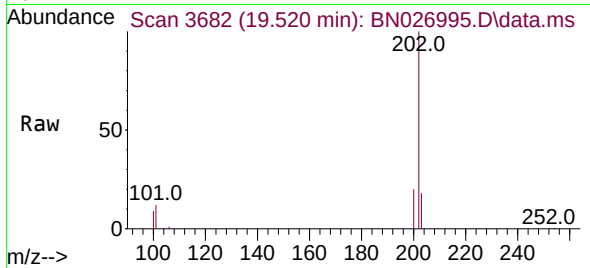


Tgt Ion:202 Resp: 70592
Ion Ratio Lower Upper
202 100
101 11.7 8.3 12.5
100 8.5 6.2 9.2

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 08/22/2023
Supervised By :mohammad ahmed 08/22/2023

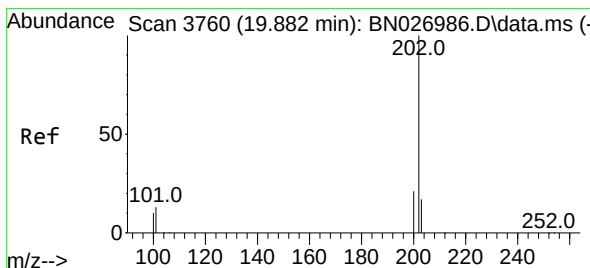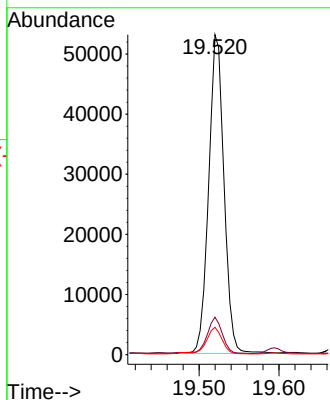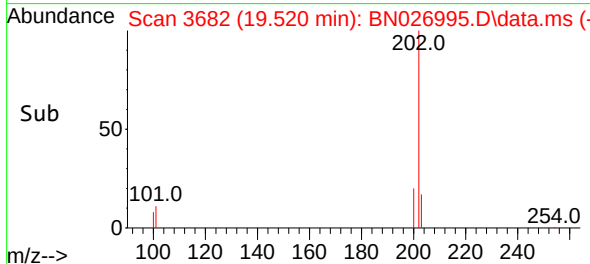


#20
Pyrene
Concen: 0.529 ng/ul m
RT: 19.887 min Scan# 3761
Delta R.T. -0.000 min
Lab File: BN026995.D
Acq: 21 Aug 2023 16:32

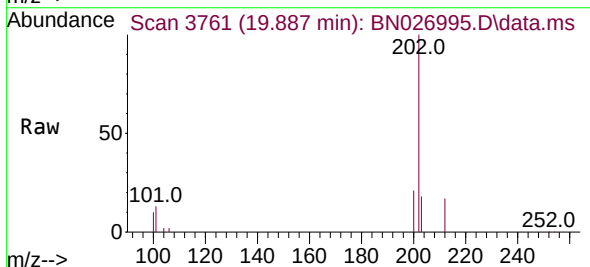


Tgt Ion:202 Resp: 62230
Ion Ratio Lower Upper
202 100
101 13.2 10.7 16.1
100 10.4 8.5 12.7

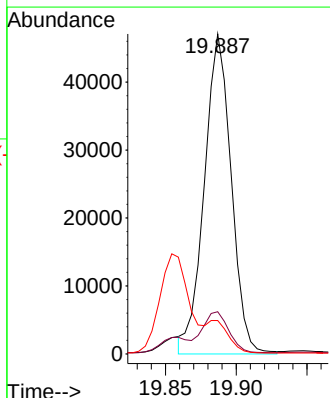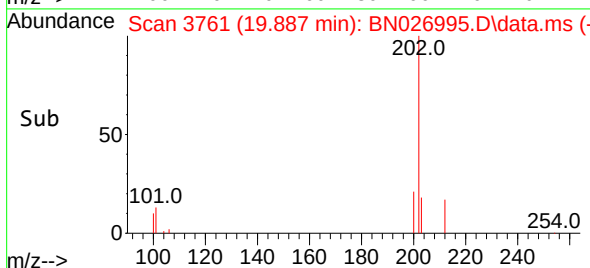

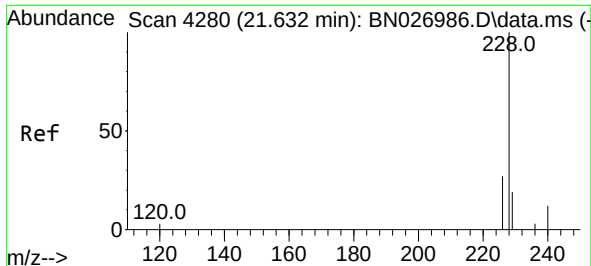

#21
Benzo(a)anthracene
Concen: 0.267 ng/ul
RT: 21.635 min Scan# 4300
Delta R.T. 0.003 min
Lab File: BN026995.D
Acq: 21 Aug 2023 16:32




Instrument :
BNA_N
ClientSampleId :
A48K5

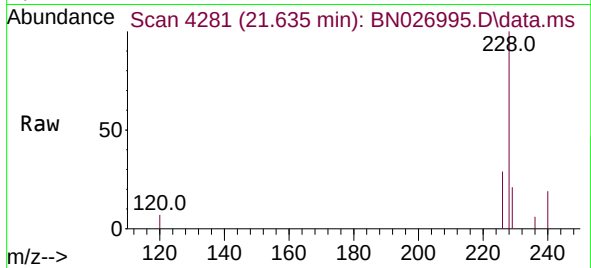


Tgt Ion:228 Resp: 28163
Ion Ratio Lower Upper
228 100
229 21.4 16.0 24.0
226 28.8 22.2 33.2

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 08/22/2023
Supervised By :mohammad ahmed 08/22/2023

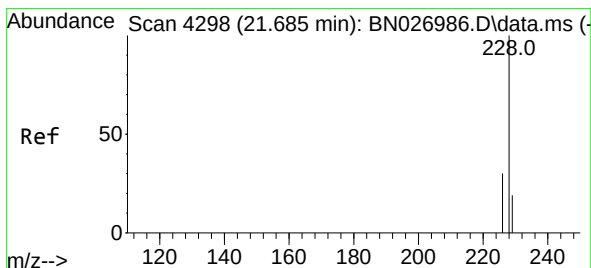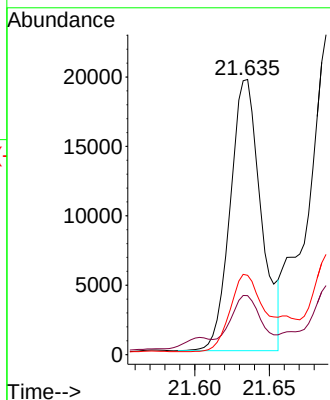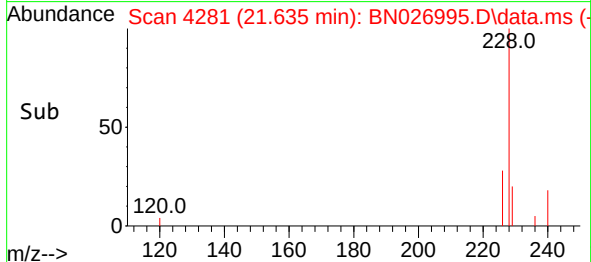


#22
Chrysene
Concen: 0.370 ng/ul
RT: 21.691 min Scan# 4300
Delta R.T. -0.000 min
Lab File: BN026995.D
Acq: 21 Aug 2023 16:32

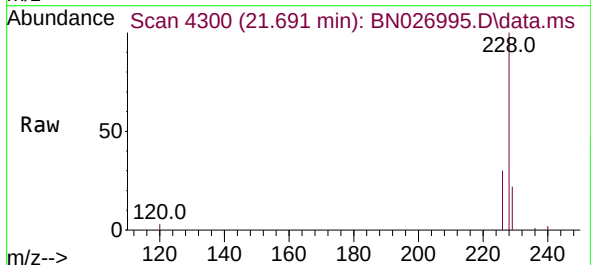


Tgt Ion:228 Resp: 38589
Ion Ratio Lower Upper
228 100
226 30.1 24.6 36.8
229 22.0 15.8 23.6

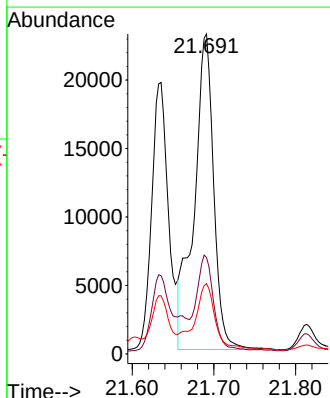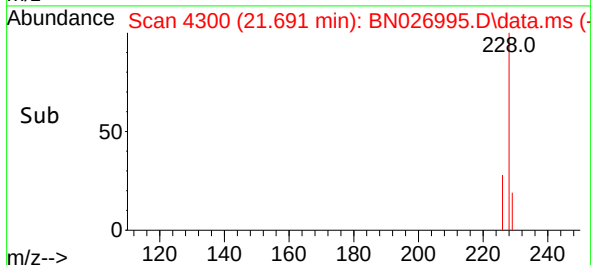

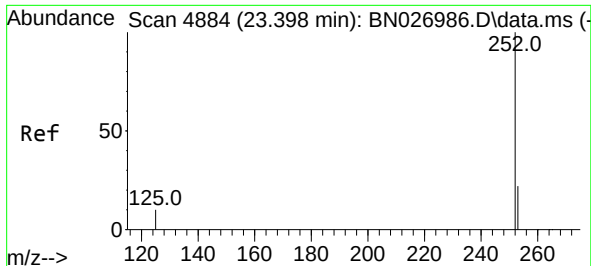

#24
Benzo(b)fluoranthene
Concen: 0.534 ng/ul m
RT: 23.404 min Scan# 4886
Delta R.T. -0.003 min
Lab File: BN026995.D
Acq: 21 Aug 2023 16:32




Instrument :
BNA_N
ClientSampleId :
A48K5

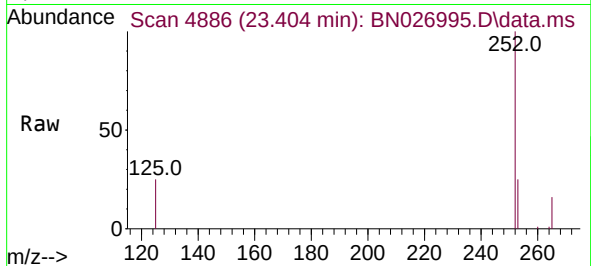

Tgt Ion:252 Resp: 55640
Ion Ratio Lower Upper
252 100
253 25.2 0.0 46.8
125 25.1 0.0 25.2




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/22/2023
Supervised By :mohammad ahmed 08/22/2023

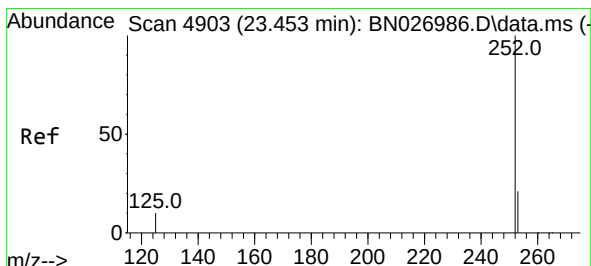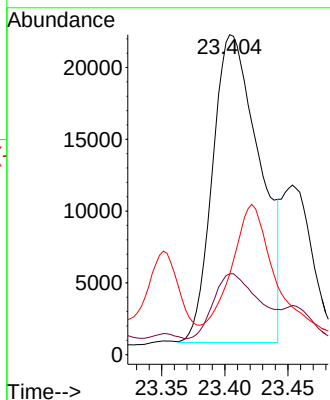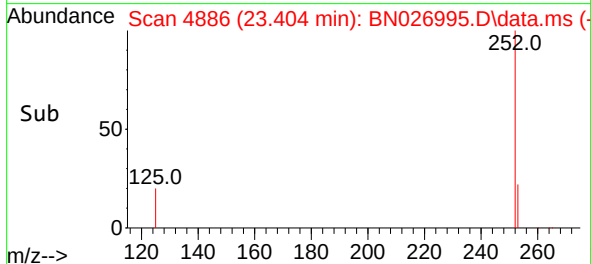

#25
Benzo(k)fluoranthene
Concen: 0.187 ng/ul m
RT: 23.454 min Scan# 4903
Delta R.T. -0.006 min
Lab File: BN026995.D
Acq: 21 Aug 2023 16:32

Tgt Ion:252 Resp: 19193
Ion Ratio Lower Upper
252 100
253 29.0 18.2 27.4#
125 28.1 9.9 14.9#

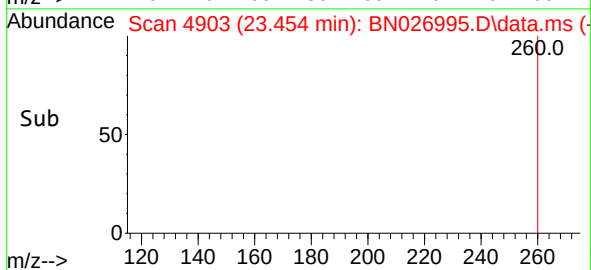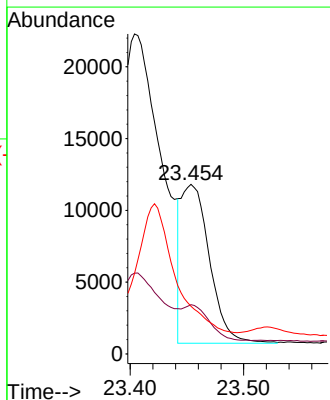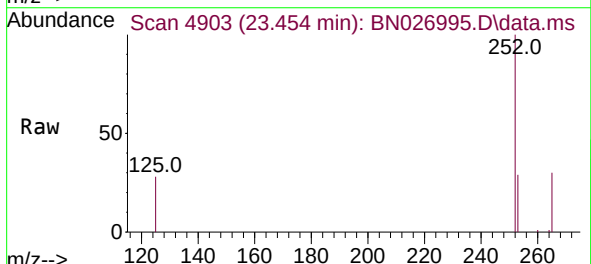

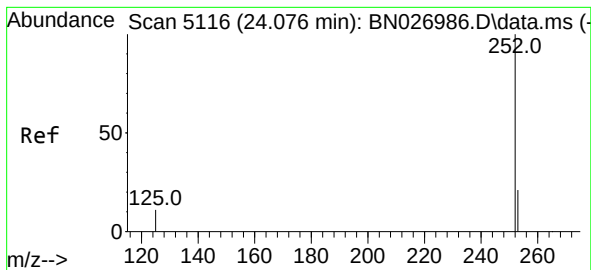

#26

Benzo(a)pyrene

Concen: 0.329 ng/ul

RT: 24.082 min Scan# 5116

Delta R.T. -0.003 min

Lab File: BN026995.D

Acq: 21 Aug 2023 16:32

Instrument :

BN026995.D

ClientSampleId :

A48K5





Tgt Ion:	252	Resp:	3088
Ion Ratio	Lower	Upper	
252	100		
253	26.4	19.0	28.6
125	18.8	11.4	17.0

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 08/22/2023

Supervised By :mohammad ahmed 08/22/2023

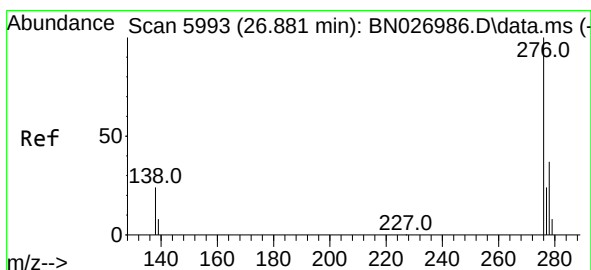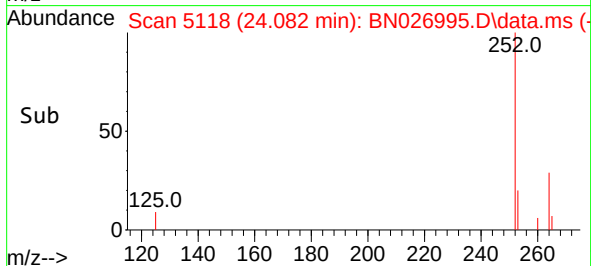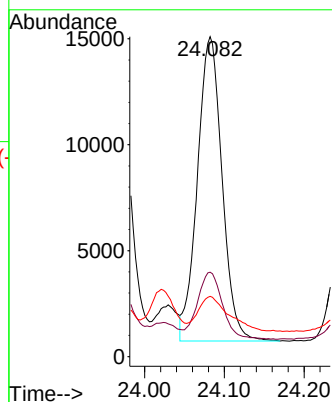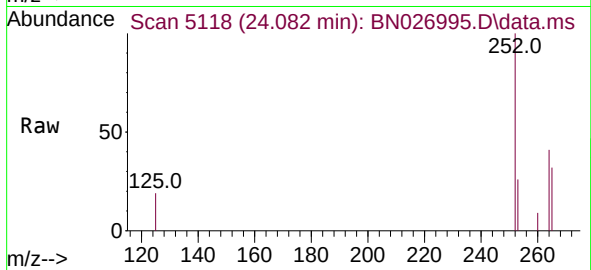

#27

Indeno(1,2,3-cd)pyrene

Concen: 0.193 ng/ul




RT: 26.884 min Scan# 5994


Delta R.T. -0.001 min

Lab File: BN026995.D

Acq: 21 Aug 2023 16:32


Tgt Ion:	276	Resp:	23696
Ion Ratio	Lower	Upper	
276	100		
138	20.0	21.6	32.4#
227	1.8	0.0	0.0#

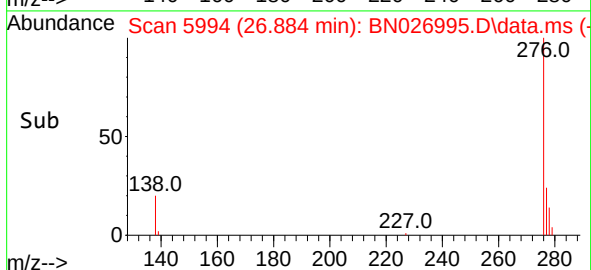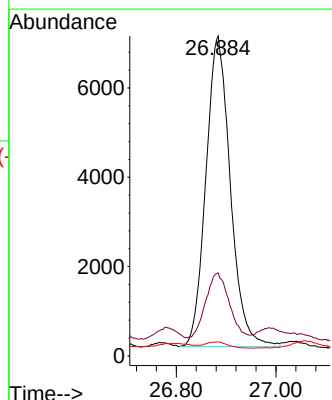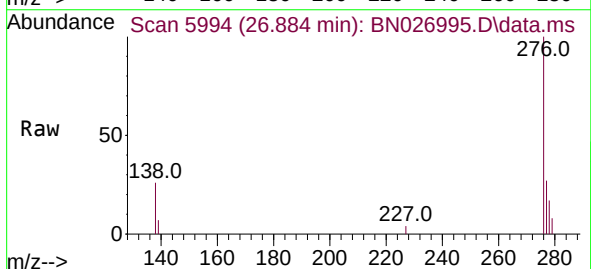

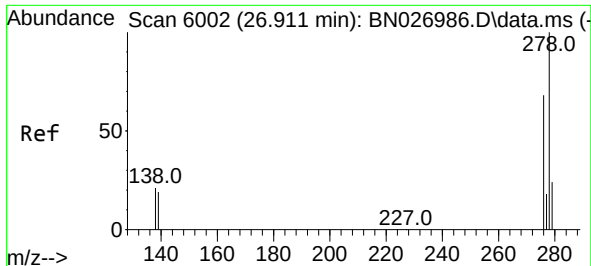

#28
Dibenzo(a,h)anthracene
Concen: 0.053 ng/ul
RT: 26.908 min Scan# 6001
Delta R.T. -0.014 min
Lab File: BN026995.D
Acq: 21 Aug 2023 16:32




Instrument :
BNA_N
ClientSampleId :
A48K5

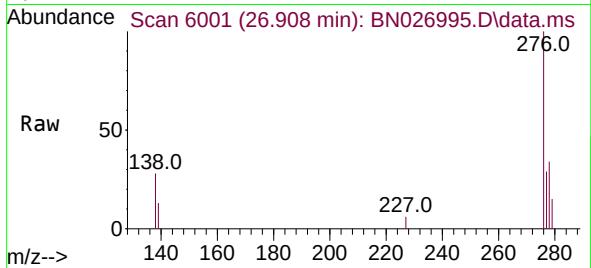


Tgt Ion:278 Resp: 5199
Ion Ratio Lower Upper
278 100
139 39.1 15.7 23.5
279 43.9 20.2 30.4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/22/2023
Supervised By :mohammad ahmed 08/22/2023

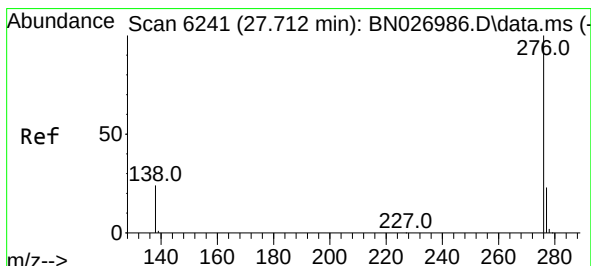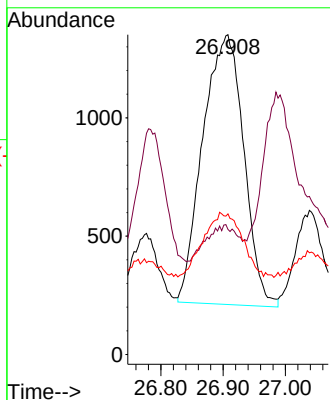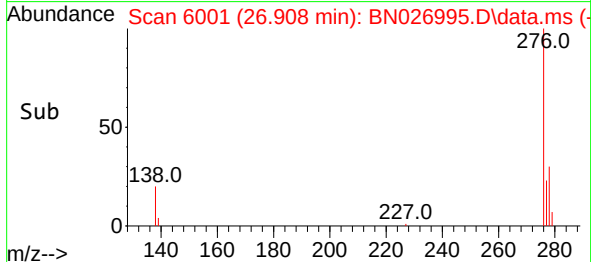

#29
Benzo(g,h,i)perylene
Concen: 0.238 ng/ul
RT: 27.723 min Scan# 6244
Delta R.T. -0.001 min
Lab File: BN026995.D
Acq: 21 Aug 2023 16:32

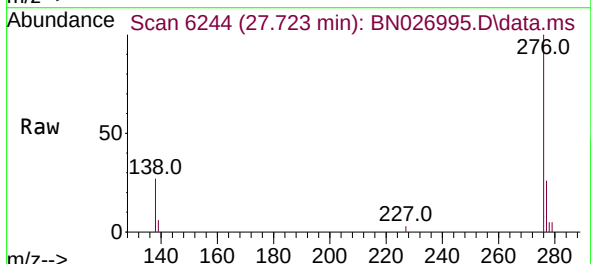

Tgt Ion:276 Resp: 24307
Ion Ratio Lower Upper
276 100
138 27.2 19.3 28.9
277 26.3 19.8 29.8

