

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN027000.D
 Acq On : 21 Aug 2023 20:16
 Operator : MA/JU
 Sample : 03967-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A48L9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/22/2023
 Supervised By :mohammad ahmed 08/22/2023

Quant Time: Aug 22 01:39:59 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 18 13:11:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.101	152	6443	0.400	ng/u1	0.00
4) Naphthalene-d8	10.927	136	21543	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.726	164	12353	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.472	188	27532	0.400	ng/u1	0.00
17) Chrysene-d12	21.644	240	21828	0.400	ng/u1	0.00
23) Perylene-d12	24.184	264	23858	0.400	ng/u1	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.439	96	60038	7.849	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.500	152	11700	0.369	ng/u1	0.00
18) Fluoranthene-d10	19.487	212	29326	0.425	ng/u1	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.977	128	1427	0.023	ng/u1#	78
15) Phenanthrene	17.515	178	5875	0.065	ng/u1	96
19) Fluoranthene	19.520	202	17216	0.190	ng/u1	98
20) Pyrene	19.887	202	16130m	0.167	ng/u1	
21) Benzo(a)anthracene	21.627	228	6086	0.070	ng/u1	96
22) Chrysene	21.682	228	9890m	0.115	ng/u1	
24) Benzo(b)fluoranthene	23.392	252	13453m	0.149	ng/u1	
25) Benzo(k)fluoranthene	23.448	252	4596m	0.052	ng/u1	
26) Benzo(a)pyrene	24.073	252	7286	0.089	ng/u1#	68
27) Indeno(1,2,3-cd)pyrene	26.871	276	5665	0.053	ng/u1#	84
29) Benzo(g,h,i)perylene	27.716	276	5809	0.065	ng/u1#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN027000.D
Acq On : 21 Aug 2023 20:16
Operator : MA/JU
Sample : 03967-11
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A48L9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/22/2023
Supervised By :mohammad ahmed 08/22/2023


Quant Time: Aug 22 01:39:59 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 18 13:11:26 2023
Response via : Initial Calibration

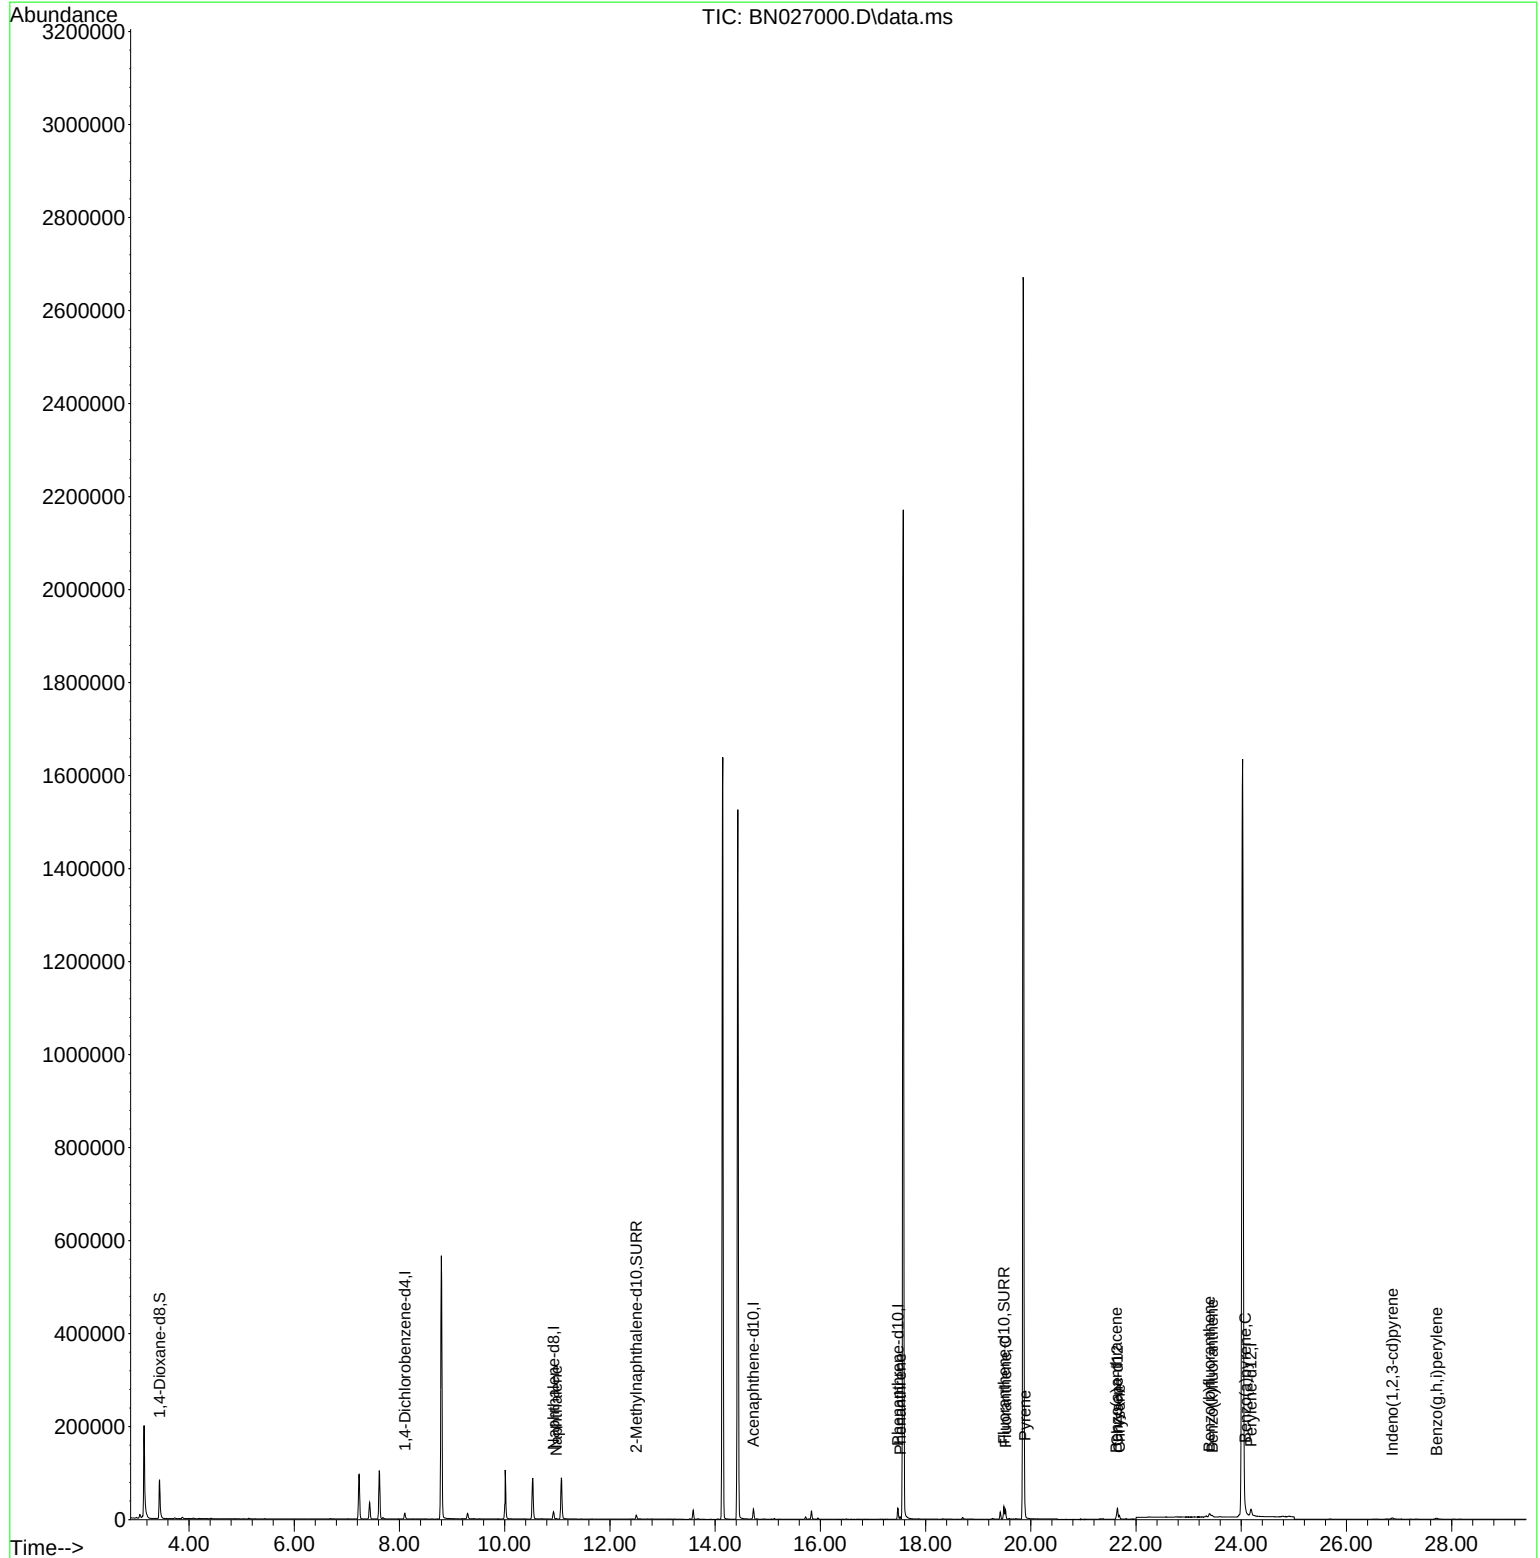

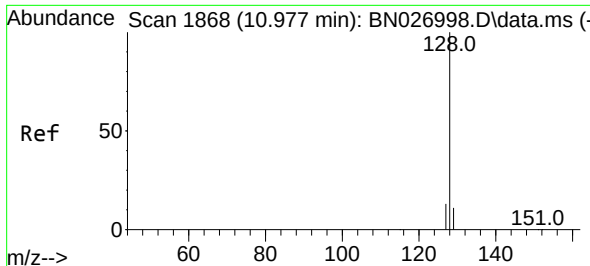

#5
Naphthalene
Concen: 0.023 ng/ul
RT: 10.977 min Scan# 1868
Delta R.T. -0.006 min
Lab File: BN027000.D
Acq: 21 Aug 2023 20:16




Instrument :
BNA_N
ClientSampleId :
A48L9

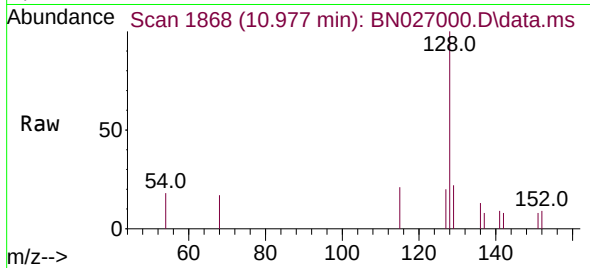

Tgt Ion:128 Resp: 1427
Ion Ratio Lower Upper
128 100
129 22.3 9.2 13.8
127 19.8 10.5 15.7




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/22/2023
Supervised By :mohammad ahmed 08/22/2023

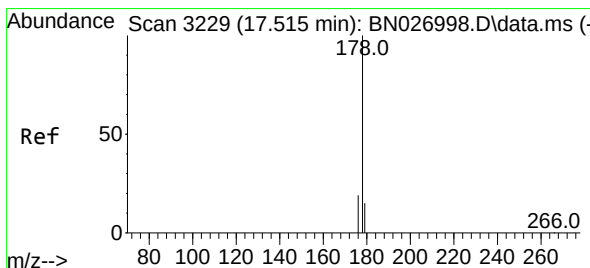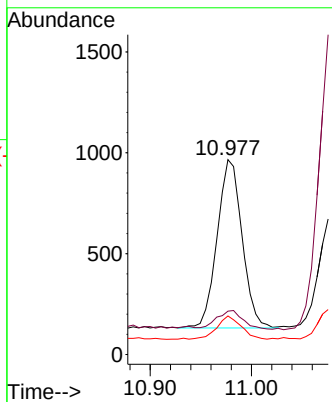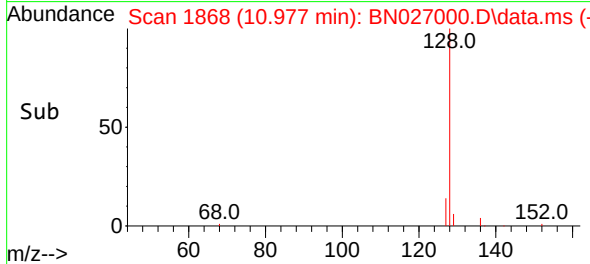

#15
Phenanthrene
Concen: 0.065 ng/ul
RT: 17.515 min Scan# 3229
Delta R.T. -0.004 min
Lab File: BN027000.D
Acq: 21 Aug 2023 20:16


Tgt Ion:178 Resp: 5875
Ion Ratio Lower Upper
178 100
179 17.7 12.6 18.8
176 21.0 15.4 23.2

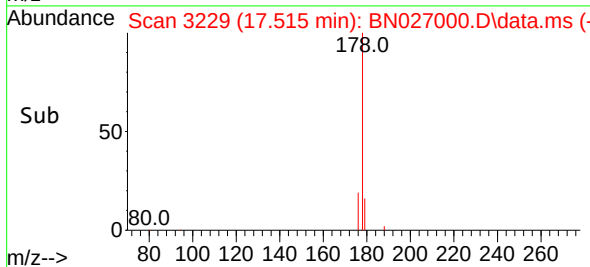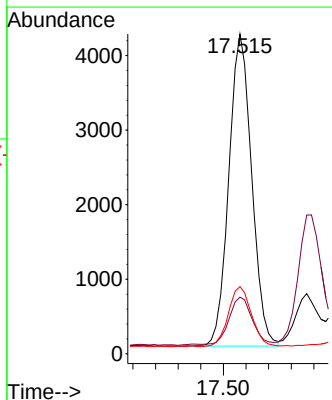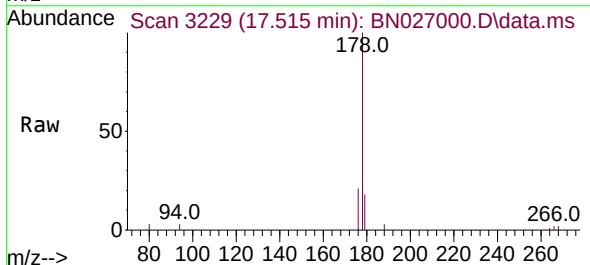

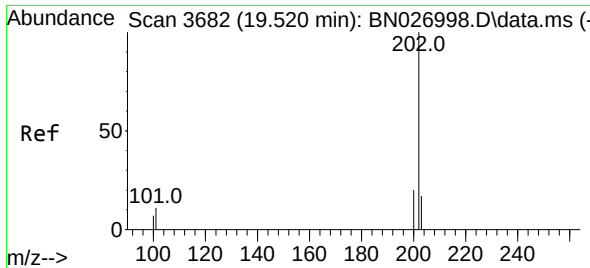

#19
Fluoranthene
Concen: 0.190 ng/ul
RT: 19.520 min Scan# 3682
Delta R.T. -0.005 min
Lab File: BN027000.D
Acq: 21 Aug 2023 20:16




Instrument :
BNA_N
ClientSampleId :
A48L9

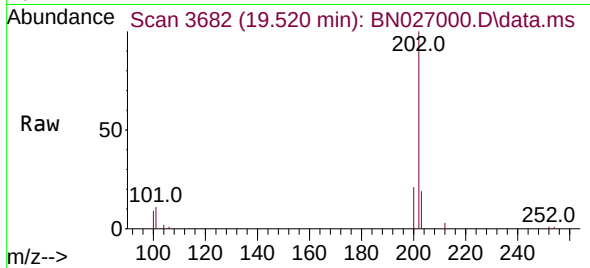


Tgt Ion:202 Resp: 17216
Ion Ratio Lower Upper
202 100
101 11.2 8.3 12.5
100 8.5 6.2 9.2

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 08/22/2023
Supervised By :mohammad ahmed 08/22/2023

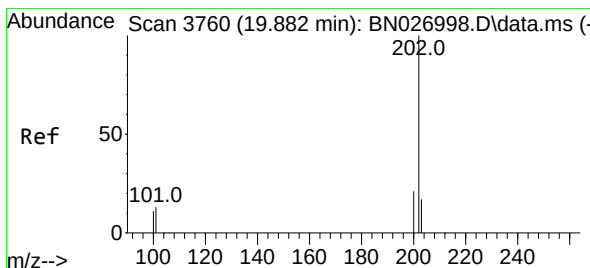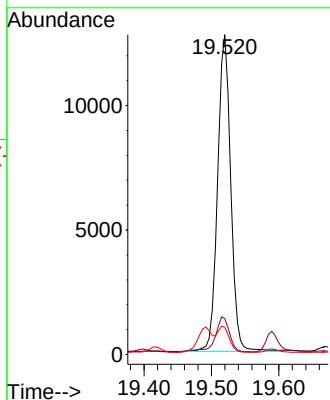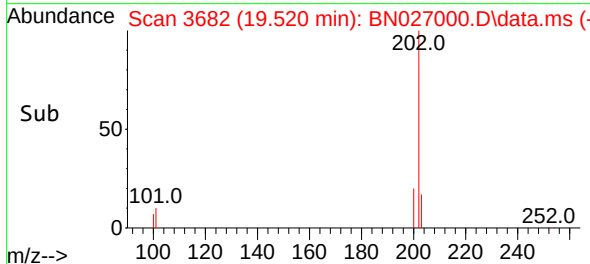


#20
Pyrene
Concen: 0.167 ng/ul m
RT: 19.887 min Scan# 3761
Delta R.T. -0.000 min
Lab File: BN027000.D
Acq: 21 Aug 2023 20:16

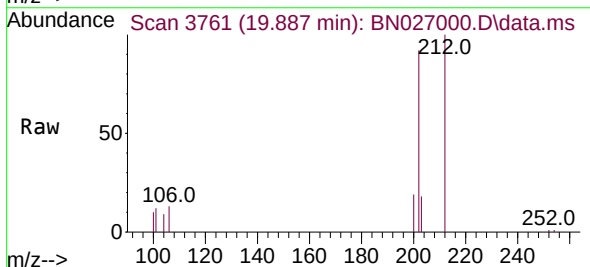


Tgt Ion:202 Resp: 16130
Ion Ratio Lower Upper
202 100
101 13.3 10.7 16.1
100 11.4 8.5 12.7

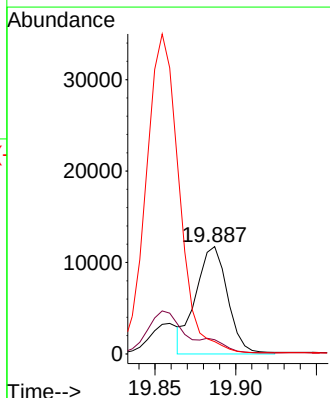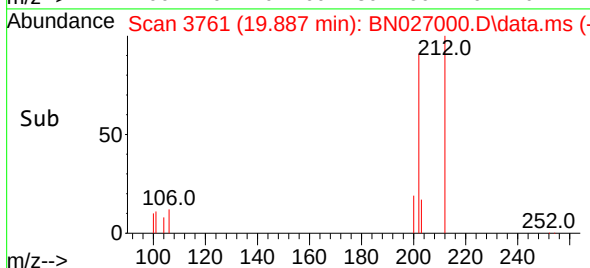

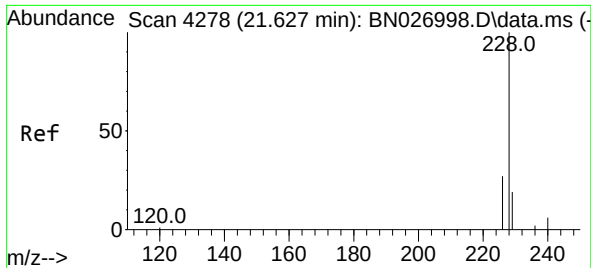

#21
Benzo(a)anthracene
Concen: 0.070 ng/ul
RT: 21.627 min Scan# 4278
Delta R.T. -0.006 min
Lab File: BN027000.D
Acq: 21 Aug 2023 20:16




Instrument :
BNA_N
ClientSampleId :
A48L9

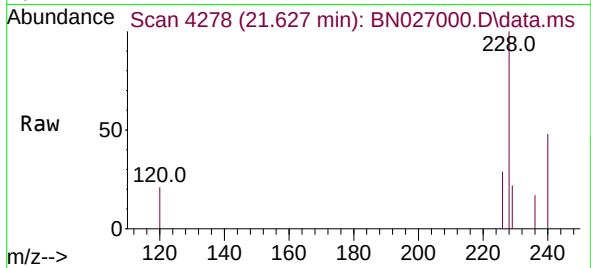


Tgt Ion:228 Resp: 6086
Ion Ratio Lower Upper
228 100
229 22.3 16.0 24.0
226 29.3 22.2 33.2

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 08/22/2023
Supervised By :mohammad ahmed 08/22/2023

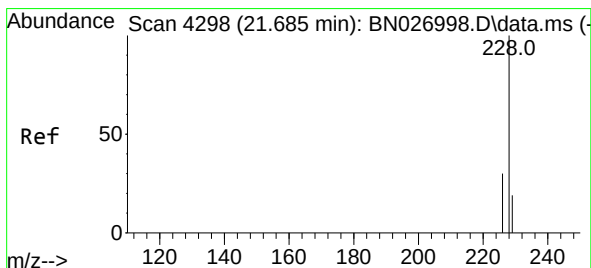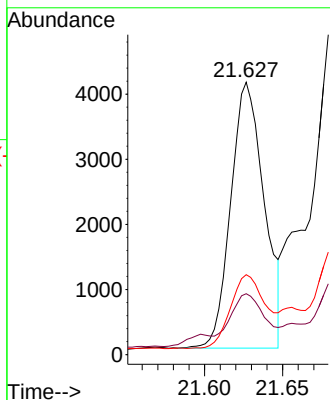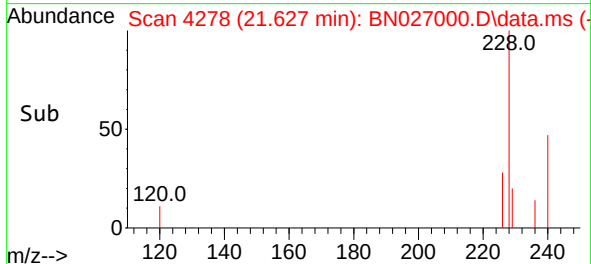


#22
Chrysene
Concen: 0.115 ng/ul m
RT: 21.682 min Scan# 4297
Delta R.T. -0.009 min
Lab File: BN027000.D
Acq: 21 Aug 2023 20:16

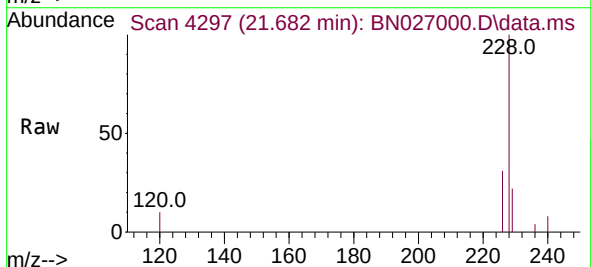


Tgt Ion:228 Resp: 9890
Ion Ratio Lower Upper
228 100
226 31.2 24.6 36.8
229 21.6 15.8 23.6

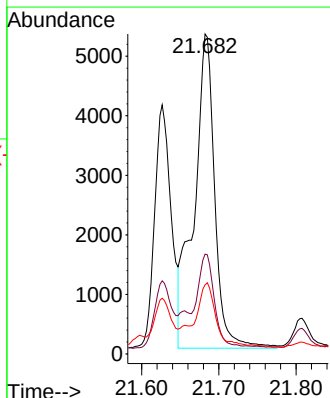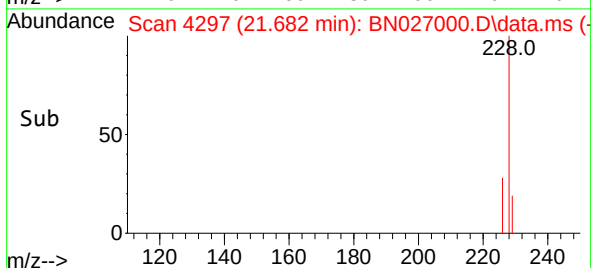

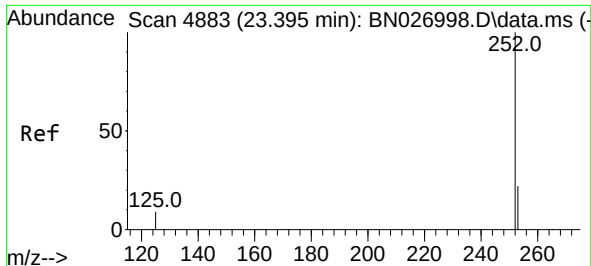

#24
Benzo(b)fluoranthene
Concen: 0.149 ng/ul m
RT: 23.392 min Scan# 4883
Delta R.T. -0.015 min
Lab File: BN027000.D
Acq: 21 Aug 2023 20:16




Instrument :
BNA_N
ClientSampleId :
A48L9

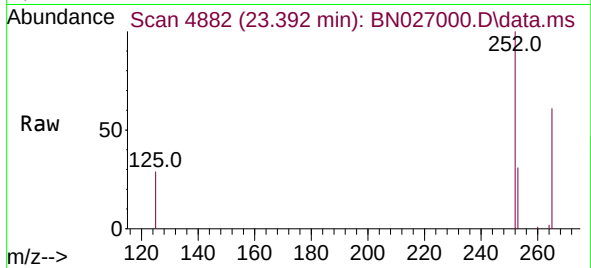

Tgt Ion:252 Resp: 13453
Ion Ratio Lower Upper
252 100
253 31.3 0.0 46.8
125 28.6 0.0 25.2




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/22/2023
Supervised By :mohammad ahmed 08/22/2023

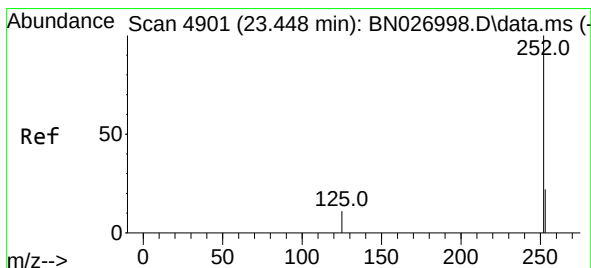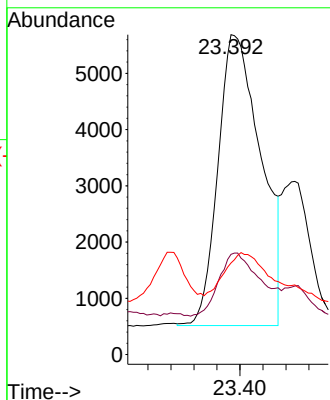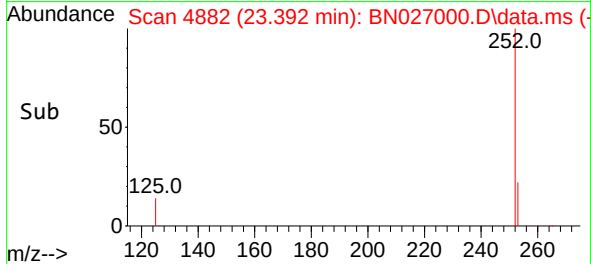

#25
Benzo(k)fluoranthene
Concen: 0.052 ng/ul m
RT: 23.448 min Scan# 4901
Delta R.T. -0.012 min
Lab File: BN027000.D
Acq: 21 Aug 2023 20:16


Tgt Ion:252 Resp: 4596
Ion Ratio Lower Upper
252 100
253 39.6 18.2 27.4#
125 40.3 9.9 14.9#

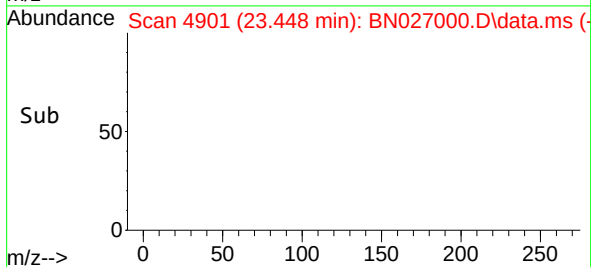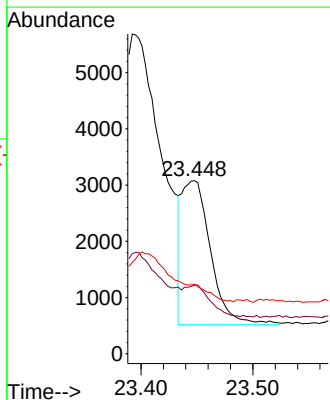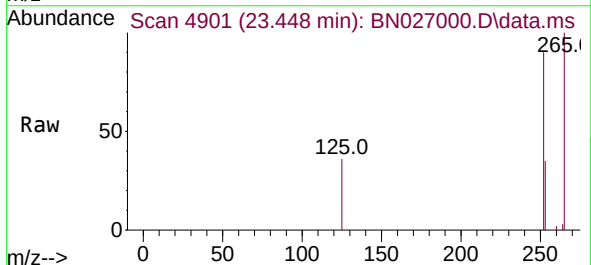

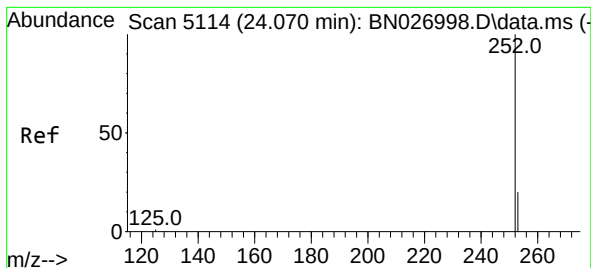

#26
Benzo(a)pyrene
Concen: 0.089 ng/ul
RT: 24.073 min Scan# 5114
Delta R.T. -0.012 min
Lab File: BN027000.D
Acq: 21 Aug 2023 20:16




Instrument :
BNA_N
ClientSampleId :
A48L9

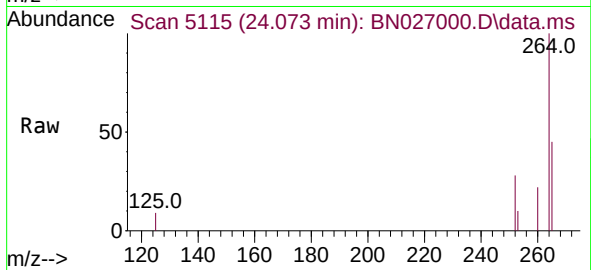

Tgt Ion:252 Resp: 7286
Ion Ratio Lower Upper
252 100
253 35.5 19.0 28.6#
125 33.0 11.4 17.0#




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/22/2023
Supervised By :mohammad ahmed 08/22/2023

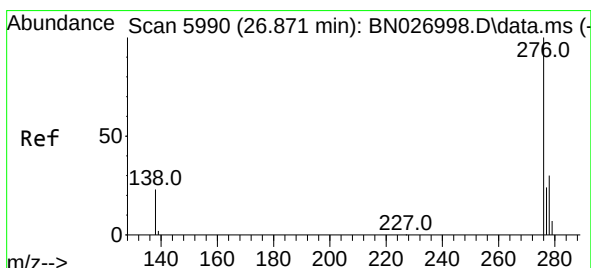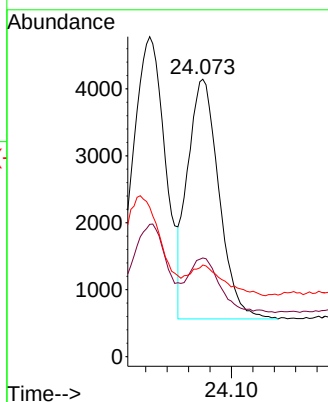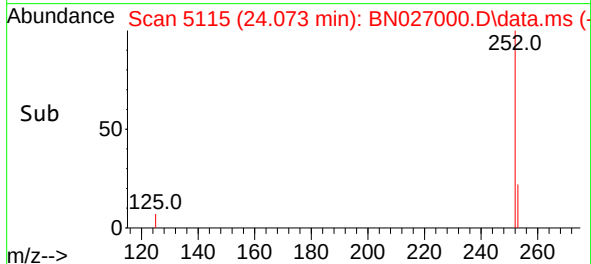

#27
Indeno(1,2,3-cd)pyrene
Concen: 0.053 ng/ul
RT: 26.871 min Scan# 5990
Delta R.T. -0.014 min
Lab File: BN027000.D
Acq: 21 Aug 2023 20:16


Tgt Ion:276 Resp: 5665
Ion Ratio Lower Upper
276 100
138 18.7 21.6 32.4#
227 0.2 0.0 0.0#

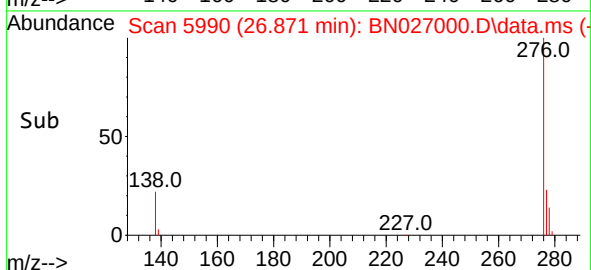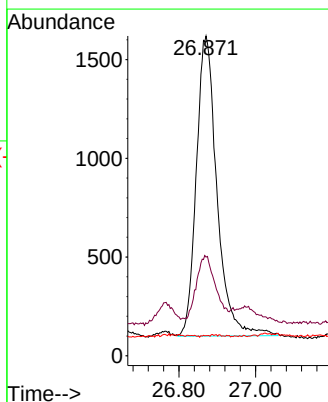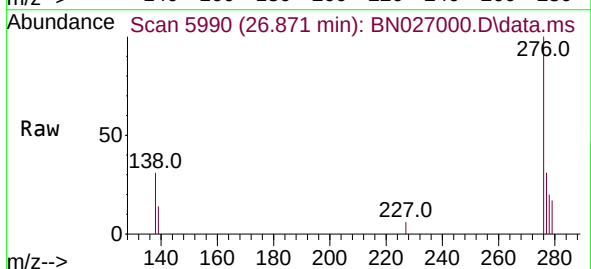

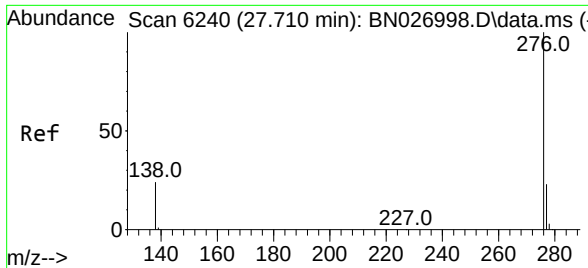

#29
 Benzo(g,h,i)perylene
 Concen: 0.065 ng/ul
 RT: 27.716 min Scan# 61
 Delta R.T. -0.007 min
 Lab File: BN027000.D
 Acq: 21 Aug 2023 20:16

Instrument :
 BNA_N
 ClientSampleId :
 A48L9

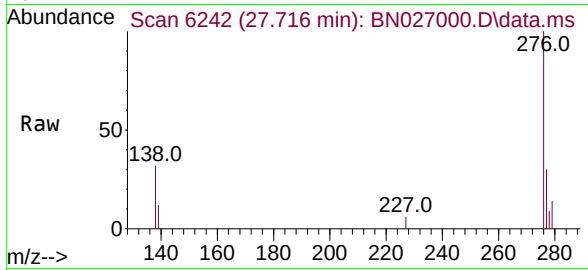

Tgt Ion:	276	Resp:	5809
Ion Ratio	Lower	Upper	
276	100		
138	31.7	19.3	28.9
277	30.4	19.8	29.8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/22/2023
 Supervised By :mohammad ahmed 08/22/2023

