

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN027035.D
 Acq On : 22 Aug 2023 20:13
 Operator : MA/JU
 Sample : 04049-07
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9T7

Quant Time: Aug 23 01:44:11 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 18 13:11:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.097	152	6659	0.400	ng/ul	0.00
4) Naphthalene-d8	10.922	136	22603	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.726	164	13179	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.472	188	28541	0.400	ng/ul	0.00
17) Chrysene-d12	21.641	240	21222	0.400	ng/ul	0.00
23) Perylene-d12	24.184	264	20380	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.439	96	23647	2.991	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.495	152	11559	0.348	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	30803	0.460	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.473	88	53358	6.611	ng/ul#	89




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN027035.D
Acq On : 22 Aug 2023 20:13
Operator : MA/JU
Sample : 04049-07
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9T7

Quant Time: Aug 23 01:44:11 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 18 13:11:26 2023
Response via : Initial Calibration

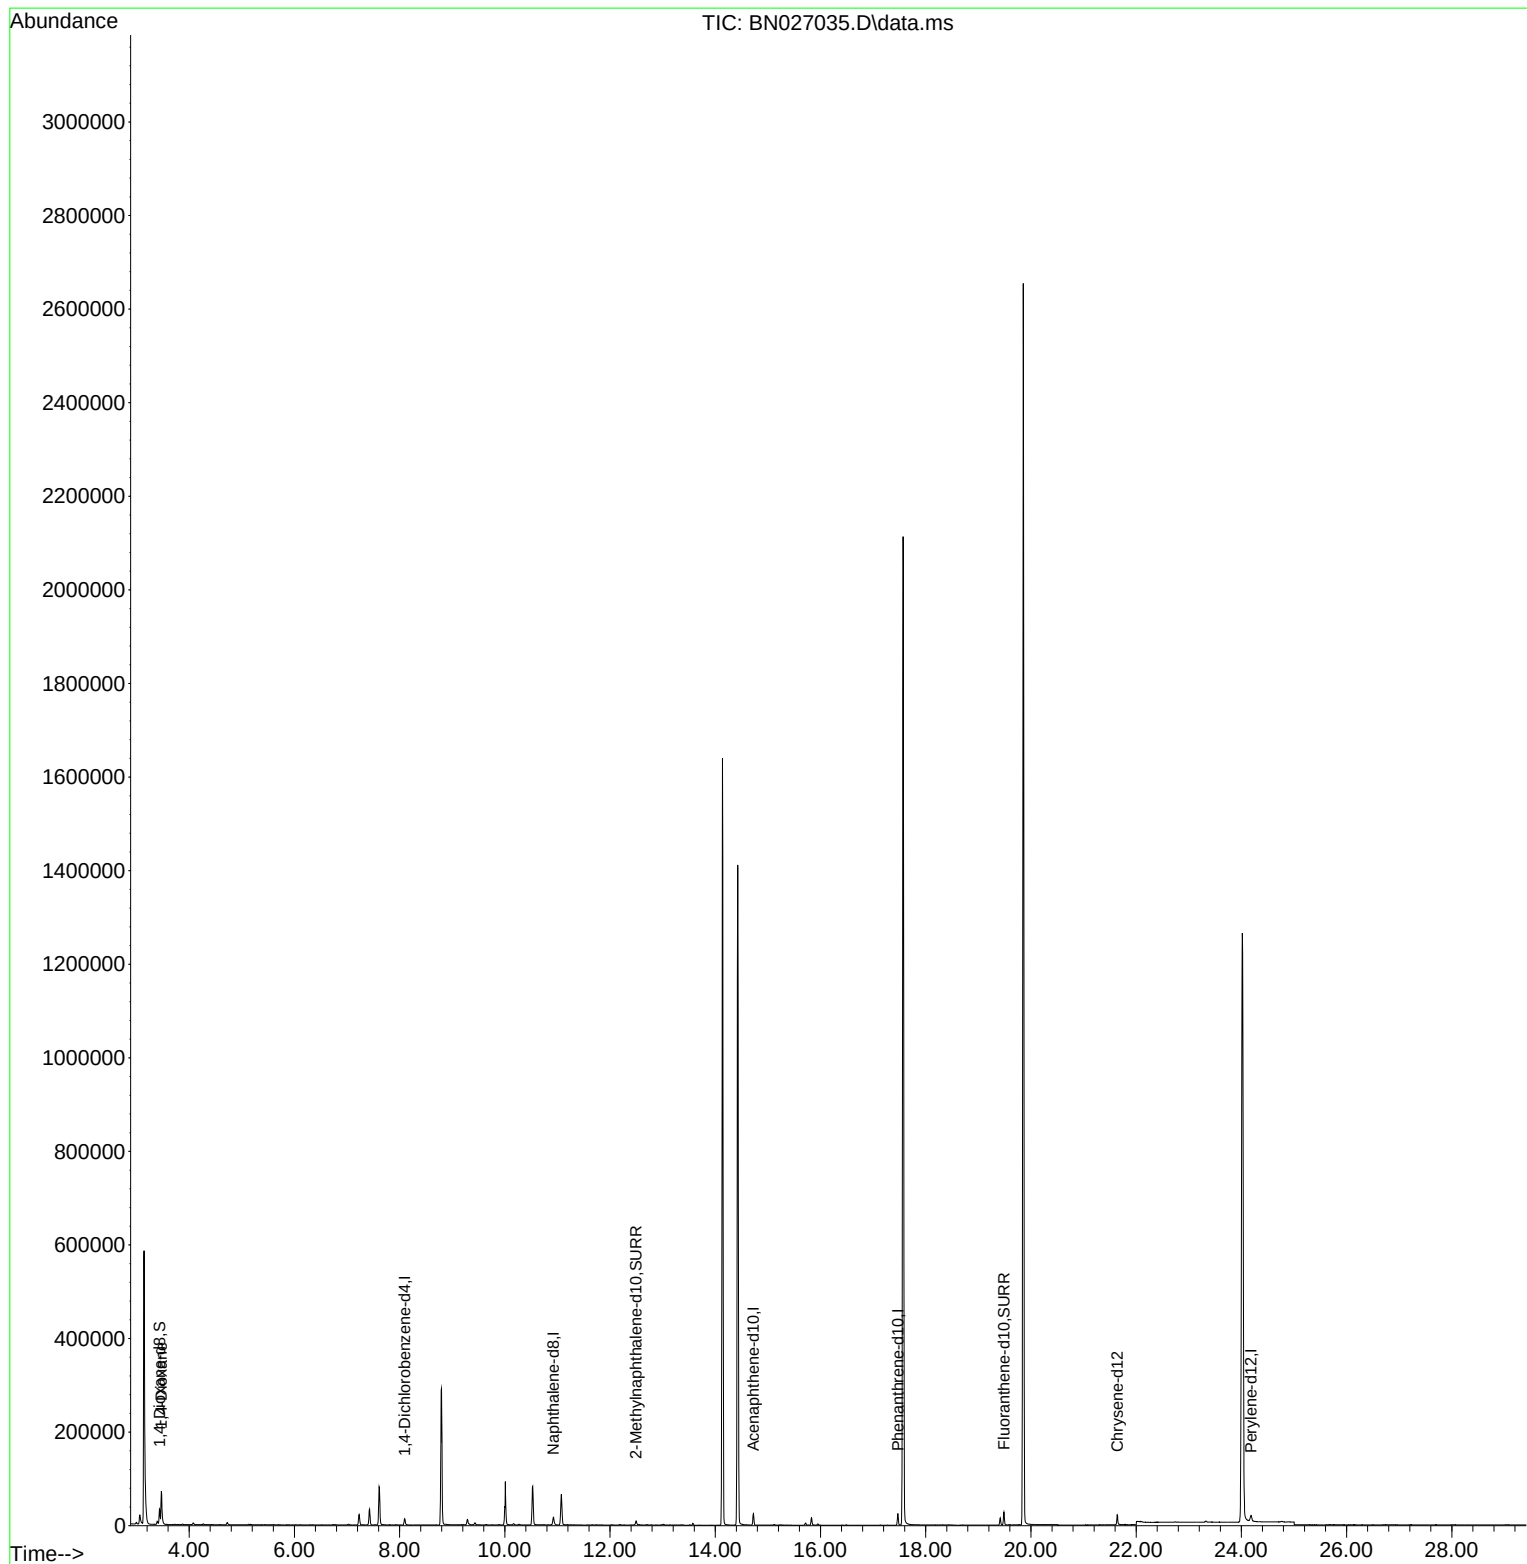

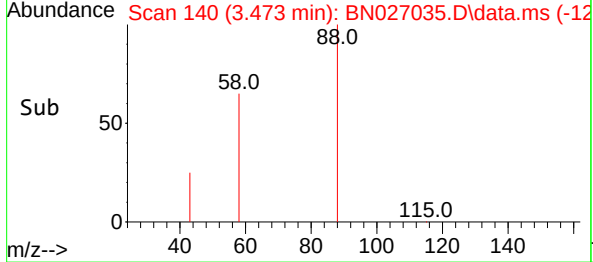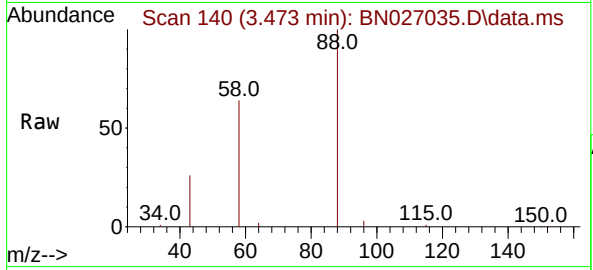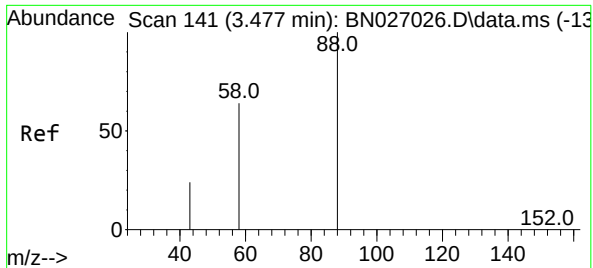

#2
1,4-Dioxane
Concen: 6.611 ng/ul
RT: 3.473 min Scan# 14
Delta R.T. -0.004 min
Lab File: BN027035.D
Acq: 22 Aug 2023 20:13

Instrument :
BNA_N
ClientSampleId :
BH9T7

Tgt Ion: 88 Resp: 53358
Ion Ratio Lower Upper
88 100
43 26.2 28.0 42.0#
58 63.7 46.0 69.0

