

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN027036.D
 Acq On : 22 Aug 2023 20:49
 Operator : MA/JU
 Sample : 04049-08
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHAL6

Quant Time: Aug 23 01:44:17 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 18 13:11:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.097	152	7403	0.400	ng/ul	0.00
4) Naphthalene-d8	10.922	136	26258	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.726	164	15667	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.468	188	31952	0.400	ng/ul	0.00
17) Chrysene-d12	21.641	240	22988	0.400	ng/ul	0.00
23) Perylene-d12	24.181	264	22372	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.439	96	20019	2.278	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.494	152	13252	0.343	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	34676	0.478	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.977	128	2462	0.033	ng/ul#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN027036.D
Acq On : 22 Aug 2023 20:49
Operator : MA/JU
Sample : 04049-08
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHAL6


Quant Time: Aug 23 01:44:17 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 18 13:11:26 2023
Response via : Initial Calibration

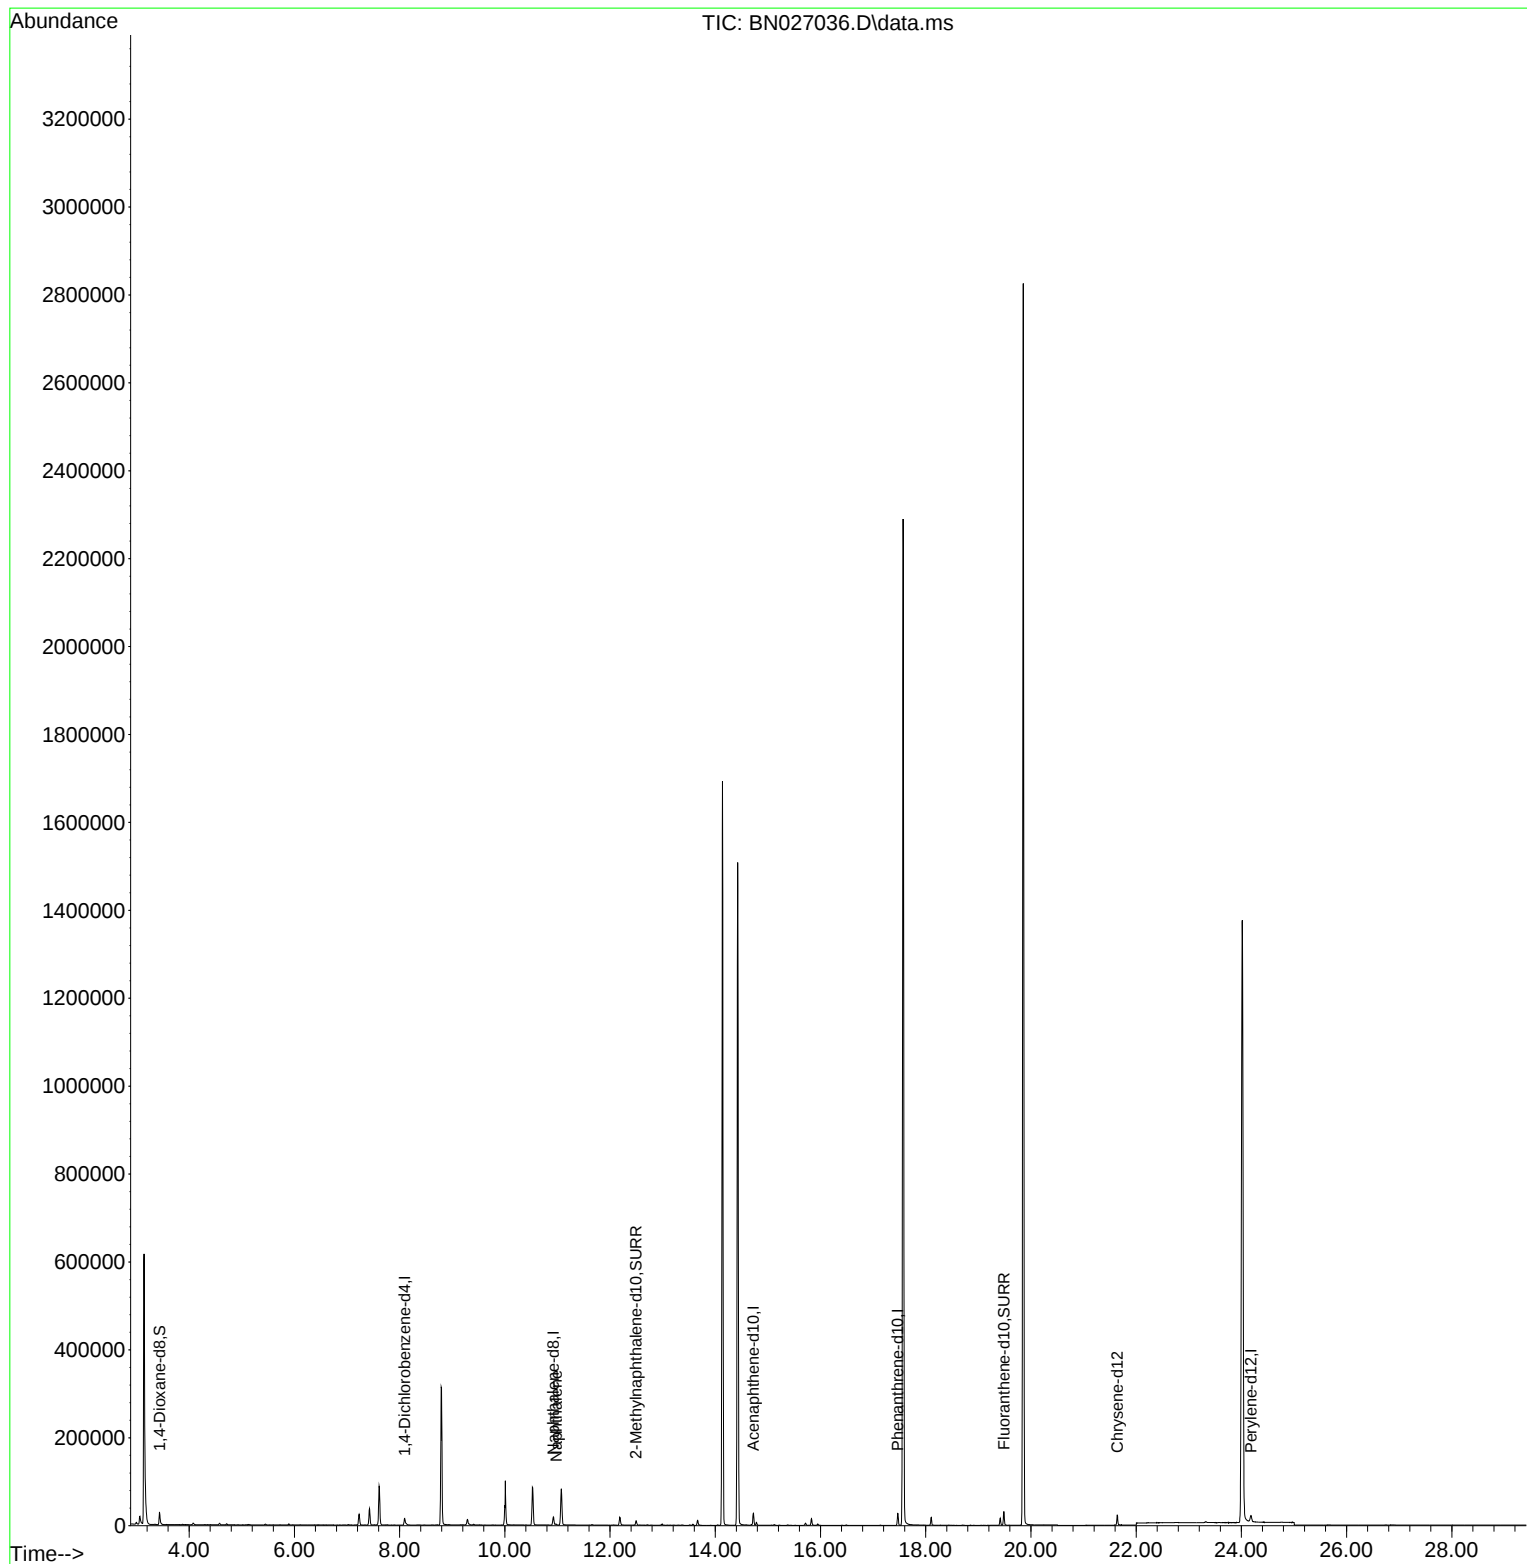

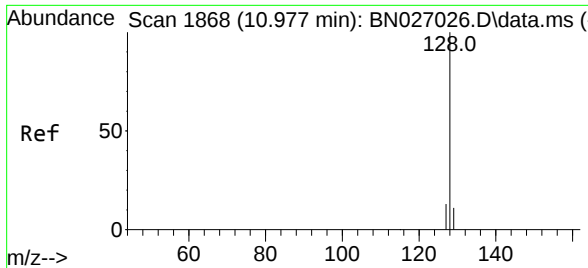

#5
Naphthalene
Concen: 0.033 ng/ul
RT: 10.977 min Scan# 11
Delta R.T. -0.006 min
Lab File: BN027036.D
Acq: 22 Aug 2023 20:49

Instrument :
BNA_N
ClientSampleId :
BHAL6

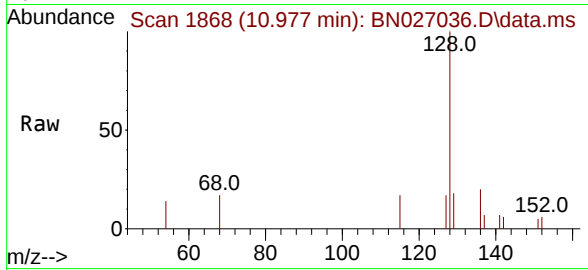

Tgt Ion:	128	Resp:	2462
Ion	Ratio	Lower	Upper
128	100		
129	18.4	9.2	13.8#
127	17.3	10.5	15.7#

