

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN027043.D
 Acq On : 23 Aug 2023 01:40
 Operator : MA/JU
 Sample : 04049-06
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9T9

Quant Time: Aug 23 02:39:16 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 23 02:28:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.093	152	7756	0.400	ng/ul	0.00
4) Naphthalene-d8	10.922	136	26381	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.721	164	15673	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.468	188	33754	0.400	ng/ul	0.00
17) Chrysene-d12	21.638	240	24048	0.400	ng/ul	0.00
23) Perylene-d12	24.173	264	23045	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.435	96	21364	2.320	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.495	152	10486	0.270	ng/ul	0.00
18) Fluoranthene-d10	19.483	212	31341	0.413	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.473	88	45973	4.891	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN027043.D
Acq On : 23 Aug 2023 01:40
Operator : MA/JU
Sample : 04049-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9T9


Quant Time: Aug 23 02:39:16 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 23 02:28:27 2023
Response via : Initial Calibration

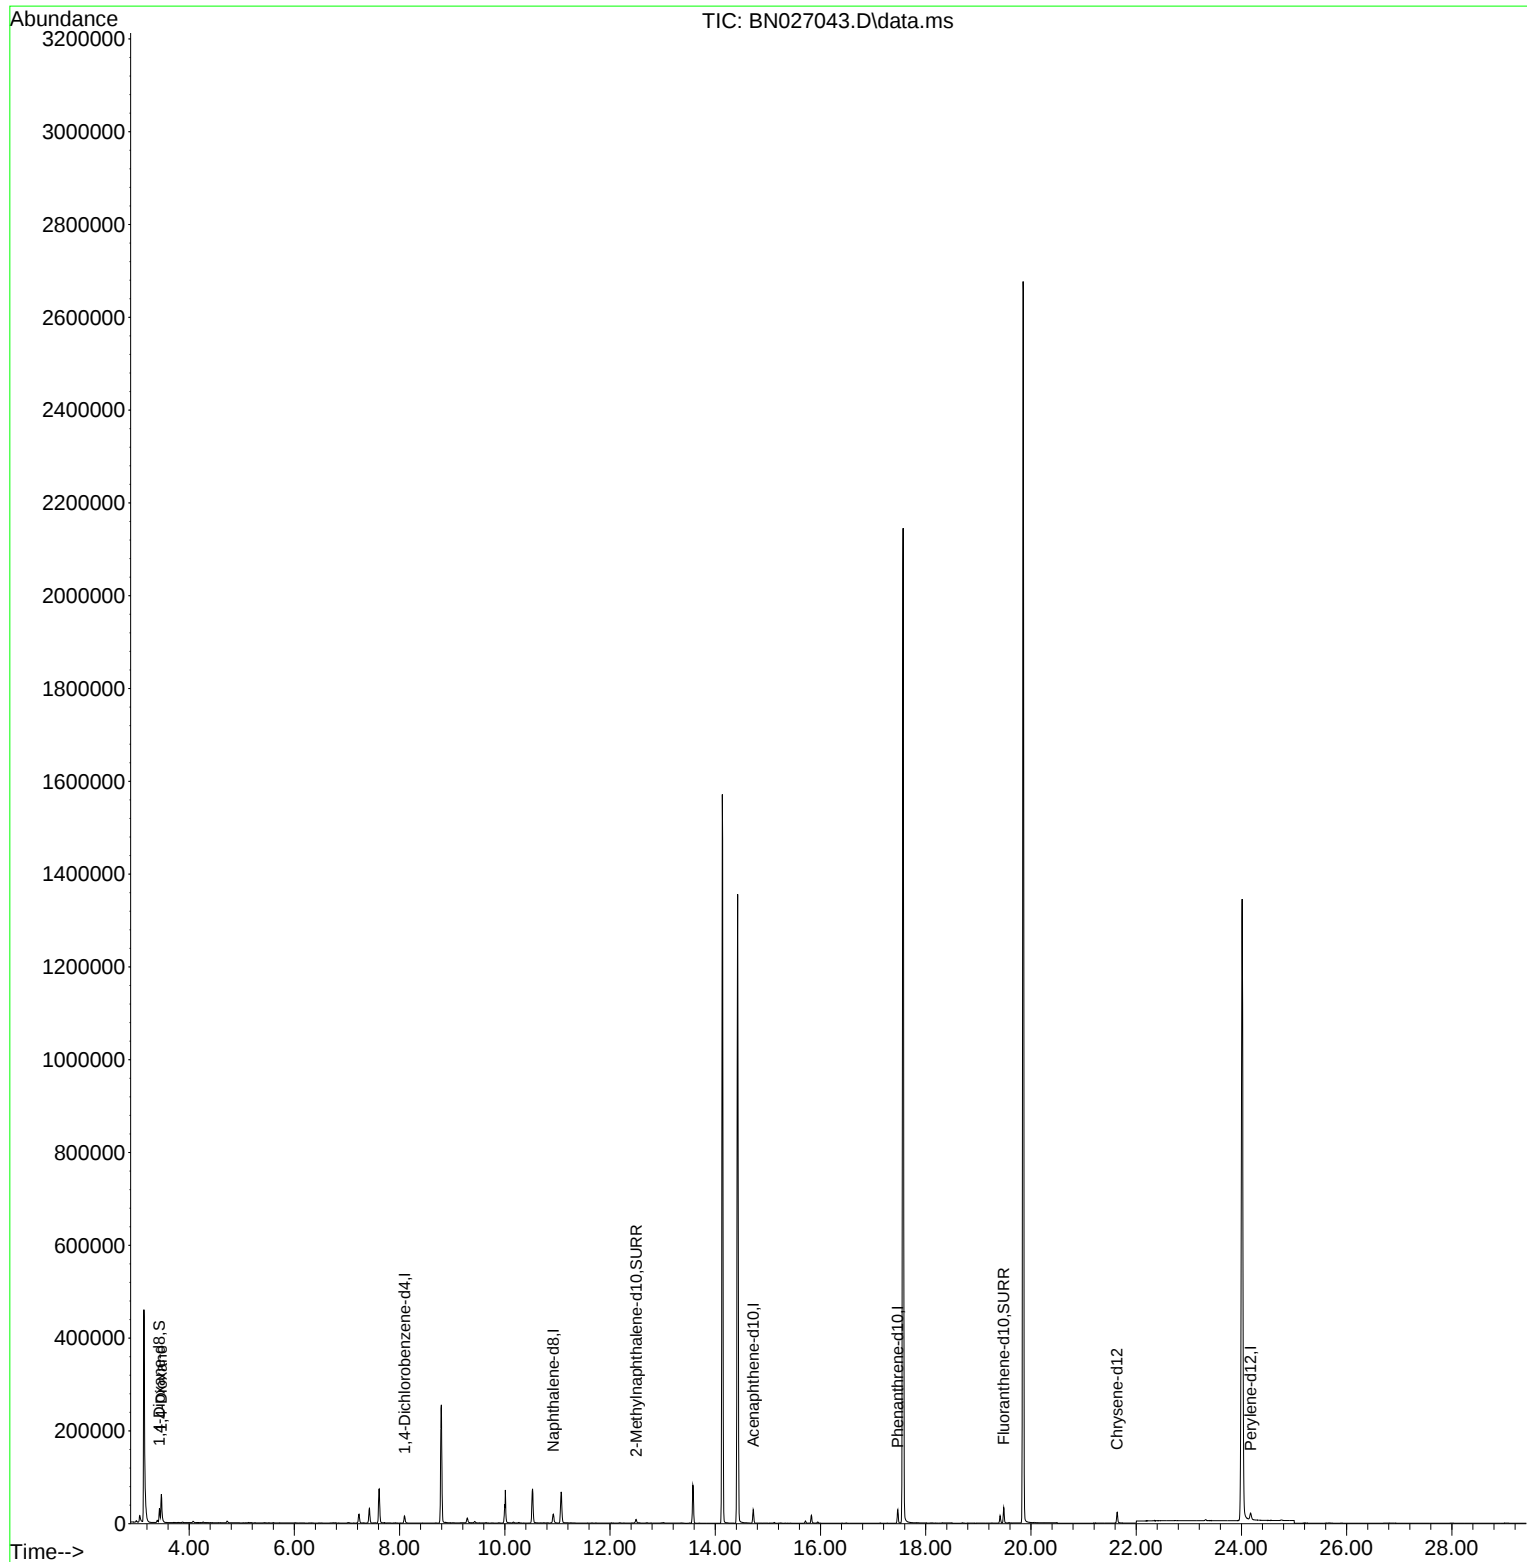

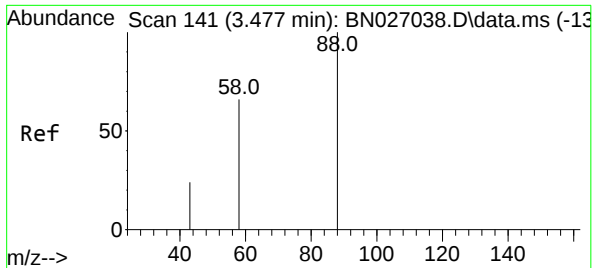

#2
 1,4-Dioxane
 Concen: 4.891 ng/ul
 RT: 3.473 min Scan# 14
 Delta R.T. -0.004 min
 Lab File: BN027043.D
 Acq: 23 Aug 2023 01:40

Instrument :
 BNA_N
 ClientSampleId :
 BH9T9

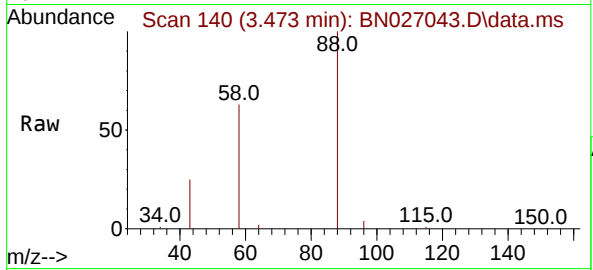

Tgt Ion:	88	Resp:	45973
Ion	Ratio	Lower	Upper
88	100		
43	25.4	28.0	42.0#
58	63.1	46.0	69.0

