

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN027045.D
 Acq On : 23 Aug 2023 02:52
 Operator : MA/JU
 Sample : 04049-04
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH946

Quant Time: Aug 23 04:15:51 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 23 02:28:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.093	152	7091	0.400	ng/ul	0.00
4) Naphthalene-d8	10.922	136	24114	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.721	164	14263	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.468	188	31926	0.400	ng/ul	0.00
17) Chrysene-d12	21.638	240	24154	0.400	ng/ul	0.00
23) Perylene-d12	24.175	264	22493	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.435	96	20062	2.383	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.495	152	10304	0.290	ng/ul	0.00
18) Fluoranthene-d10	19.492	212	32278	0.423	ng/ul	0.00
Target Compounds						
15) Phenanthrene	17.510	178	2344	0.022	ng/ul#	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN027045.D
Acq On : 23 Aug 2023 02:52
Operator : MA/JU
Sample : 04049-04
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH946

Quant Time: Aug 23 04:15:51 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 23 02:28:27 2023
Response via : Initial Calibration

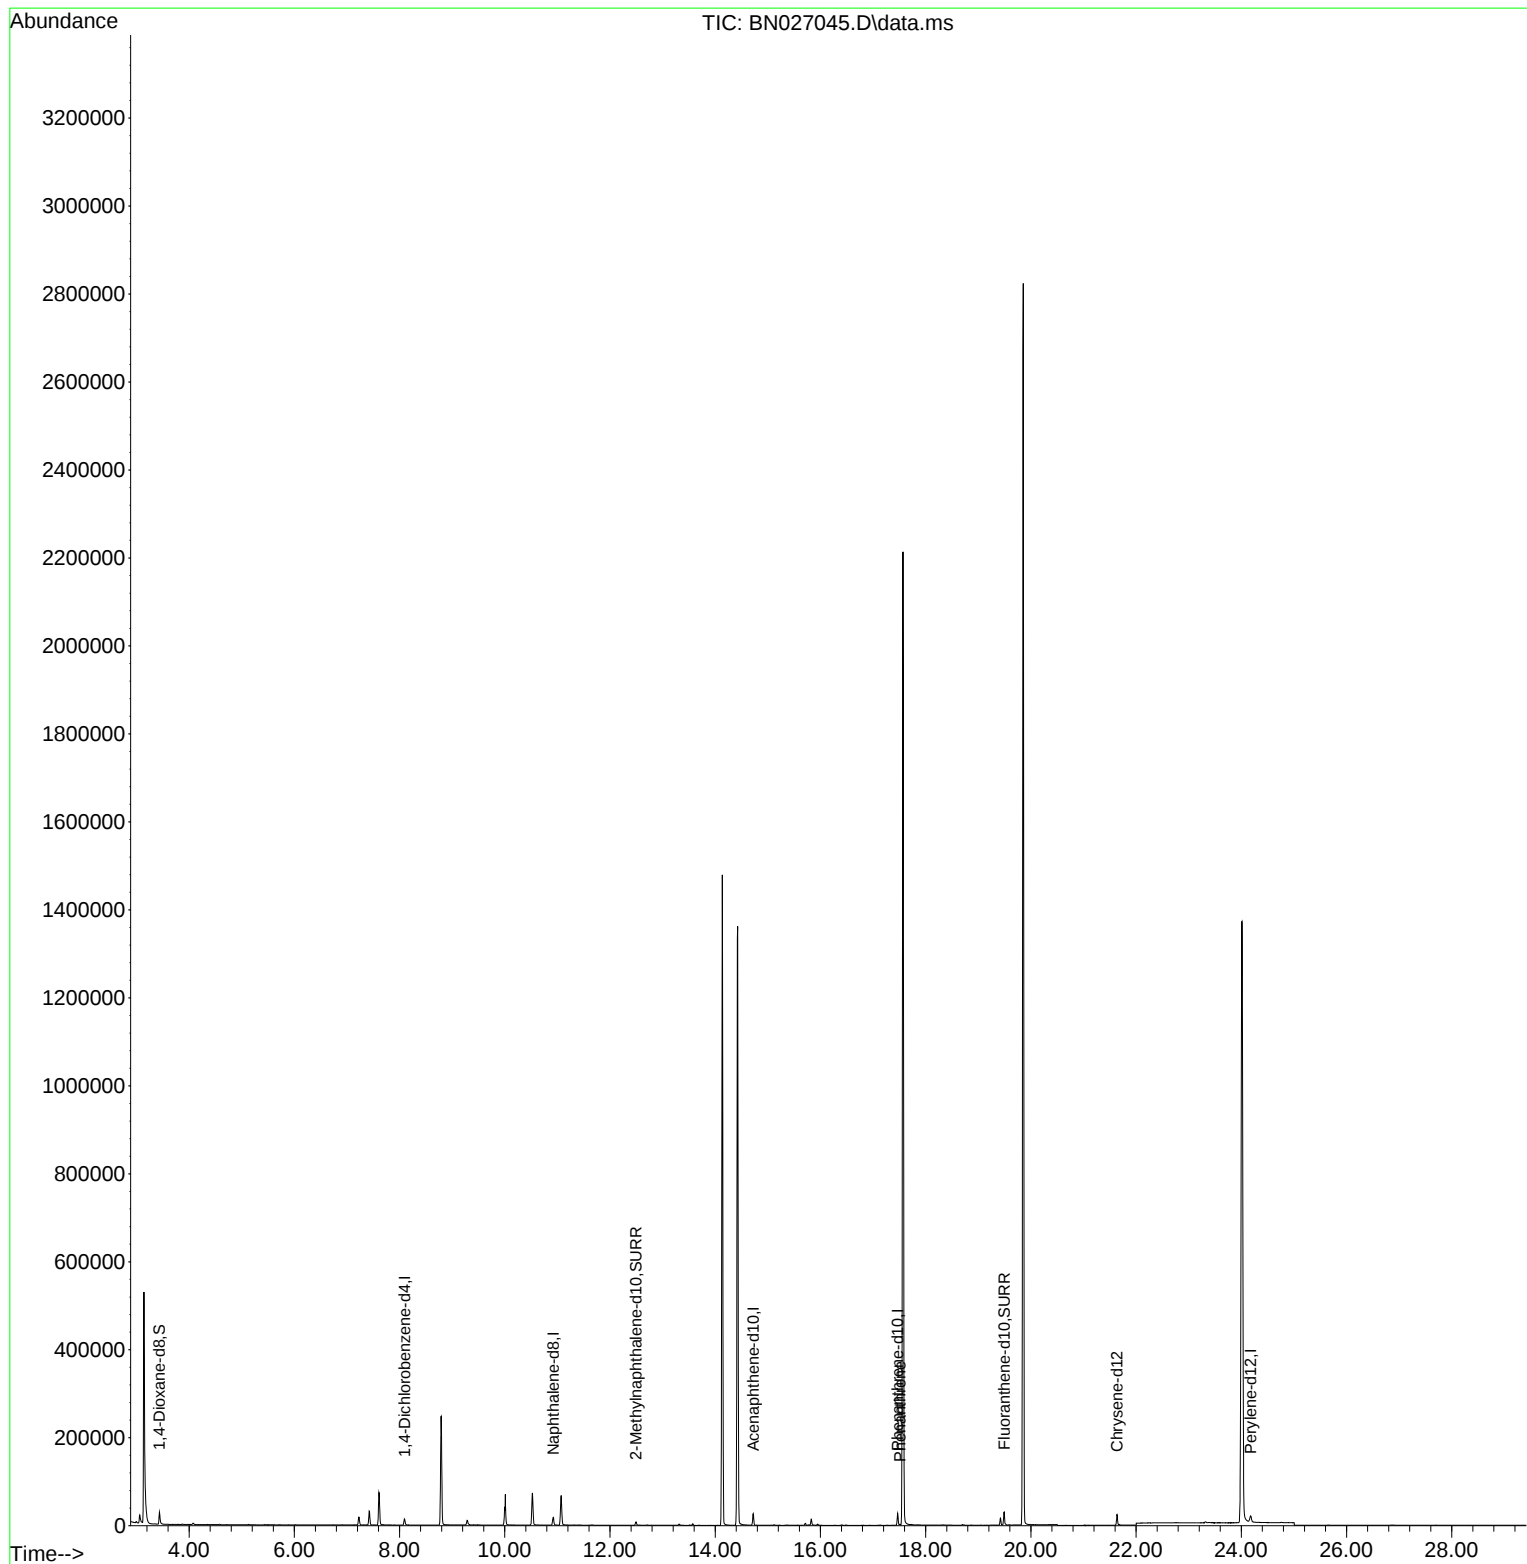

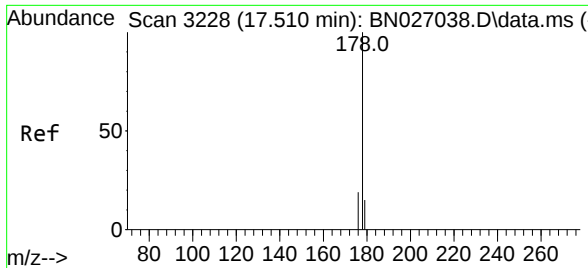

#15
 Phenanthrene
 Concen: 0.022 ng/ul
 RT: 17.510 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN027045.D
 Acq: 23 Aug 2023 02:52

Instrument :
 BNA_N
 ClientSampleId :
 BH946

Tgt Ion:	178	Resp:	2344
Ion Ratio	Lower	Upper	
178	100		
179	23.3	12.6	18.8#
176	24.4	15.4	23.2#

