

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN027046.D
 Acq On : 23 Aug 2023 03:29
 Operator : MA/JU
 Sample : 04049-05
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9T5

Quant Time: Aug 23 04:17:18 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 23 02:28:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.093	152	6769	0.400	ng/ul	0.00
4) Naphthalene-d8	10.916	136	23094	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.721	164	14124	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.468	188	29405	0.400	ng/ul	0.00
17) Chrysene-d12	21.635	240	21200	0.400	ng/ul #	0.00
23) Perylene-d12	24.173	264	20454	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.435	96	26435	3.290	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.495	152	12472	0.367	ng/ul	0.00
18) Fluoranthene-d10	19.483	212	30061	0.449	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.473	88	1745	0.213	ng/ul#	83
19) Fluoranthene	19.511	202	1788	0.020	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN027046.D
Acq On : 23 Aug 2023 03:29
Operator : MA/JU
Sample : 04049-05
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9T5

Quant Time: Aug 23 04:17:18 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 23 02:28:27 2023
Response via : Initial Calibration




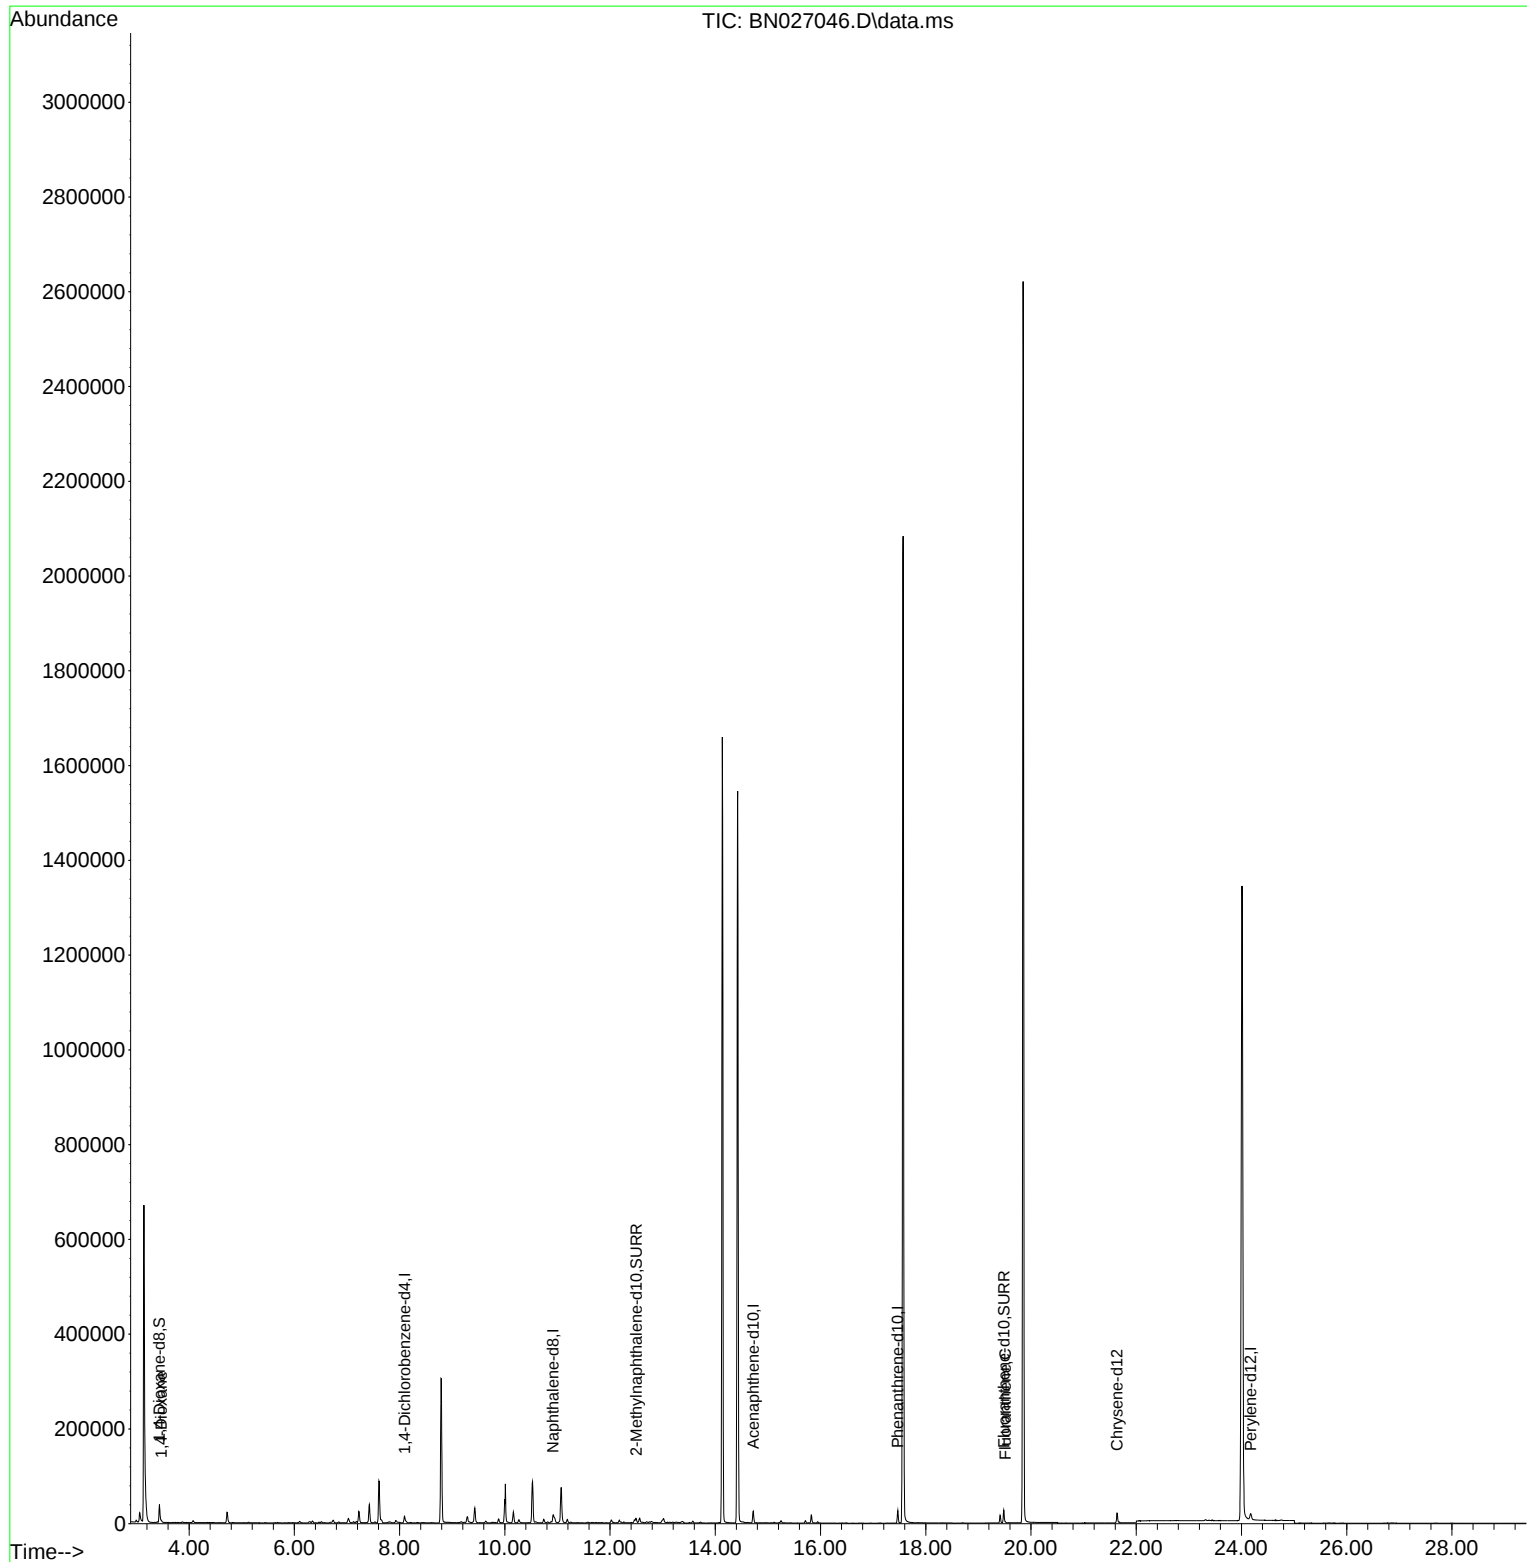


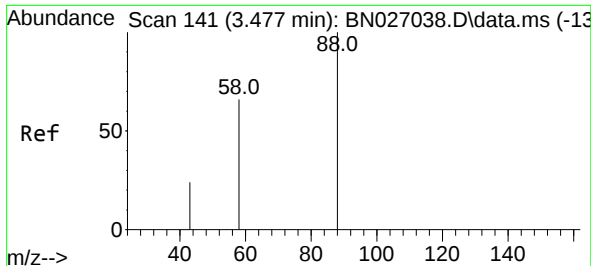

#2
1,4-Dioxane
Concen: 0.213 ng/ul
RT: 3.473 min Scan# 141
Delta R.T. -0.004 min
Lab File: BN027046.D
Acq: 23 Aug 2023 03:29

Instrument :
BNA_N
ClientSampleId :
BH9T5

Tgt Ion: 88 Resp: 1745
Ion Ratio Lower Upper
88 100
43 45.3 28.0 42.0#
58 45.2 46.0 69.0#

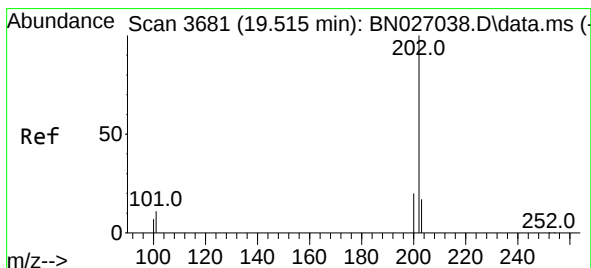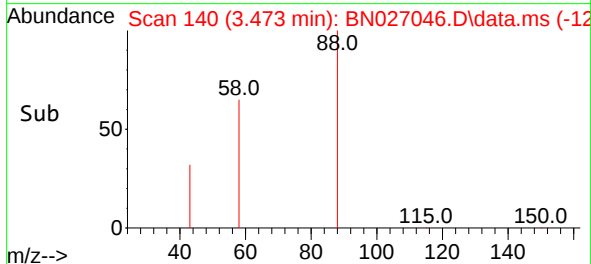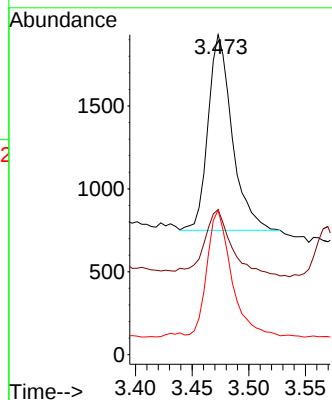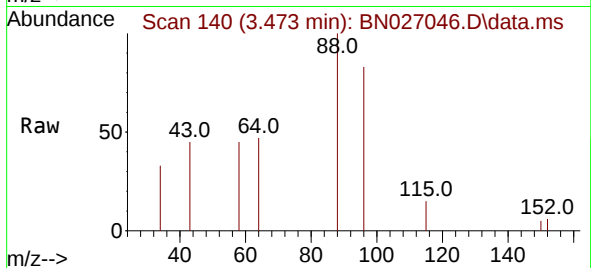

#19
Fluoranthene
Concen: 0.020 ng/ul
RT: 19.511 min Scan# 3680
Delta R.T. -0.005 min
Lab File: BN027046.D
Acq: 23 Aug 2023 03:29

Tgt Ion: 202 Resp: 1788
Ion Ratio Lower Upper
202 100
101 19.2 8.3 12.5#
100 13.8 6.2 9.2#

