

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN027069.D
 Acq On : 23 Aug 2023 19:42
 Operator : MA/JU
 Sample : 03901-02
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH316

Quant Time: Aug 24 01:39:35 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 23 02:28:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.093	152	7297	0.400	ng/u1	0.00
4) Naphthalene-d8	10.916	136	24049	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.717	164	14511	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.464	188	32504	0.400	ng/u1	0.00
17) Chrysene-d12	21.644	240	24297	0.400	ng/u1	0.00
23) Perylene-d12	24.182	264	26458	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.435	96	42055	4.855	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.489	152	11286	0.319	ng/u1	0.00
18) Fluoranthene-d10	19.483	212	30328	0.395	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.469	88	6429	0.727	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN027069.D
Acq On : 23 Aug 2023 19:42
Operator : MA/JU
Sample : 03901-02
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH316

Quant Time: Aug 24 01:39:35 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 23 02:28:27 2023
Response via : Initial Calibration

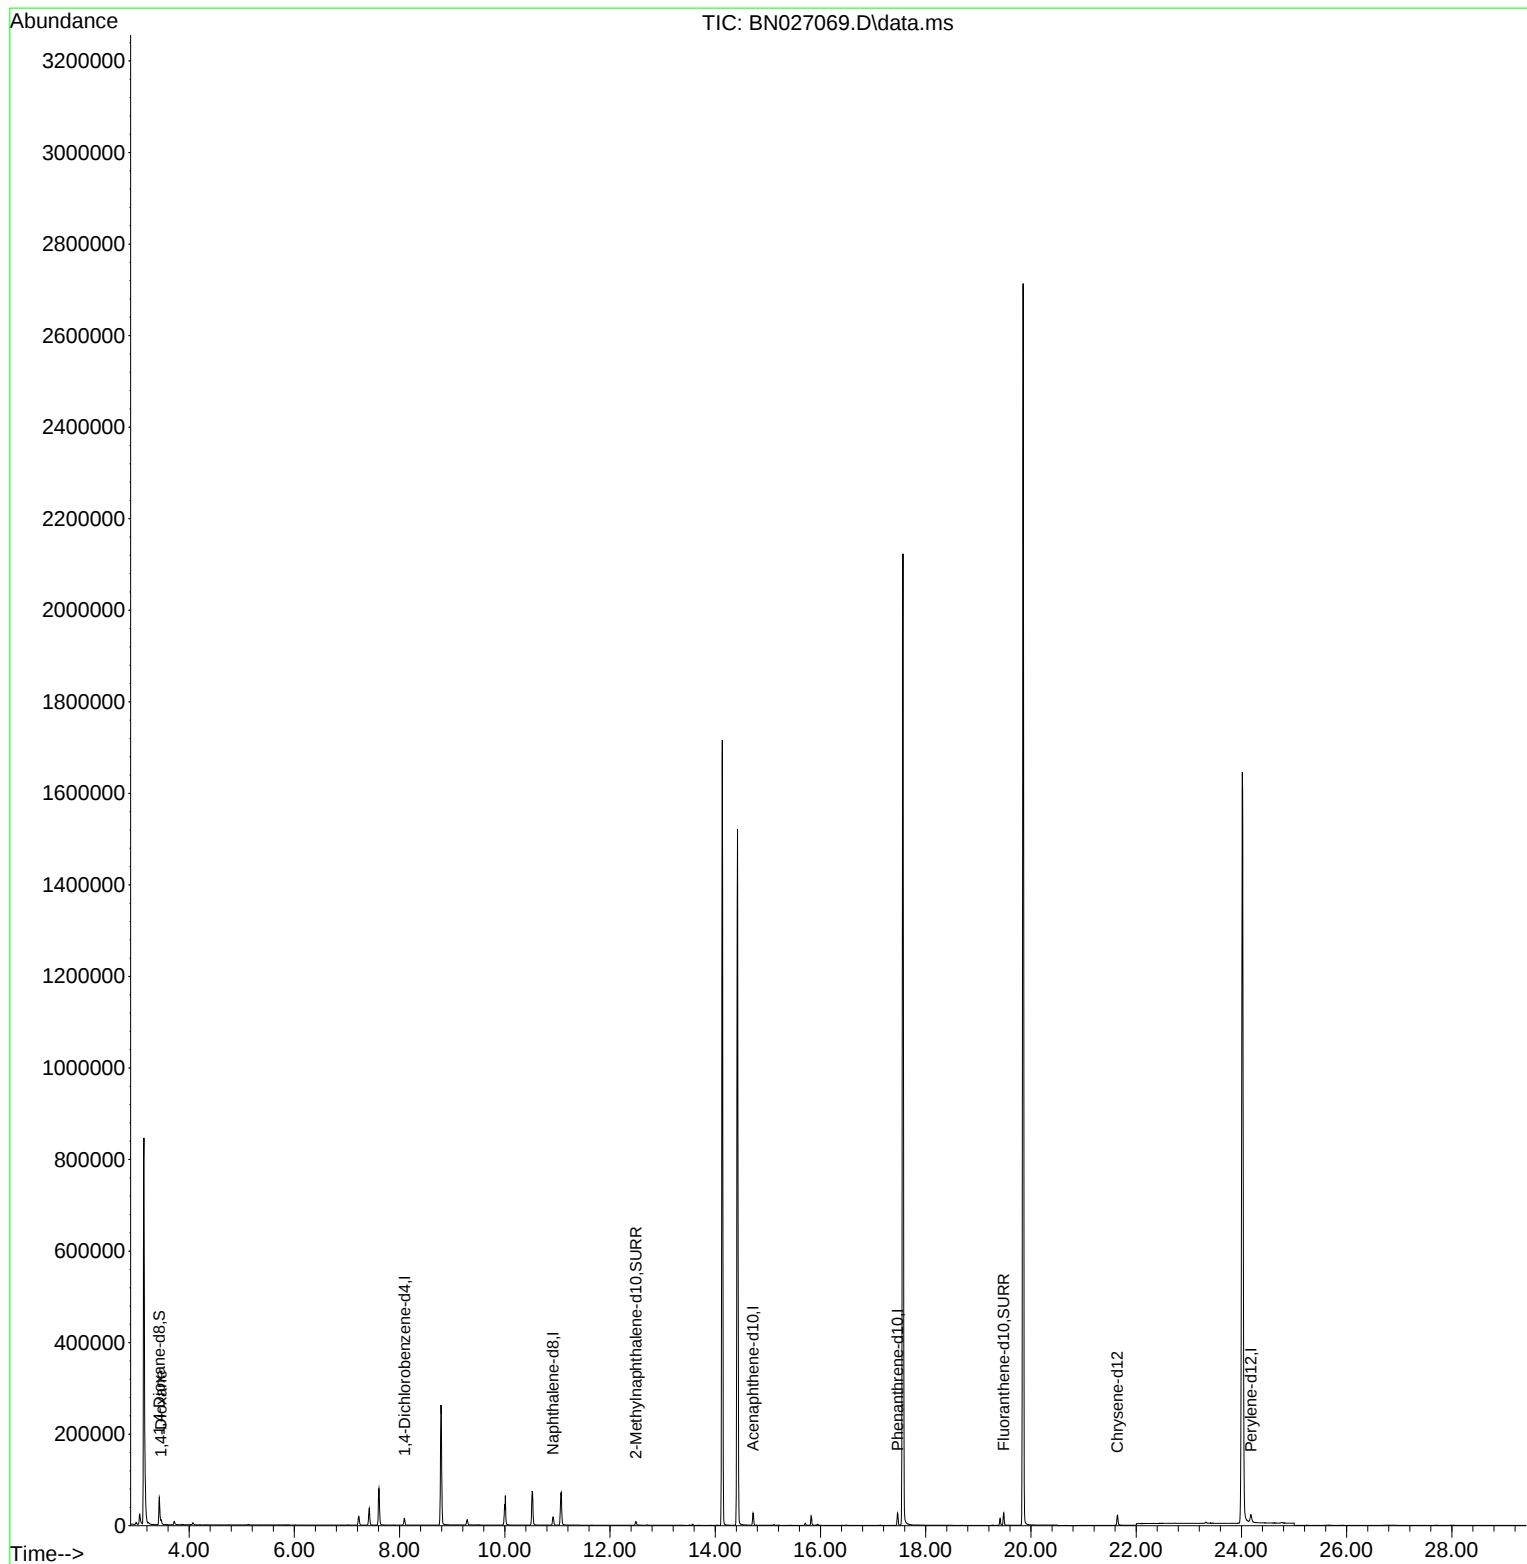

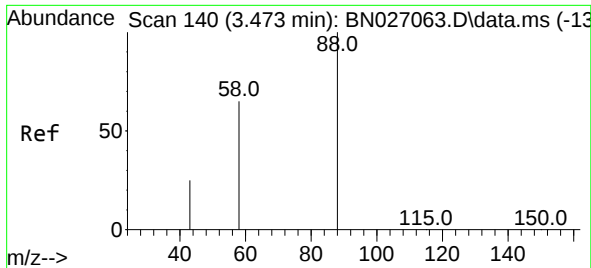

#2
 1,4-Dioxane
 Concen: 0.727 ng/ul
 RT: 3.469 min Scan# 11
 Delta R.T. -0.009 min
 Lab File: BN027069.D
 Acq: 23 Aug 2023 19:42

Instrument :
 BNA_N
 ClientSampleId :
 BH316

Tgt Ion: 88 Resp: 6429

Ion	Ratio	Lower	Upper
88	100		
43	33.8	28.0	42.0
58	58.4	46.0	69.0

