

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
 Data File : BN027085.D
 Acq On : 24 Aug 2023 06:04
 Operator : MA/JU
 Sample : 04105-02
 Misc :
 ALS Vial : 105 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9F7

Quant Time: Aug 24 06:53:53 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 23 02:28:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.088	152	7727	0.400	ng/ul	0.00
4) Naphthalene-d8	10.911	136	26015	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.717	164	15822	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.464	188	34601	0.400	ng/ul	0.00
17) Chrysene-d12	21.635	240	25697	0.400	ng/ul	0.00
23) Perylene-d12	24.170	264	25334	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.435	96	41793	4.556	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.489	152	11036	0.288	ng/ul	0.00
18) Fluoranthene-d10	19.478	212	32834	0.405	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.473	88	27119	2.896	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082123\
Data File : BN027085.D
Acq On : 24 Aug 2023 06:04
Operator : MA/JU
Sample : 04105-02
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9F7

Quant Time: Aug 24 06:53:53 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 23 02:28:27 2023
Response via : Initial Calibration

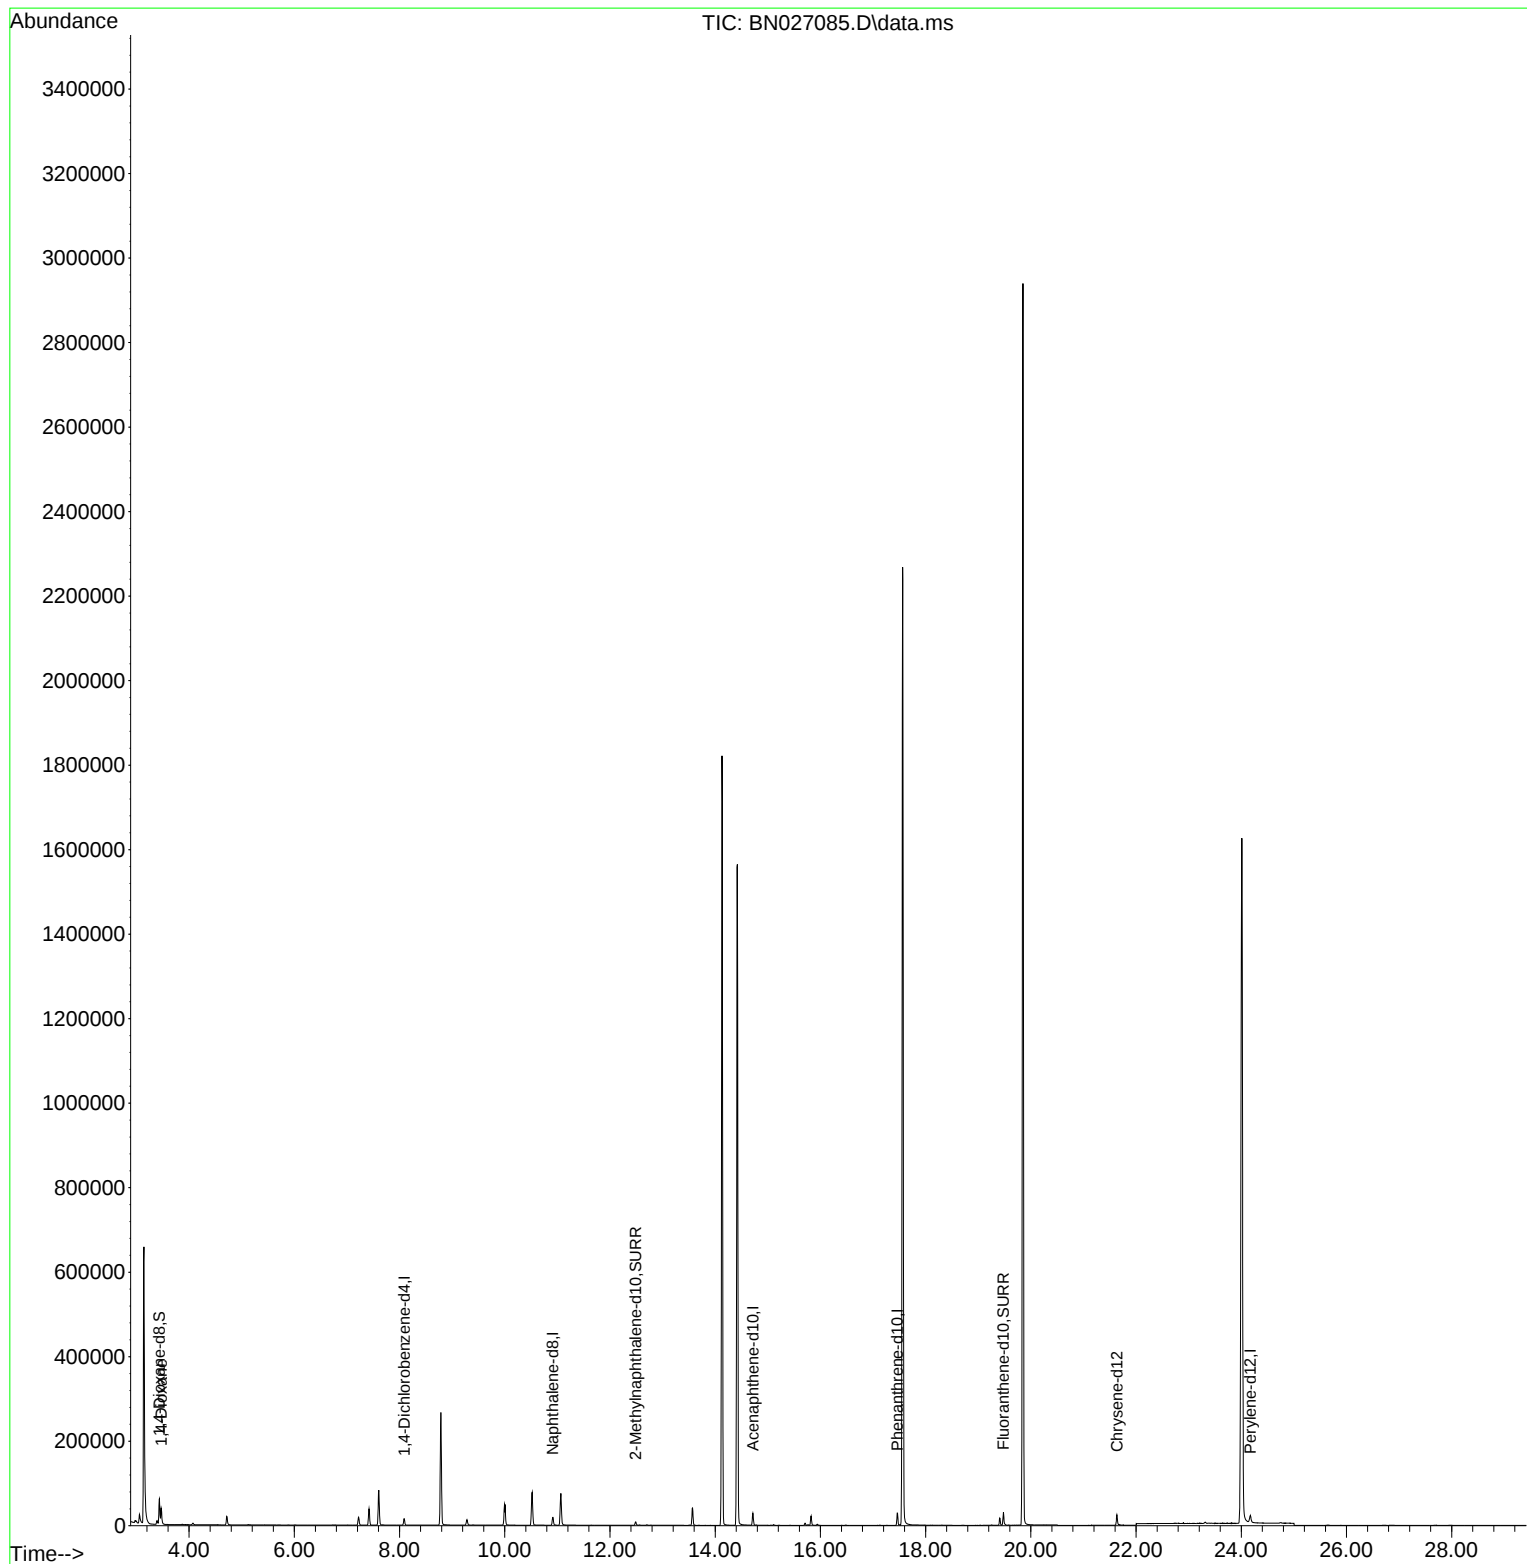

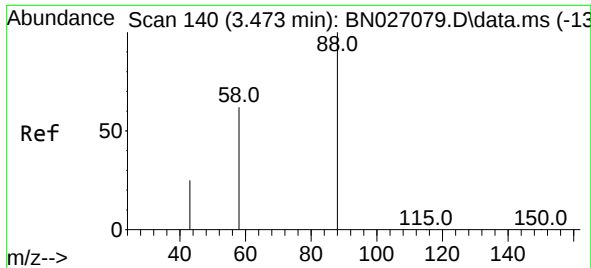

#2
 1,4-Dioxane
 Concen: 2.896 ng/ul
 RT: 3.473 min Scan# 14
 Delta R.T. -0.004 min
 Lab File: BN027085.D
 Acq: 24 Aug 2023 06:04

Instrument :
 BNA_N
 ClientSampleId :
 BH9F7

Tgt Ion: 88 Resp: 27119
 Ion Ratio Lower Upper
 88 100
 43 24.5 28.0 42.0#
 58 58.9 46.0 69.0

