

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082218\
 Data File : BN002453.D
 Acq On : 22 Aug 2018 12:44
 Operator : JU/SJ
 Sample : J4514-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0335

Quant Time: Aug 23 04:49:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 23 04:38:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	146542	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	694431	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	443764	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	1076258	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1208309	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	1242628	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.24	96	23094	7.44	ng/uL	0.00
5) Phenol-d5	6.85	99	125909	9.37	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	331328	39.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	329076	32.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	225458	20.99	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	213219	38.57	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	225582	38.80	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	369992	34.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	24056	2.08	ng/ul	0.02
43) Dimethylphthalate-d6	13.72	166	1496713	40.69	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	1819379	40.32	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	38572	5.55	ng/ul	0.01
57) Fluorene-d10	15.30	176	1304326	40.90	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	212348	30.99	ng/ul	0.00
70) Anthracene-d10	17.15	188	2094895	40.74	ng/ul	0.00
78) Pyrene-d10	19.45	212	2350380	40.65	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	2636496	40.58	ng/ul	0.00


Target Compounds					Ovalue	
2) 1,4-Dioxane	3.27	88	47565	14.320	ng/uL	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082218\
Data File : BN002453.D
Acq On : 22 Aug 2018 12:44
Operator : JU/SJ
Sample : J4514-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0335

Quant Time: Aug 23 04:49:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 23 04:38:12 2018
Response via : Initial Calibration

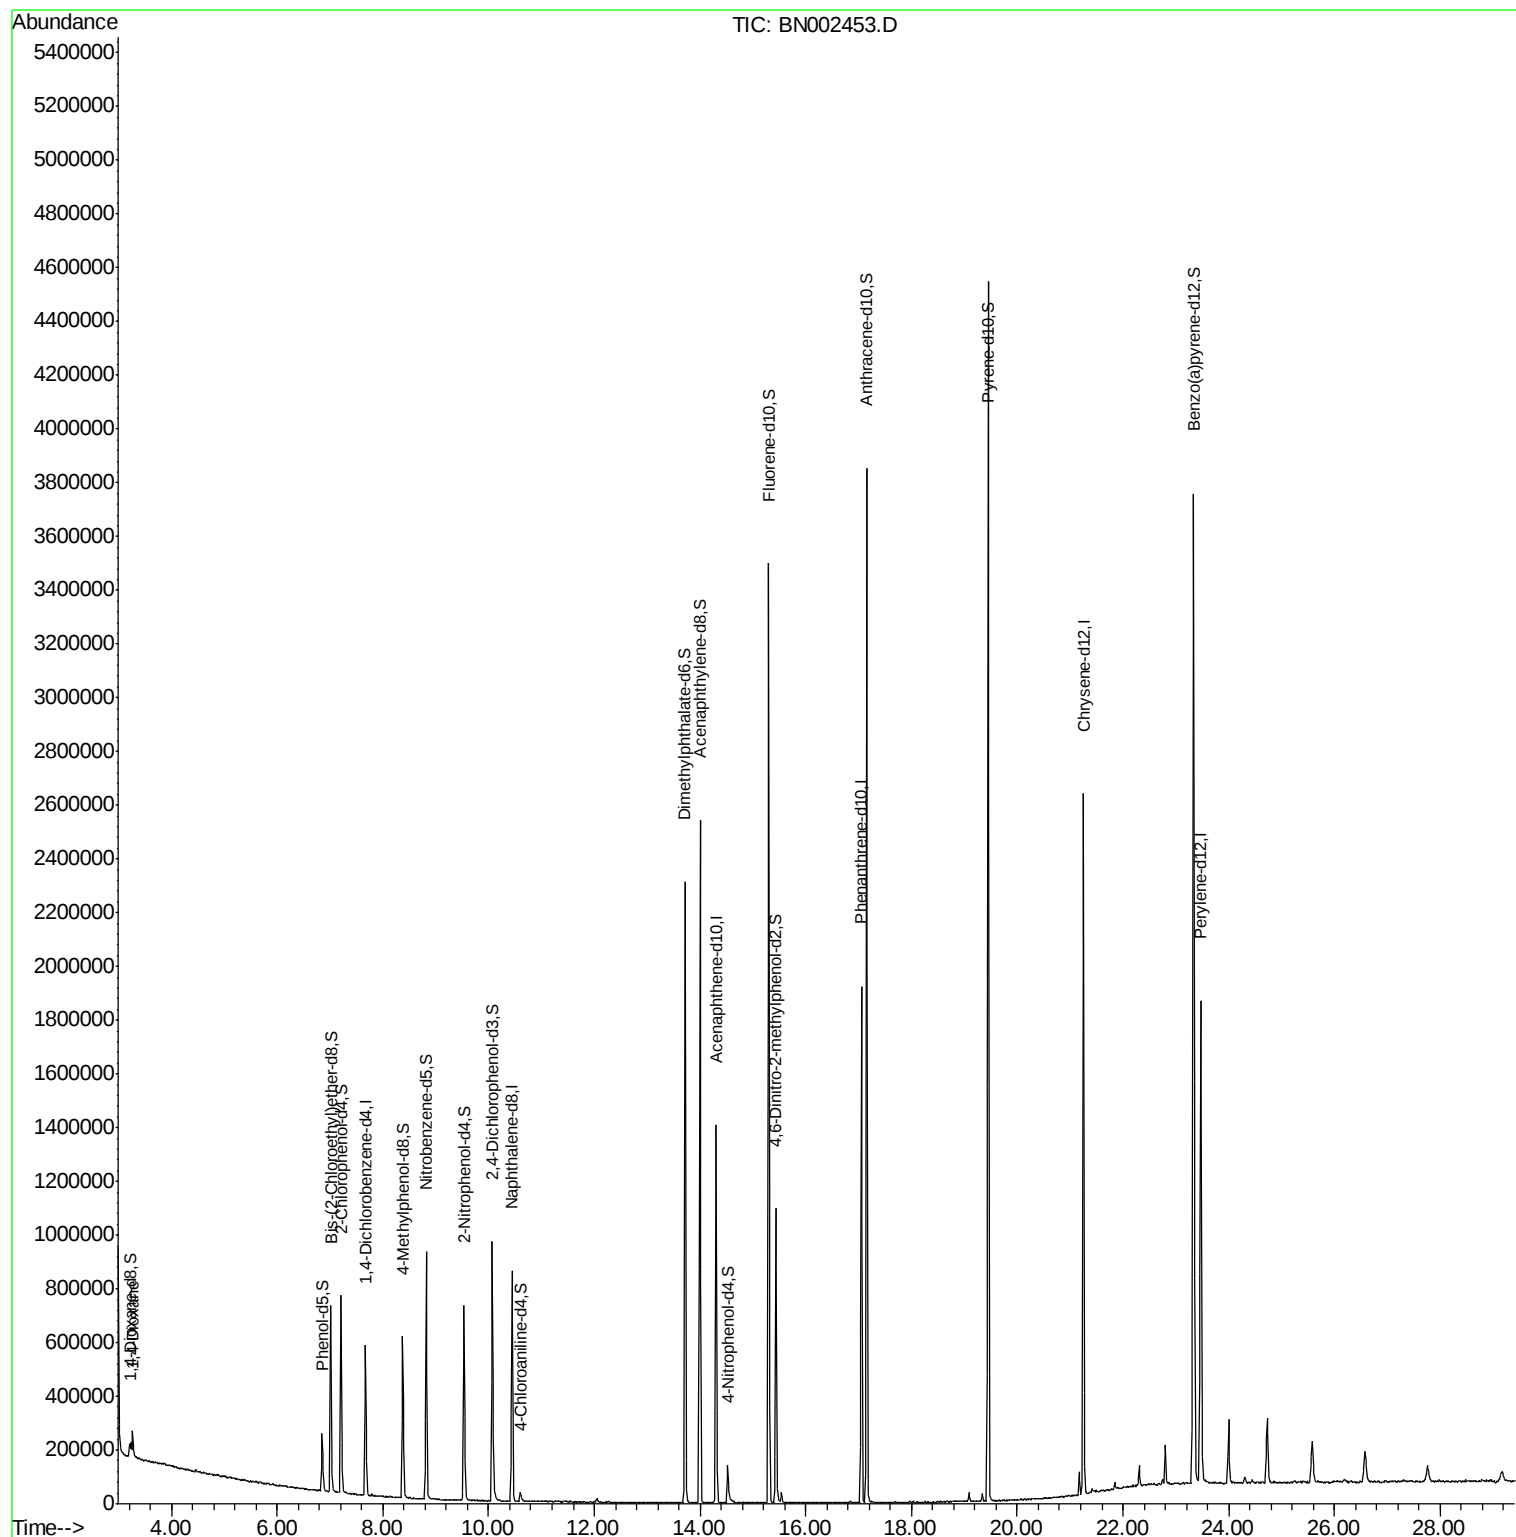

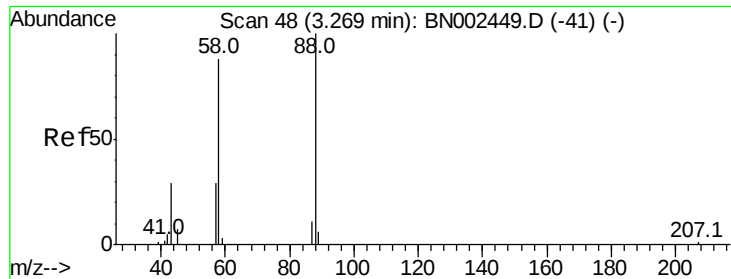

#2
 1,4-Dioxane
 Concen: 14.320 ng/uL
 RT: 3.27 min Scan# 48
 Delta R.T. -0.00 min
 Lab File: BN002453.D
 Acq: 22 Aug 2018 12:44

Instrument :
 BNA_N
 ClientSampleId :
 C0335

Tot Ion: 88 Resp: 47565
 Ion Ratio Lower Upper
 88 100
 43 33.6 32.0 48.0
 58 88.0 72.0 108.0

