

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002480.D
 Acq On : 23 Aug 2018 23:36
 Operator : JU/SJ
 Sample : PB112072BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 24 00:56:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 00:52:48 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	2067	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.44	136	8850	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.31	164	5682	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.15	188	2058486	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.26
20) Perylene-d12	23.48	264	13456	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	8228	0.59	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.31	166	3529	0.152	ng/ul#	19
23) Benzo(a)pyrene	23.34	252	8258	0.182	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
Data File : BN002480.D
Acq On : 23 Aug 2018 23:36
Operator : JU/SJ
Sample : PB112072BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 24 00:56:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 24 00:52:48 2018
Response via : Initial Calibration




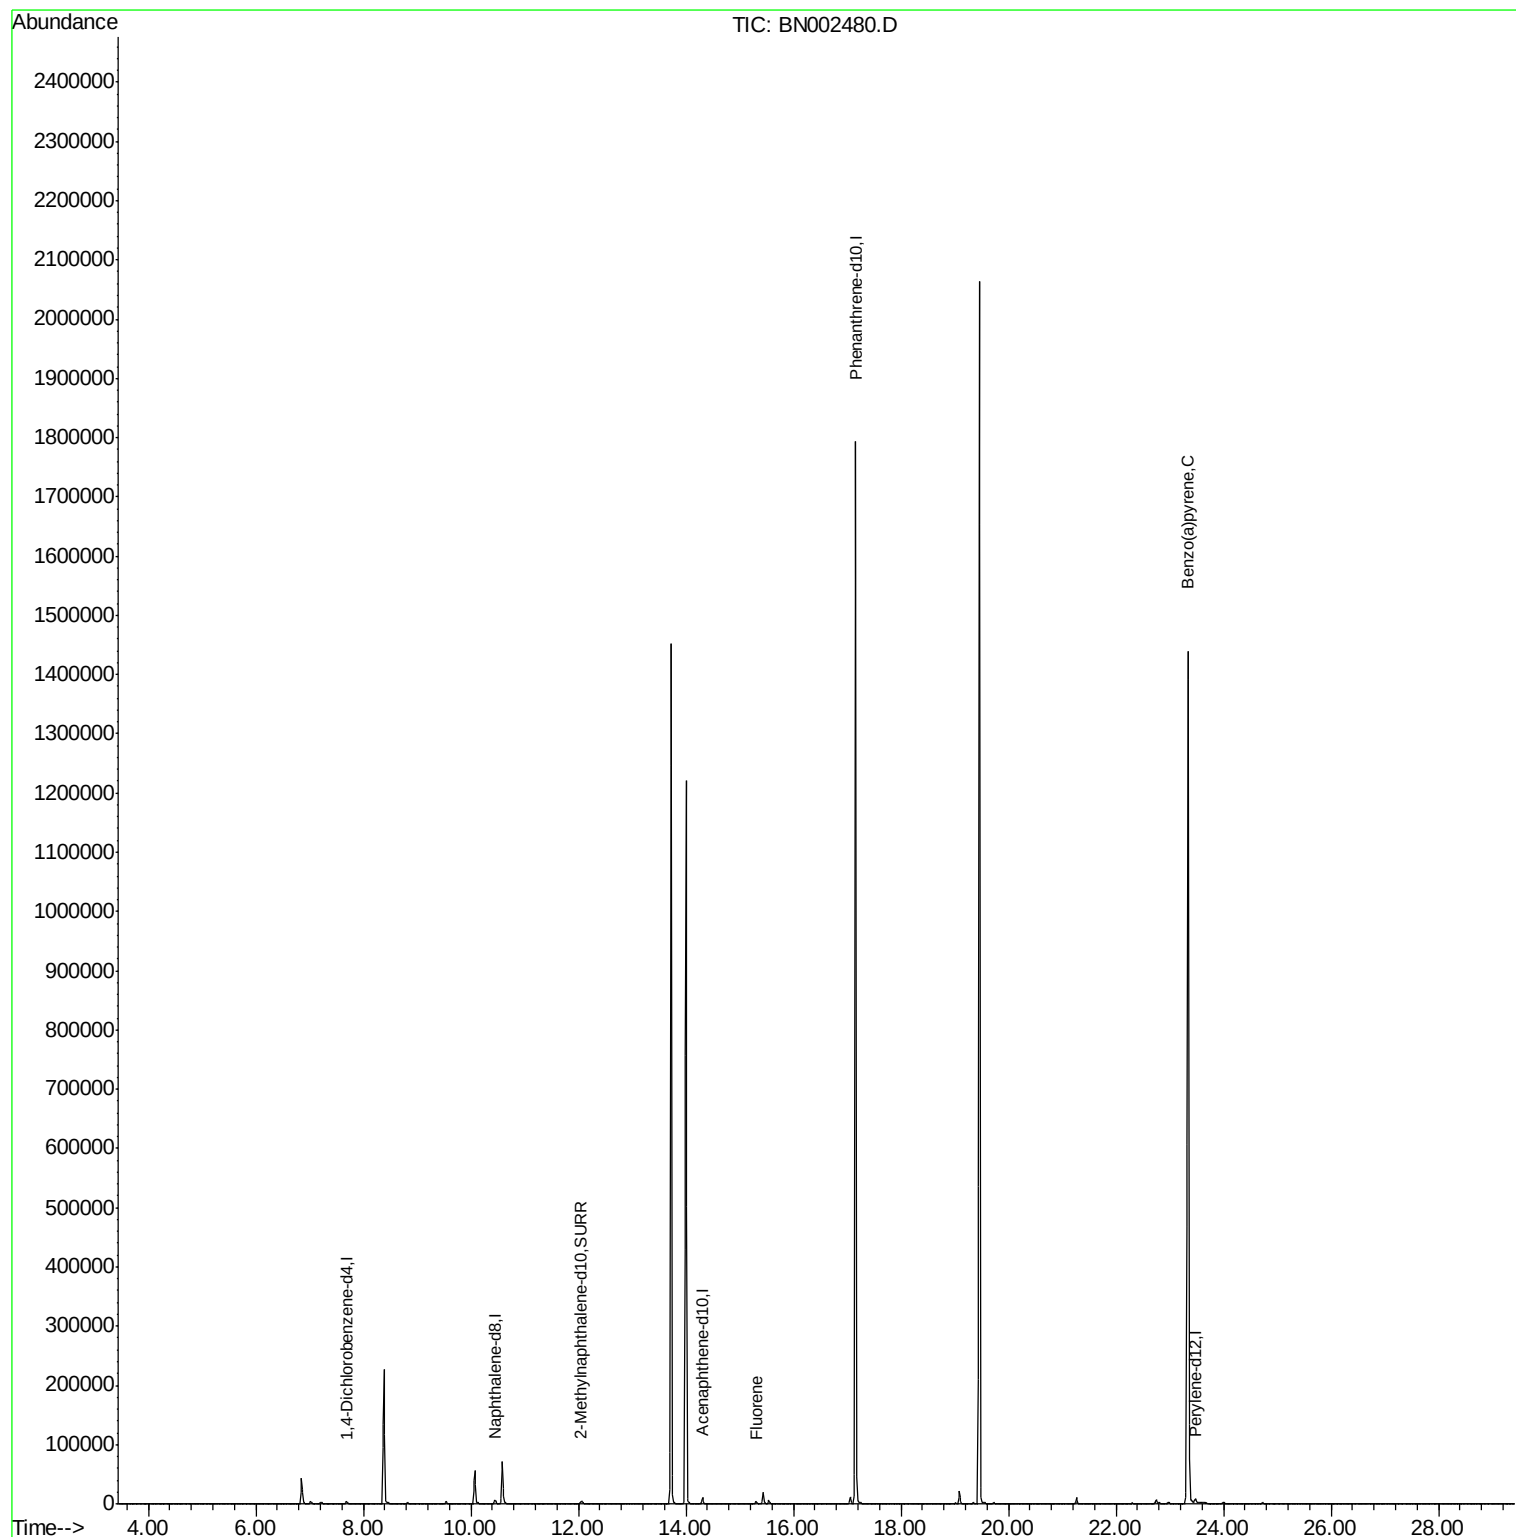


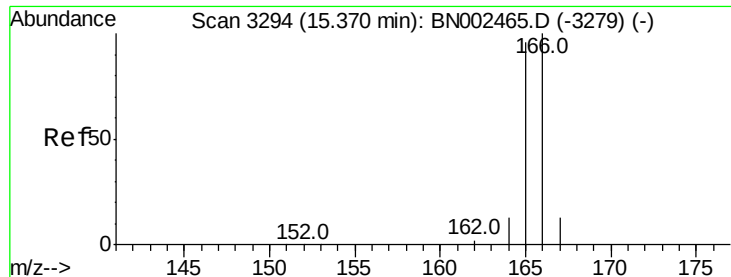

#9
Fluorene
 Concen: 0.152 ng/ul
 RT: 15.31 min Scan# 3280
 Delta R.T. -0.06 min
 Lab File: BN002480.D
 Acq: 23 Aug 2018 23:36

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion:166 Resp: 3529
 Ion Ratio Lower Upper
 166 100
 165 5.3 73.4 110.2#
 167 32.2 14.6 22.0#

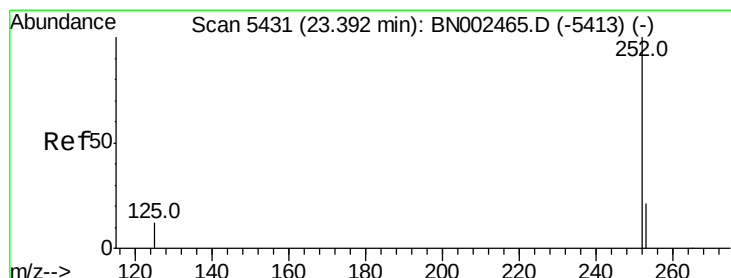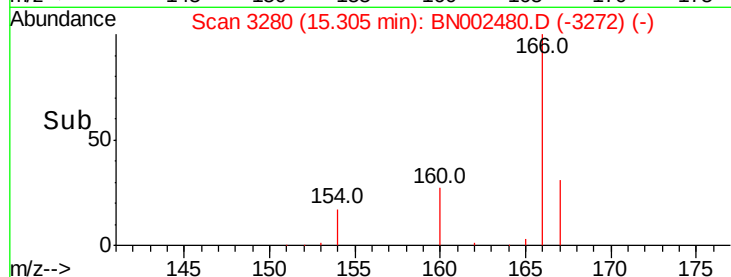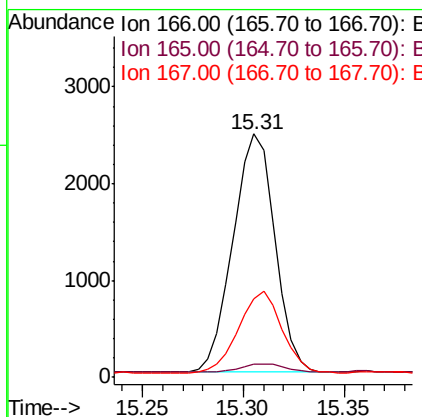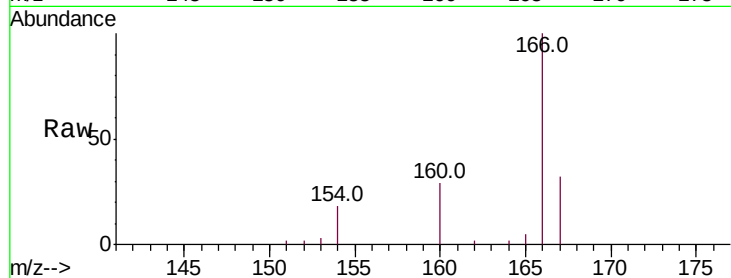

#23
Benzo(a)pyrene
 Concen: 0.182 ng/ul
 RT: 23.34 min Scan# 5412
 Delta R.T. -0.06 min
 Lab File: BN002480.D
 Acq: 23 Aug 2018 23:36

Tgt Ion:252 Resp: 8258
 Ion Ratio Lower Upper
 252 100
 253 32.5 16.0 24.0#
 125 26.2 12.0 18.0#

