

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:32:52 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

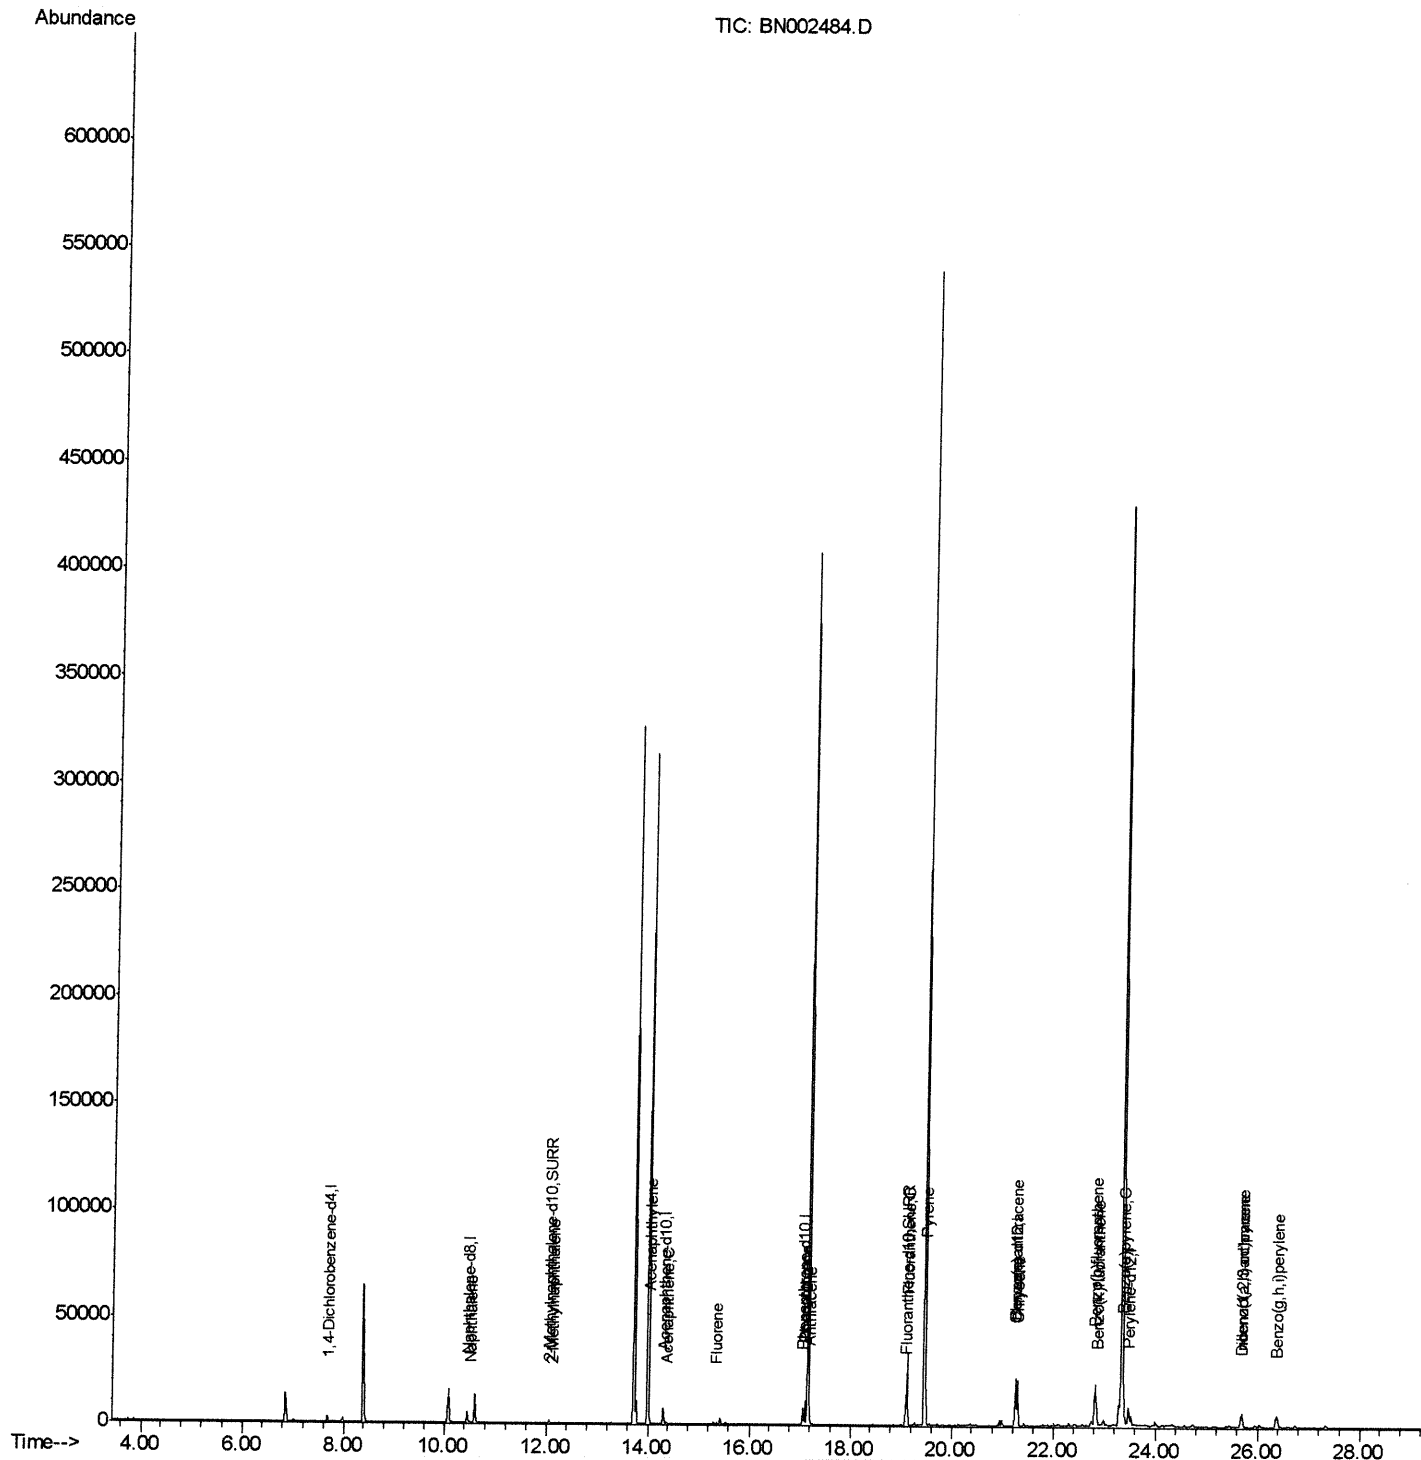

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:18:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

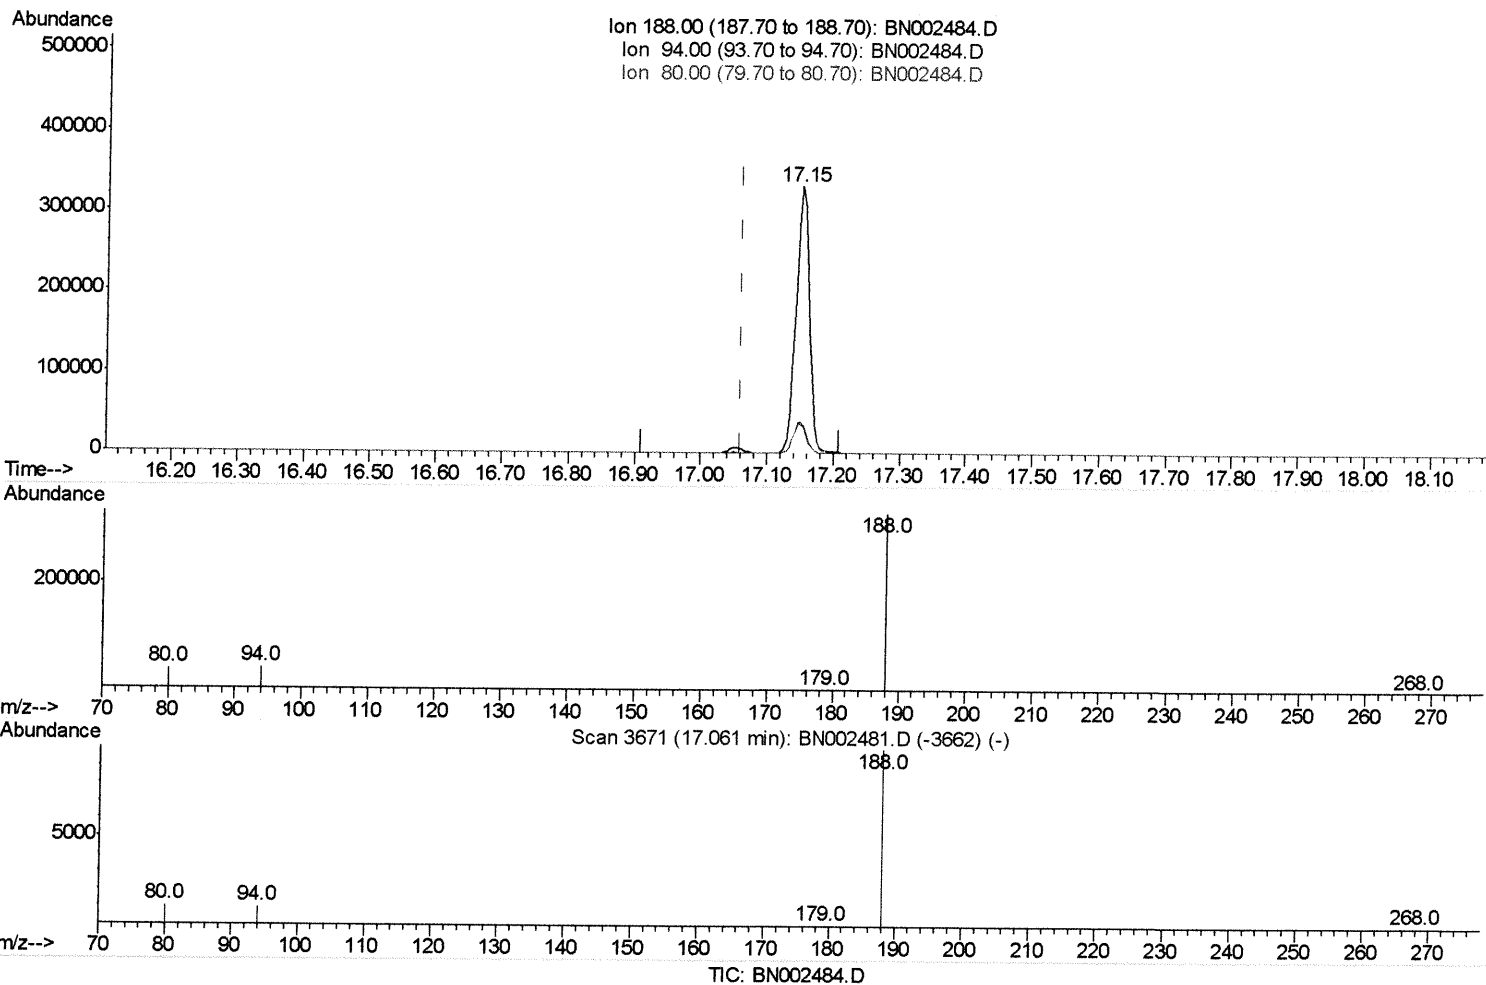

(10) Phenanthrene-d10 (I)

17.150min (+0.089) 0.40ng/ul

response 461175

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.79
80.00	11.80	11.13
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:18:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

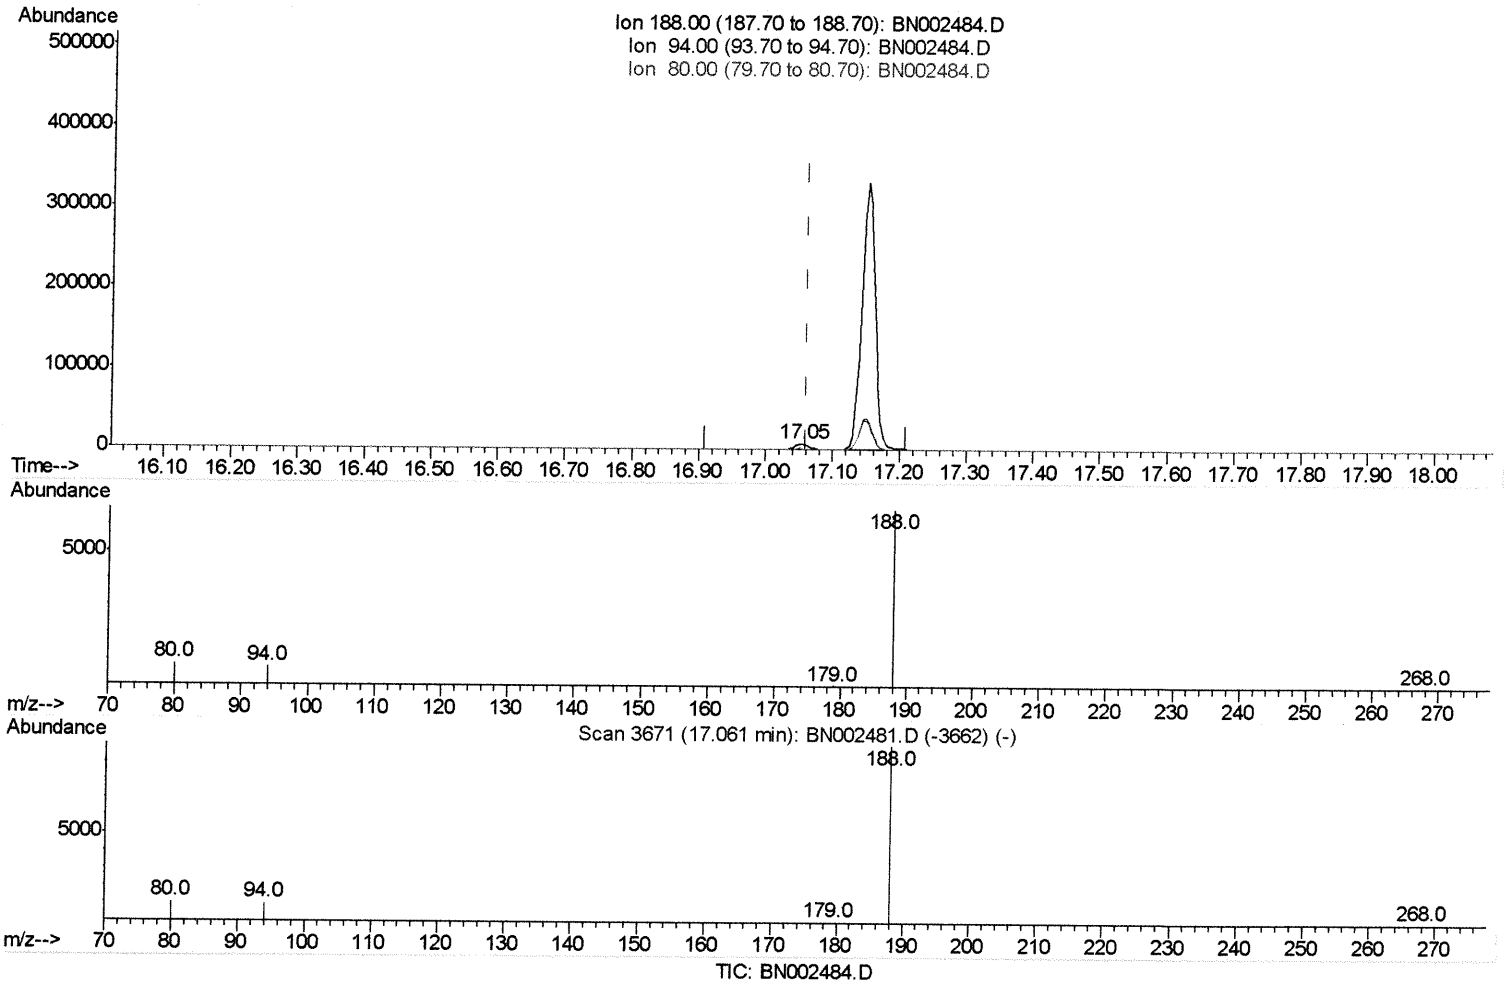

(10) Phenanthrene-d10 (I)

17.052min (-0.008) 0.40ng/ul m

SJ 8/27/18

response 9668

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.77
80.00	11.80	12.45
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:28:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

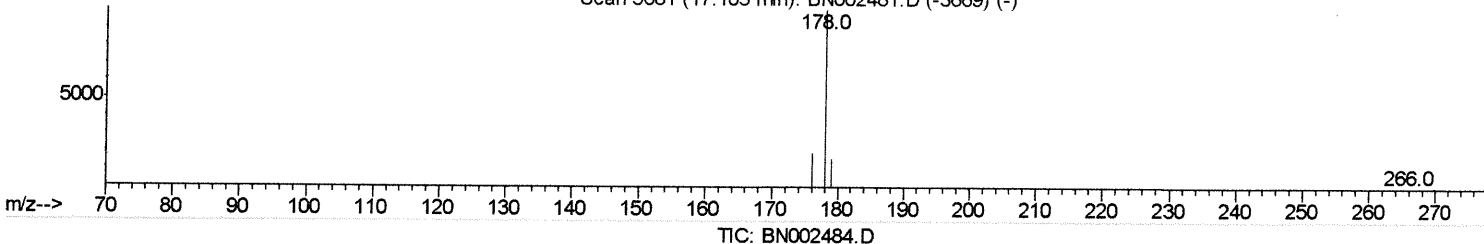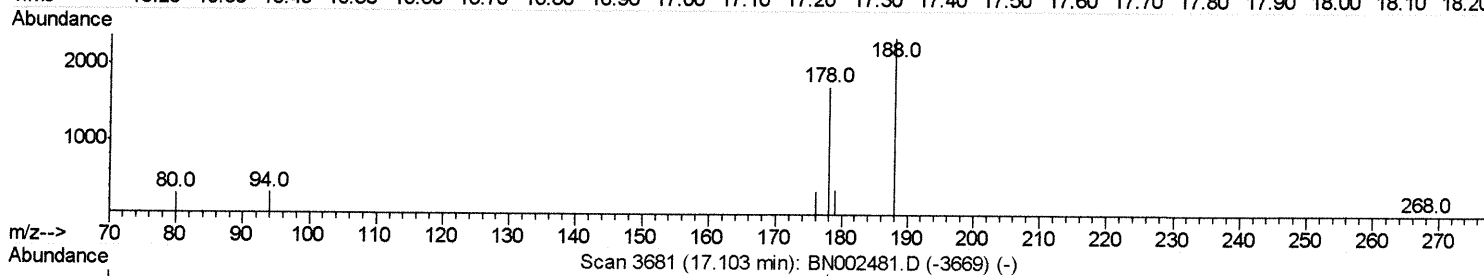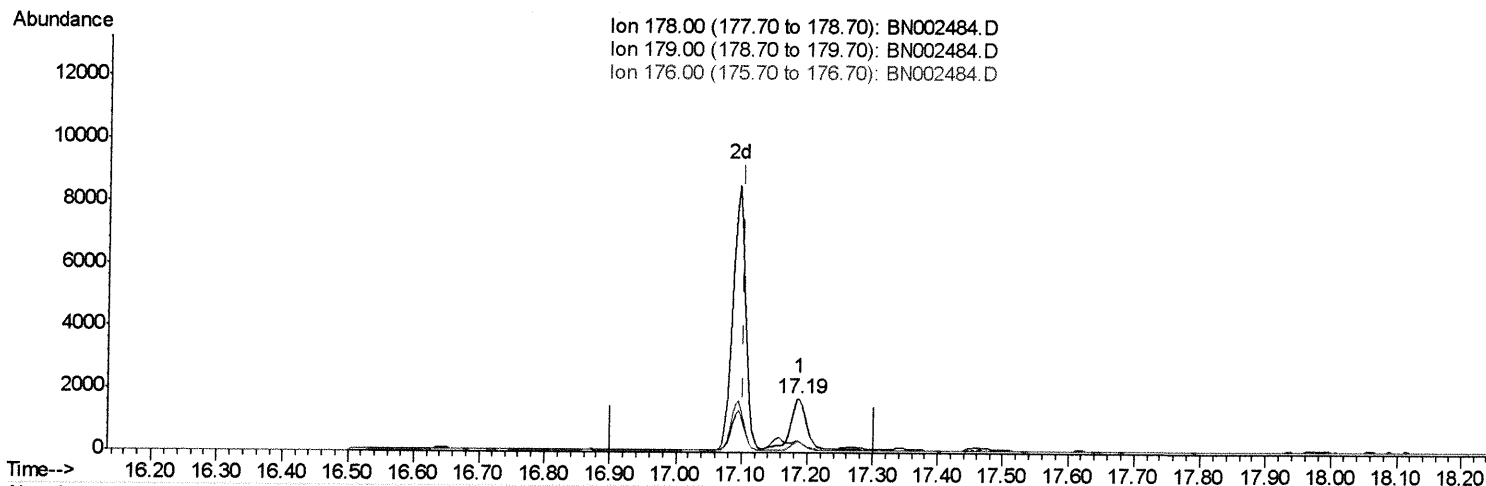

(12) Phenanthrene

17.188min (+0.085) 0.10ng/ul

response 2820

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	20.97
176.00	17.00	20.62#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:28:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

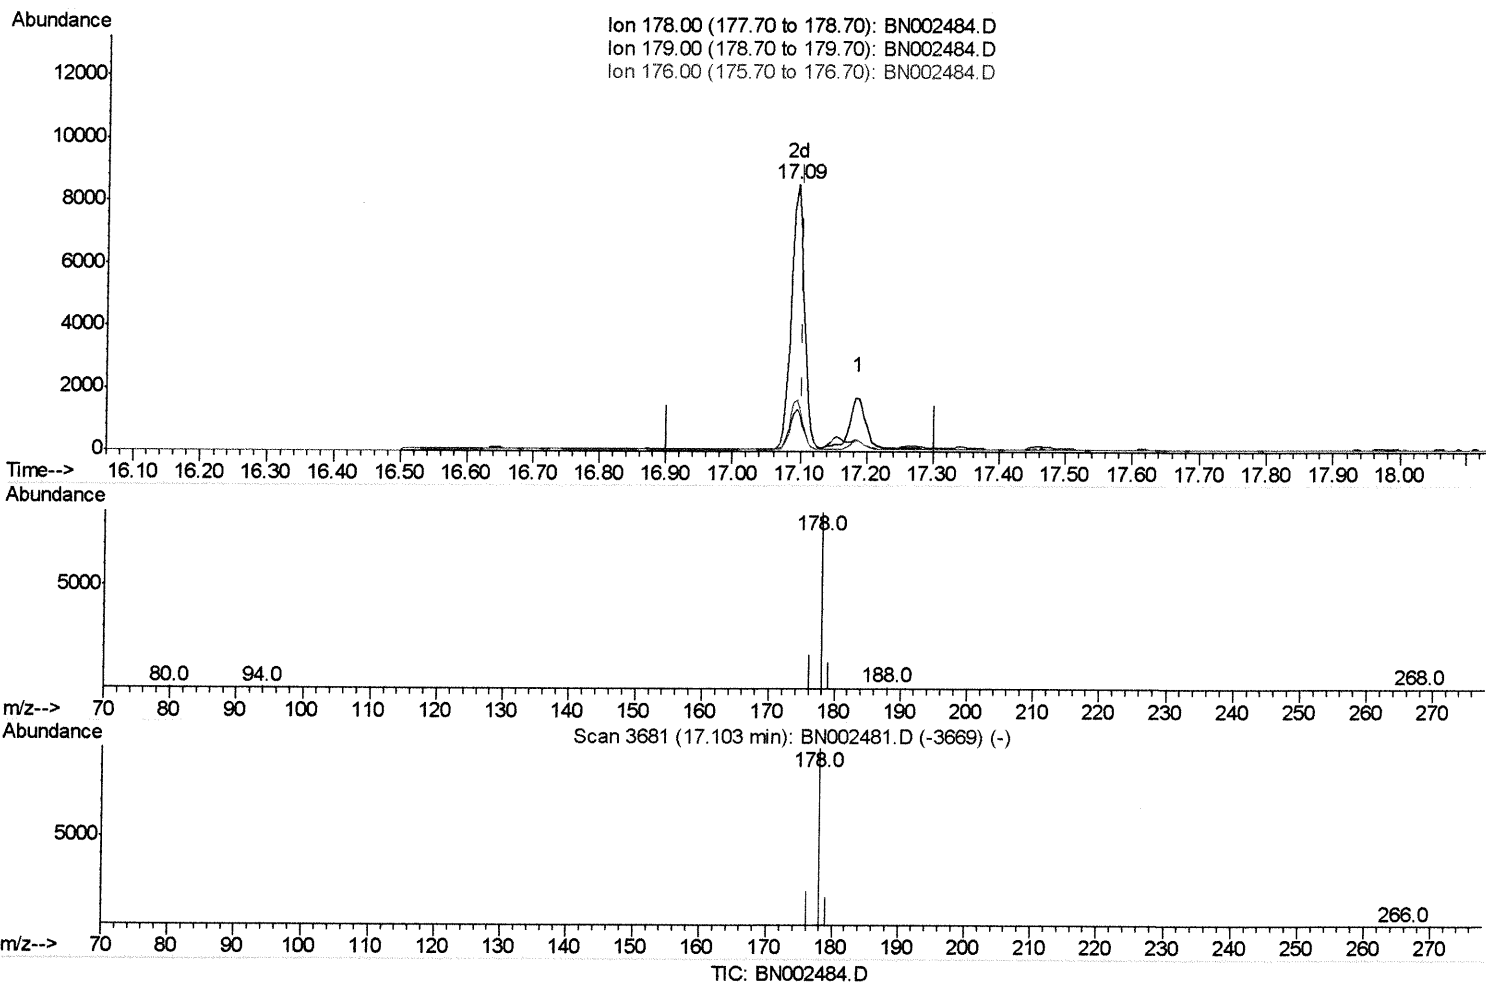

(12) Phenanthrene

17.095min (-0.008) 0.40ng/ul m

SJ 8/27/18

response 11549

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	15.84#
176.00	17.00	19.56
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:28:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

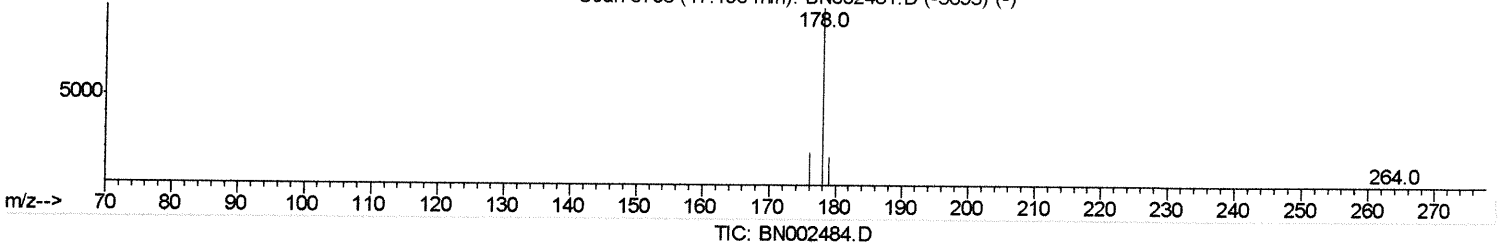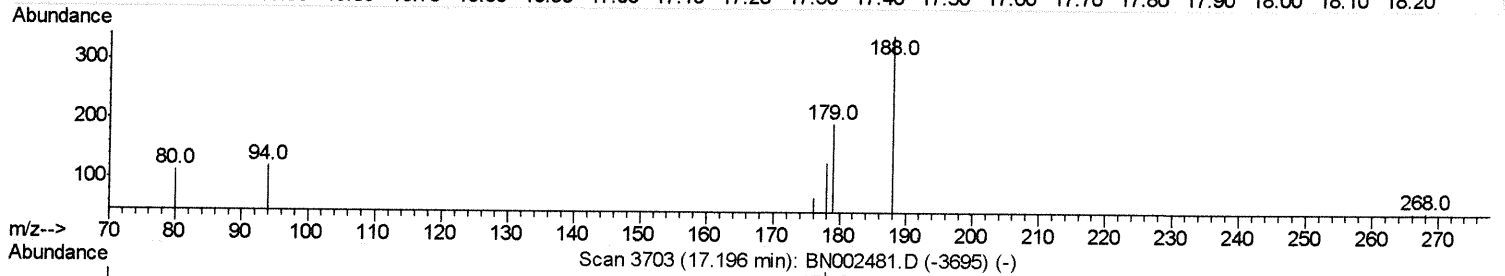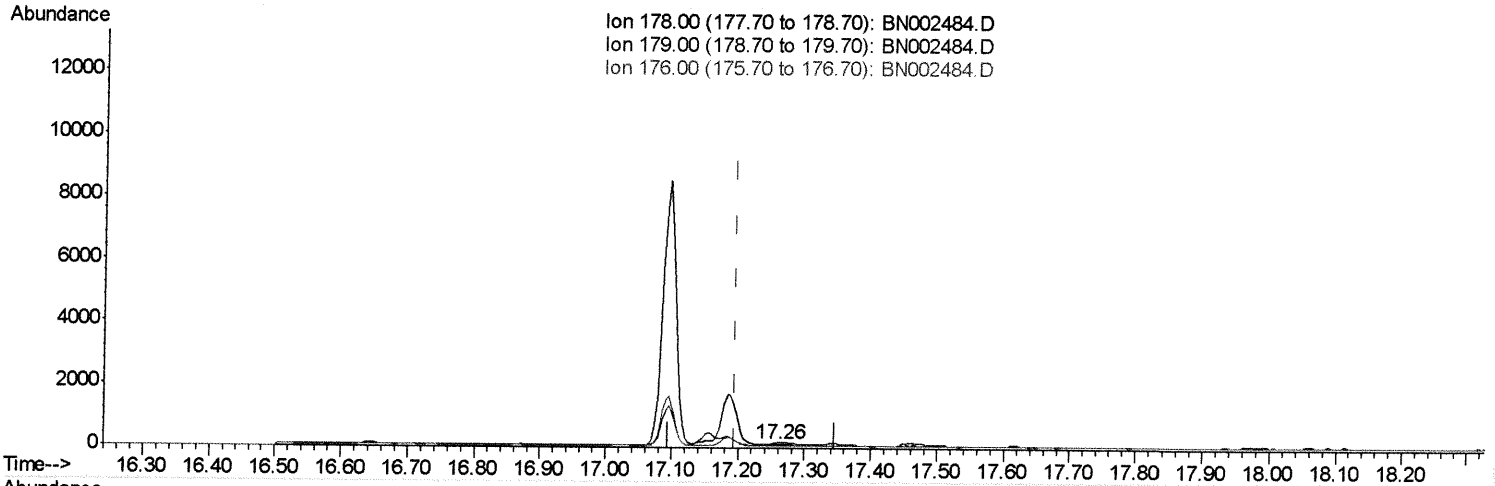

(13) Anthracene

17.259min (+0.063) 0.00ng/ul

response 81

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	150.39#
176.00	18.40	55.04#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
Data File : BN002484.D
Acq On : 24 Aug 2018 02:01
Operator : JU/SJ
Sample : J4421-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA8

Manual Integrations
APPROVED

Sohil
8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:28:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 24 02:20:09 2018
Response via : Initial Calibration

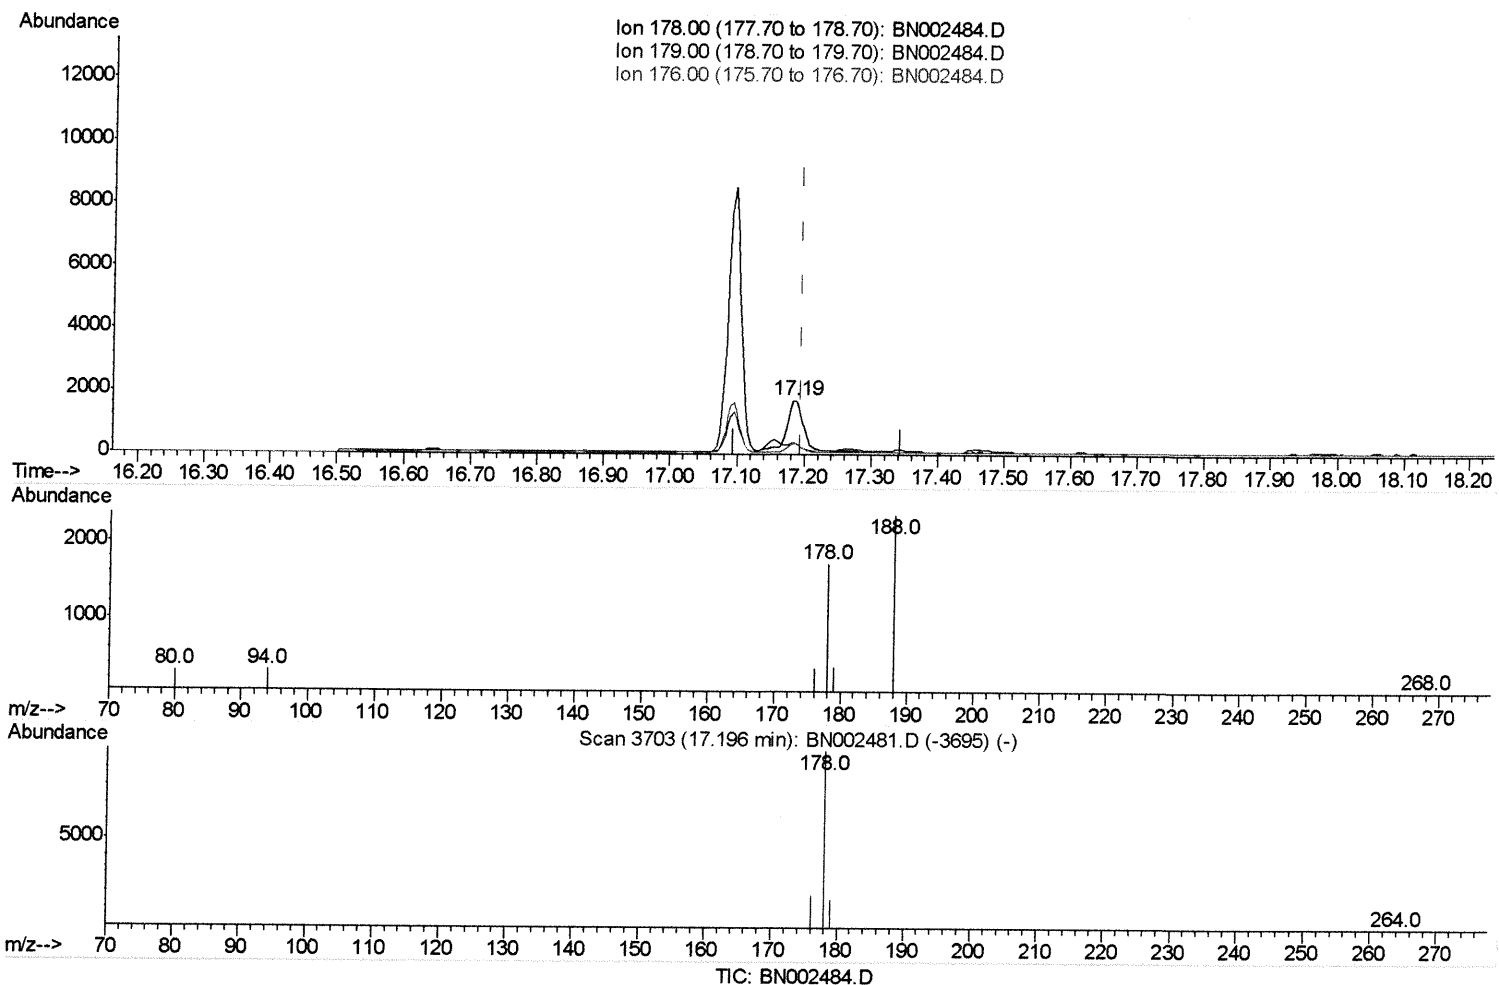

(13) Anthracene

17.188min (-0.008) 0.11ng/ul m

SJ 8/27/18

response 2619

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	20.97
176.00	18.40	20.62
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:28:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

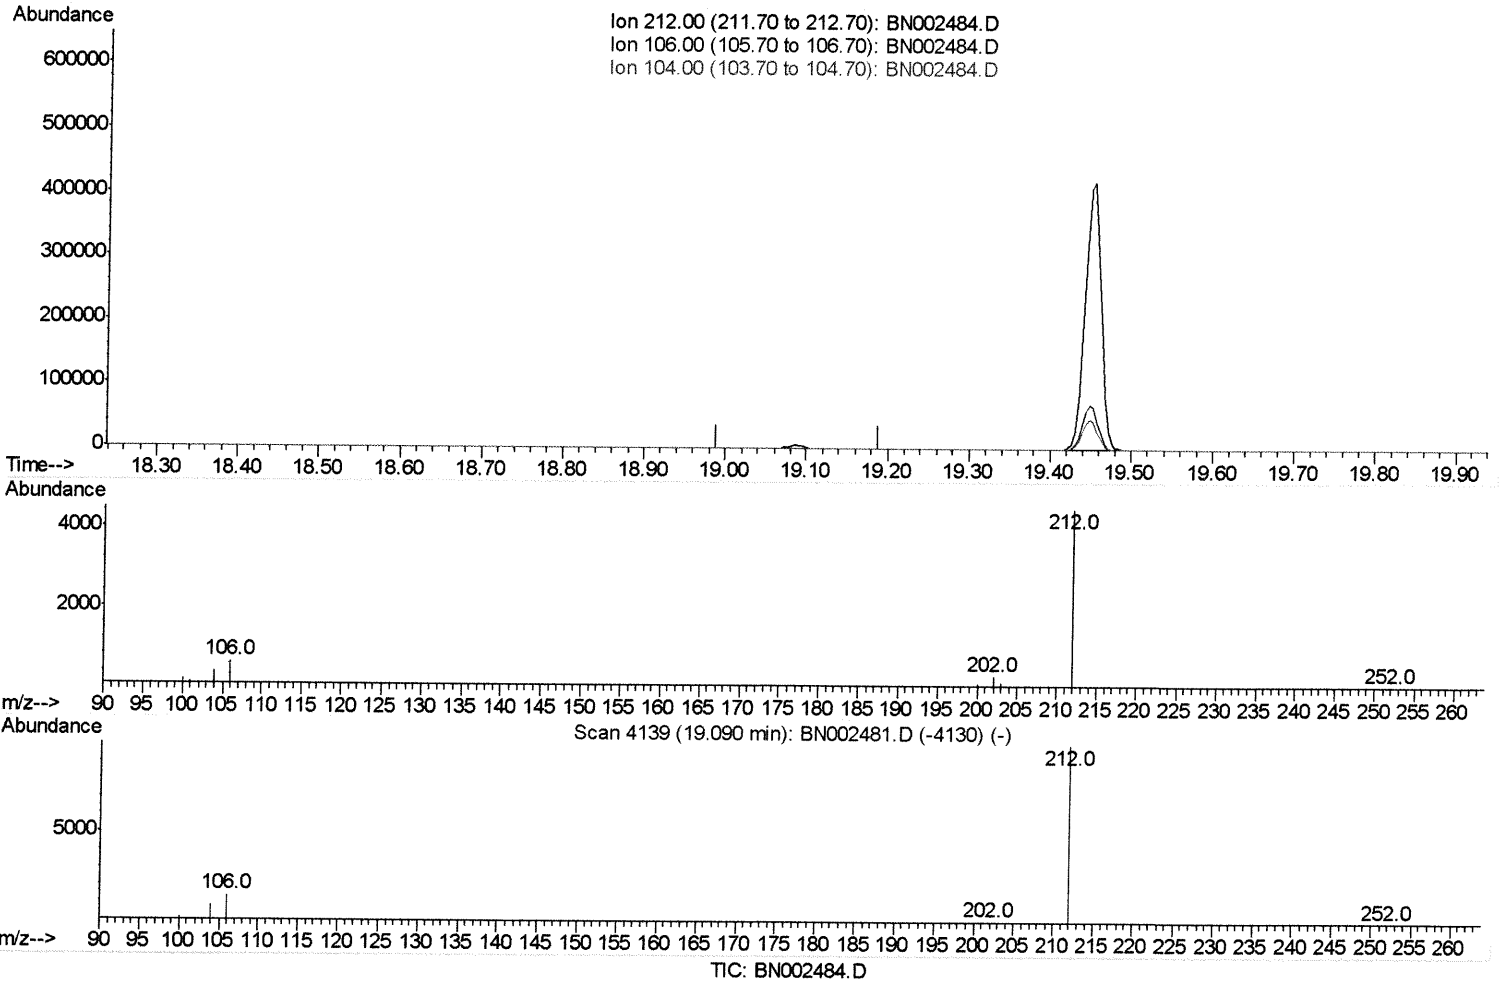

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:28:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

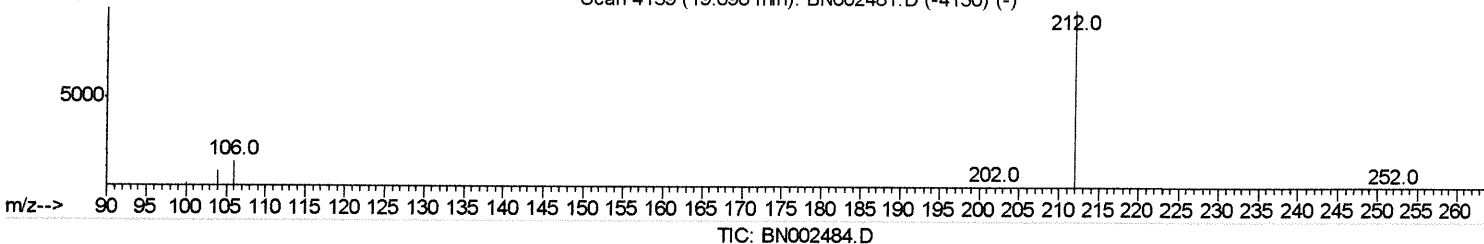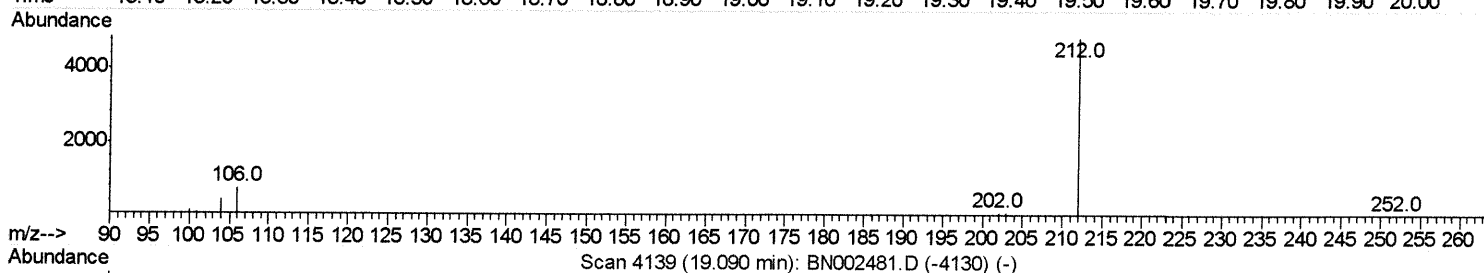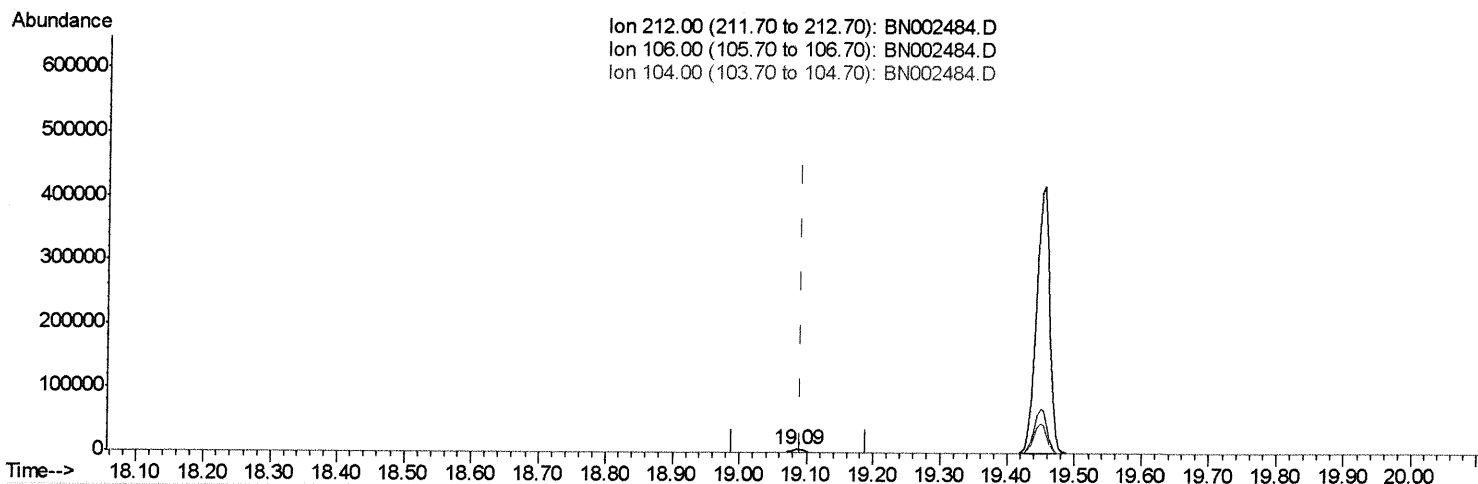

(14) Fluoranthene-d10 (SURR)

19.086min (-0.005) 0.23ng/ul m

SJ 8/27/18

response 6637

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:28:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

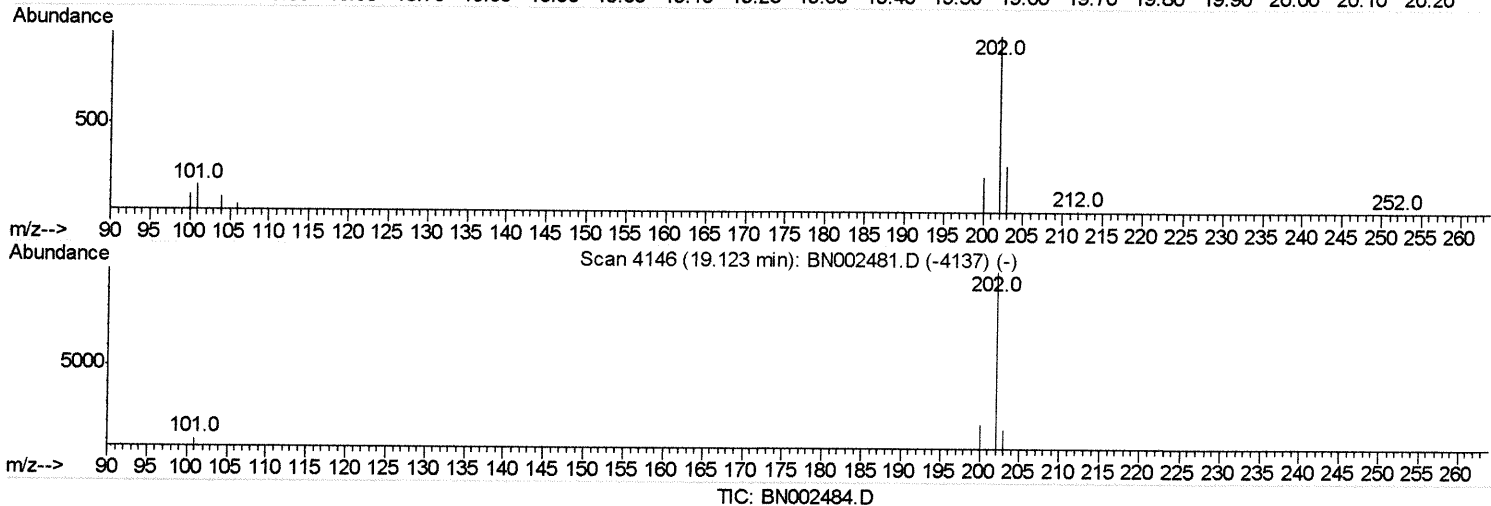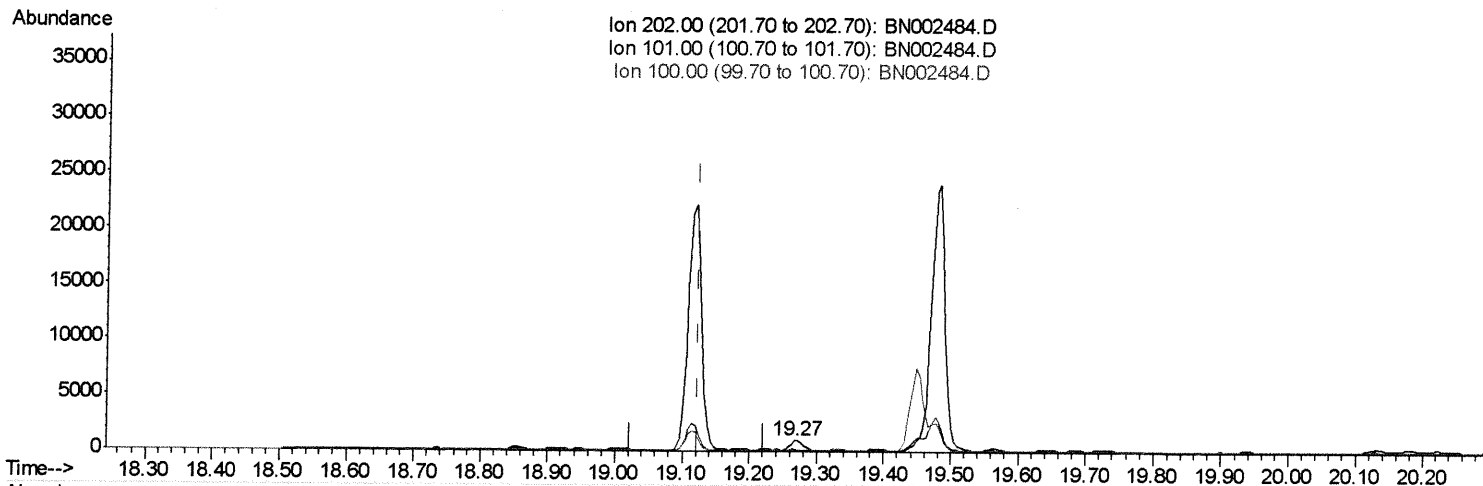

(15) Fluoranthene (C)

19.267min (+0.144) 0.03ng/ul

response 1131

Ion	Exp%	Act%
202.00	100	100
101.00	10.00	19.42
100.00	10.00	14.30
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:28:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

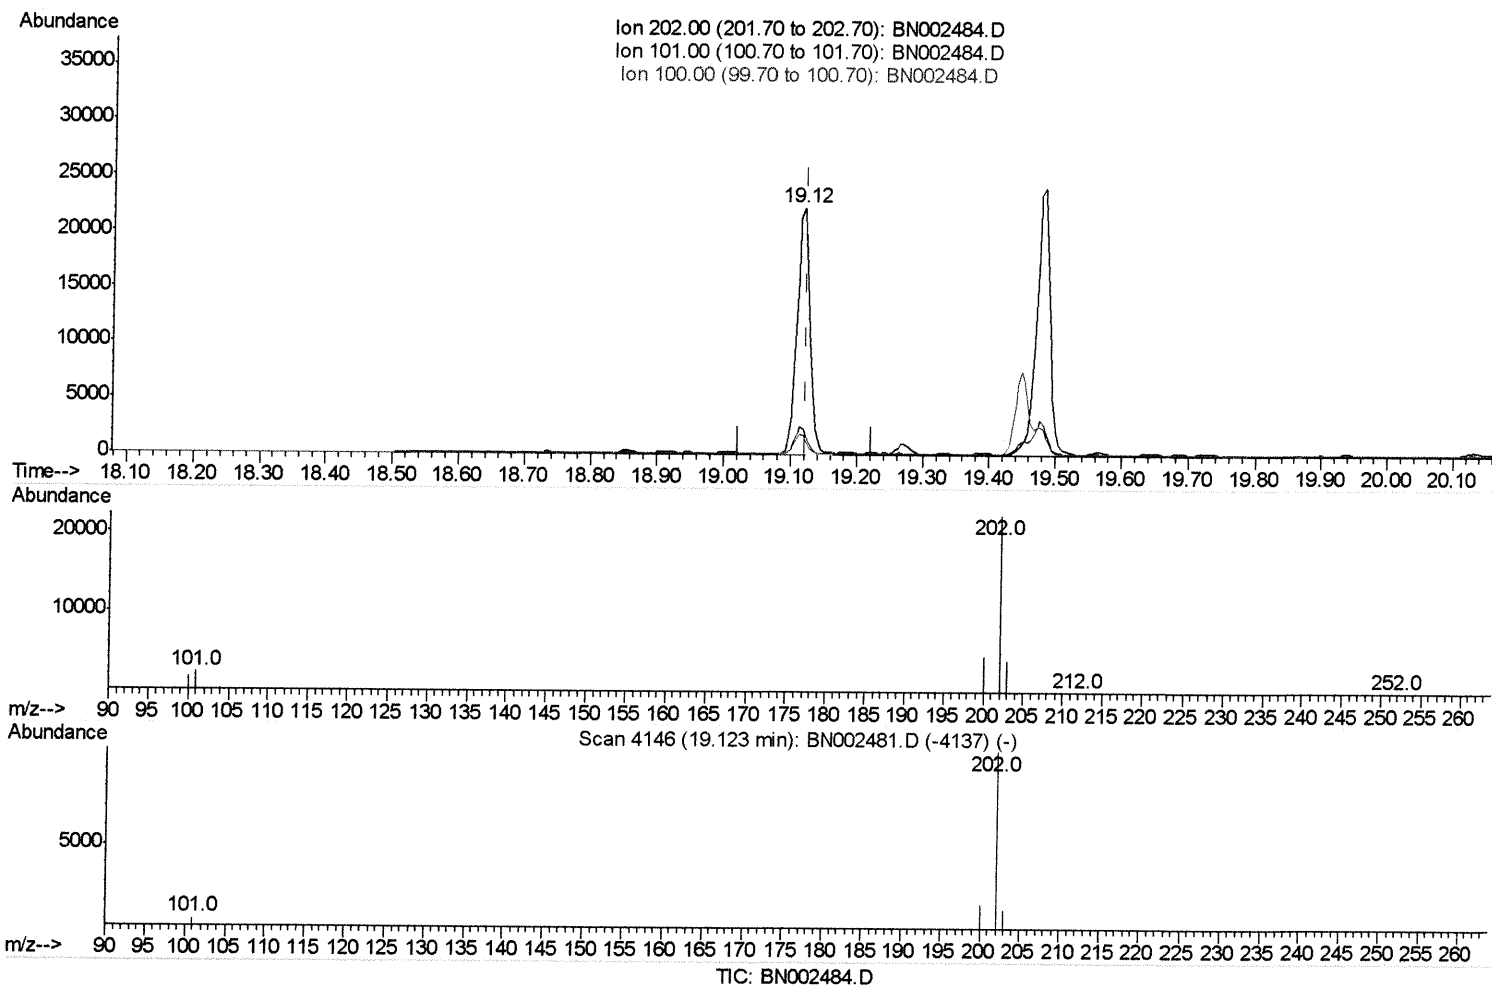

(15) Fluoranthene (C)

19.118min (-0.005) 0.90ng/ul m

SJ 8/27/18

response 30213

Ion	Exp%	Act%
202.00	100	100
101.00	10.00	10.42
100.00	10.00	7.86
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:28:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

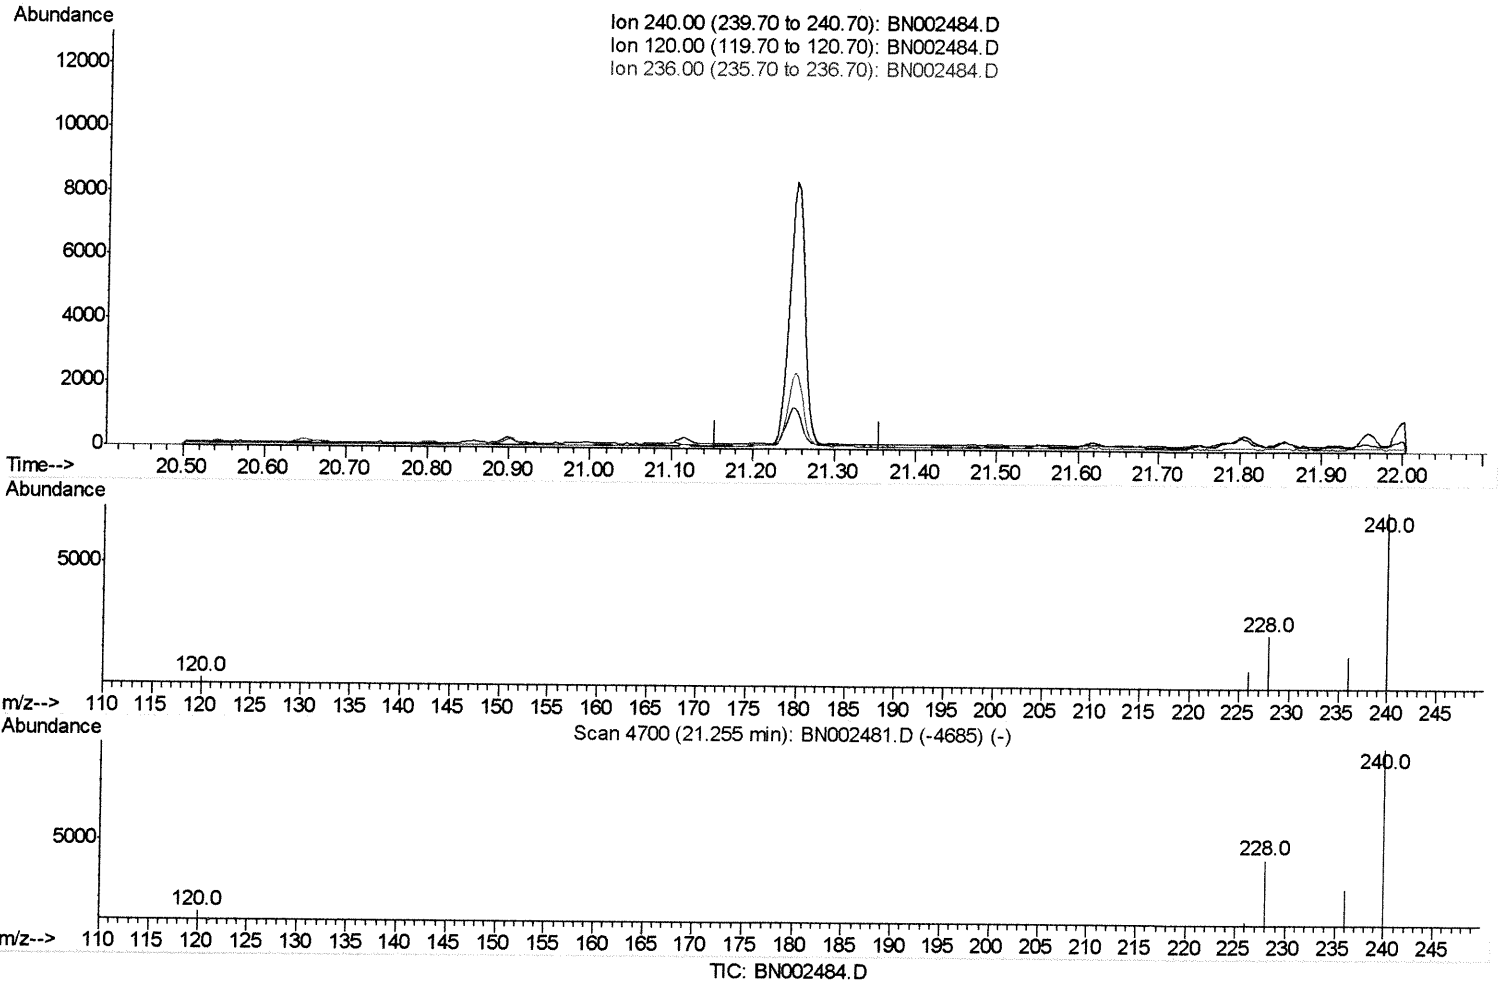

(16) Chrysene-d12 (I)

21.255min (-21.255) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.60	0.00#
236.00	34.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:28:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

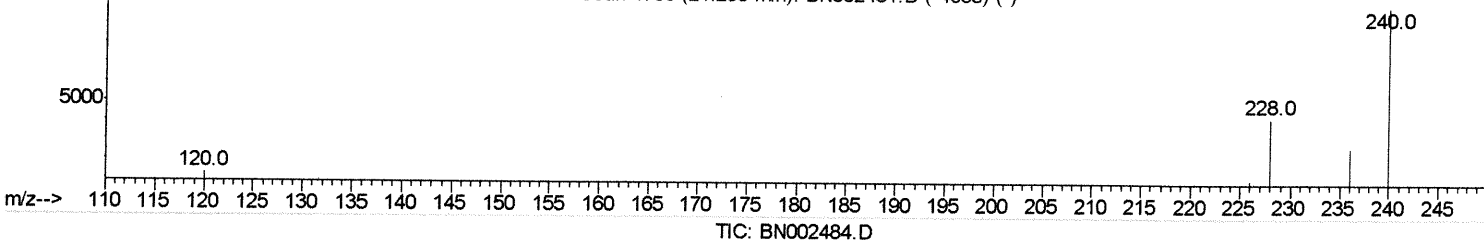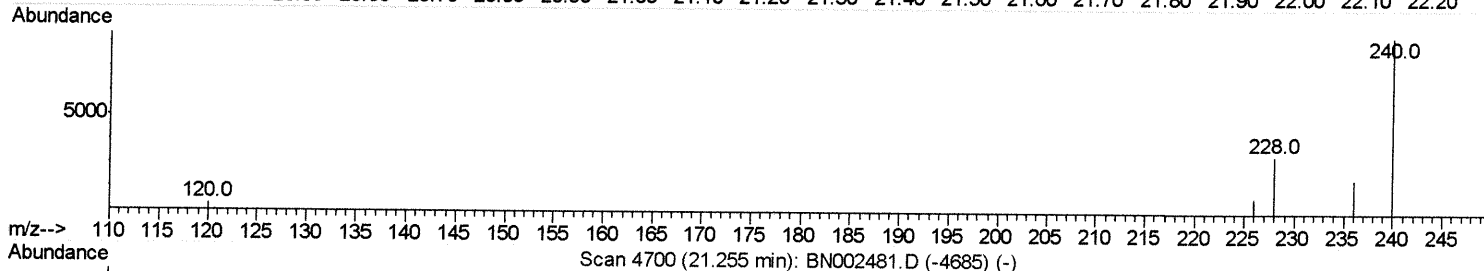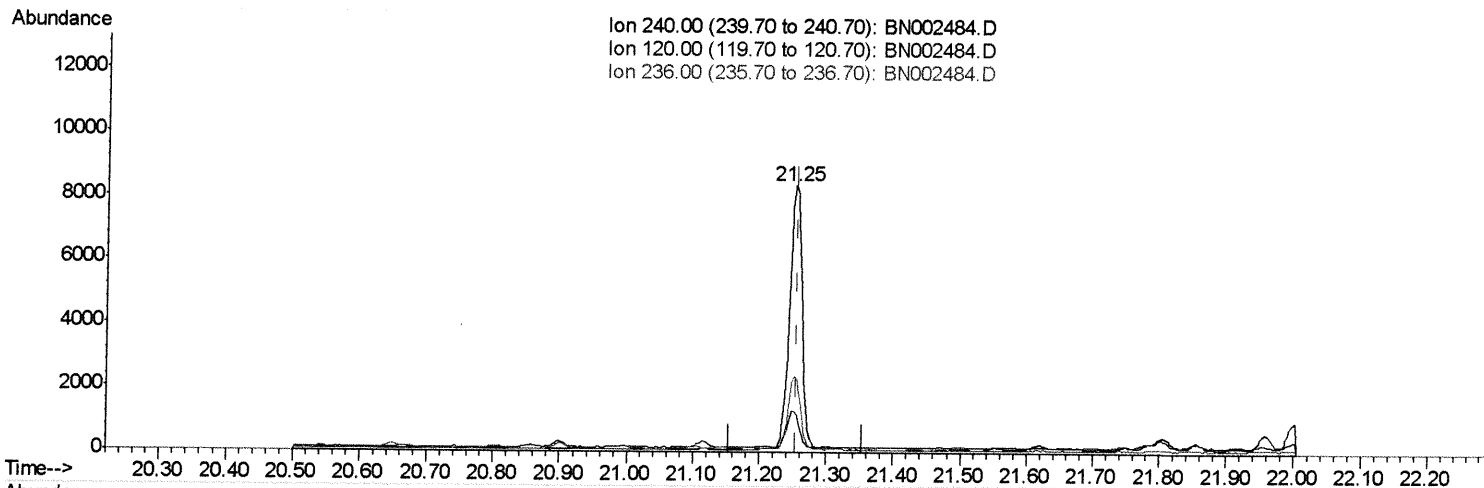

(16) Chrysene-d12 (I)

21.251min (-0.005) 0.40ng/ul m

SJ 8/27/18

response 10532

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	15.45#
236.00	34.90	28.62
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:31:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

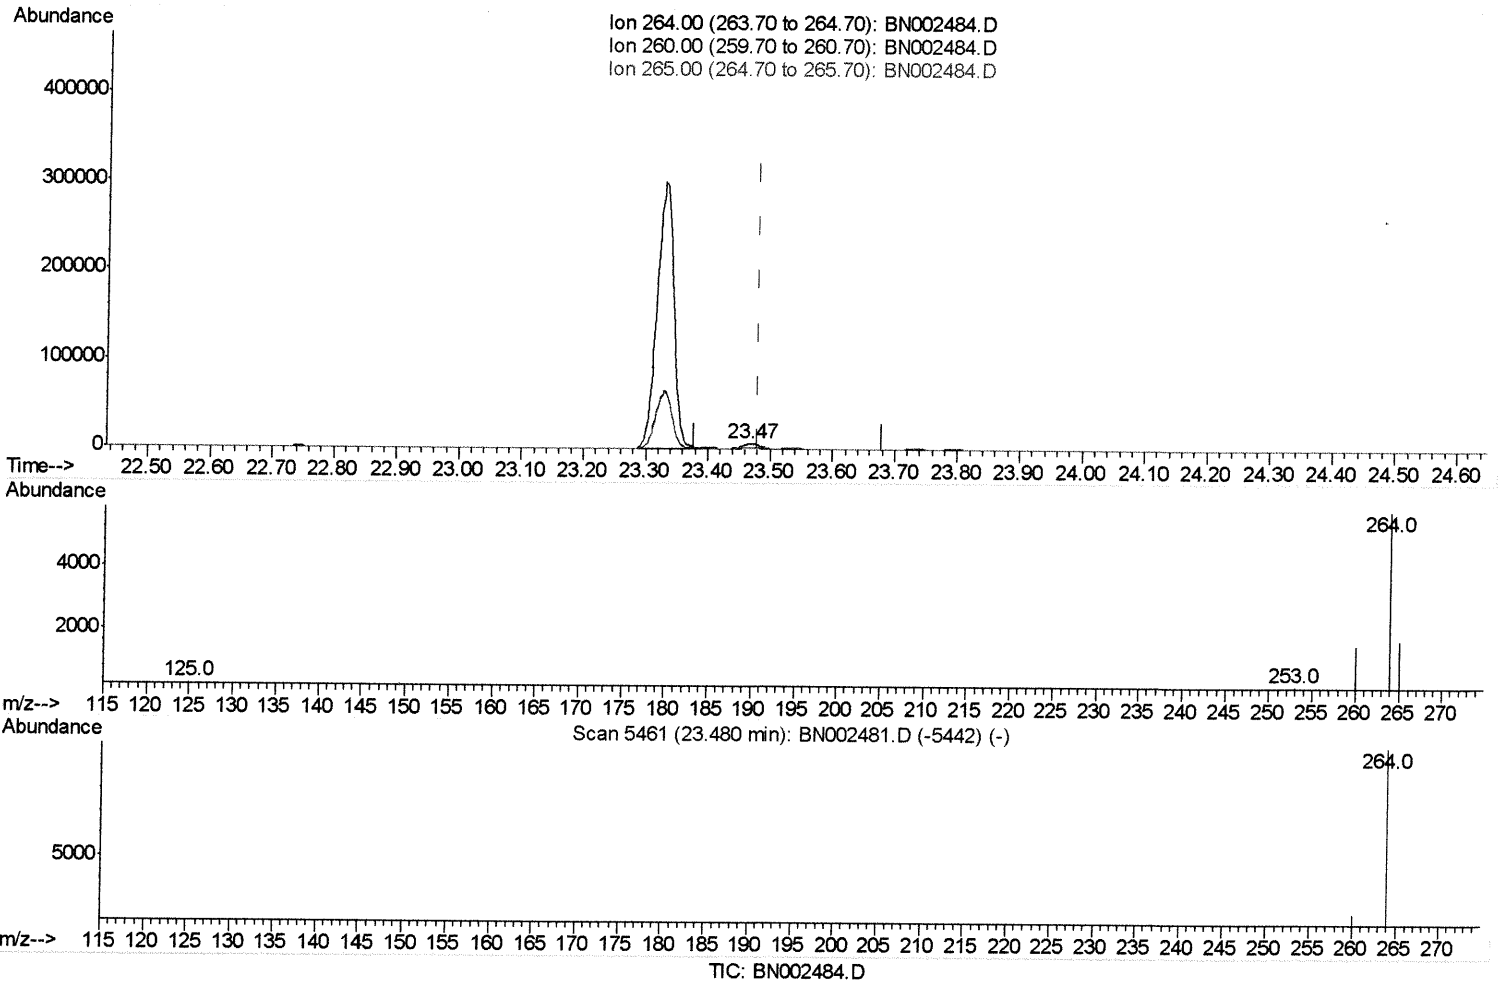

(20) Perylene-d12 (I)

23.469min (-0.010) 0.40ng/ul

response 12238

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.75
265.00	103.50	29.31#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:31:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

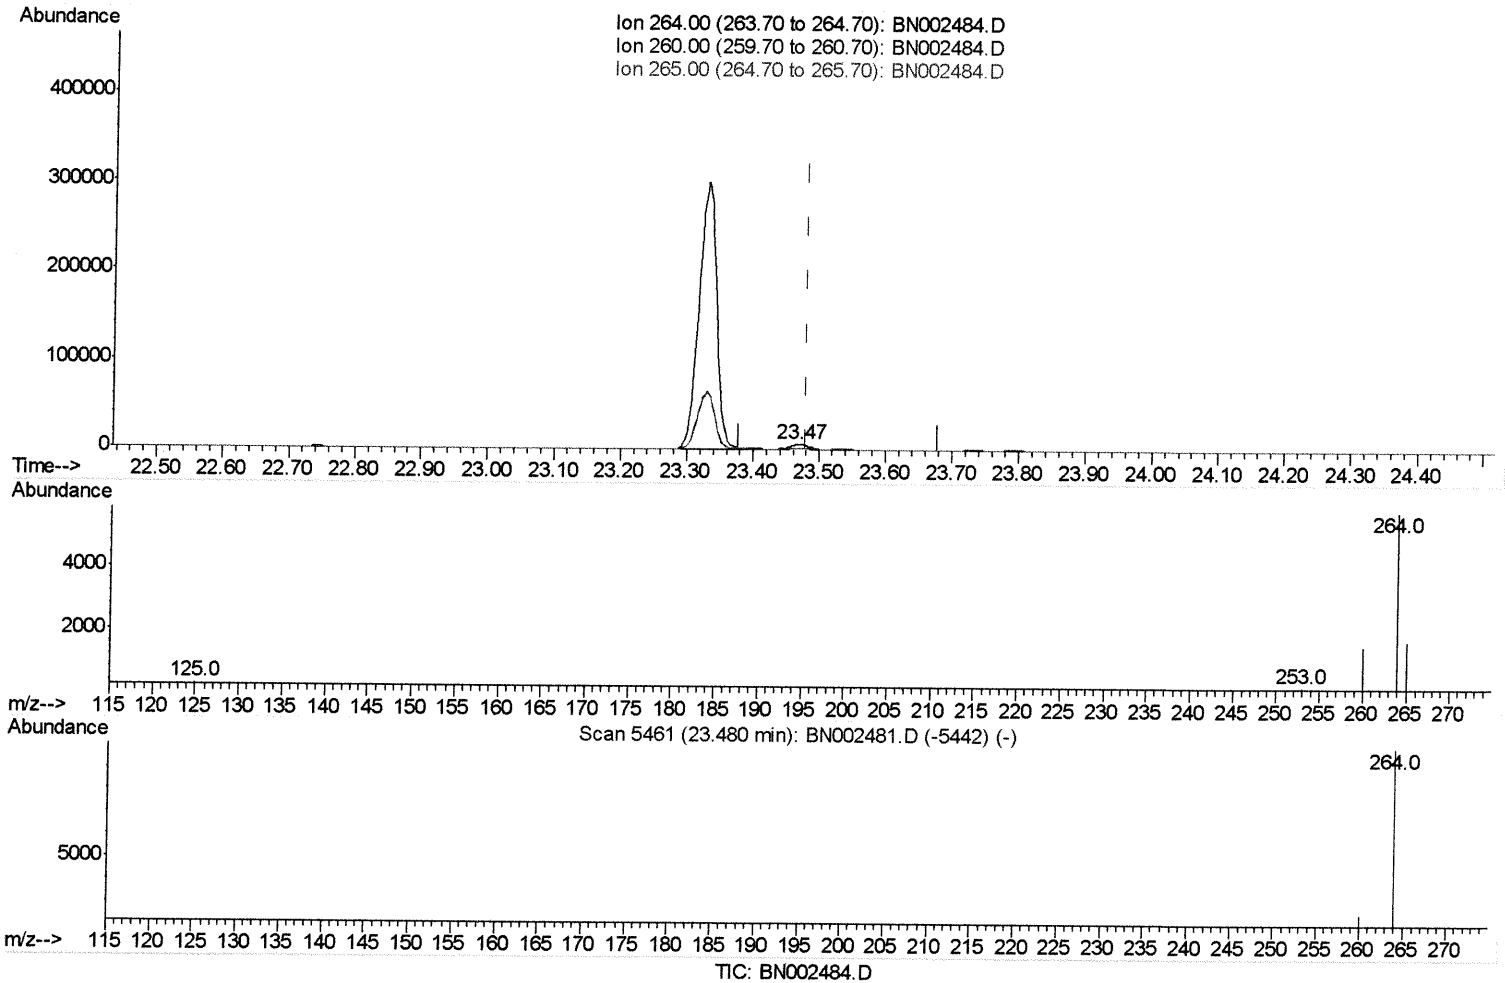

(20) Perylene-d12 (I)

23.469min (-0.010) 0.40ng/ul m

SJ 8/27/18

response 9829

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.75
265.00	103.50	29.31#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:31:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

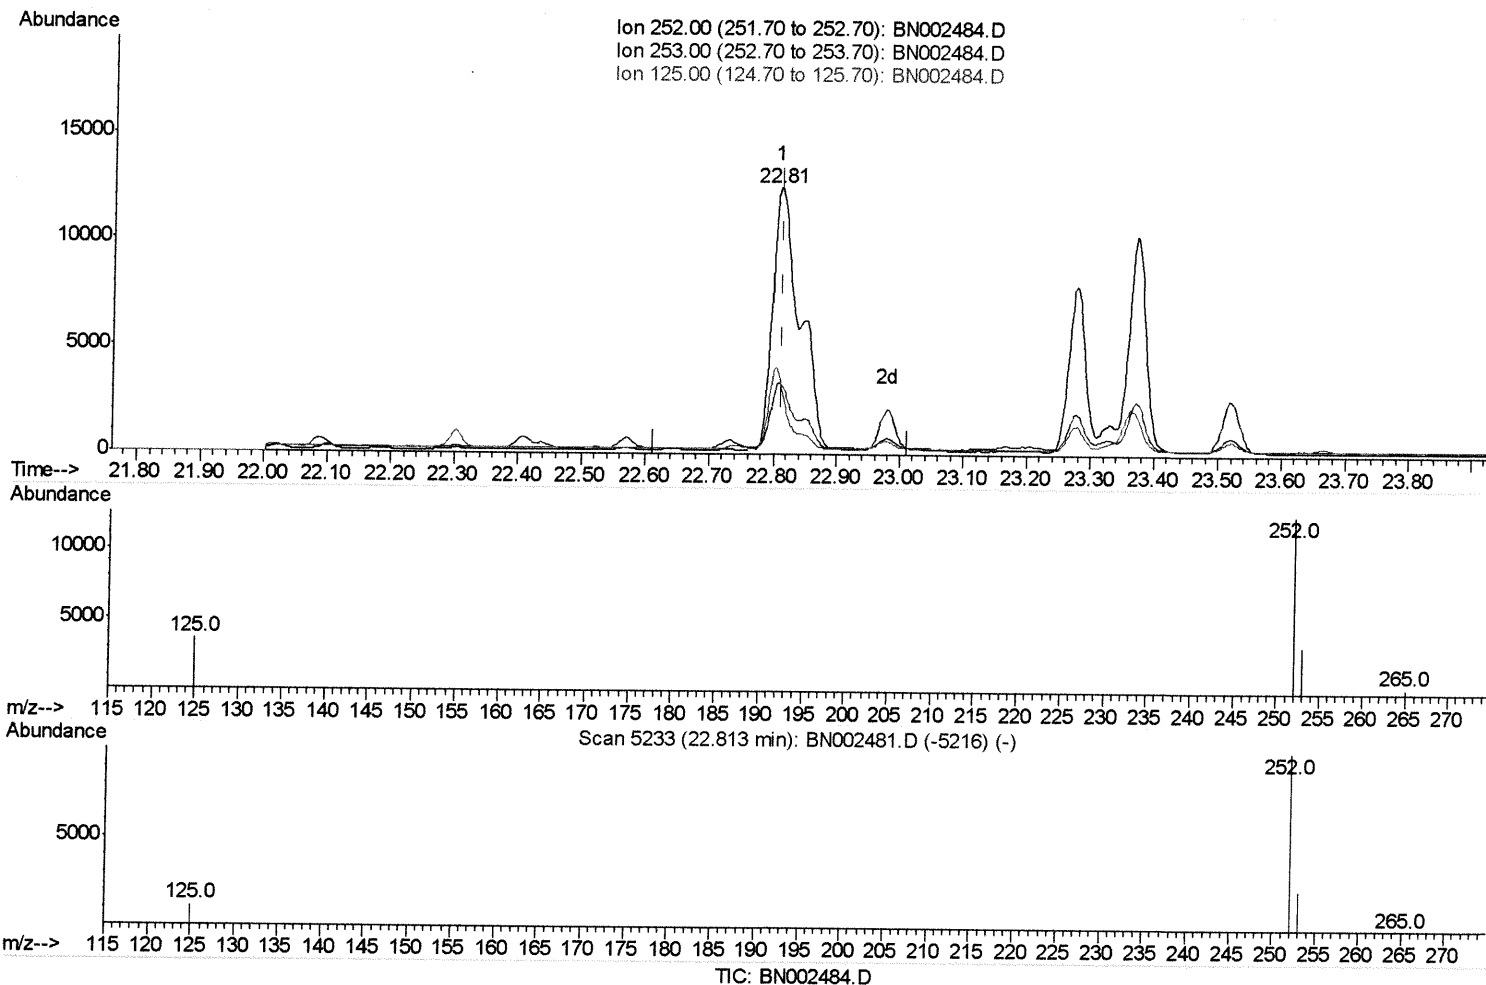

(21) Benzo(b)fluoranthene
 22.808min (-0.005) 1.04ng/ul
 response 36659

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	26.77
125.00	17.50	29.24
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:31:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

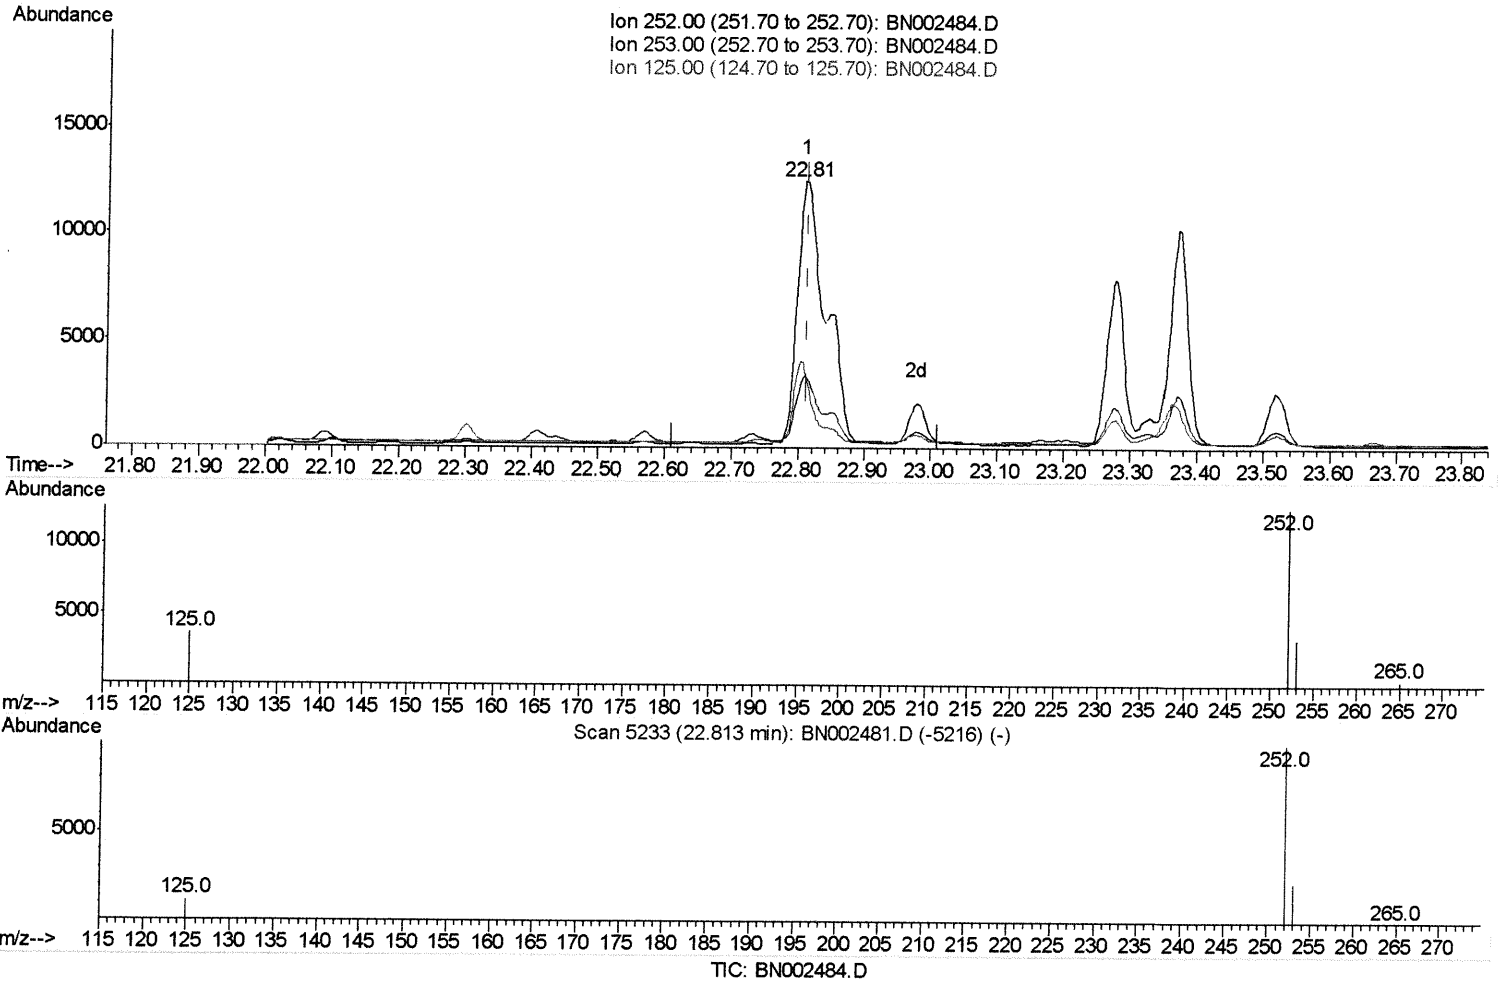

(21) Benzo(b)fluoranthene

22.808min (-0.005) 0.79ng/ul m

SJ 8/27/18

response 28016

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	26.77
125.00	17.50	29.24
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:31:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

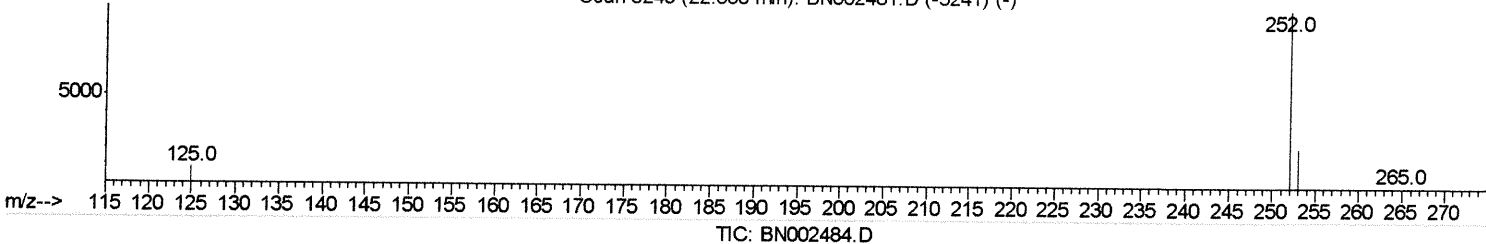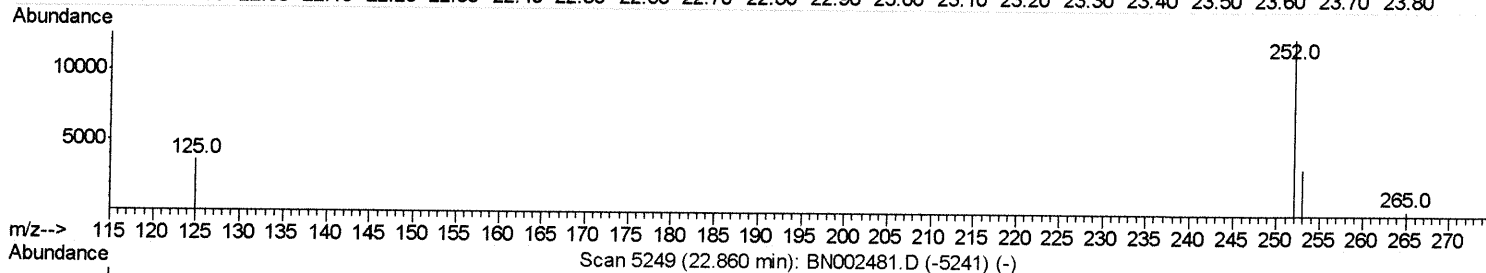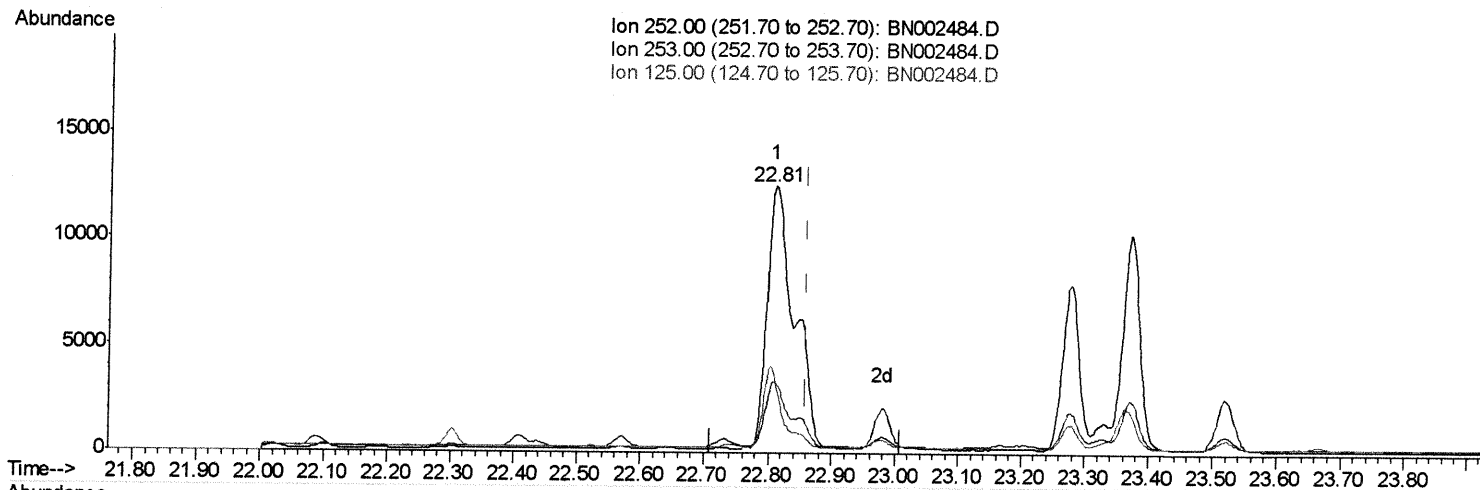

(22) Benzo(k)fluoranthene
 22.808min (-0.051) 1.00ng/ul
 response 36659

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	26.77
125.00	17.10	29.24#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:31:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

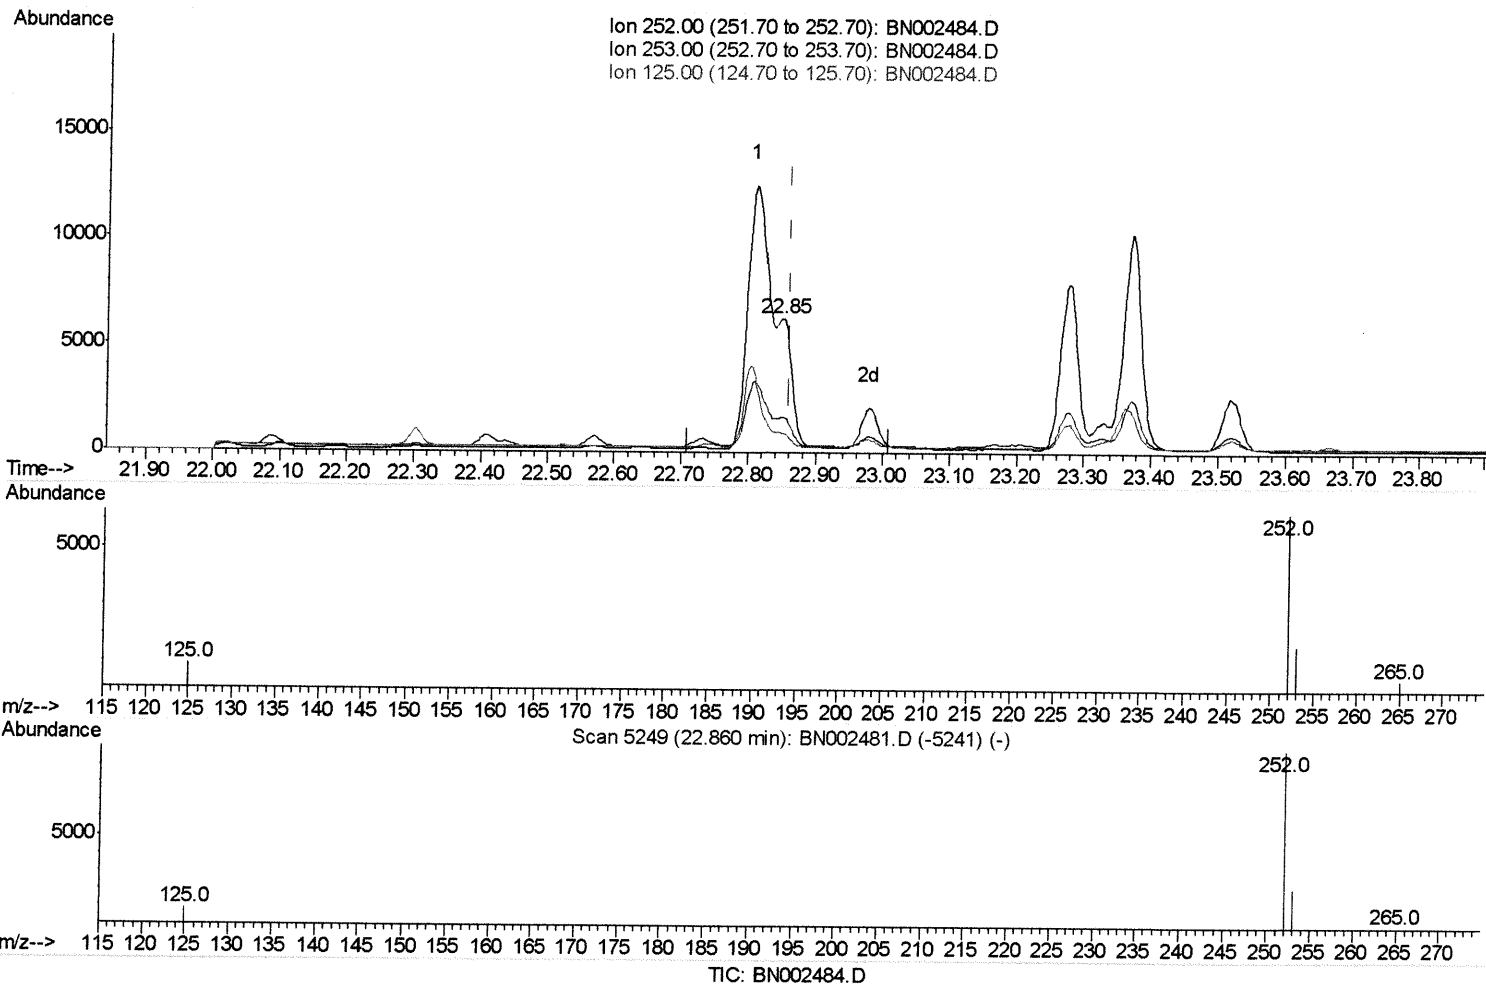

(22) Benzo(k)fluoranthene

22.849min (-0.010) 0.23ng/ul m

SJ 8/27/18

response 8277

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	26.24
125.00	17.10	14.69
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082318\
 Data File : BN002484.D
 Acq On : 24 Aug 2018 02:01
 Operator : JU/SJ
 Sample : J4421-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Manual Integrations
 APPROVED

Sohil
 8/24/2018 5:11:54 PM

Quant Time: Aug 24 04:32:52 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 02:20:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	1773	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	7122	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.31	164	4026	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	9668m	0.40	ng/ul	0.00
16) Chrysene-d12	21.25	240	10532m	0.40	ng/ul	0.00
20) Perylene-d12	23.47	264	9829m	0.40	ng/ul	-0.01

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.05	152	2382	0.21	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	6637m	0.23	ng/ul	0.00

Target Compounds

					Ovalue
3) Naphthalene	10.49	128	777	0.042	ng/ul# 78
5) 2-Methylnaphthalene	12.13	142	437	0.034	ng/ul 100
7) Acenaphthylene	14.02	152	2925	0.155	ng/ul 99
8) Acenaphthene	14.37	153	643	0.045	ng/ul# 93
9) Fluorene	15.36	166	683	0.041	ng/ul# 91
12) Phenanthrene	17.09	178	11549m	0.404	ng/ul
13) Anthracene	17.19	178	2619m	0.107	ng/ul
15) Fluoranthene	19.12	202	30213m	0.899	ng/ul
17) Pyrene	19.48	202	33721	0.939	ng/ul# 95
18) Benzo(a)anthracene	21.23	228	17817	0.566	ng/ul# 86
19) Chrysene	21.29	228	21406	0.601	ng/ul 97
21) Benzo(b)fluoranthene	22.81	252	28016m	0.793	ng/ul
22) Benzo(k)fluoranthene	22.85	252	8277m	0.227	ng/ul
23) Benzo(a)pyrene	23.37	252	18716	0.564	ng/ul# 89
24) Indeno(1,2,3-cd)pyrene	25.69	276	11149	0.322	ng/ul# 77
25) Dibenzo(a,h)anthracene	25.69	278	2749	0.101	ng/ul# 90
26) Benzo(g,h,i)perylene	26.37	276	11863	0.400	ng/ul 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed