


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082319\
 Data File : BN007332.D
 Acq On : 23 Aug 2019 18:27
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 24 00:38:17 2019

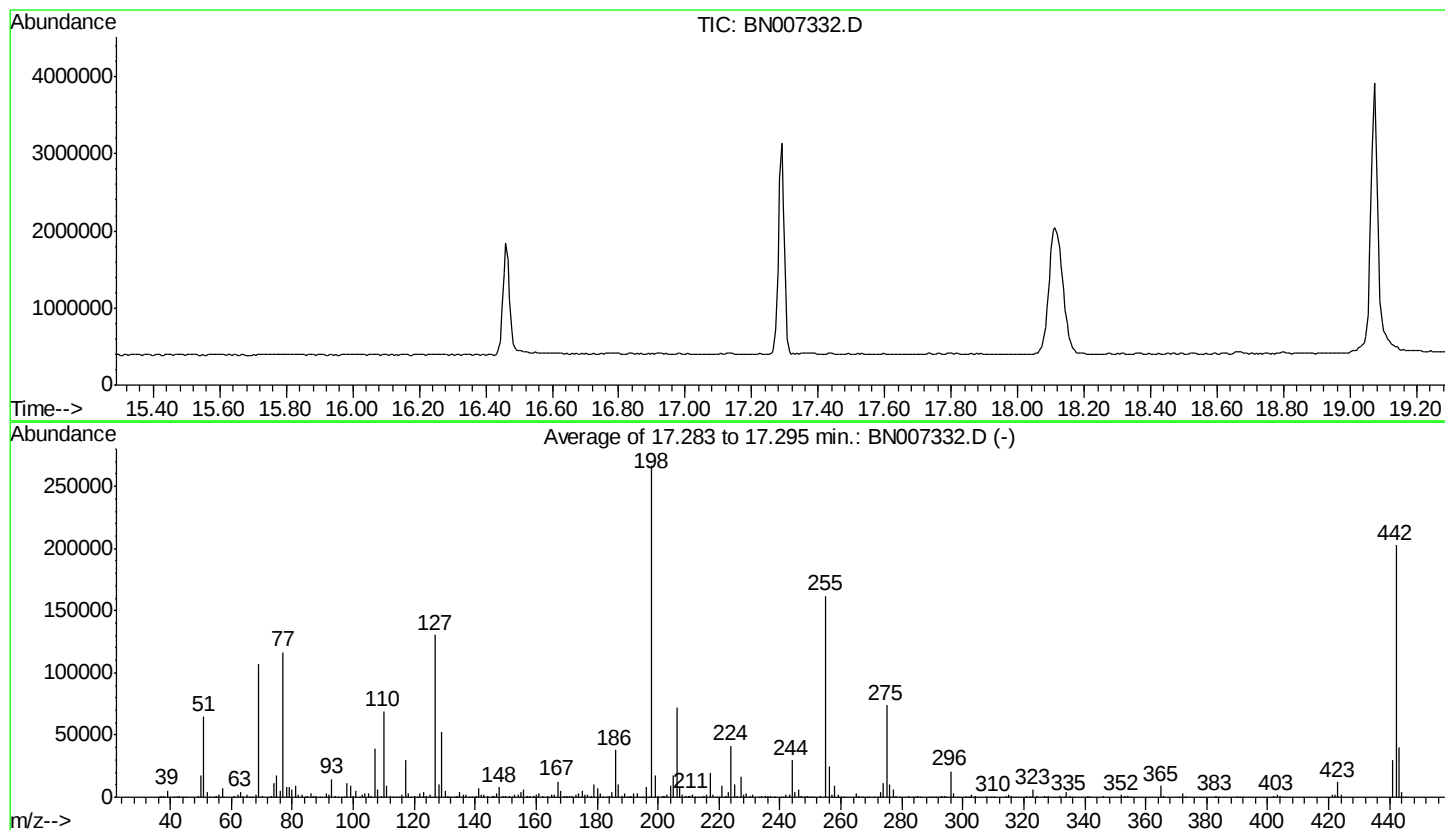

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.3	64816	PASS
68	69	0.00	2	1.6	1731	PASS
69	198	0.00	100	40.0	106698	PASS
70	69	0.00	2	0.6	591	PASS
127	198	10	80	48.9	130490	PASS
197	198	0.00	2	0.2	543	PASS
198	198	100	100	100.0	266710	PASS
199	198	5	9	6.8	18043	PASS
275	198	10	60	27.8	74021	PASS
365	198	1	100	3.4	9026	PASS
441	198	0.01	100	11.3	30120	PASS
442	198	50	100	76.0	202709	PASS
443	442	15	24	19.6	39736	PASS