

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082418\
 Data File : BN002512.D
 Acq On : 24 Aug 2018 21:45
 Operator : JU/SJ
 Sample : J4628-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB3F3

Manual Integrations
 APPROVED

Sohil
 8/27/2018 1:19:50 PM

Quant Time: Aug 25 03:52:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 25 01:30:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	141296	20.00	ng/ul	0.00
18) Naphthalene-d8	10.44	136	672911	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	426532	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	1023836	20.00	ng/ul	0.00
77) Chrysene-d12	21.24	240	1202019	20.00	ng/ul	0.00
85) Perylene-d12	23.46	264	1300949	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	9362	3.13	ng/uL	0.00
5) Phenol-d5	6.85	99	225108	17.38	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.01	67	149823	18.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	174094	17.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	184855	17.85	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	92653	17.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	98851	17.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	181323	17.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	174477	15.59	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	617940	17.48	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	766952	17.68	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	90513m	13.54	ng/ul	0.00
57) Fluorene-d10	15.30	176	539670	17.60	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	76497	11.74	ng/ul	0.00
70) Anthracene-d10	17.15	188	852826	17.44	ng/ul	0.00
78) Pyrene-d10	19.44	212	1005933	17.49	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.32	264	1198944	17.62	ng/ul	-0.01

Target Compounds				Ovalue
44) Dimethylphthalate	13.76	163	122598	3.535 ng/ul 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082418\
Data File : BN002512.D
Acq On : 24 Aug 2018 21:45
Operator : JU/SJ
Sample : J4628-08
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DB3F3

Manual Integrations
APPROVED

Sohil
8/27/2018 1:19:50 PM

Quant Time: Aug 25 03:52:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 25 01:30:26 2018
Response via : Initial Calibration

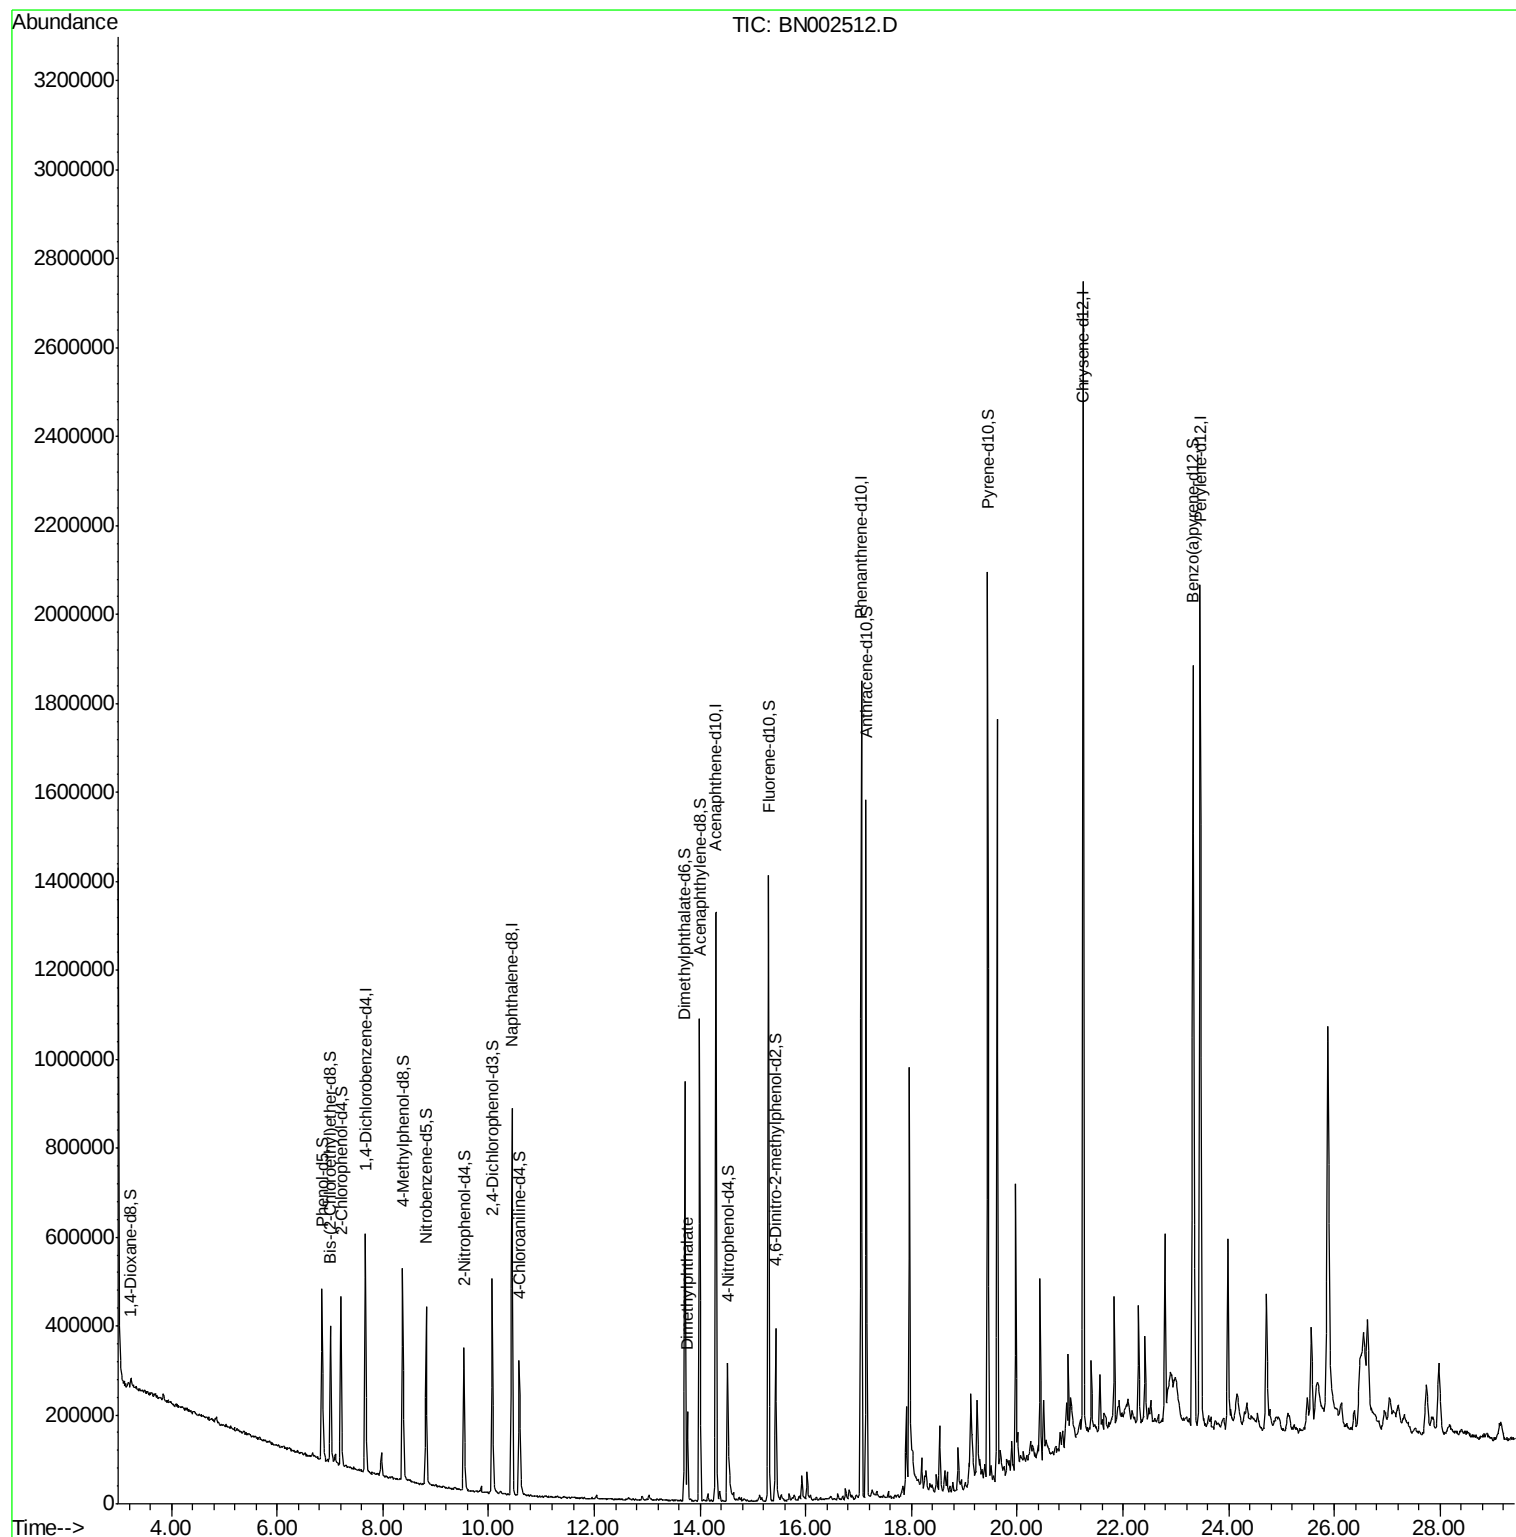

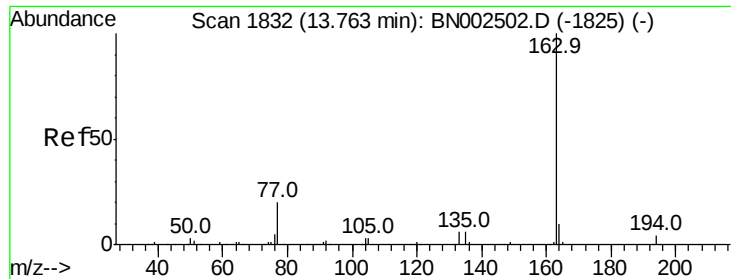

#44
 Dimethylphthalate
 Concen: 3.535 ng/ul
 RT: 13.76 min Scan# 1832
 Delta R.T. -0.00 min
 Lab File: BN002512.D
 Acq: 24 Aug 2018 21:45

Instrument :
 BNA_N
 ClientSampleId :
 DB3F3

Tot Ion	Ratio	Resp	Lower	Upper
163	100	122598		
194	4.8		3.2	4.8
164	10.2		7.8	11.8

Manual Integrations
 APPROVED

Sohil
 8/27/2018 1:19:50 PM

