

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082418\
 Data File : BN002520.D
 Acq On : 25 Aug 2018 02:38
 Operator : JU/SJ
 Sample : J4628-12
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB3F7

Manual Integrations
 APPROVED

Sohil
 8/27/2018 1:19:56 PM

Quant Time: Aug 25 05:09:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 25 04:34:18 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	115137	20.00	ng/ul	0.00
18) Naphthalene-d8	10.44	136	550748	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	335228	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	823944	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1057395	20.00	ng/ul	0.00
85) Perylene-d12	23.46	264	1181562	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	9157	3.75	ng/uL	0.00
5) Phenol-d5	6.85	99	200020	18.95	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.01	67	133967	20.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	154809	19.25	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	163613	19.39	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	83038	18.94	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	85618	18.57	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	162641	19.20	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	199345	21.77	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	563060	20.26	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	708090	20.77	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	74421m	14.17	ng/ul	0.00
57) Fluorene-d10	15.30	176	513716	21.32	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	60780	11.59	ng/ul	0.00
70) Anthracene-d10	17.15	188	808512	20.54	ng/ul	0.00
78) Pyrene-d10	19.45	212	1001423	19.79	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.32	264	1310051	21.20	ng/ul	0.00

Target Compounds

				Ovalue	
6) Phenol	6.88	94	19662	1.829	ng/ul# 86
44) Dimethylphthalate	13.76	163	239323	8.781	ng/ul 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082418\
Data File : BN002520.D
Acq On : 25 Aug 2018 02:38
Operator : JU/SJ
Sample : J4628-12
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DB3F7

Manual Integrations
APPROVED

Sohil
8/27/2018 1:19:56 PM

Quant Time: Aug 25 05:09:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 25 04:34:18 2018
Response via : Initial Calibration

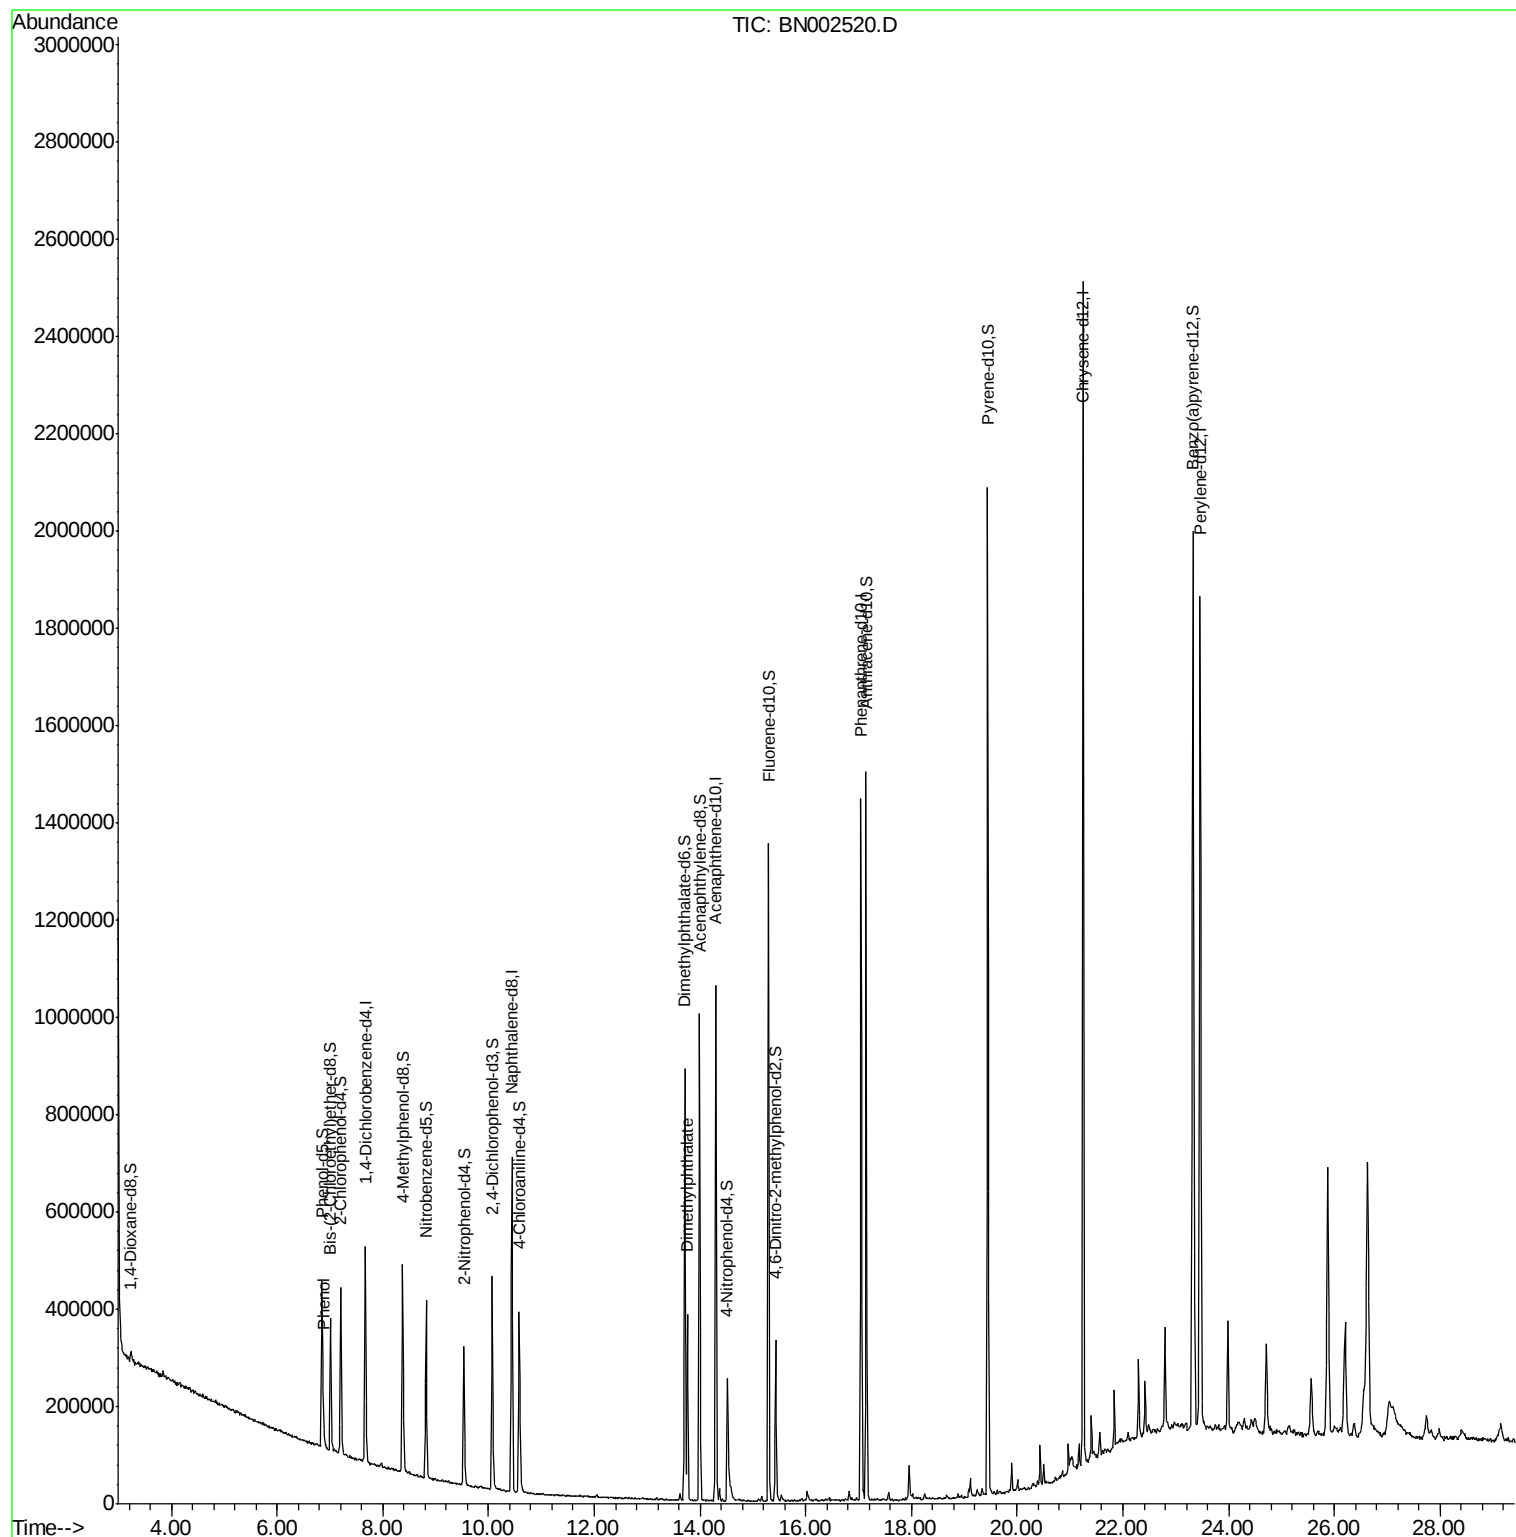

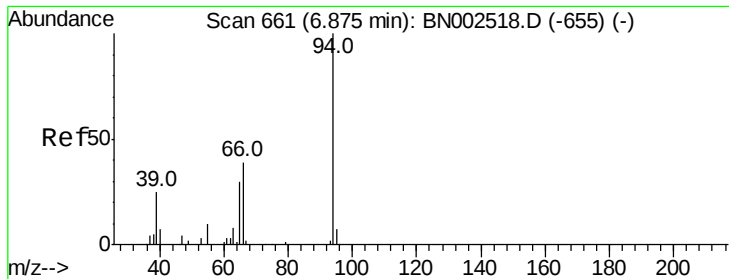

#6

Phenol

Concen: 1.829 ng/ul

RT: 6.88 min Scan# 661

Delta R.T. -0.00 min

Lab File: BN002520.D

Acq: 25 Aug 2018 02:38

Instrument :

BNA_N





ClientSampled :

DB3F7

Tot Ion:	94	Resp:	19662
Ion Ratio	Lower	Upper	
94	100		
65	36.8	21.0	31.6#
66	42.6	29.3	43.9

Manual Integrations
APPROVED

Sohil
8/27/2018 1:19:56 PM

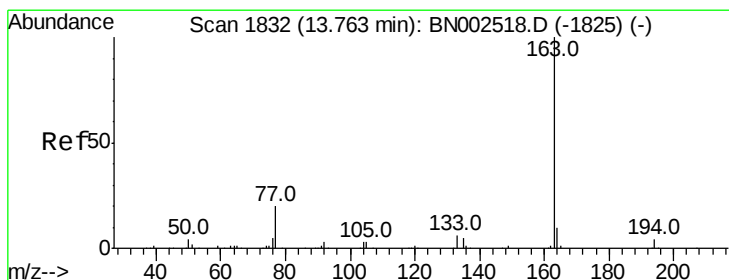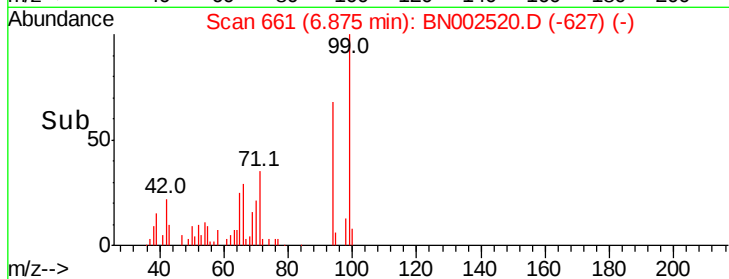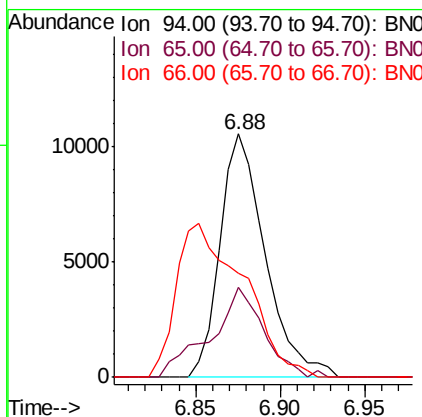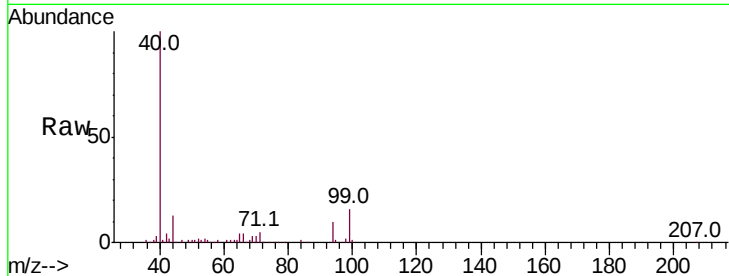

#44

Dimethylphthalate

Concen: 8.781 ng/ul

RT: 13.76 min Scan# 1832

Delta R.T. -0.00 min

Lab File: BN002520.D

Acq: 25 Aug 2018 02:38

Tgt Ion:	163	Resp:	239323
Ion Ratio	Lower	Upper	
163	100		
194	4.2	3.2	4.8
164	9.8	7.8	11.8

