

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082419\
 Data File : BN007381.D
 Acq On : 25 Aug 2019 03:07
 Operator : HP/JU
 Sample : PB122525BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB122525BL

Quant Time: Aug 25 05:25:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 24 00:38:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	7216	0.40	ng	0.00
7) Naphthalene-d8	10.15	136	27600	0.40	ng	-0.01
13) Acenaphthene-d10	14.04	164	11972	0.40	ng	-0.01
19) Phenanthrene-d10	16.80	188	22924	0.40	ng	0.00
27) Chrysene-d12	21.02	240	24639	0.40	ng	0.00
34) Perylene-d12	23.12	264	30134	0.40	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.04	112	5280	0.20	ng	0.00
5) Phenol-d6	6.60	99	6215	0.18	ng	0.00
8) Nitrobenzene-d5	8.53	82	4592	0.19	ng	0.00
11) 2-Methylnaphthalene-d10	11.76	152	9735	0.21	ng	0.00
14) 2,4,6-Tribromophenol	15.56	330	808	0.13	ng	0.00
15) 2-Fluorobiphenyl	12.66	172	11016	0.23	ng	0.00
25) Fluoranthene-d10	18.84	212	16971	0.23	ng	0.00
29) Terphenyl-d14	19.46	244	12491	0.19	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
32) Bis(2-ethylhexyl)phthalate	20.96	149	217	Below Cal	#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082419\
Data File : BN007381.D
Acq On : 25 Aug 2019 03:07
Operator : HP/JU
Sample : PB122525BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB122525BL

Quant Time: Aug 25 05:25:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 24 00:38:17 2019
Response via : Initial Calibration

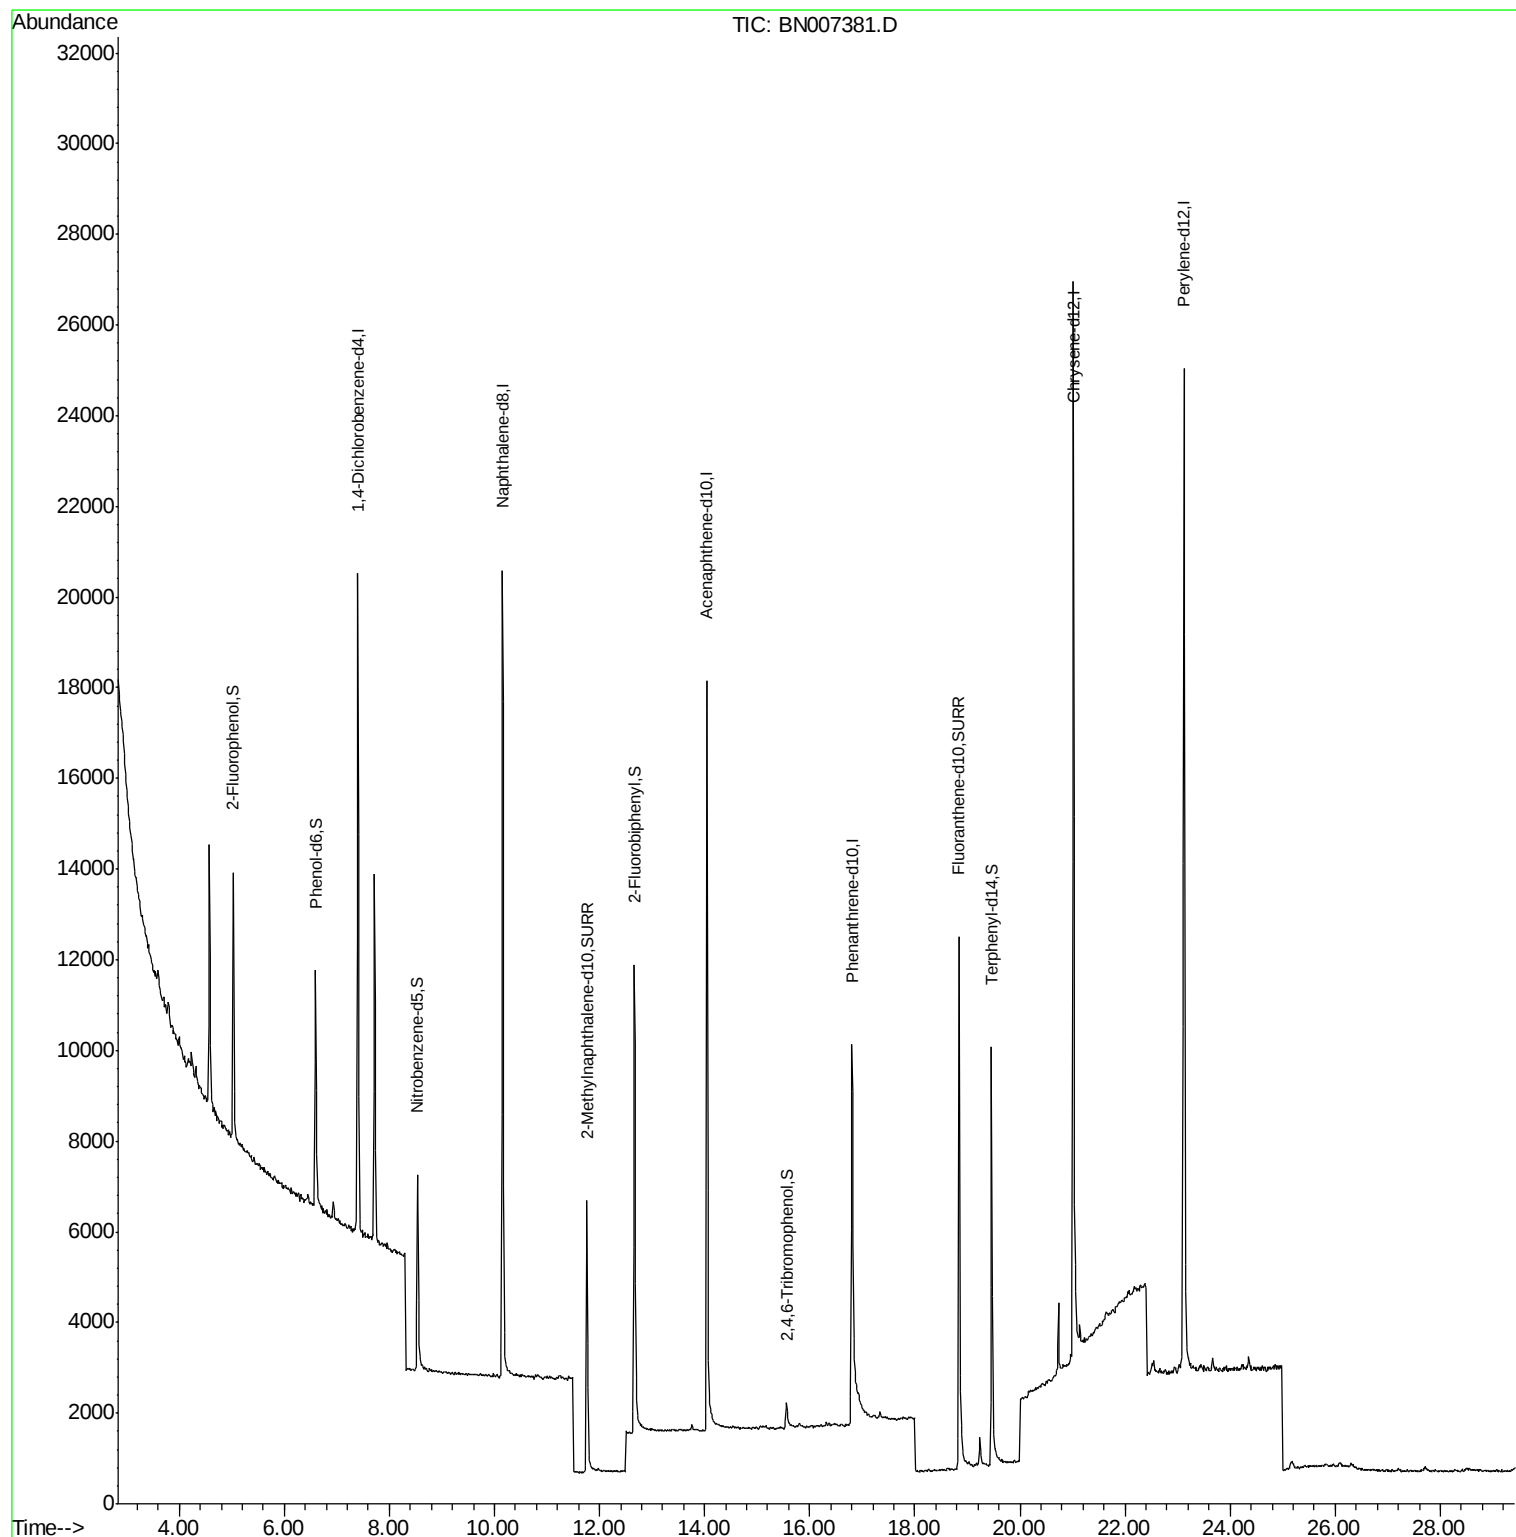



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.40 min Scan# 568

Delta R.T. 0.00 min

Lab File: BN007381.D

Acq: 25 Aug 2019 03:07

Instrument :

BNA_N

ClientSampleId :

PB122525BL


Tgt Ion:152 Resp: 7216

Ion Ratio Lower Upper

152 100

150 151.5 109.1 163.7




115 69.5 59.6 89.4

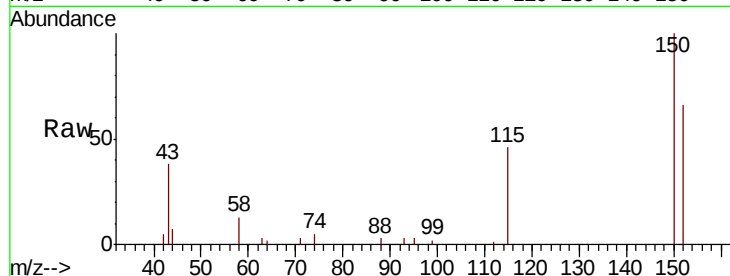

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

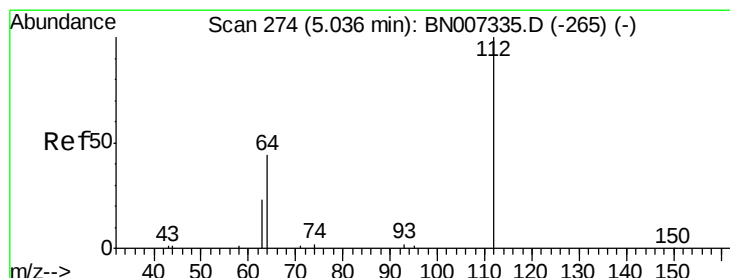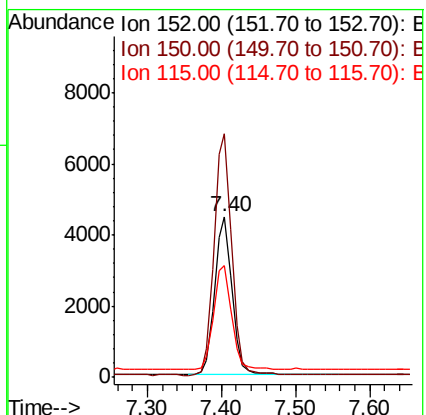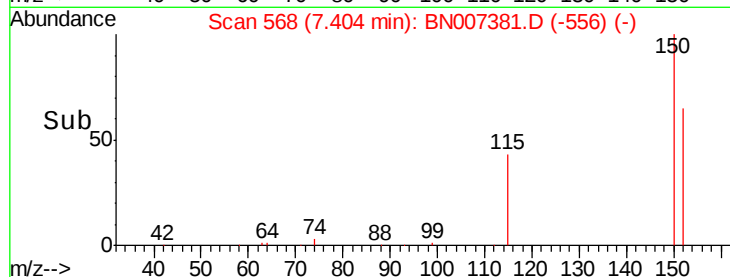

#4

2-Fluorophenol

Concen: 0.196 ng

RT: 5.04 min Scan# 274

Delta R.T. 0.00 min

Lab File: BN007381.D

Acq: 25 Aug 2019 03:07


Tgt Ion:112 Resp: 5280

Ion Ratio Lower Upper

112 100

64 50.9 42.3 63.5



63 27.8 23.6 35.4

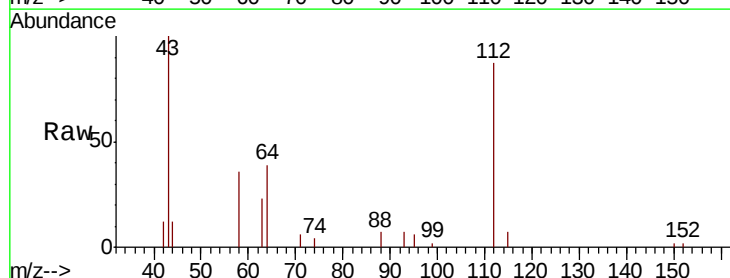

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BNC

Ion 63.00 (62.70 to 63.70): BNC

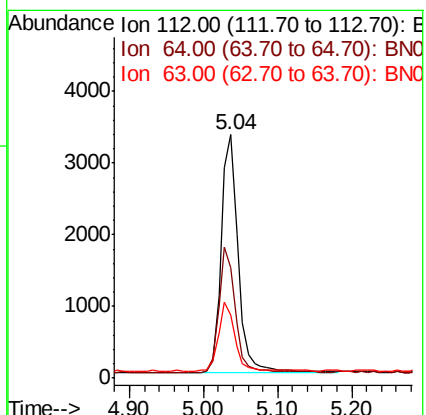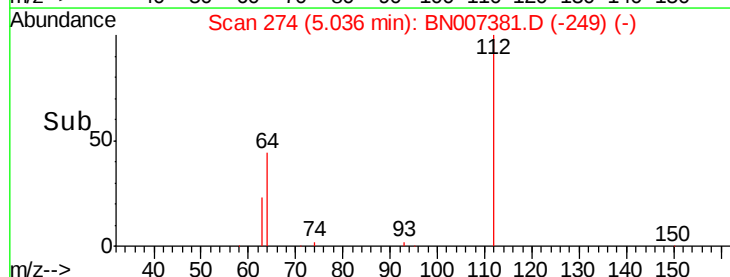



#5

Phenol-d6

Concen: 0.178 ng

RT: 6.60 min Scan# 468

Delta R.T. 0.01 min

Lab File: BN007381.D

Acq: 25 Aug 2019 03:07

Instrument :

BNA_N

ClientSampleId :

PB122525BL


Tgt Ion: 99 Resp: 6215

Ion Ratio Lower Upper

99 100

42 12.5 11.2 16.8




71 35.3 31.8 47.8

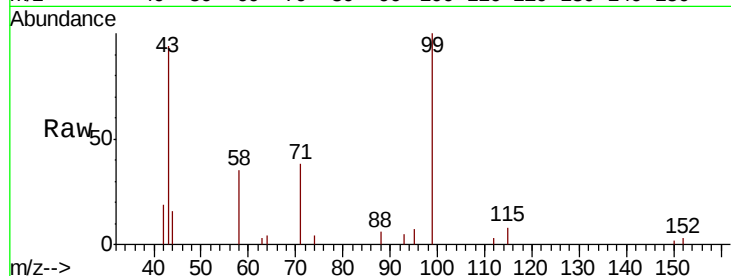

Abundance Ion 99.00 (98.70 to 99.70): BN007335.D (-462) (-)

Ion 42.00 (41.70 to 42.70): BN007335.D (-462) (-)

Ion 71.00 (70.70 to 71.70): BN007335.D (-462) (-)

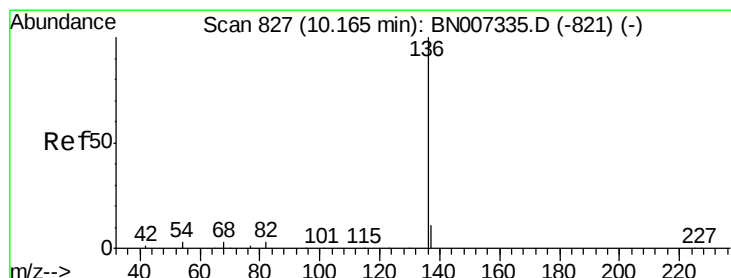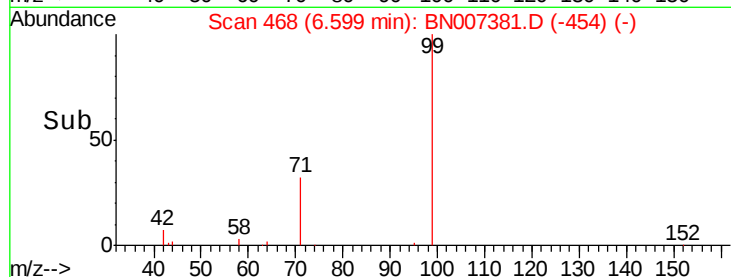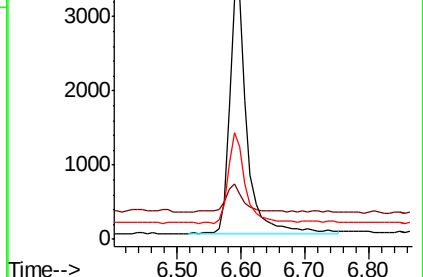

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.15 min Scan# 826

Delta R.T. -0.01 min

Lab File: BN007381.D

Acq: 25 Aug 2019 03:07

Tgt Ion: 136 Resp: 27600


Ion Ratio Lower Upper

136 100

137 11.3 12.9 19.3#

54 5.7 8.6 12.8#

68 7.1 17.0 25.4#


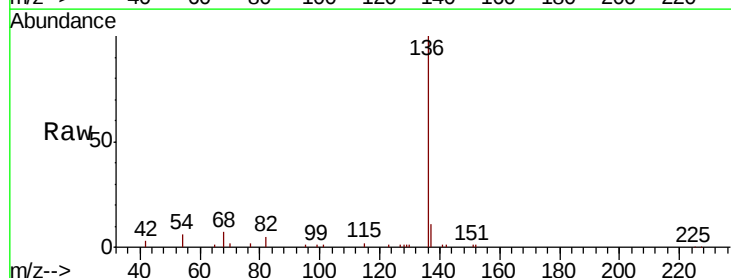


Abundance Ion 136.00 (135.70 to 136.70): BN007335.D (-821) (-)

Ion 137.00 (136.70 to 137.70): BN007335.D (-821) (-)

Ion 54.00 (53.70 to 54.70): BN007335.D (-821) (-)

Ion 68.00 (67.70 to 68.70): BN007335.D (-821) (-)

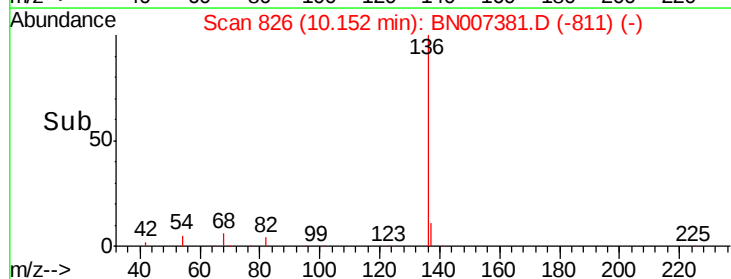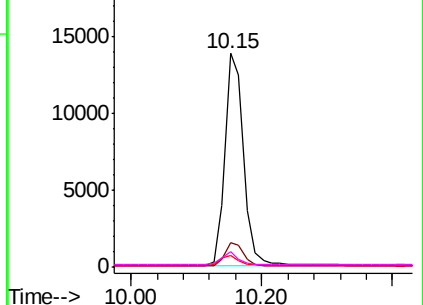







#8
 Nitrobenzene-d5
 Concen: 0.191 ng
 RT: 8.53 min Scan# 698
 Delta R.T. 0.00 min
 Lab File: BN007381.D
 Acq: 25 Aug 2019 03:07

Instrument :
 BNA_N
 ClientSampleId :
 PB122525BL

Tgt Ion: 82 Resp: 4592
 Ion Ratio Lower Upper
 82 100
 128 33.6 19.7 29.5#
 54 39.6 25.8 38.6#

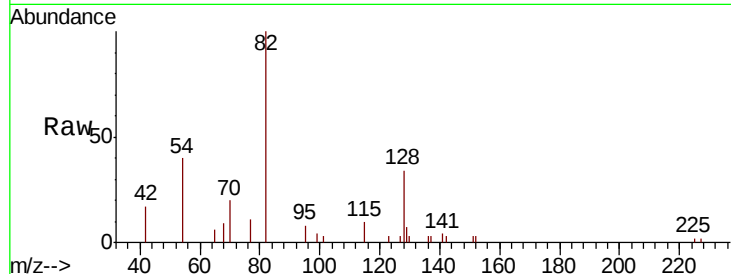


Abundance Ion 82.00 (81.70 to 82.70): BN0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BN0

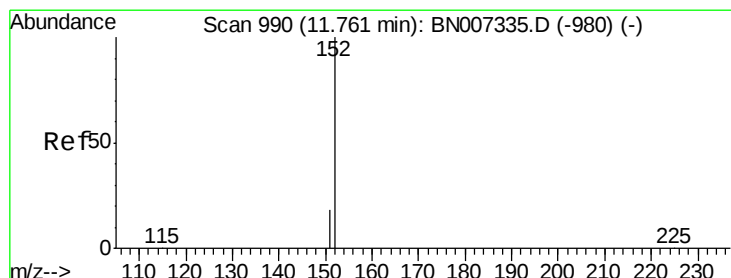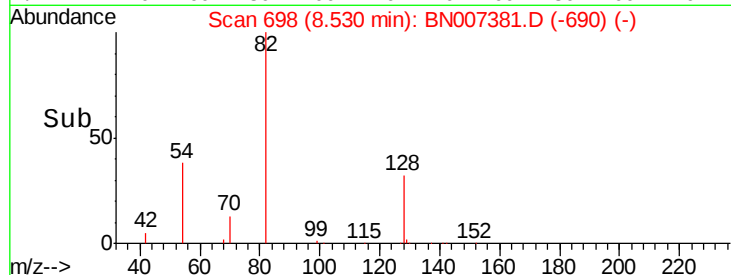
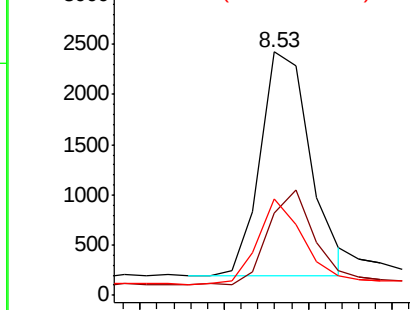


#11
 2-Methylnaphthalene-d10
 Concen: 0.212 ng
 RT: 11.76 min Scan# 990
 Delta R.T. 0.00 min
 Lab File: BN007381.D
 Acq: 25 Aug 2019 03:07

Tgt Ion: 152 Resp: 9735
 Ion Ratio Lower Upper
 152 100
 151 18.8 16.2 24.2

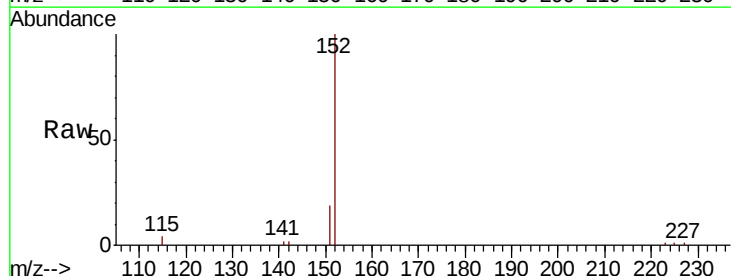

Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 151.00 (150.70 to 151.70): E

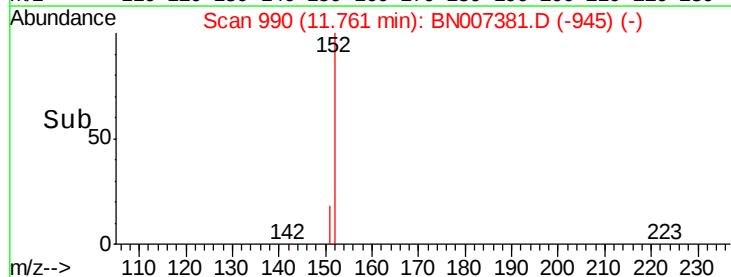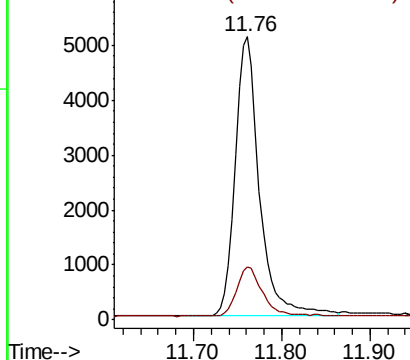



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.04 min Scan# 1295

Delta R.T. -0.01 min

Lab File: BN007381.D

Acq: 25 Aug 2019 03:07

Instrument :

BNA_N

ClientSampleId :

PB122525BL


Tgt Ion:164 Resp: 11972

Ion Ratio Lower Upper

164 100

162 105.7 83.5 125.3




160 48.4 38.2 57.4

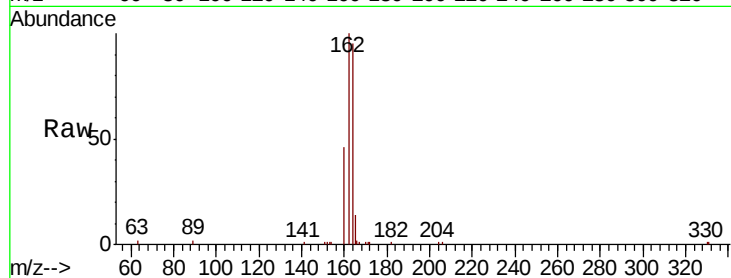

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

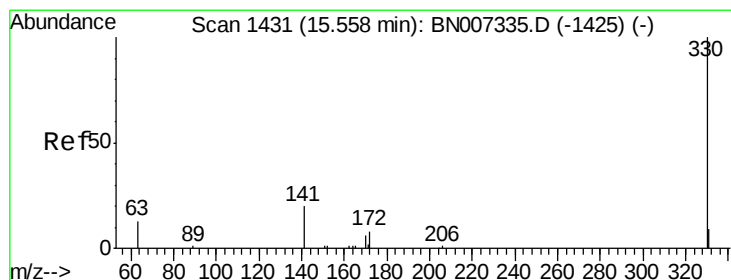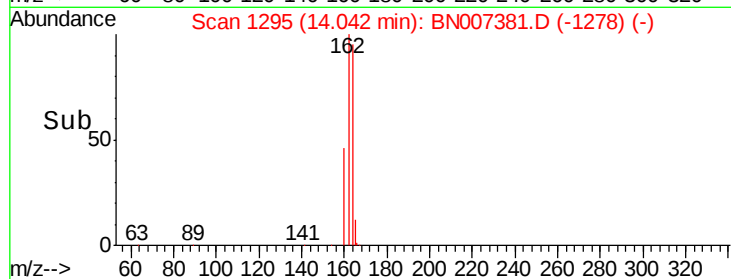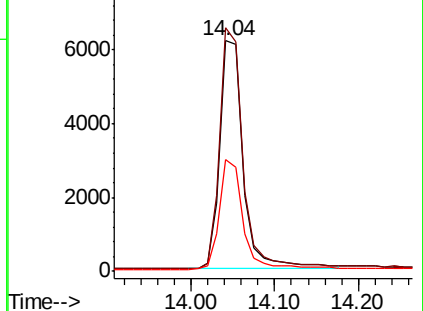

#14

2,4,6-Tribromophenol

Concen: 0.129 ng

RT: 15.56 min Scan# 1431

Delta R.T. 0.00 min

Lab File: BN007381.D

Acq: 25 Aug 2019 03:07


Tgt Ion:330 Resp: 808

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0



141 31.4 26.9 40.3

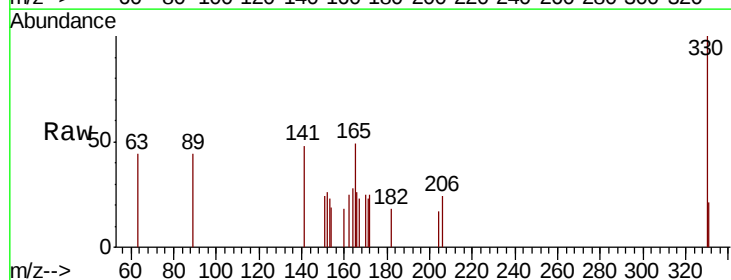


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

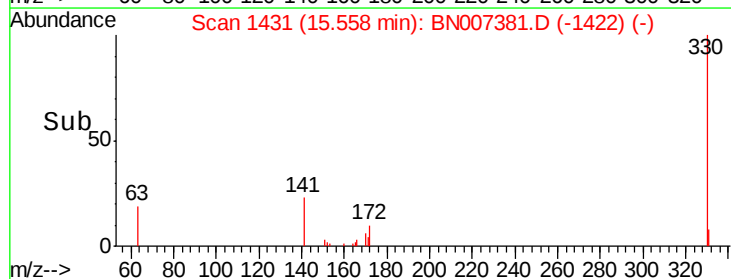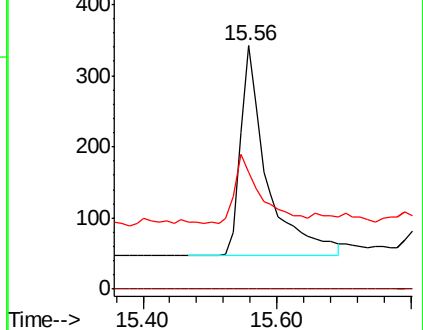

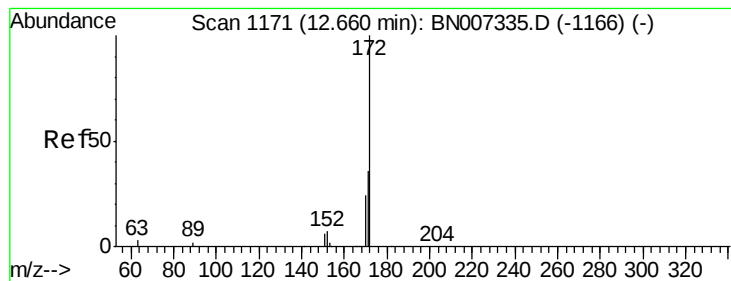

#15

2-Fluorobiphenyl

Concen: 0.228 ng

RT: 12.66 min Scan# 1171

Delta R.T. 0.00 min

Lab File: BN007381.D

Acq: 25 Aug 2019 03:07

Instrument :

BNA_N

ClientSampleId :

PB122525BL


Tgt Ion:172 Resp: 11016

Ion Ratio Lower Upper

172 100

171 35.6 30.3 45.5




170 23.6 20.7 31.1

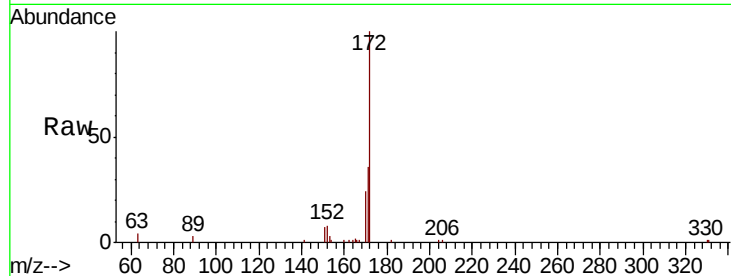

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

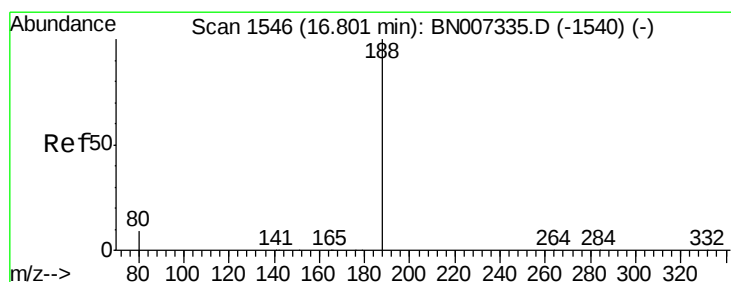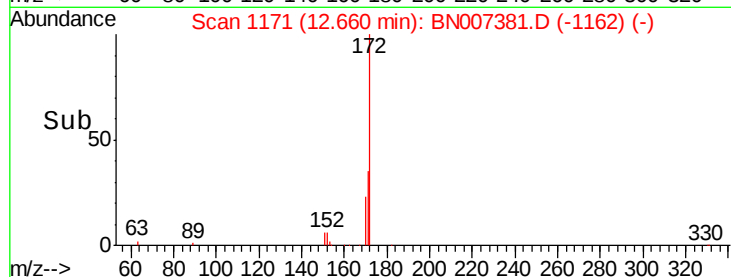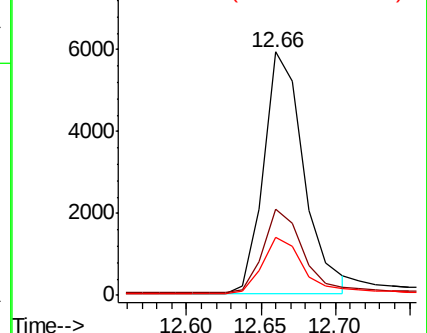

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.80 min Scan# 1546

Delta R.T. 0.00 min

Lab File: BN007381.D

Acq: 25 Aug 2019 03:07


Tgt Ion:188 Resp: 22924

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0



80 11.6 11.8 17.8#

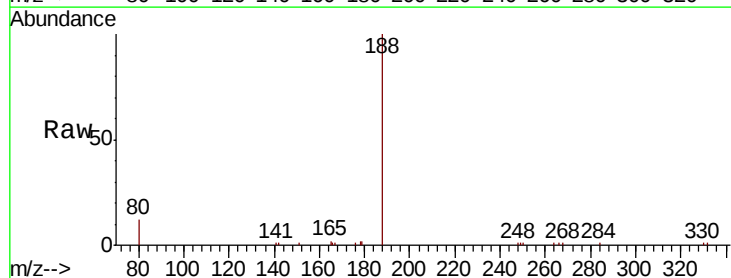


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

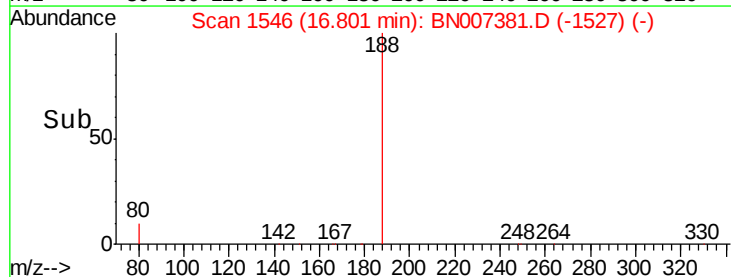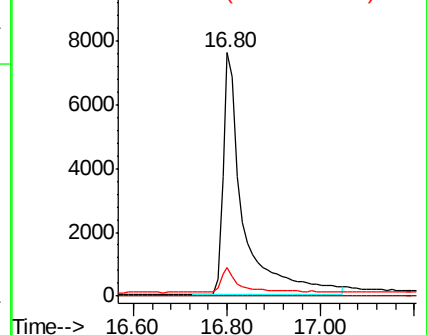


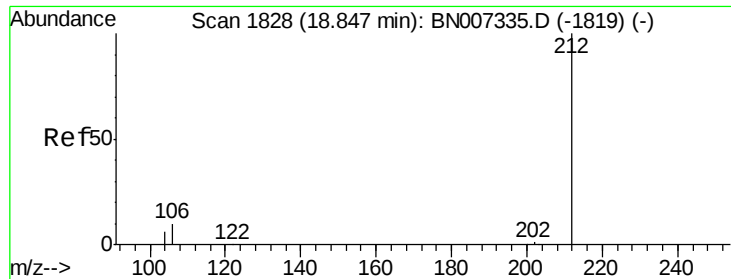




#25
Fluoranthene-d10
Concen: 0.230 ng
RT: 18.84 min Scan# 1827
Delta R.T. -0.00 min
Lab File: BN007381.D
Acq: 25 Aug 2019 03:07

Instrument :
BNA_N
ClientSampleId :
PB122525BL

Tgt Ion:212 Resp: 16971
Ion Ratio Lower Upper
212 100
106 11.2 9.0 13.4
104 6.3 5.4 8.2

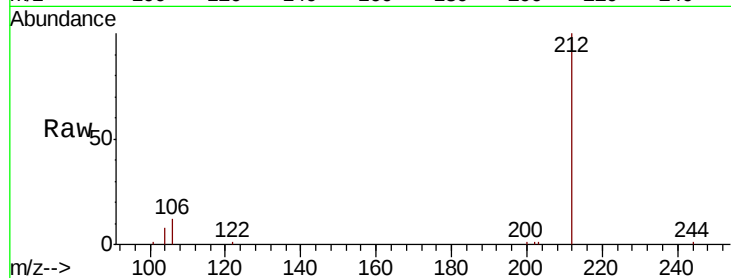


Abundance Ion 212.00 (211.70 to 212.70): E
Ion 106.00 (105.70 to 106.70): E
Ion 104.00 (103.70 to 104.70): E

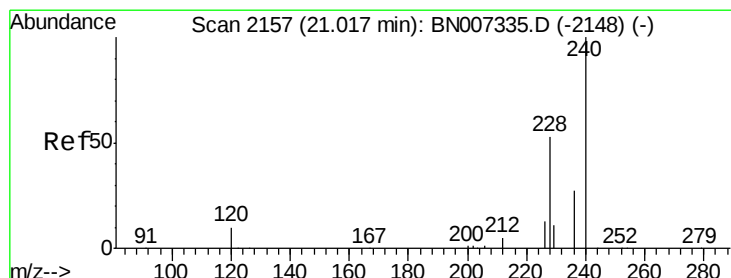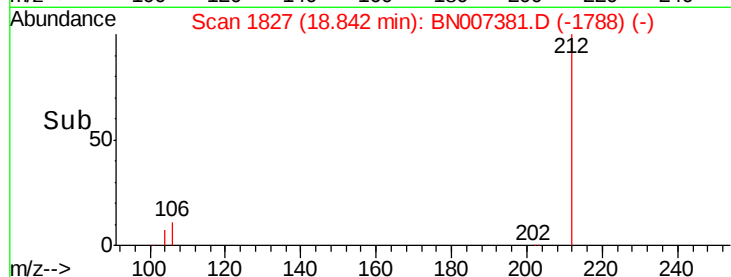
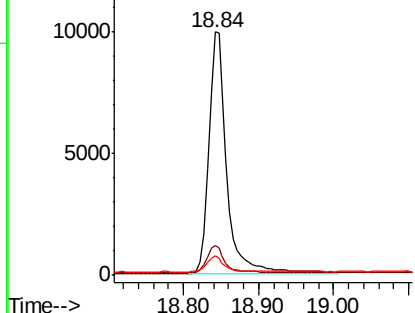



#27
Chrysene-d12
Concen: 0.400 ng
RT: 21.02 min Scan# 2157
Delta R.T. 0.00 min
Lab File: BN007381.D
Acq: 25 Aug 2019 03:07

Tgt Ion:240 Resp: 24639
Ion Ratio Lower Upper
240 100
120 8.4 9.6 14.4#
236 27.0 22.2 33.2

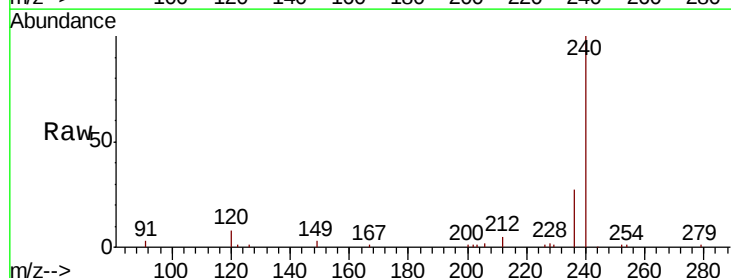

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

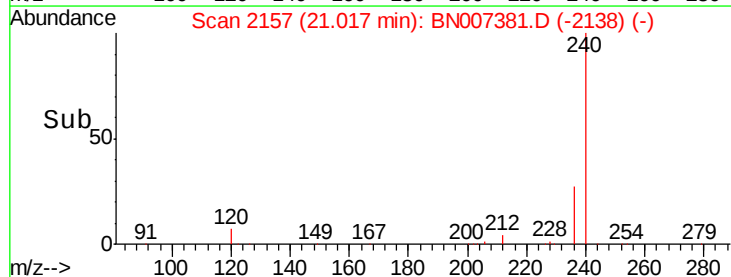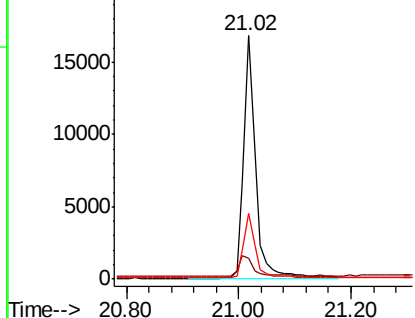

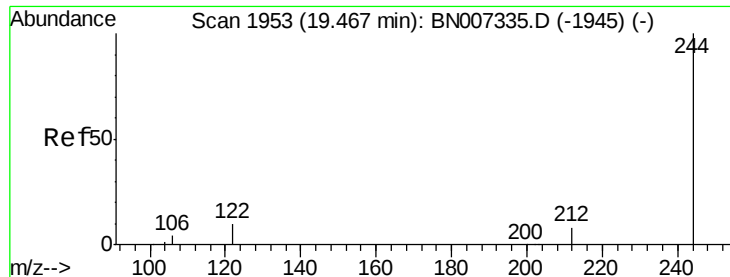

#29

Terphenyl-d14

Concen: 0.194 ng

RT: 19.46 min Scan# 1952

Delta R.T. -0.00 min

Lab File: BN007381.D

Acq: 25 Aug 2019 03:07

Instrument :

BNA_N

ClientSampleId :

PB122525BL


Tgt Ion:244 Resp: 12491

Ion Ratio Lower Upper




244 100

212 8.6 7.0 10.6

122 11.9 9.6 14.4

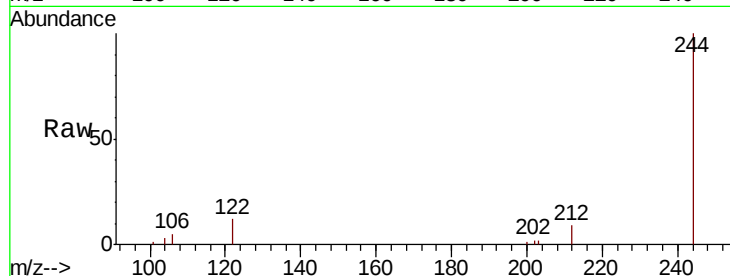

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

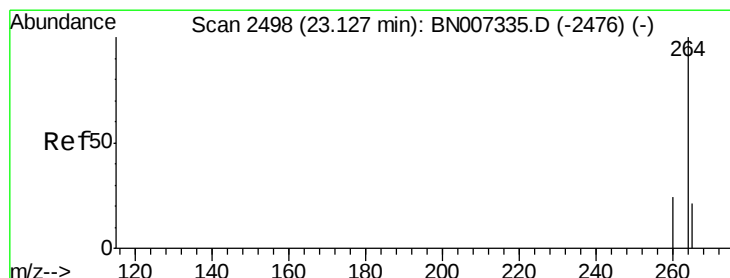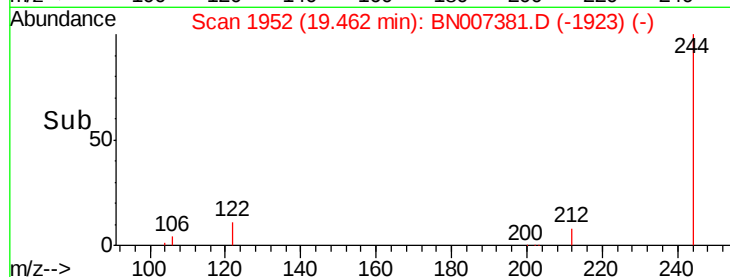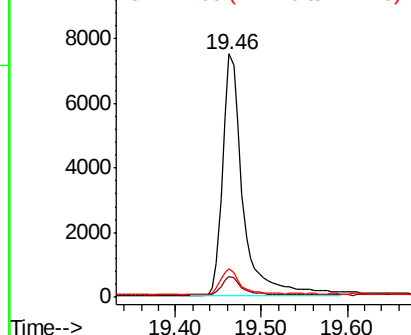

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.12 min Scan# 2496

Delta R.T. -0.01 min

Lab File: BN007381.D

Acq: 25 Aug 2019 03:07


Tgt Ion:264 Resp: 30134

Ion Ratio Lower Upper

264 100

260 24.2 19.7 29.5

265 32.1 29.9 44.9

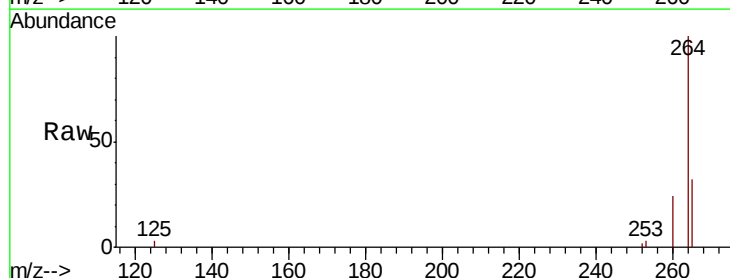

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

