


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082419\
 Data File : BN007359.D
 Acq On : 24 Aug 2019 11:20
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 24 00:38:17 2019

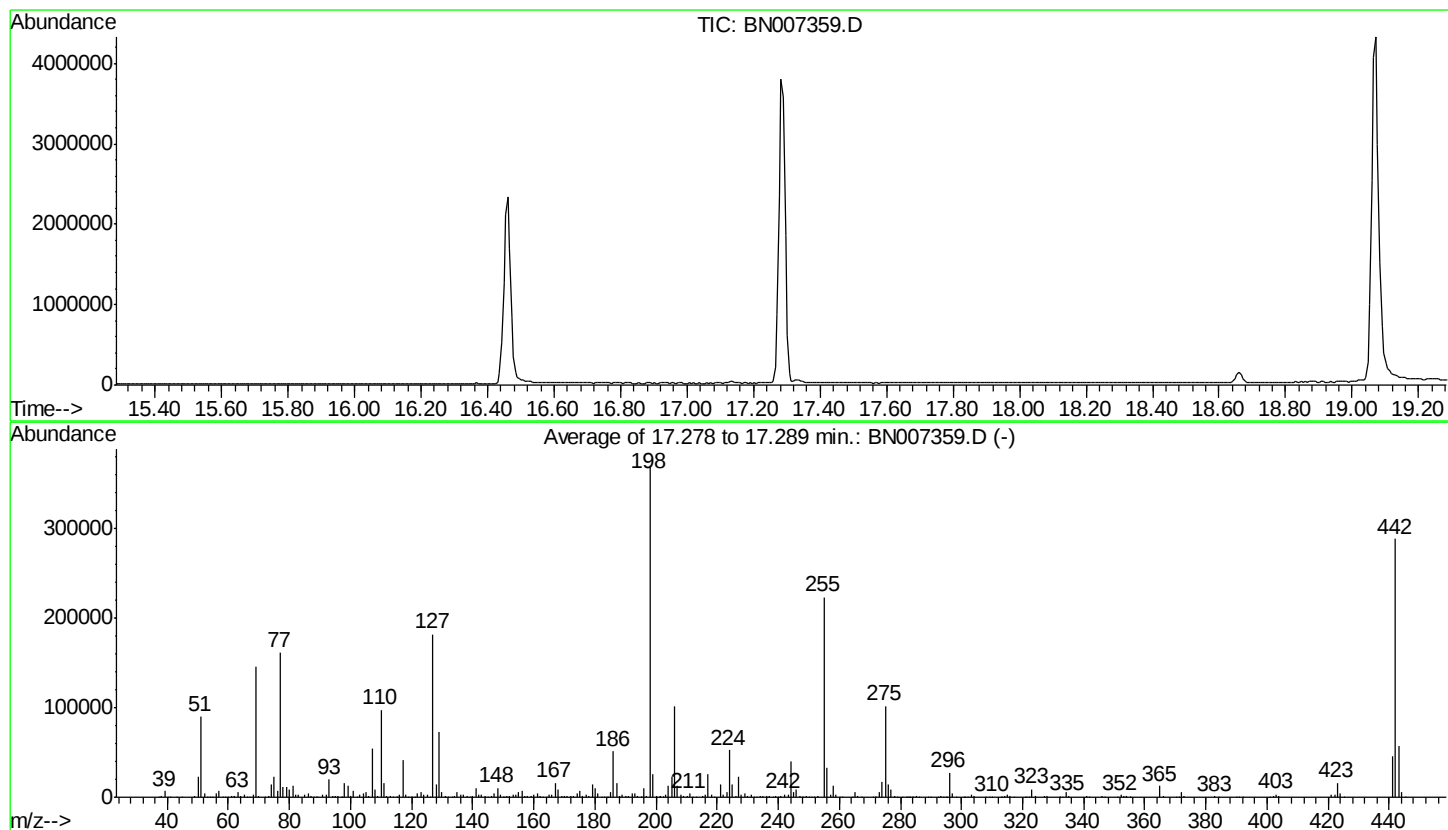

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.2	89586	PASS
68	69	0.00	2	2.0	2871	PASS
69	198	0.00	100	39.2	145431	PASS
70	69	0.00	2	0.5	775	PASS
127	198	10	80	49.1	181866	PASS
197	198	0.00	2	0.2	813	PASS
198	198	100	100	100.0	370624	PASS
199	198	5	9	6.9	25581	PASS
275	198	10	60	27.4	101682	PASS
365	198	1	100	3.4	12694	PASS
441	198	0.01	100	12.2	45165	PASS
442	198	50	100	78.0	289002	PASS
443	442	15	24	19.8	57176	PASS