


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082420\
 Data File : BN011599.D
 Acq On : 24 Aug 2020 16:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 25 03:31:11 2020

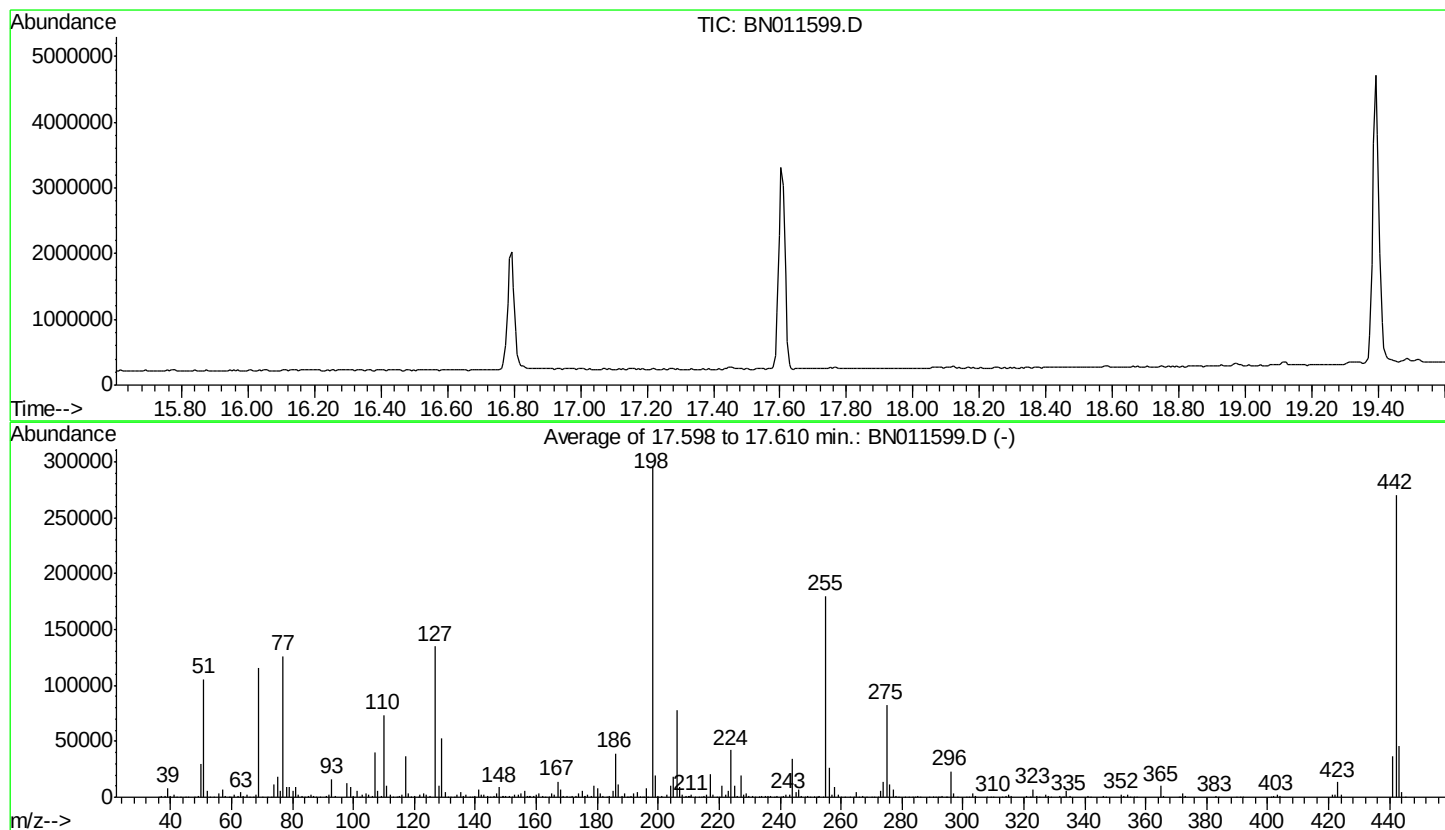

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	105558	PASS
68	69	0.00	2	1.9	2140	PASS
69	198	0.00	100	39.0	115537	PASS
70	69	0.00	2	0.2	282	PASS
127	198	10	80	45.4	134535	PASS
197	198	0.00	2	0.2	492	PASS
198	198	100	100	100.0	296448	PASS
199	198	5	9	6.7	19804	PASS
275	198	10	60	27.9	82802	PASS
365	198	1	100	3.5	10258	PASS
441	198	0.01	100	12.4	36858	PASS
442	198	50	100	91.3	270677	PASS
443	442	15	24	17.0	46141	PASS