

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082423\
 Data File : BN027100.D
 Acq On : 24 Aug 2023 16:47
 Operator : MA/JU
 Sample : PB154650BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK973

Quant Time: Aug 25 03:50:55 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 23 02:28:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.088	152	8812	0.400	ng/ul	0.00
4) Naphthalene-d8	10.916	136	28558	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.717	164	16761	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.460	188	37078	0.400	ng/ul	0.00
17) Chrysene-d12	21.635	240	28072	0.400	ng/ul	0.00
23) Perylene-d12	24.170	264	33311	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.431	96	45506	4.350	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.489	152	9835	0.234	ng/ul	0.00
18) Fluoranthene-d10	19.478	212	25805	0.291	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.845	202	4106	0.033	ng/ul#	1
26) Benzo(a)pyrene	24.009	252	8975	0.079	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082423\
Data File : BN027100.D
Acq On : 24 Aug 2023 16:47
Operator : MA/JU
Sample : PB154650BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK973

Quant Time: Aug 25 03:50:55 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 23 02:28:27 2023
Response via : Initial Calibration




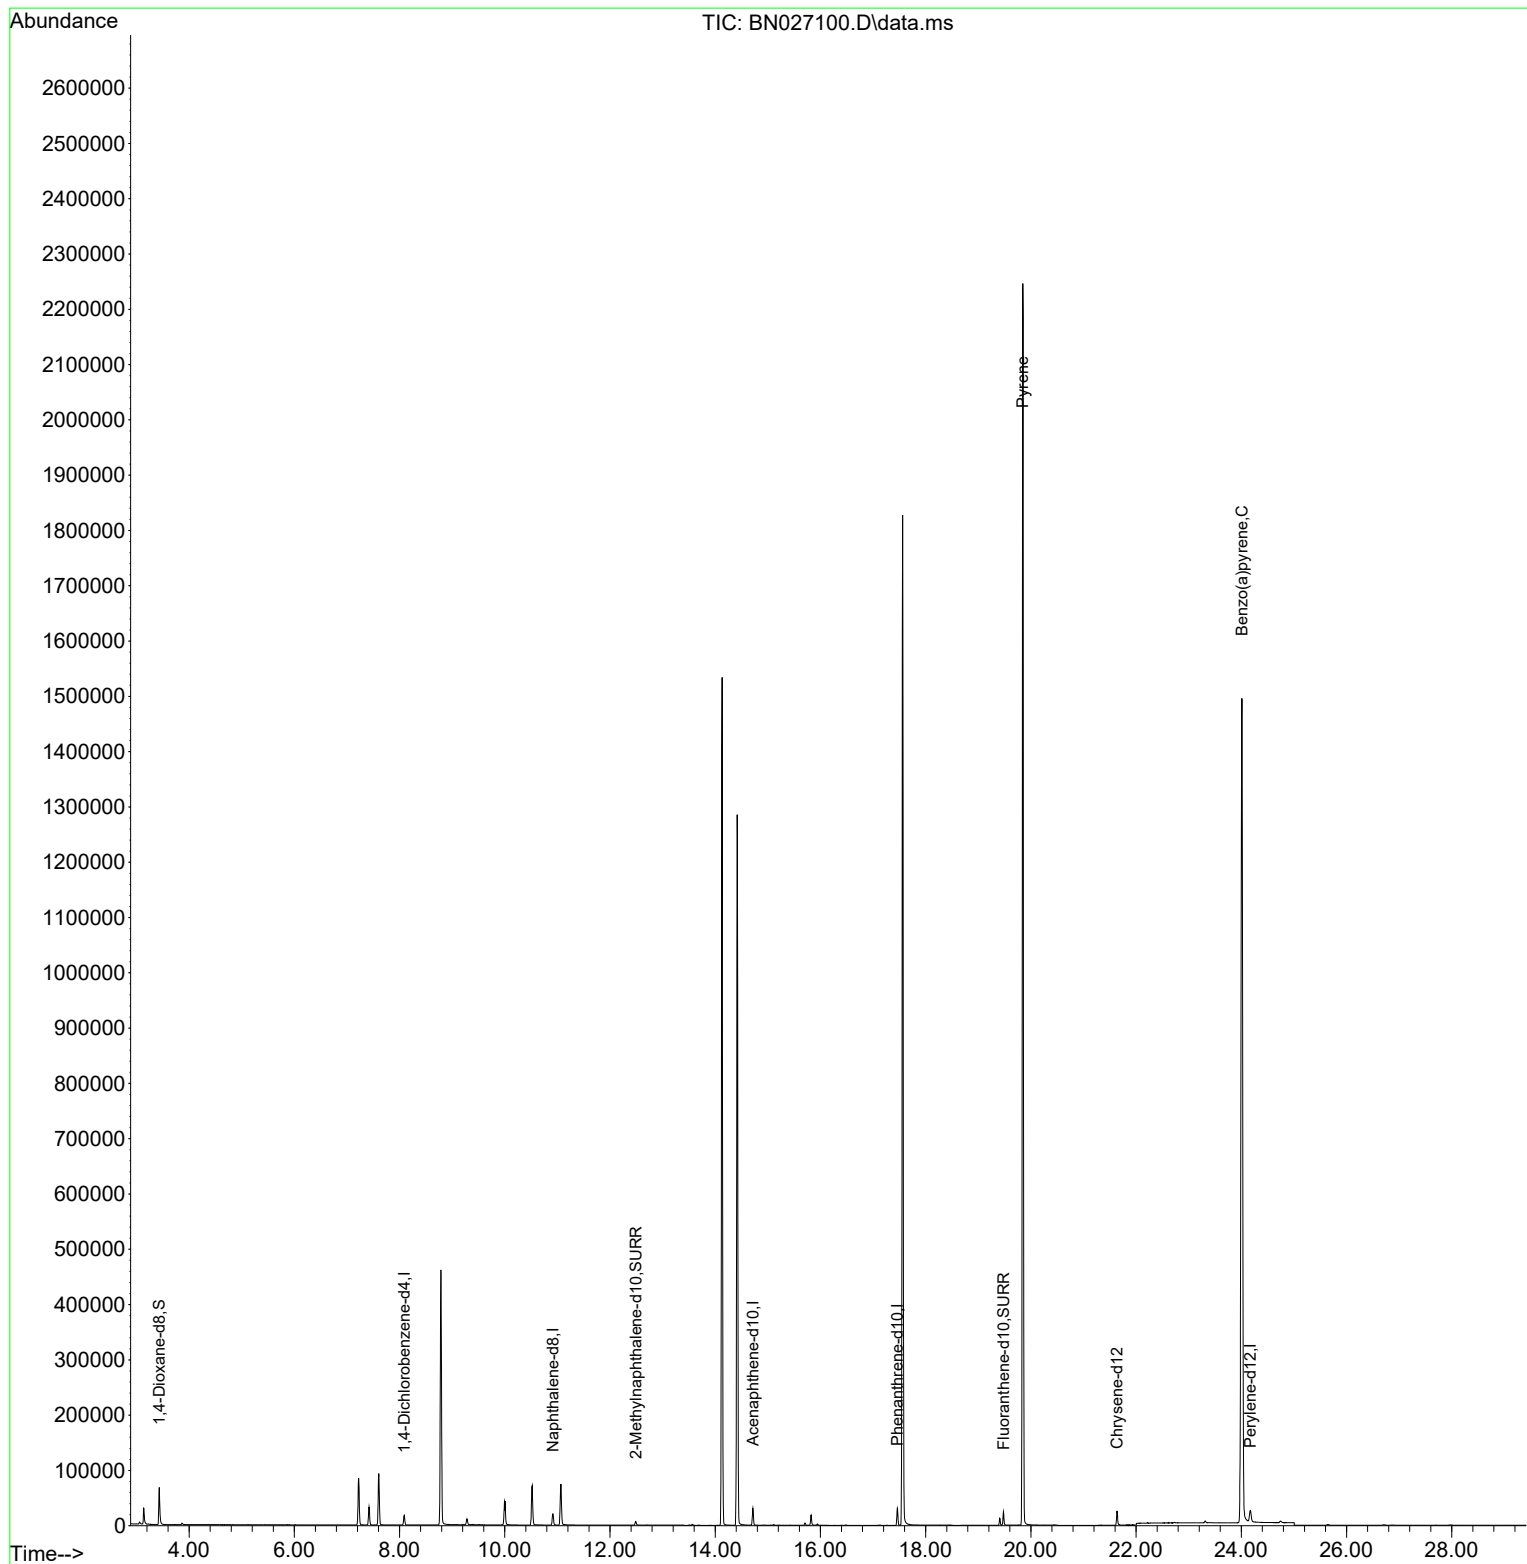


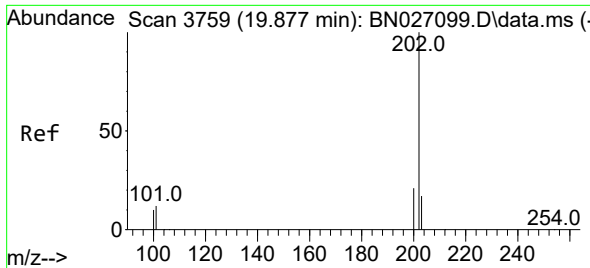

#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.845 min Scan# 31
Delta R.T. -0.037 min
Lab File: BN027100.D
Acq: 24 Aug 2023 16:47

Instrument :
BNA_N
ClientSampleId :
SBLK973

Tgt Ion:202 Resp: 4106
Ion Ratio Lower Upper
202 100
101 159.1 10.7 16.1#
100 1196.6 8.5 12.7#

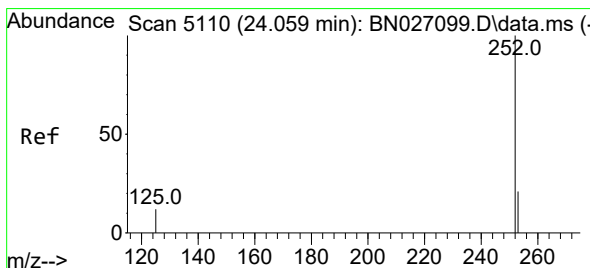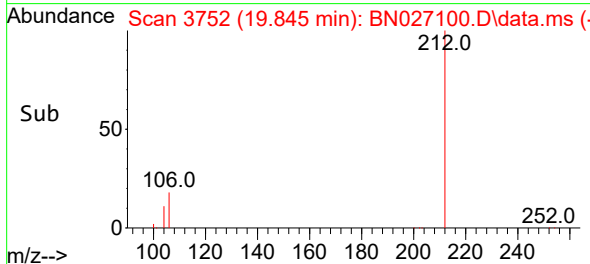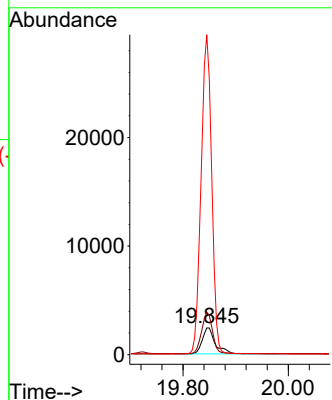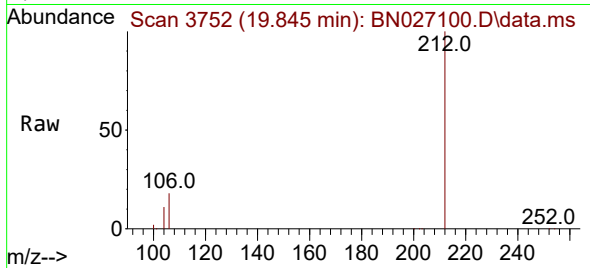

#26
Benzo(a)pyrene
Concen: 0.079 ng/ul
RT: 24.009 min Scan# 5093
Delta R.T. -0.053 min
Lab File: BN027100.D
Acq: 24 Aug 2023 16:47

Tgt Ion:252 Resp: 8975
Ion Ratio Lower Upper
252 100
253 41.1 19.0 28.6#
125 39.7 11.4 17.0#

