

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082423\
 Data File : BN027105.D
 Acq On : 24 Aug 2023 19:52
 Operator : MA/JU
 Sample : 03968-28
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A48P7

Quant Time: Aug 25 03:51:42 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 23 02:28:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.089	152	7701	0.400	ng/ul	0.00
4) Naphthalene-d8	10.911	136	25813	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.717	164	15623	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.459	188	34381	0.400	ng/ul	0.00
17) Chrysene-d12	21.635	240	28540	0.400	ng/ul	0.00
23) Perylene-d12	24.170	264	33275	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.431	96	45641	4.992	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.489	152	9419	0.248	ng/ul	0.00
18) Fluoranthene-d10	19.478	212	26989	0.299	ng/ul	0.00
Target Compounds						
					Qvalue	
24) Benzo(b)fluoranthene	23.380	252	2789	0.022	ng/ul#	1
26) Benzo(a)pyrene	24.006	252	7138	0.063	ng/ul#	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082423\
Data File : BN027105.D
Acq On : 24 Aug 2023 19:52
Operator : MA/JU
Sample : 03968-28
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A48P7


Quant Time: Aug 25 03:51:42 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 23 02:28:27 2023
Response via : Initial Calibration

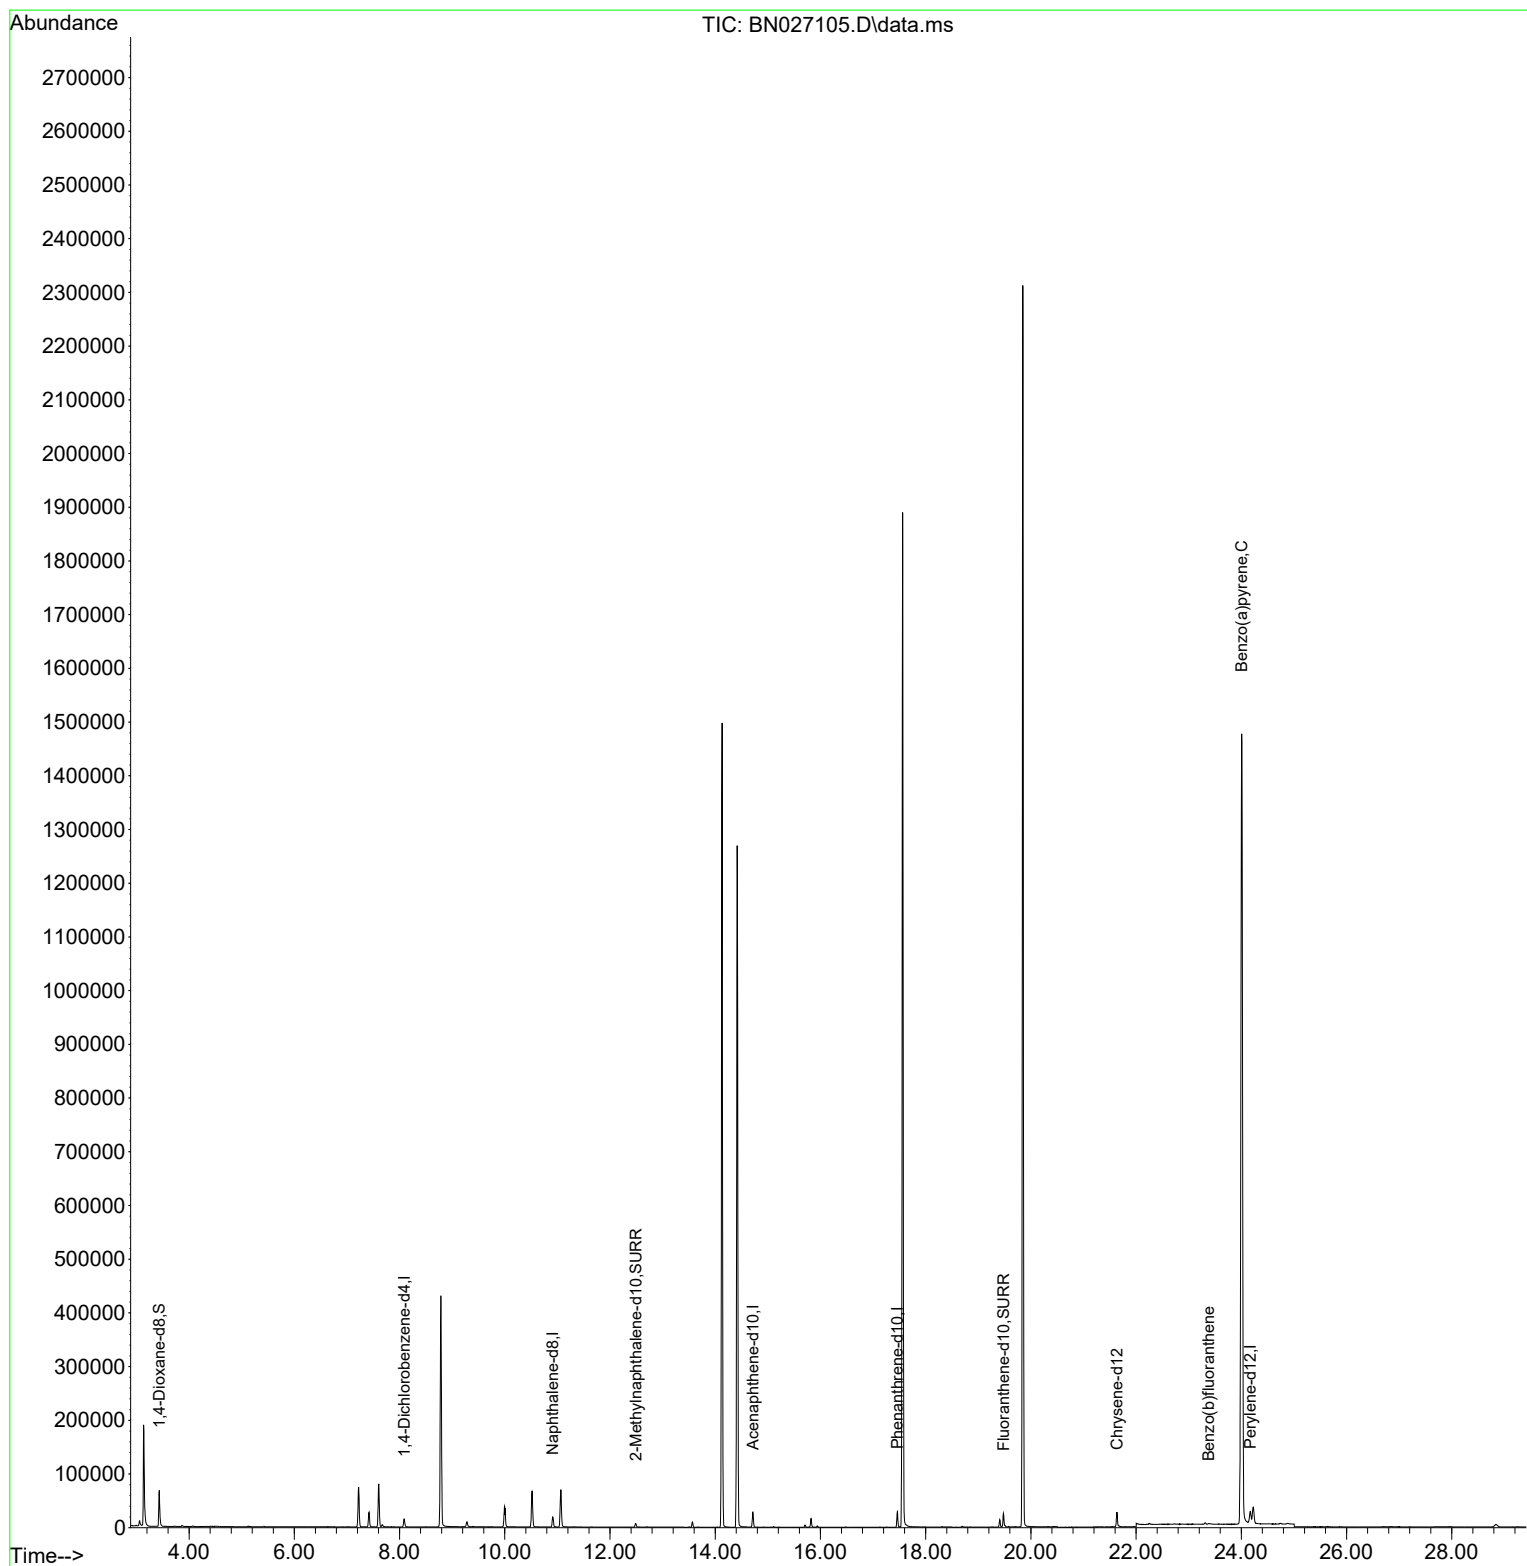



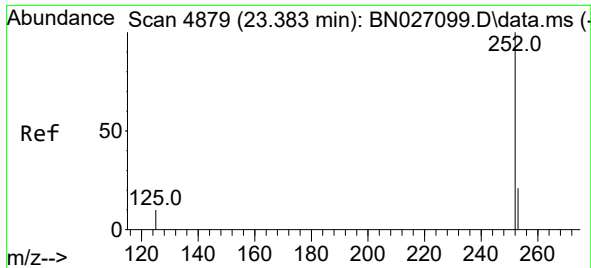


#24
Benzo(b)fluoranthene
Concen: 0.022 ng/ul
RT: 23.380 min Scan# 41
Delta R.T. -0.006 min
Lab File: BN027105.D
Acq: 24 Aug 2023 19:52

Instrument :
BNA_N
ClientSampleId :
A48P7

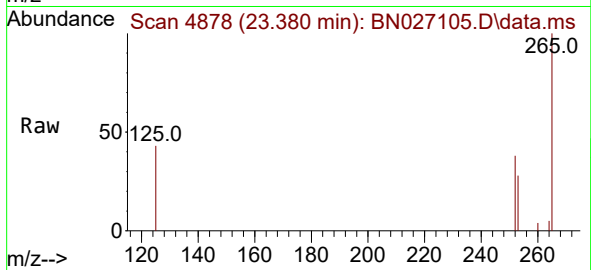

Tgt Ion:252 Resp: 2789
Ion Ratio Lower Upper
252 100
253 73.5 0.0 46.8#
125 110.6 0.0 25.2#

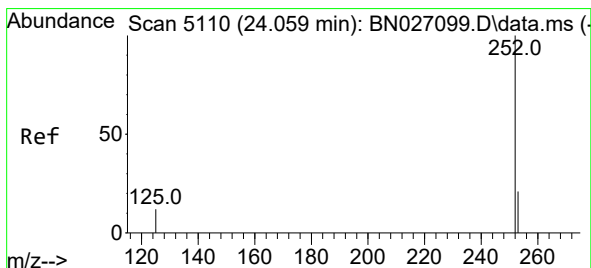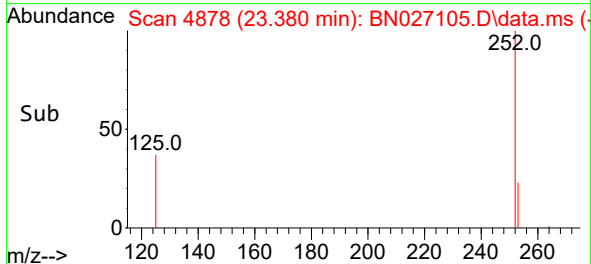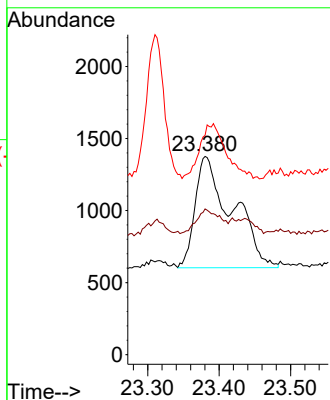

#26
Benzo(a)pyrene
Concen: 0.063 ng/ul
RT: 24.006 min Scan# 5092
Delta R.T. -0.056 min
Lab File: BN027105.D
Acq: 24 Aug 2023 19:52

Tgt Ion:252 Resp: 7138
Ion Ratio Lower Upper
252 100
253 44.2 19.0 28.6#
125 46.1 11.4 17.0#

