
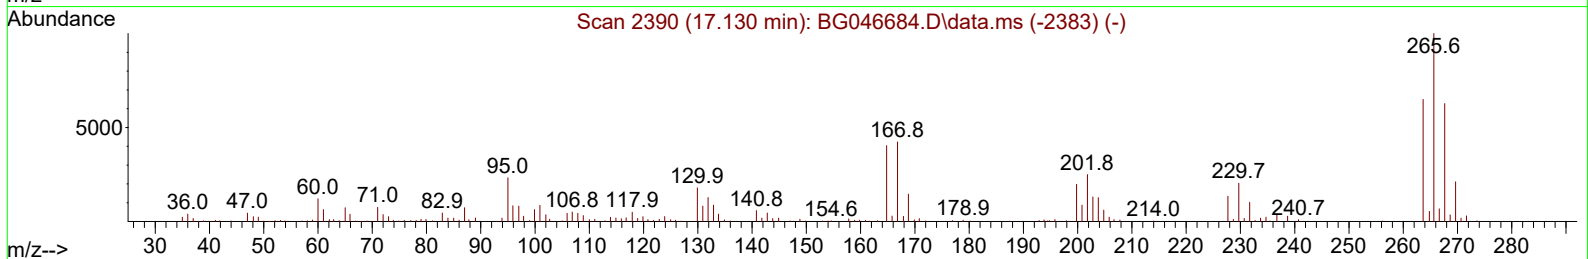
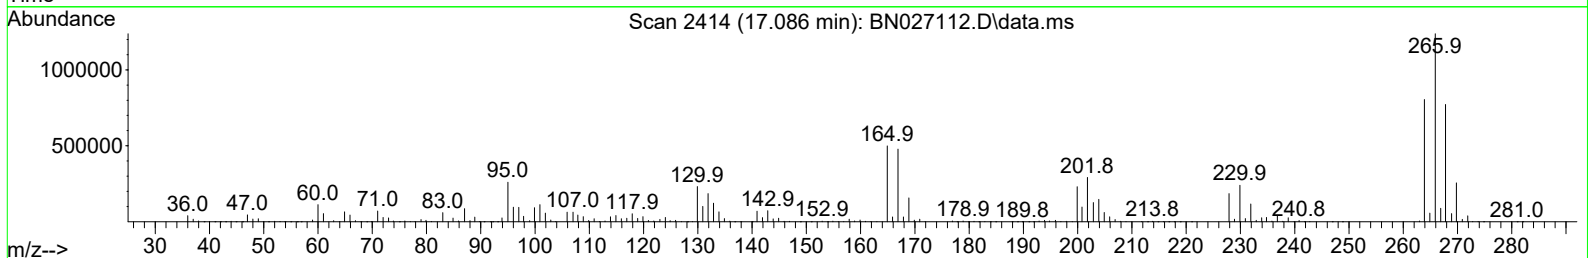


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
Data File : BN027112.D
Acq On : 25 Aug 2023 09:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 06:49:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 26 06:49:43 2023
Response via : Initial Calibration

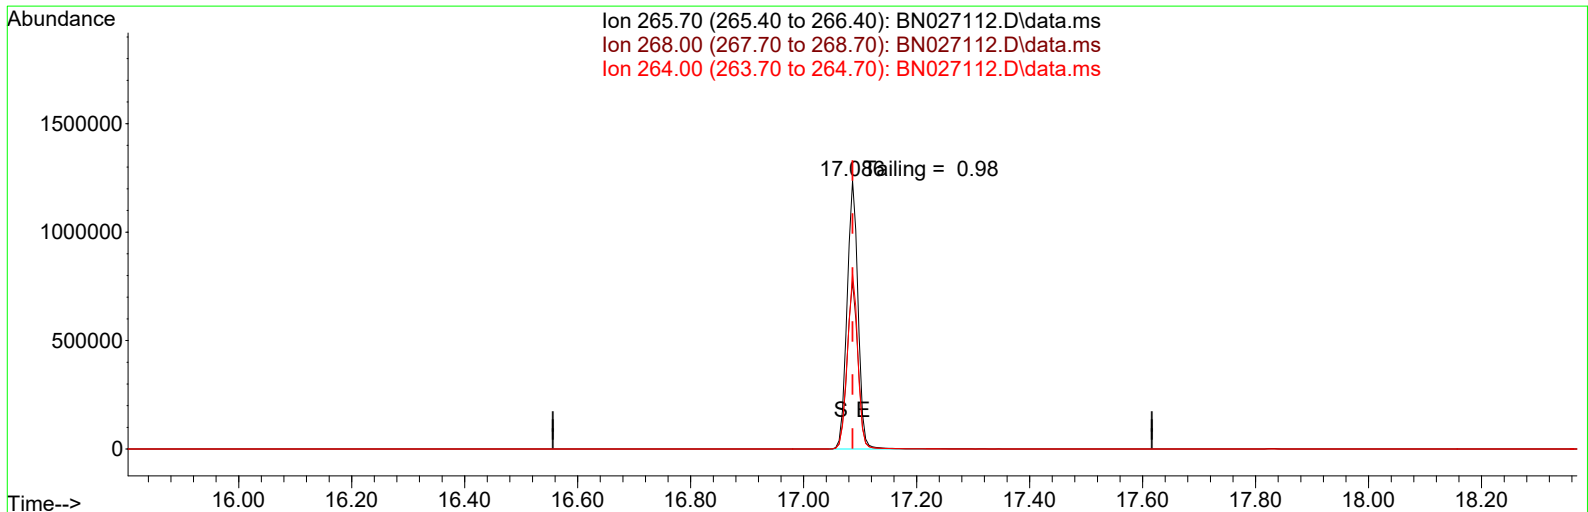

TIC: BN027112.D\data.ms

(70) Pentachlorophenol (C)




17.086min (0.000) 39288.13 ng

response 1678204

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.35
264.00	61.60	65.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
 Data File : BN027112.D
 Acq On : 25 Aug 2023 09:55
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 06:49:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 26 06:49:43 2023
 Response via : Initial Calibration

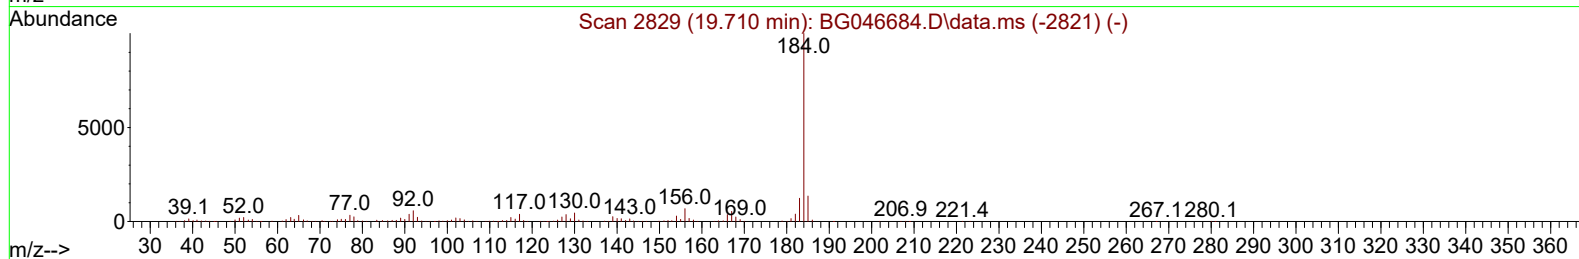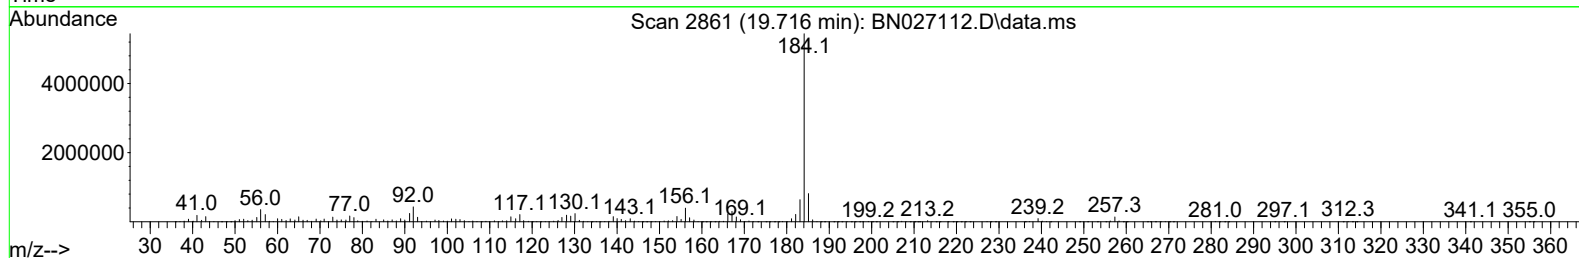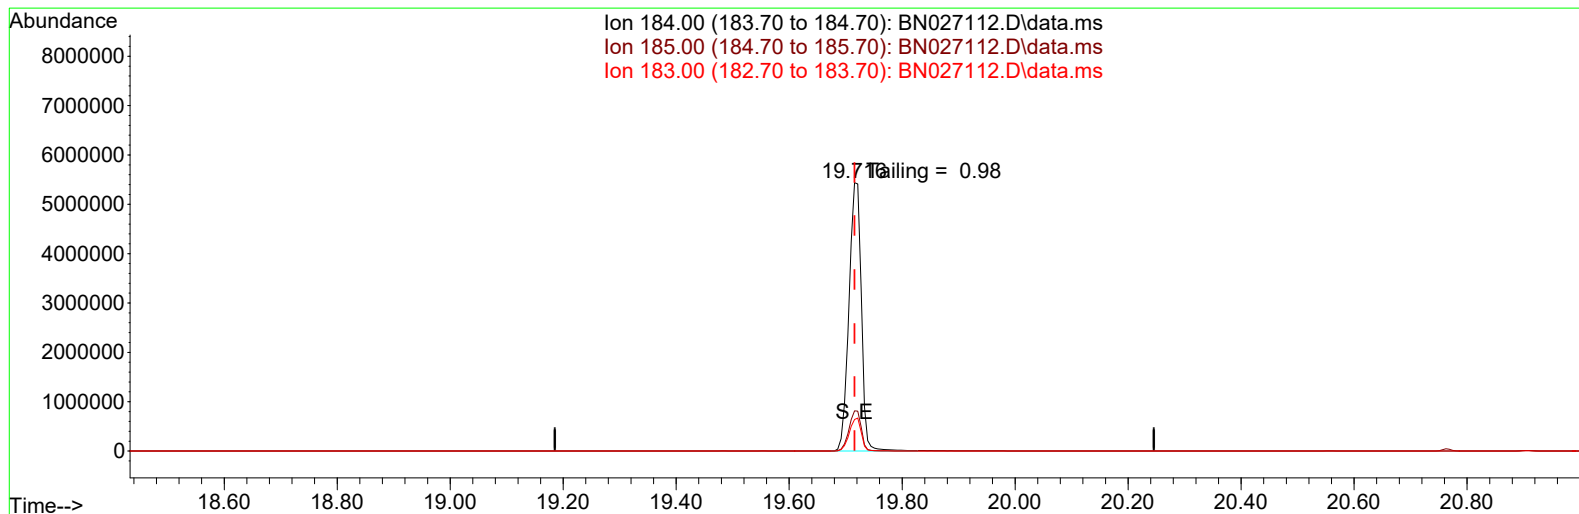

TIC: BN027112.D\data.ms

(77) Benzidine

19.716min (0.000) 1880129.62 ng

response 8345620

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.00
183.00	13.20	11.75
0.00	0.00	0.00