
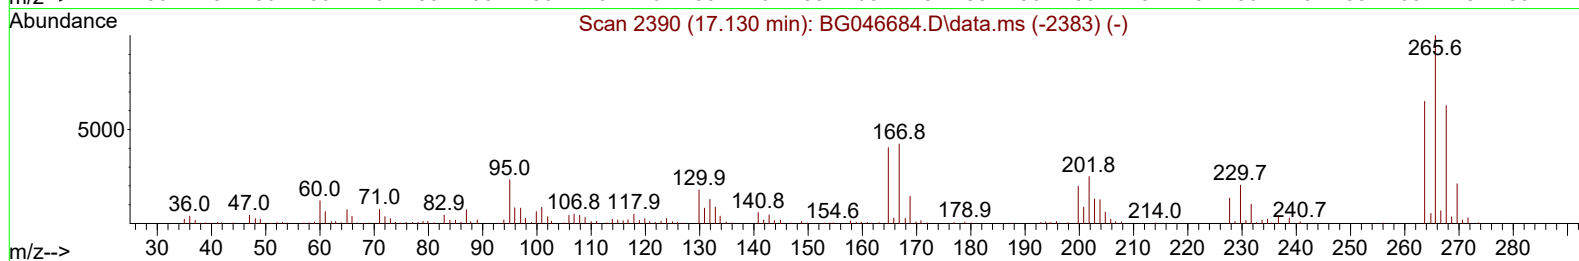
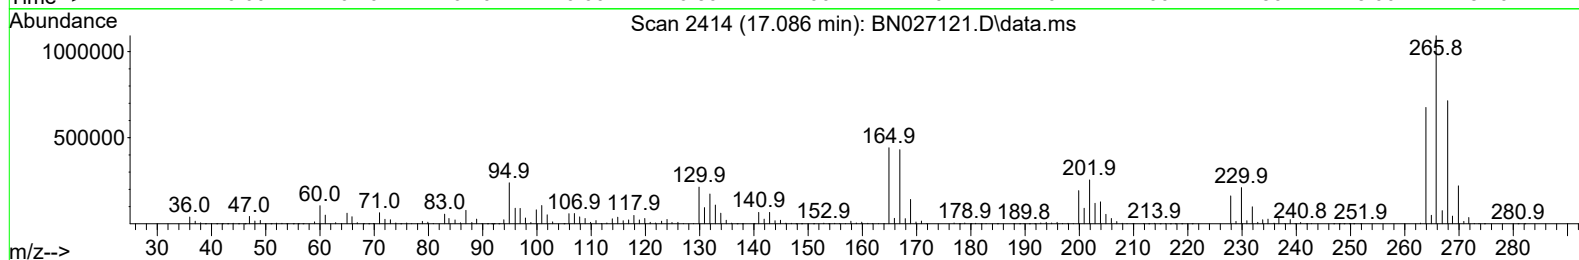


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
Data File : BN027121.D
Acq On : 25 Aug 2023 16:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 06:51:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 26 06:49:43 2023
Response via : Initial Calibration

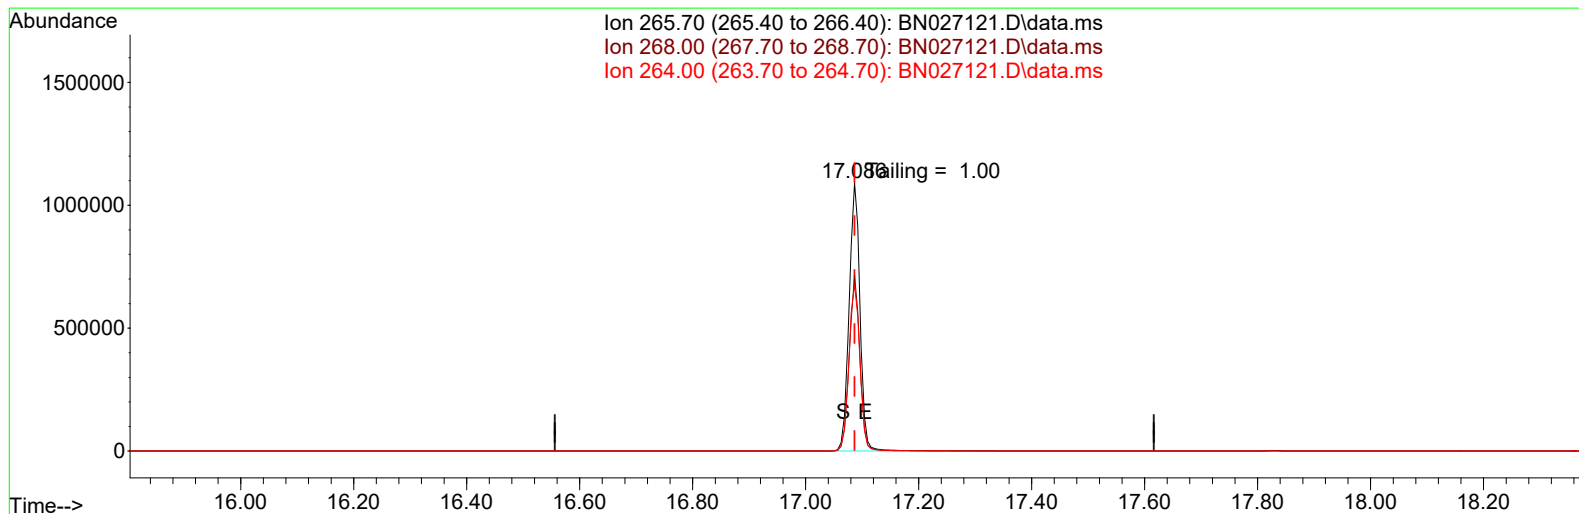

TIC: BN027121.D\data.ms

(70) Pentachlorophenol (C)




17.086min (-0.000) 35809.85 ng

response 1464430

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.48
264.00	61.60	61.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
 Data File : BN027121.D
 Acq On : 25 Aug 2023 16:32
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 06:51:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 26 06:49:43 2023
 Response via : Initial Calibration

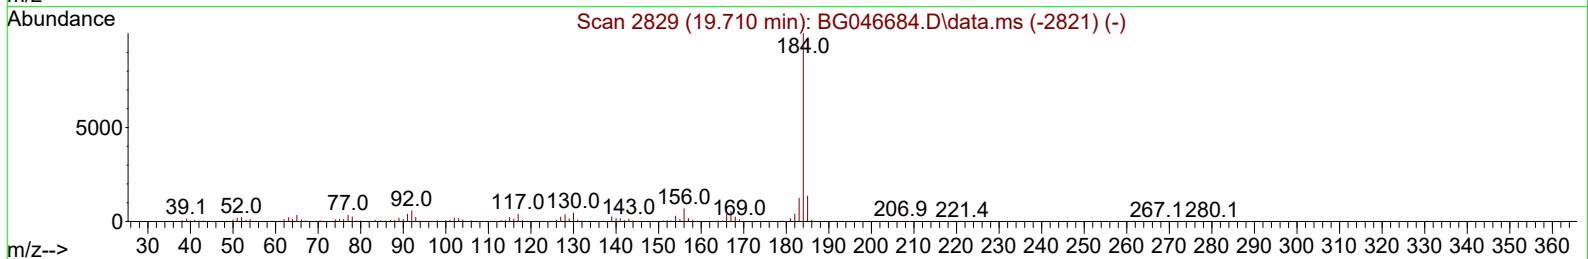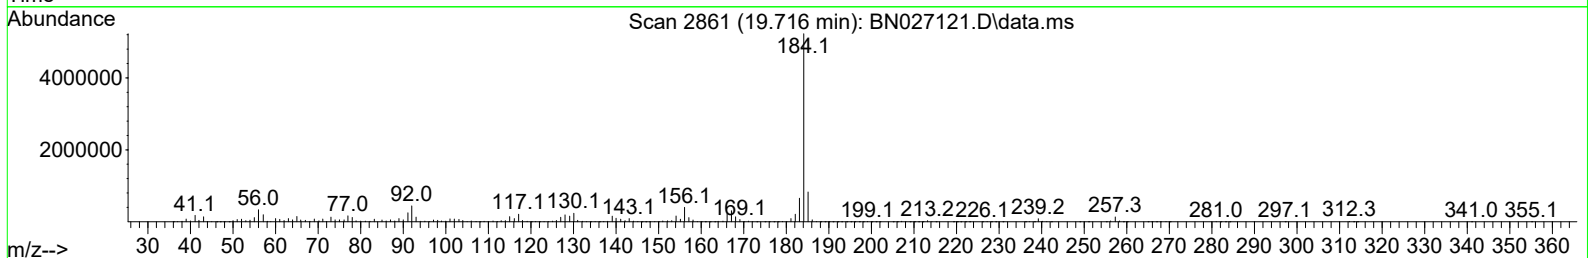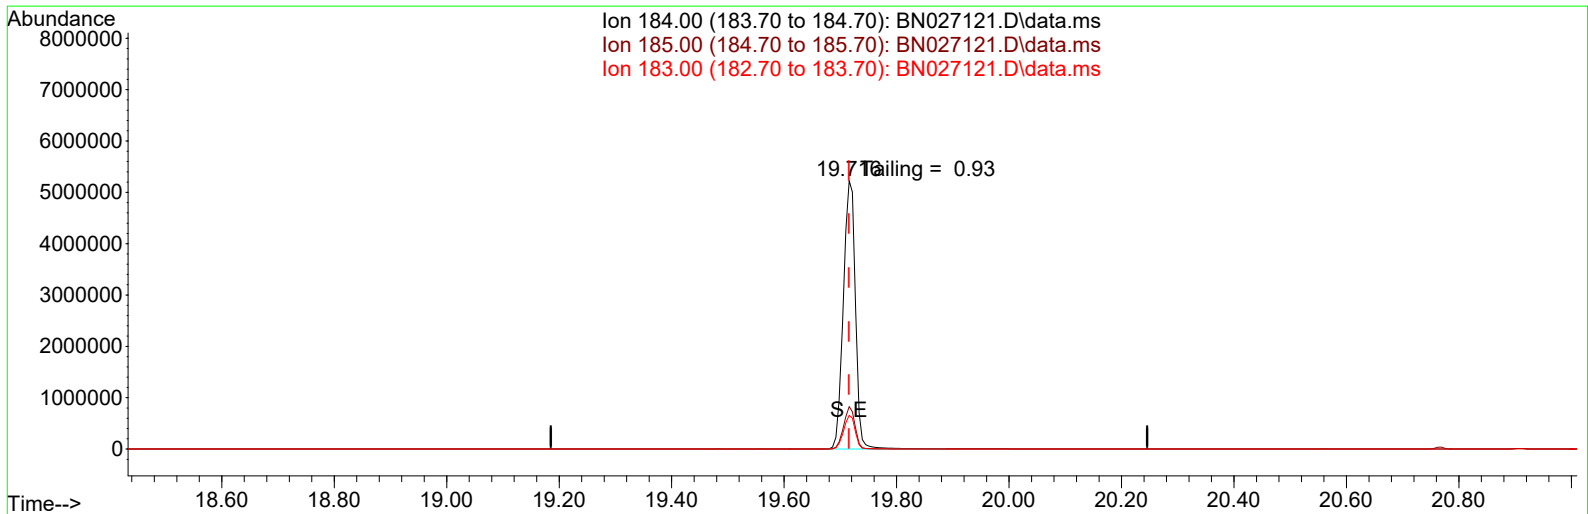

TIC: BN027121.D\data.ms

(77) Benzidine**19.716min (-0.000) 4380034.99 ng****response 7830940**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.83
183.00	13.20	12.53
0.00	0.00	0.00