
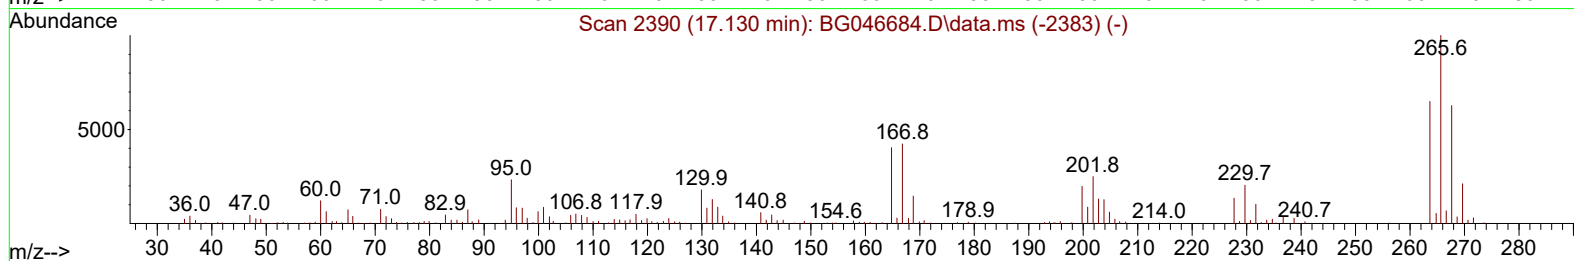
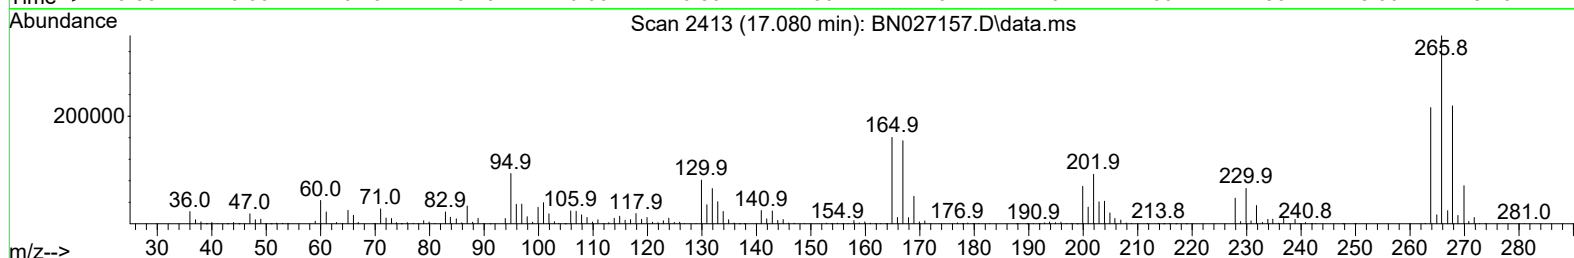


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
Data File : BN027157.D
Acq On : 26 Aug 2023 16:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 46 Sample Multiplier: 1

Quant Time: Aug 27 04:49:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 27 04:48:19 2023
Response via : Initial Calibration

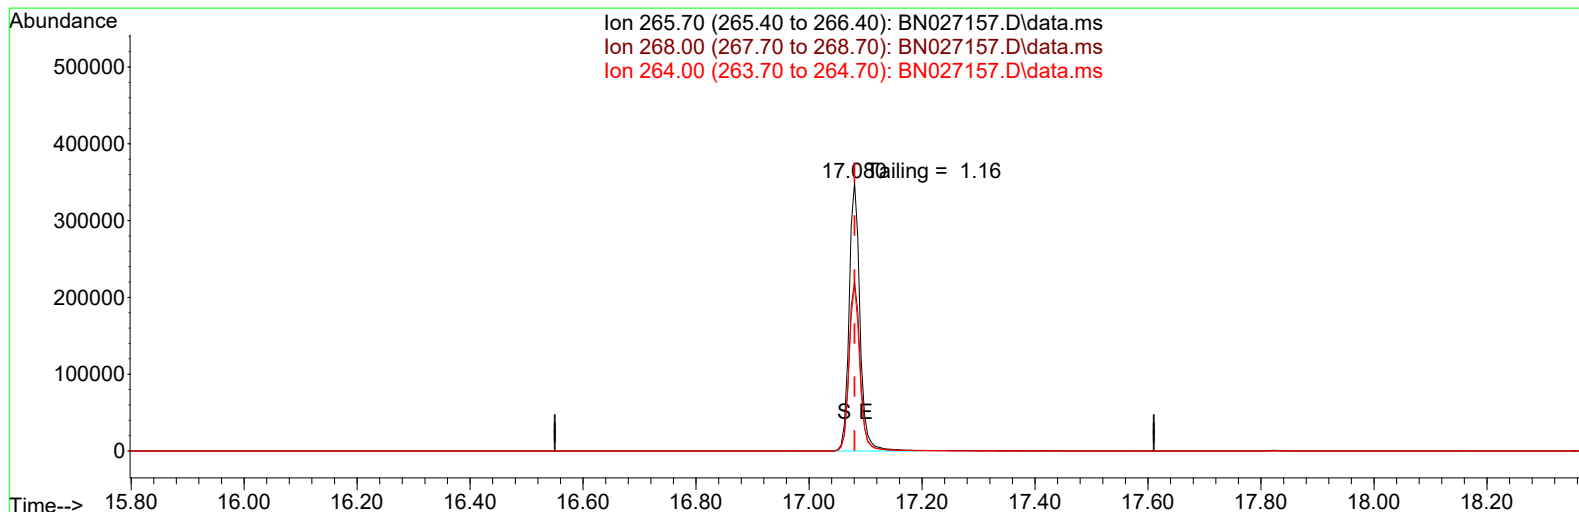

TIC: BN027157.D\data.ms

(70) Pentachlorophenol (C)




17.080min (-0.000) 22025.85 ng

response 468951

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.78
264.00	61.60	61.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
Data File : BN027157.D
Acq On : 26 Aug 2023 16:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 46 Sample Multiplier: 1

Quant Time: Aug 27 04:49:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 27 04:48:19 2023
Response via : Initial Calibration

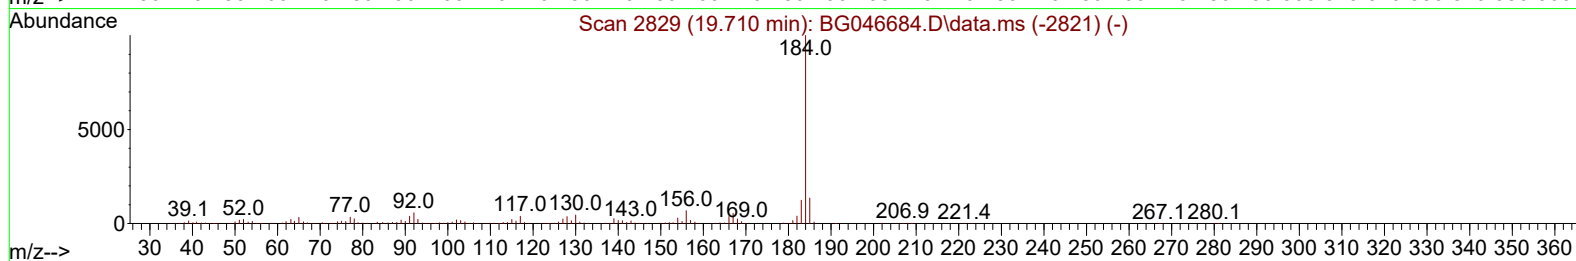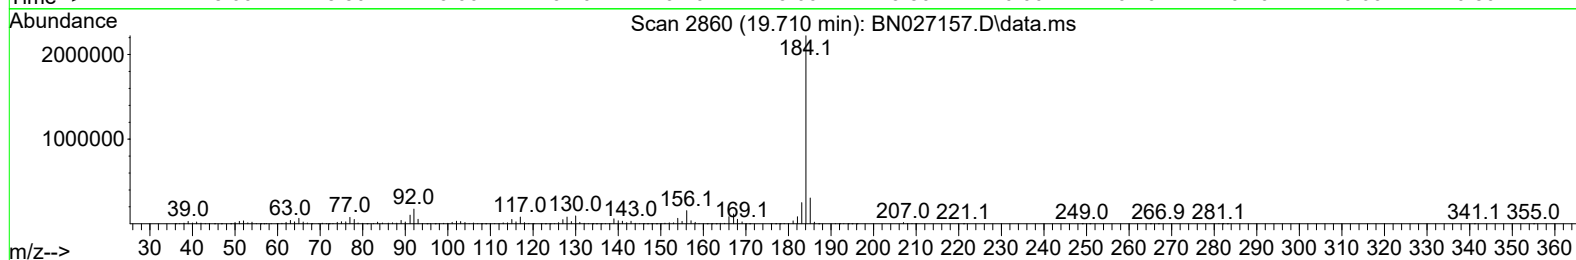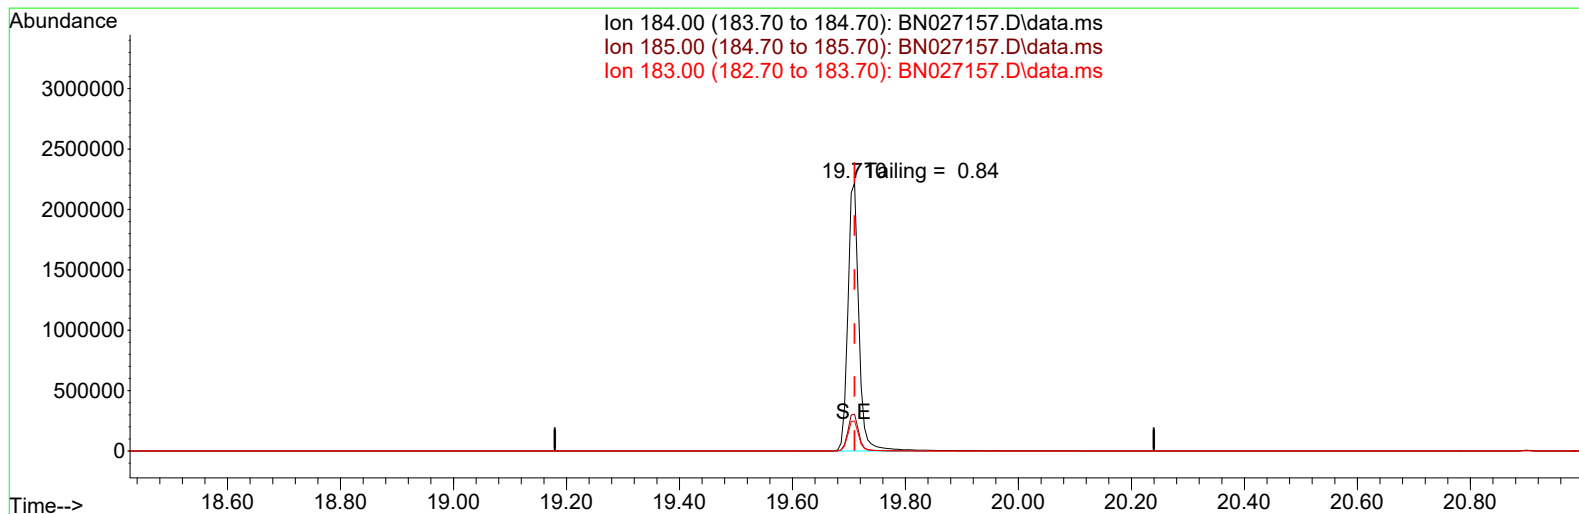

TIC: BN027157.D\data.ms

(77) Benzidine

19.710min (-0.000) 0.00 ng

response 3014282

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.73
183.00	13.20	11.22
0.00	0.00	0.00