
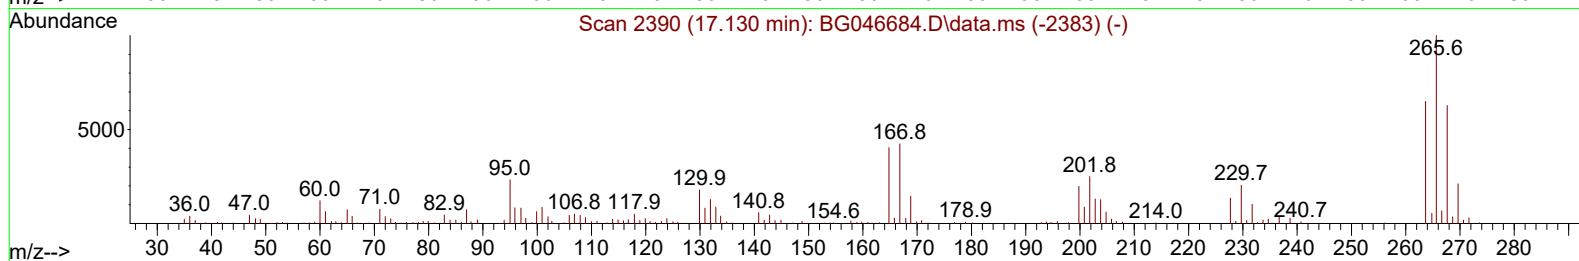
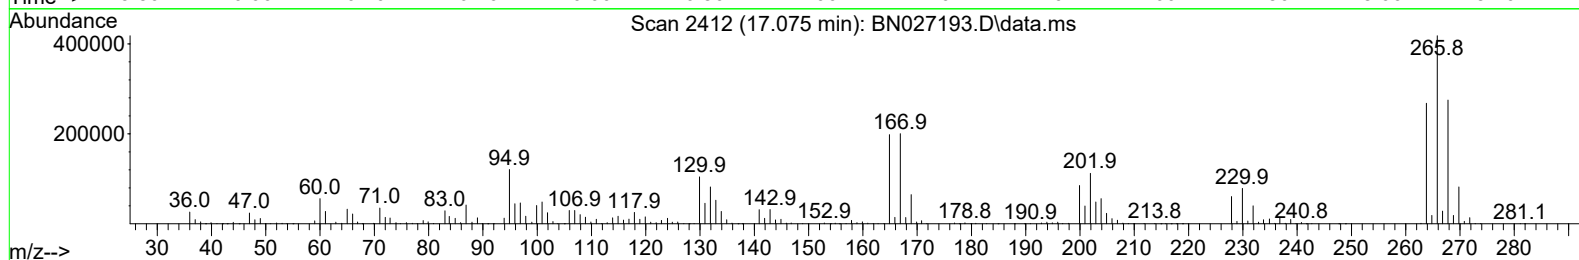


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
Data File : BN027193.D
Acq On : 27 Aug 2023 17:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 84 Sample Multiplier: 1

Quant Time: Aug 28 01:21:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 01:21:07 2023
Response via : Initial Calibration

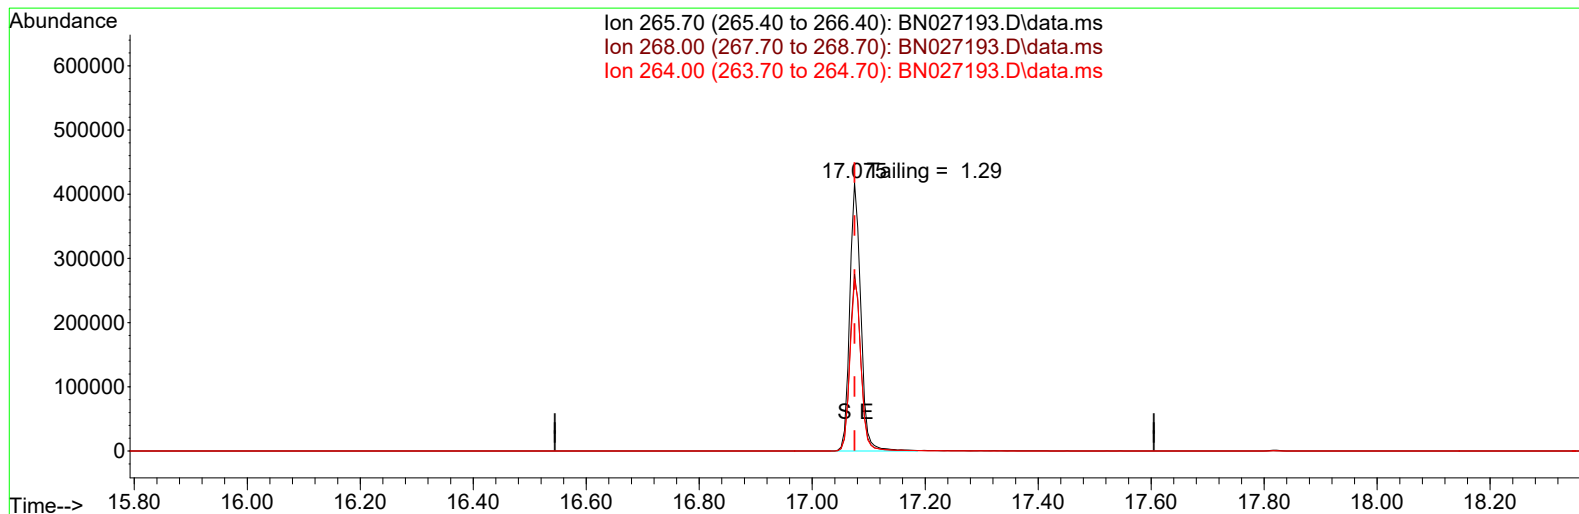

TIC: BN027193.D\data.ms

(70) Pentachlorophenol (C)




17.075min (0.000) 20760.76 ng

response 570727

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.80
264.00	61.60	64.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
Data File : BN027193.D
Acq On : 27 Aug 2023 17:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 84 Sample Multiplier: 1

Quant Time: Aug 28 01:21:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 01:21:07 2023
Response via : Initial Calibration

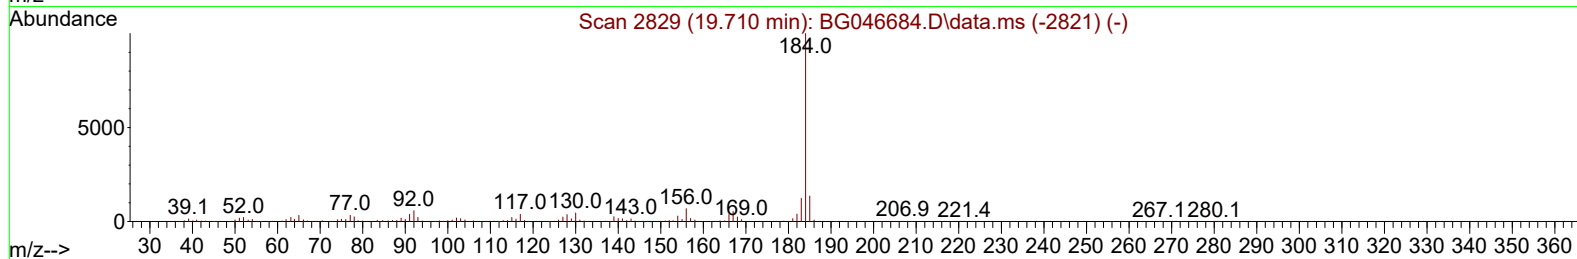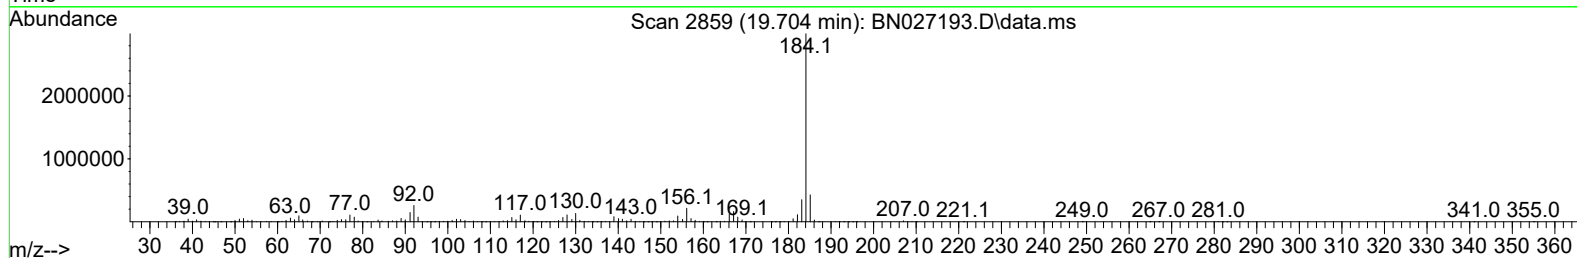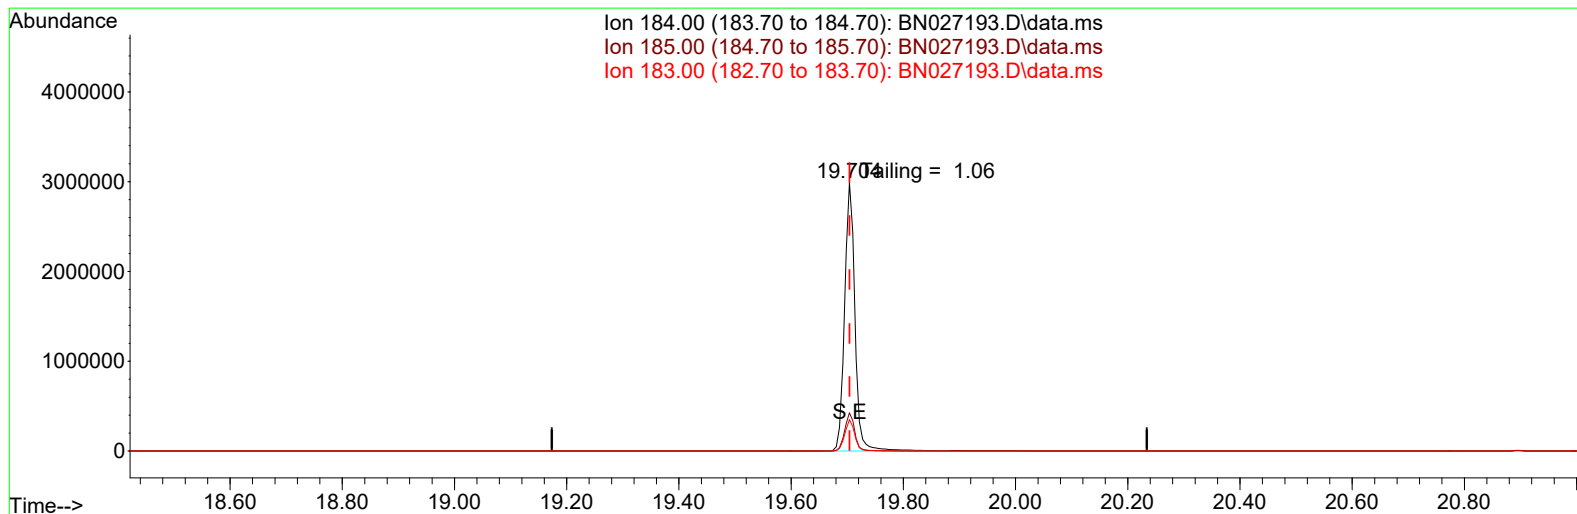

TIC: BN027193.D\data.ms

(77) Benzidine

19.704min (0.000) 0.00 ng

response 3850520

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	11.72
0.00	0.00	0.00