
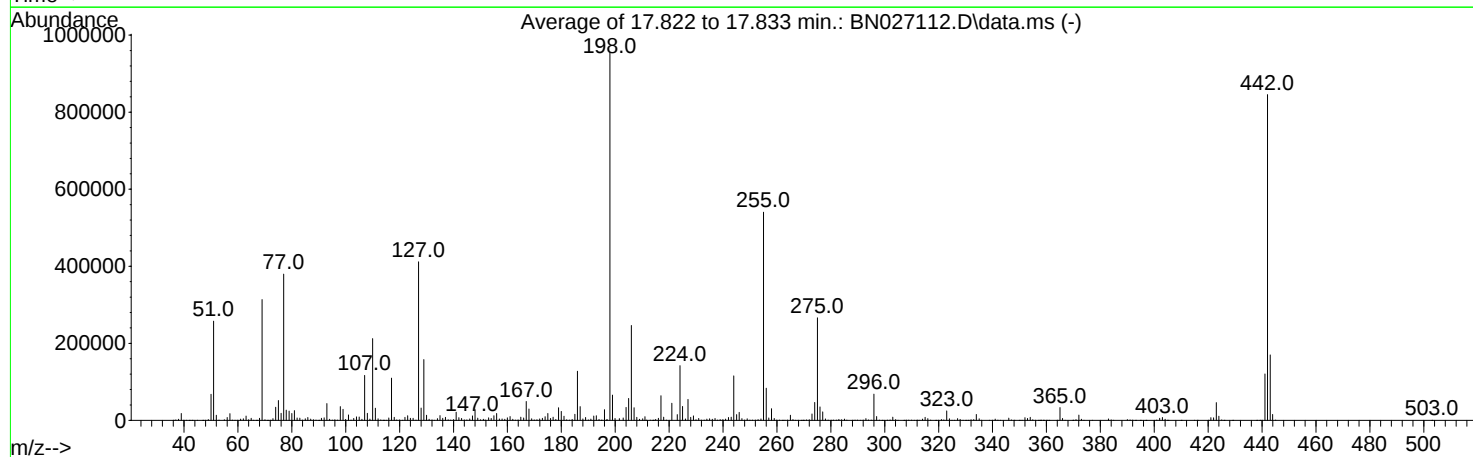


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
 Data File : BN027112.D
 Acq On : 25 Aug 2023 09:55
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 26 02:13:59 2023

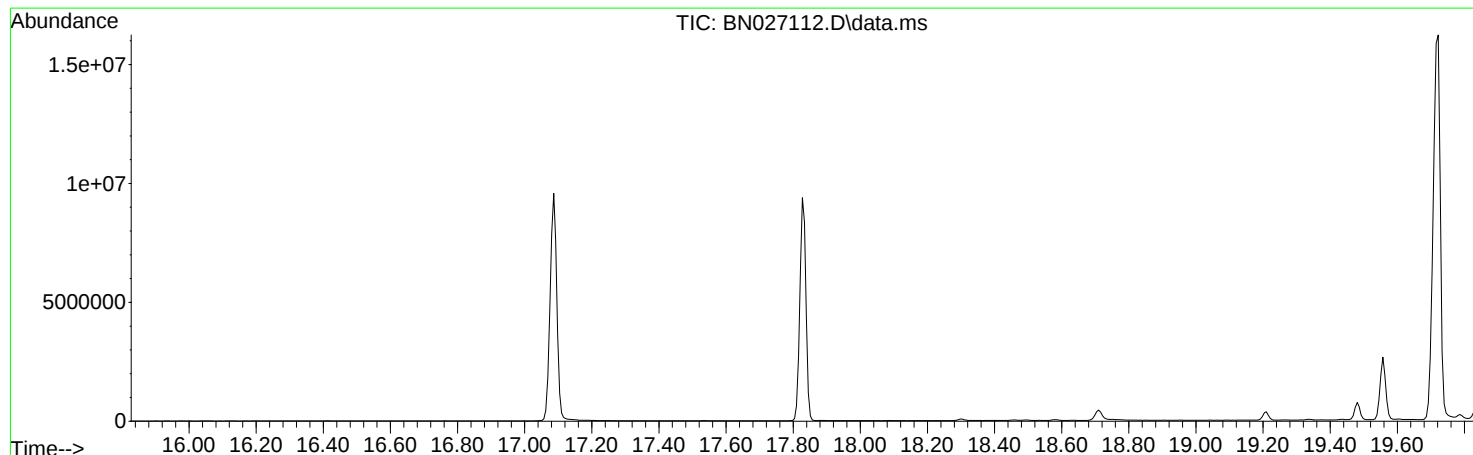




AutoFind: Scans 2539, 2540, 2541; Background Corrected with Scan 2532

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	257570	PASS
68	69	0.00	2	1.8	5554	PASS
69	198	0.00	100	32.8	313436	PASS
70	69	0.00	2	0.5	1610	PASS
127	198	10	80	43.1	411627	PASS
197	198	0.00	2	0.2	2086	PASS
198	198	100	100	100.0	954923	PASS
199	198	5	9	6.9	65680	PASS
275	198	10	60	27.9	266261	PASS
365	198	1	100	3.5	33405	PASS
441	198	0.01	100	12.6	120592	PASS
442	442	50	100	100.0	845611	PASS
443	442	15	24	20.1	169811	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
Data File : BN027112.D
Acq On : 25 Aug 2023 09:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 26 06:49:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 26 06:49:43 2023
Response via : Initial Calibration

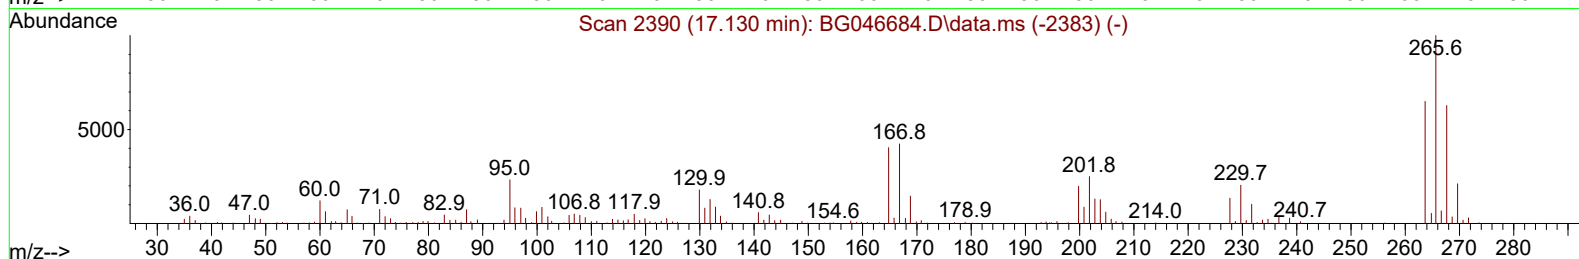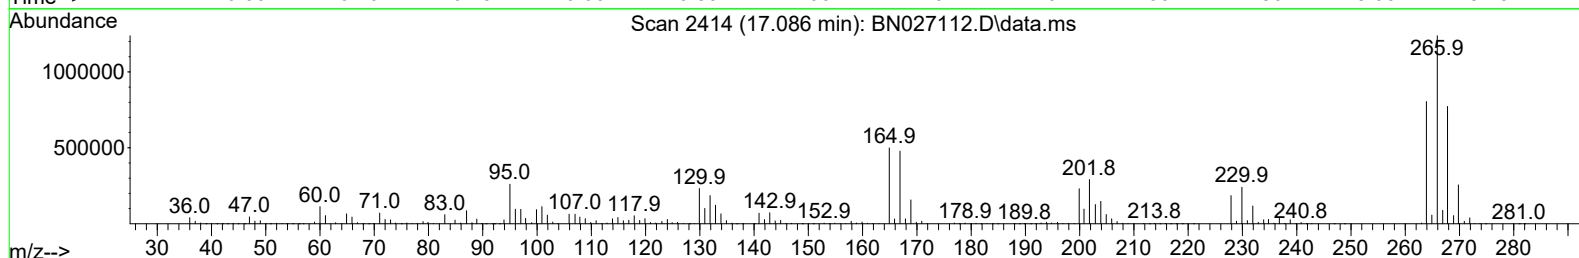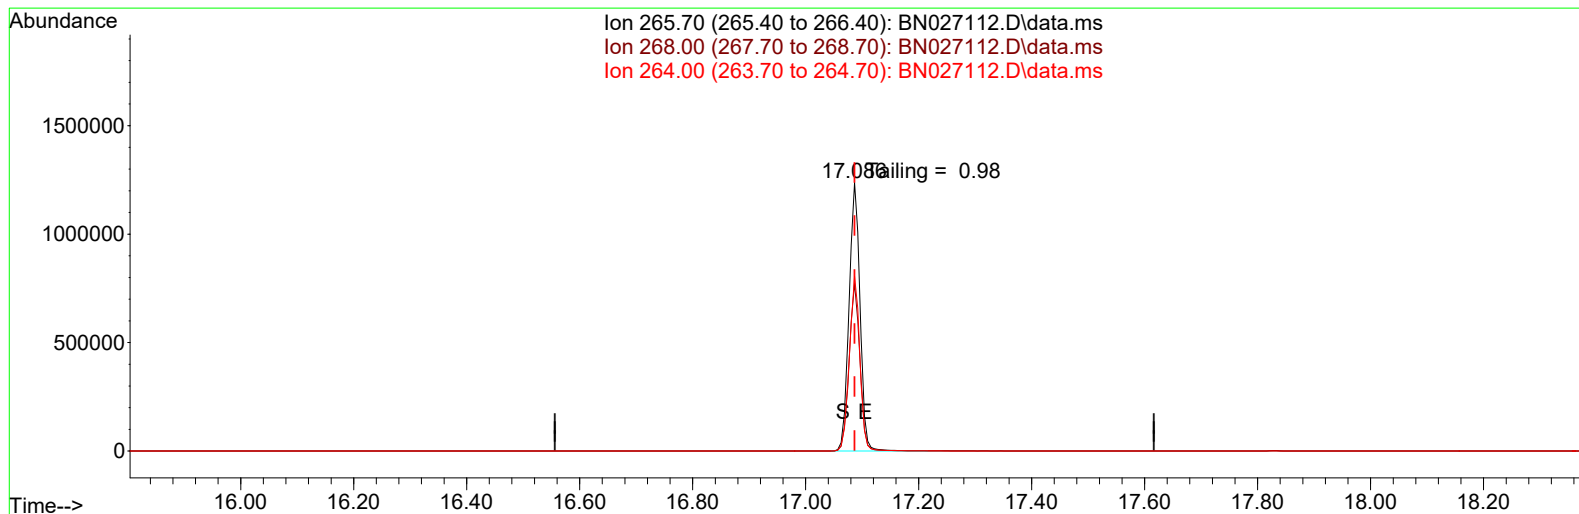

TIC: BN027112.D\data.ms

(70) Pentachlorophenol (C)

17.086min (0.000) 39288.13 ng




response 1678204

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.35
264.00	61.60	65.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
Data File : BN027112.D
Acq On : 25 Aug 2023 09:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 26 06:49:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 26 06:49:43 2023
Response via : Initial Calibration

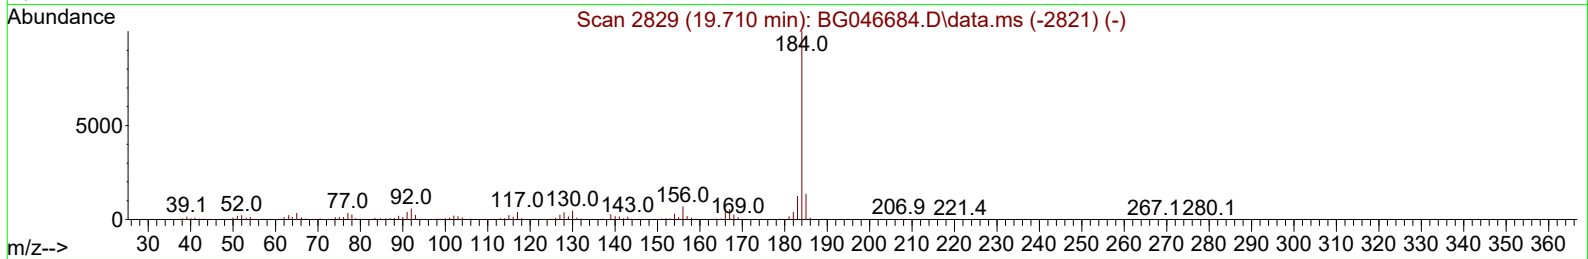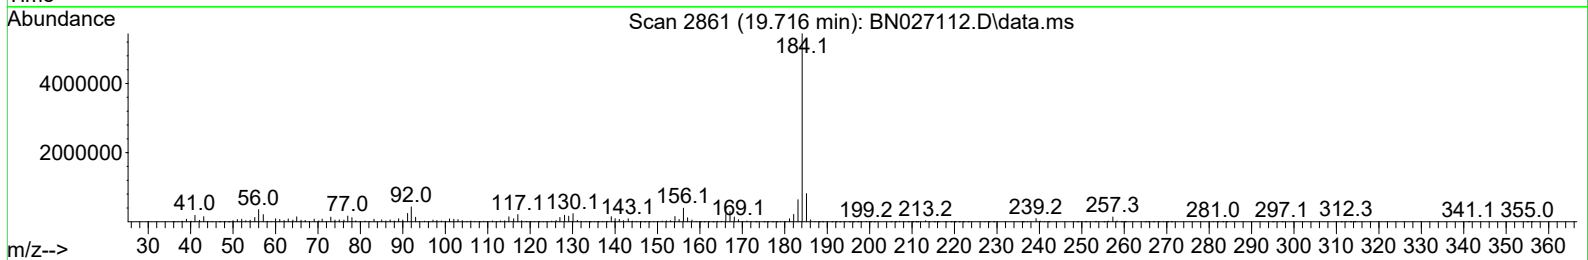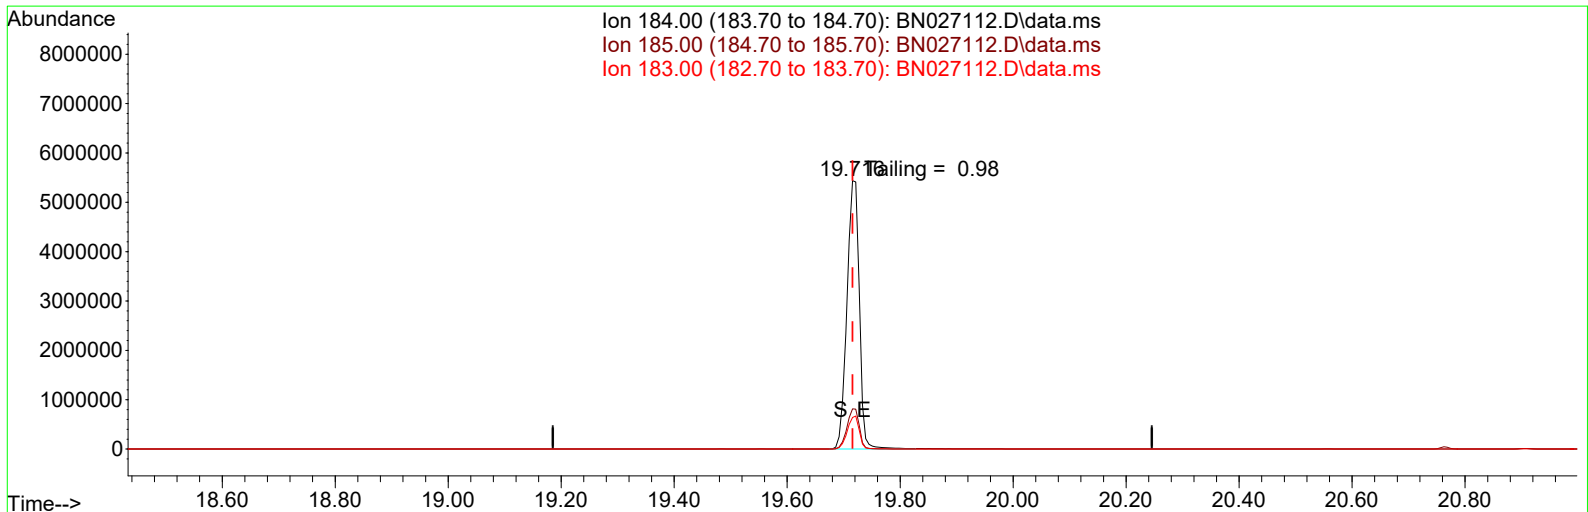

TIC: BN027112.D\data.ms

(77) Benzidine

19.716min (0.000) 1880129.62 ng

response 8345620

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.00
183.00	13.20	11.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2023	BNA_N	<u>BN027112.D</u>
Compound Name	Response	Retention Time
DDT	4204734	20.91
DDD	95892	20.469
DDE	1544	19.957
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
97436	4302170	2.26

Instrument :
BNA_N
ClientSampleId :
DFTPP