
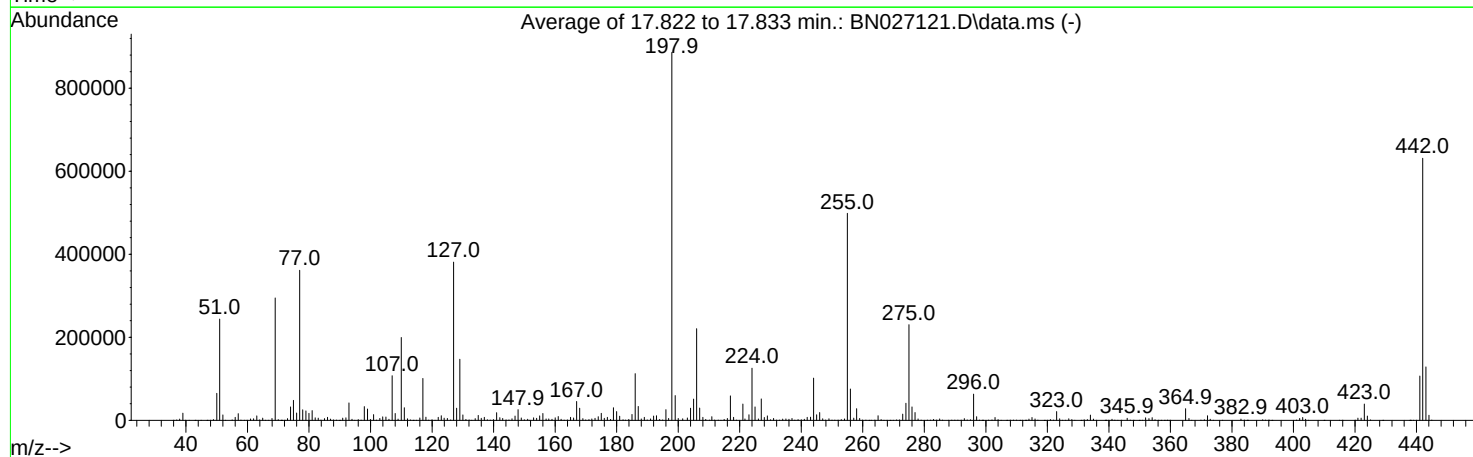


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
 Data File : BN027121.D
 Acq On : 25 Aug 2023 16:32
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 26 02:13:59 2023

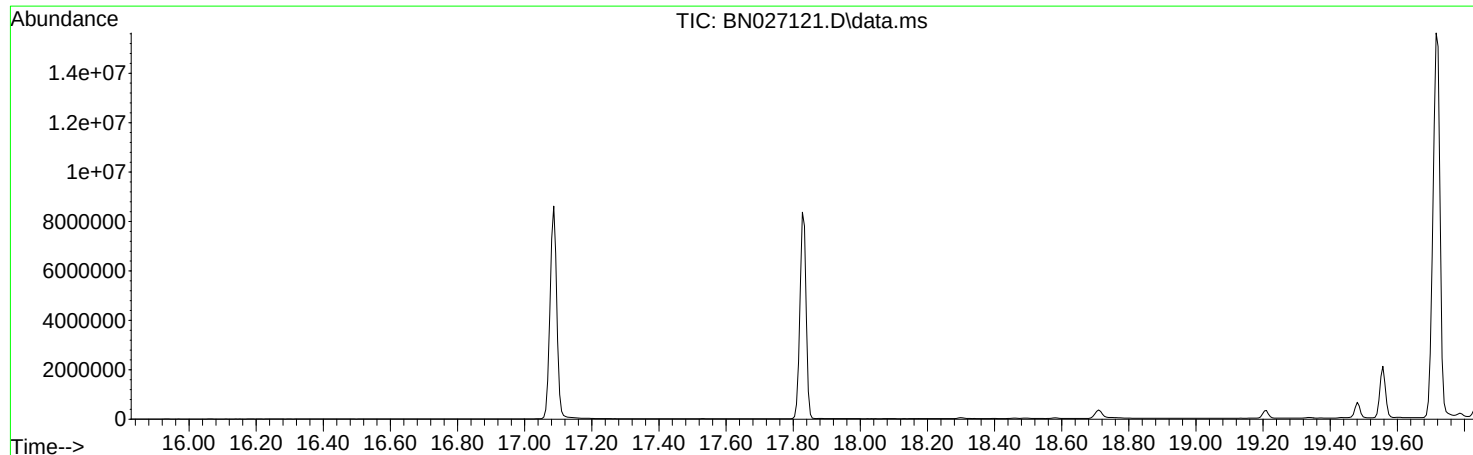




AutoFind: Scans 2539, 2540, 2541; Background Corrected with Scan 2532

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	243944	PASS
68	69	0.00	2	1.6	4739	PASS
69	198	0.00	100	33.3	294899	PASS
70	69	0.00	2	0.6	1776	PASS
127	198	10	80	43.0	381056	PASS
197	198	0.00	2	0.5	4681	PASS
198	198	100	100	100.0	886123	PASS
199	198	5	9	6.7	59765	PASS
275	198	10	60	26.0	230315	PASS
365	198	1	100	3.2	28045	PASS
441	198	0.01	100	12.0	106725	PASS
442	442	50	100	100.0	631147	PASS
443	442	15	24	20.4	128952	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
Data File : BN027121.D
Acq On : 25 Aug 2023 16:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 26 06:51:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 26 06:49:43 2023
Response via : Initial Calibration

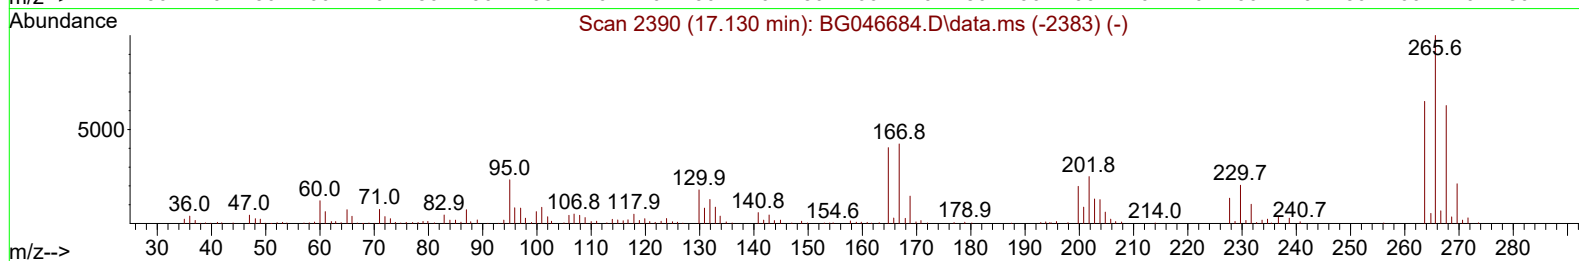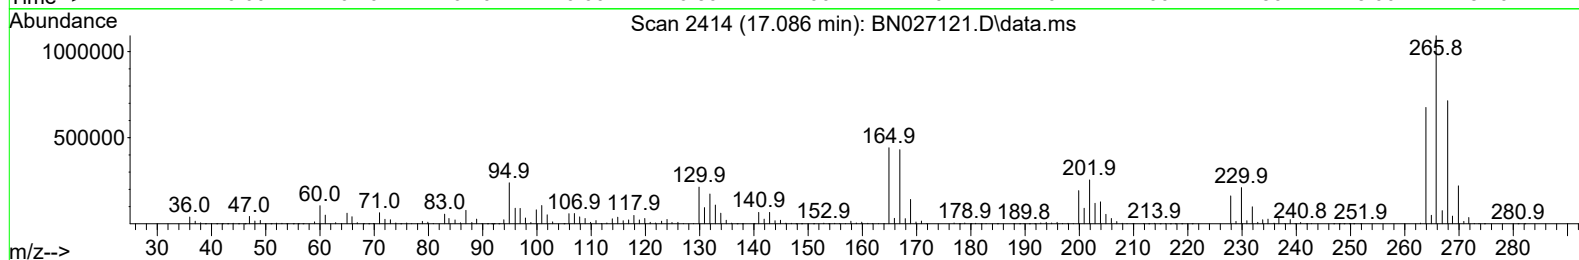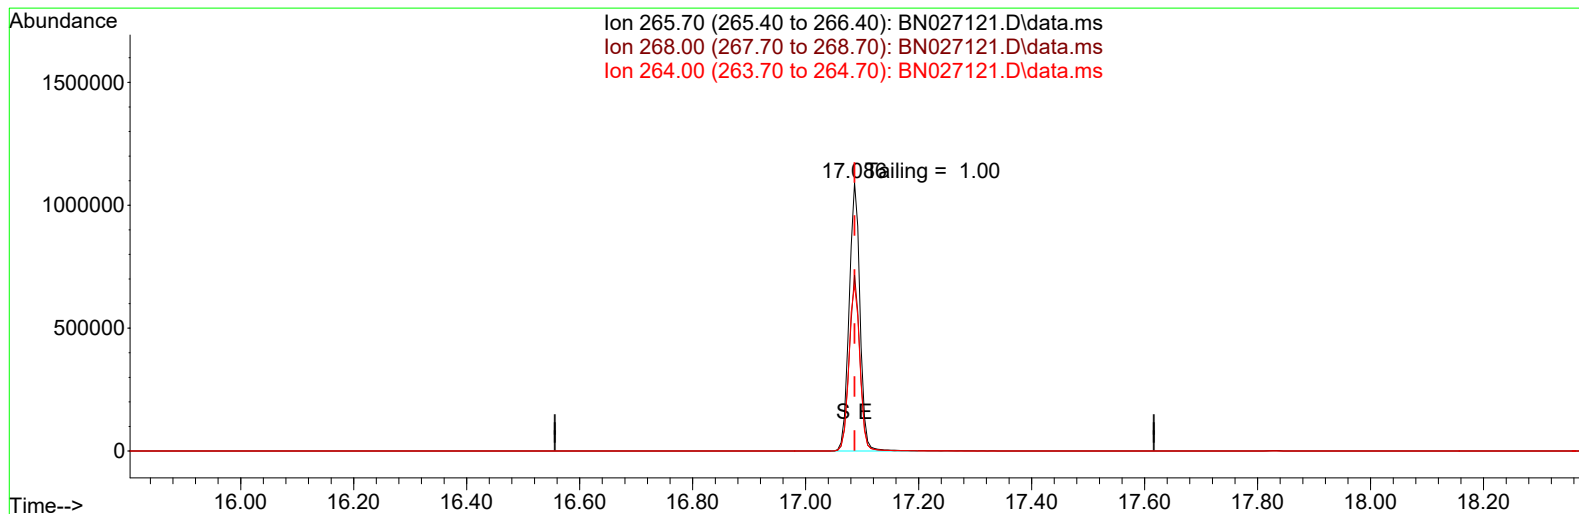

TIC: BN027121.D\data.ms

(70) Pentachlorophenol (C)

17.086min (-0.000) 35809.85 ng




response 1464430

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.48
264.00	61.60	61.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
Data File : BN027121.D
Acq On : 25 Aug 2023 16:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 26 06:51:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 26 06:49:43 2023
Response via : Initial Calibration

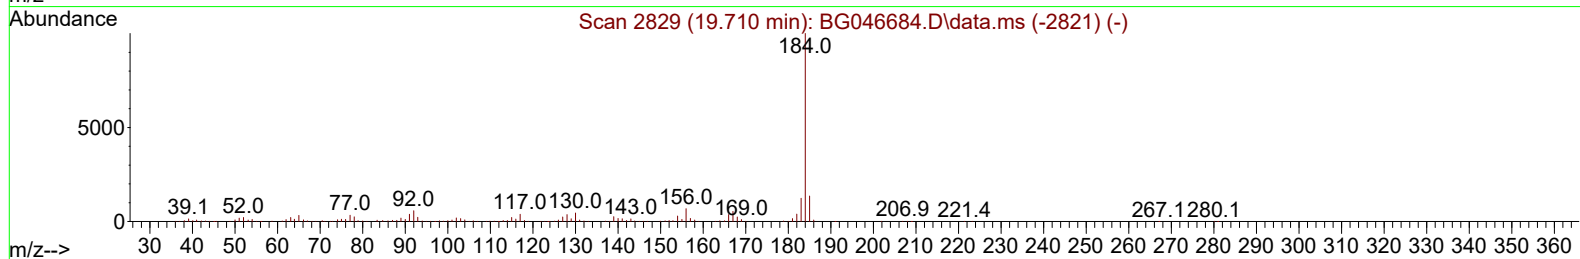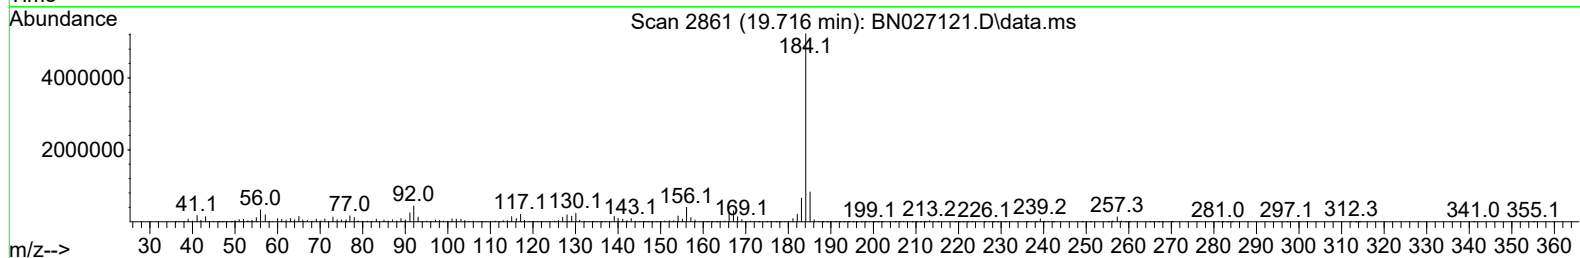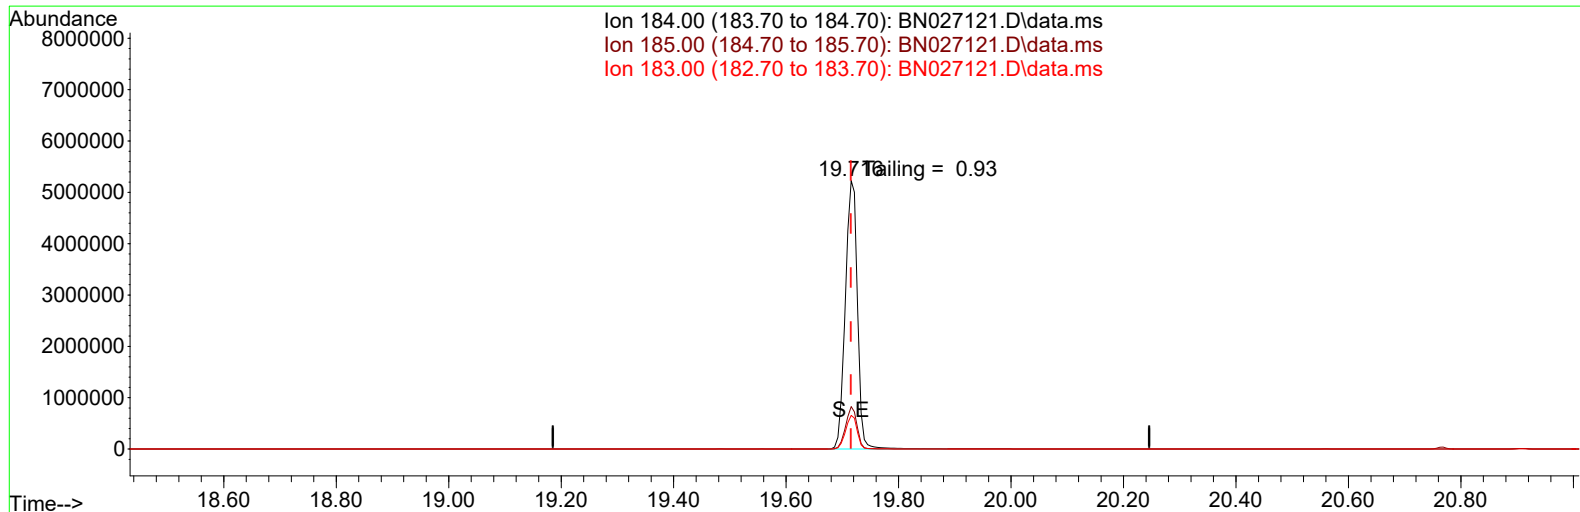

TIC: BN027121.D\data.ms

(77) Benzidine**19.716min (-0.000) 4380034.99 ng****response 7830940**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.83
183.00	13.20	12.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2023	BNA_N	<u>BN027121.D</u>
Compound Name	Response	Retention Time
DDT	3862224	20.91
DDD	56506	20.468
DDE	1236	19.957
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
57742	3919966	1.47

Instrument :
BNA_N
ClientSampleId :
DFTPP