
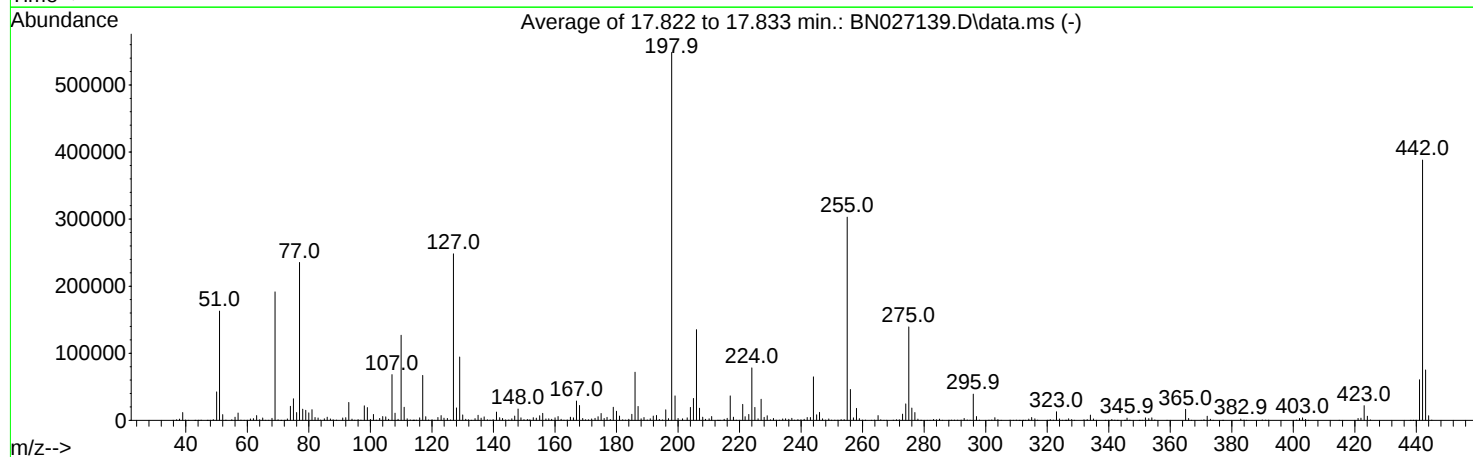


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
Data File : BN027139.D
Acq On : 26 Aug 2023 04:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Aug 26 02:13:59 2023

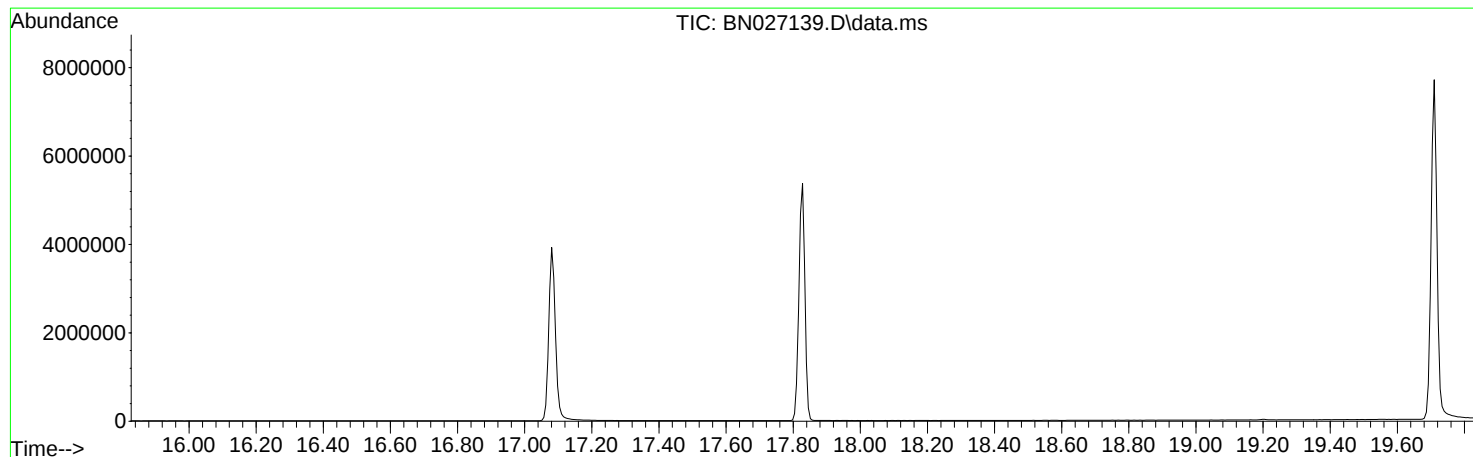




AutoFind: Scans 2539, 2540, 2541; Background Corrected with Scan 2531

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	162829	PASS
68	69	0.00	2	1.7	3203	PASS
69	198	0.00	100	34.9	191595	PASS
70	69	0.00	2	0.5	1007	PASS
127	198	10	80	45.3	248320	PASS
197	198	0.00	2	0.5	2579	PASS
198	198	100	100	100.0	548373	PASS
199	198	5	9	6.7	36555	PASS
275	198	10	60	25.4	139275	PASS
365	198	1	100	3.0	16471	PASS
441	198	0.01	100	11.1	60611	PASS
442	442	50	100	100.0	388181	PASS
443	442	15	24	19.3	75067	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
Data File : BN027139.D
Acq On : 26 Aug 2023 04:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 27 04:48:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 27 04:48:19 2023
Response via : Initial Calibration

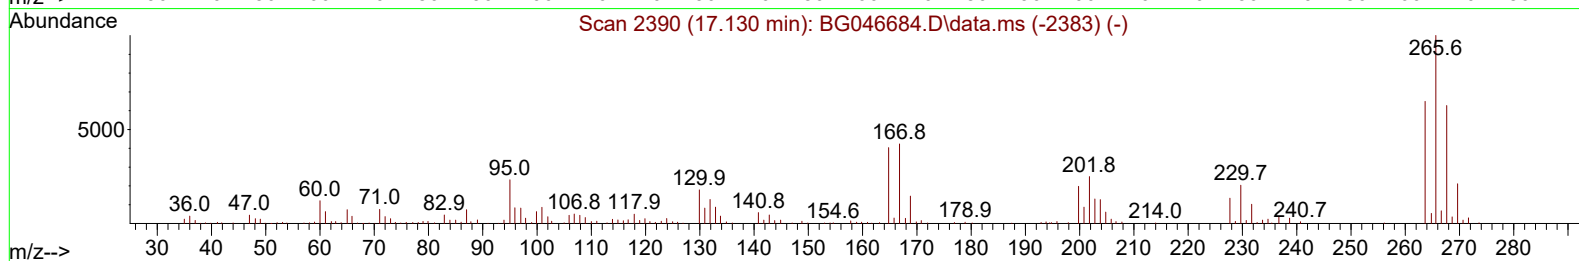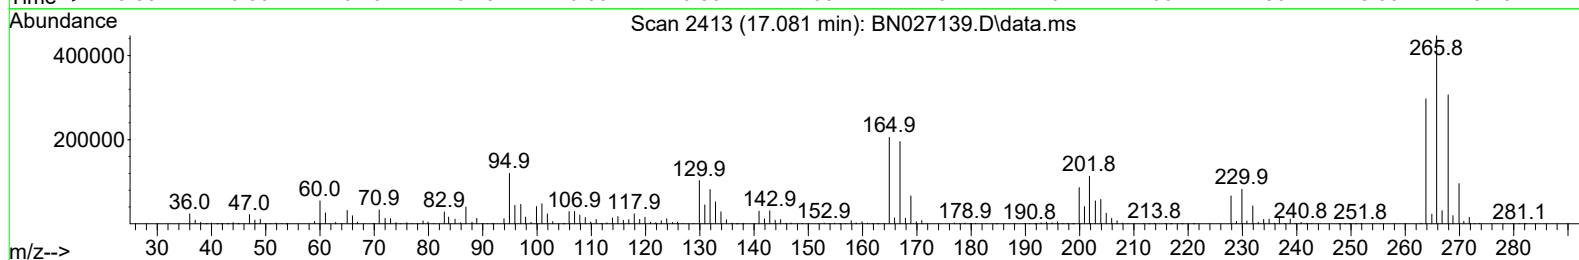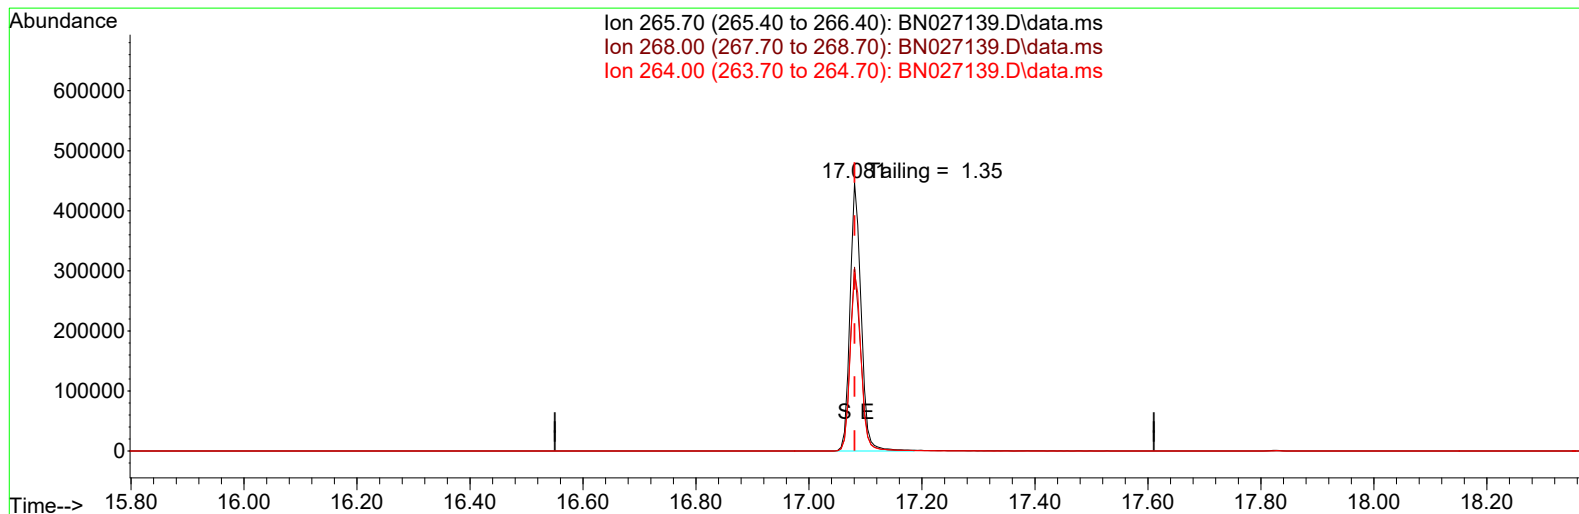

TIC: BN027139.D\data.ms

(70) Pentachlorophenol (C)

17.081min (0.000) 22851.79 ng




response 614940

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.53
264.00	61.60	66.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
 Data File : BN027139.D
 Acq On : 26 Aug 2023 04:22
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 27 04:48:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Aug 27 04:48:19 2023
 Response via : Initial Calibration

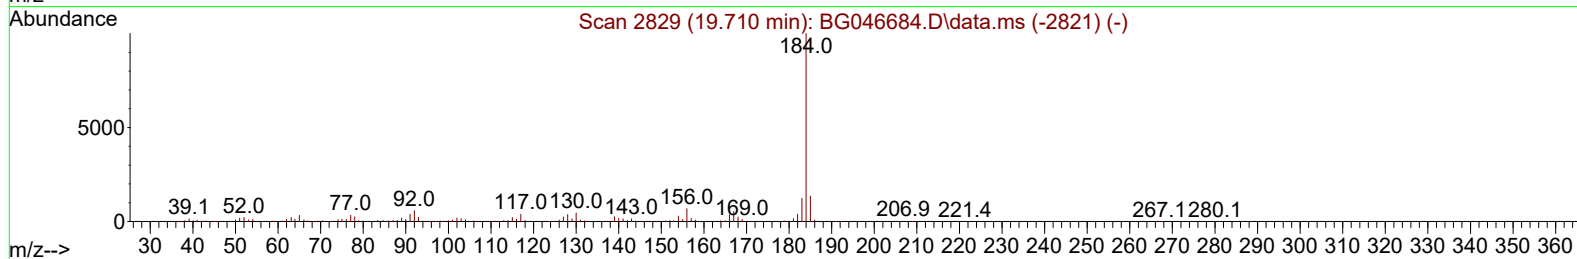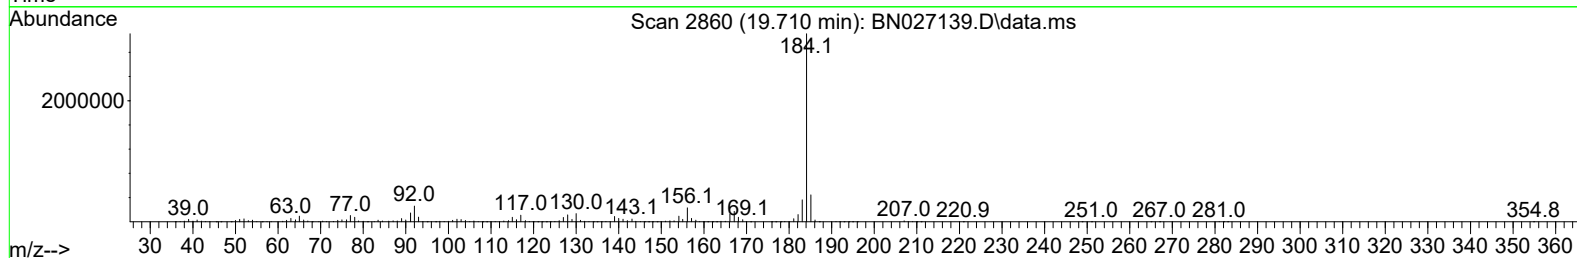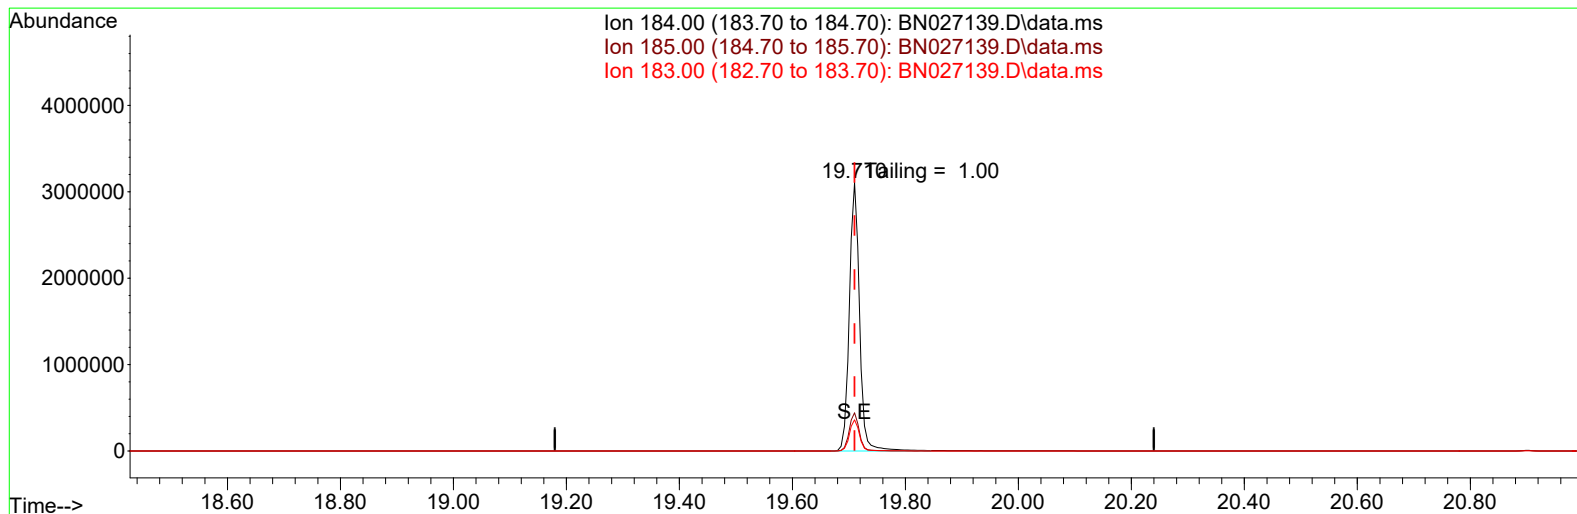

TIC: BN027139.D\data.ms

(77) Benzidine

19.710min (0.000) 0.00 ng

response 3928269

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.26
183.00	13.20	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2023	BNA_N	<u>BN027139.D</u>
Compound Name	Response	Retention Time
DDT	1906133	20.904
DDD	26914	20.463
DDE	929	19.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27843	1933976	1.44

Instrument :
BNA_N
ClientSampleId :
DFTPP