
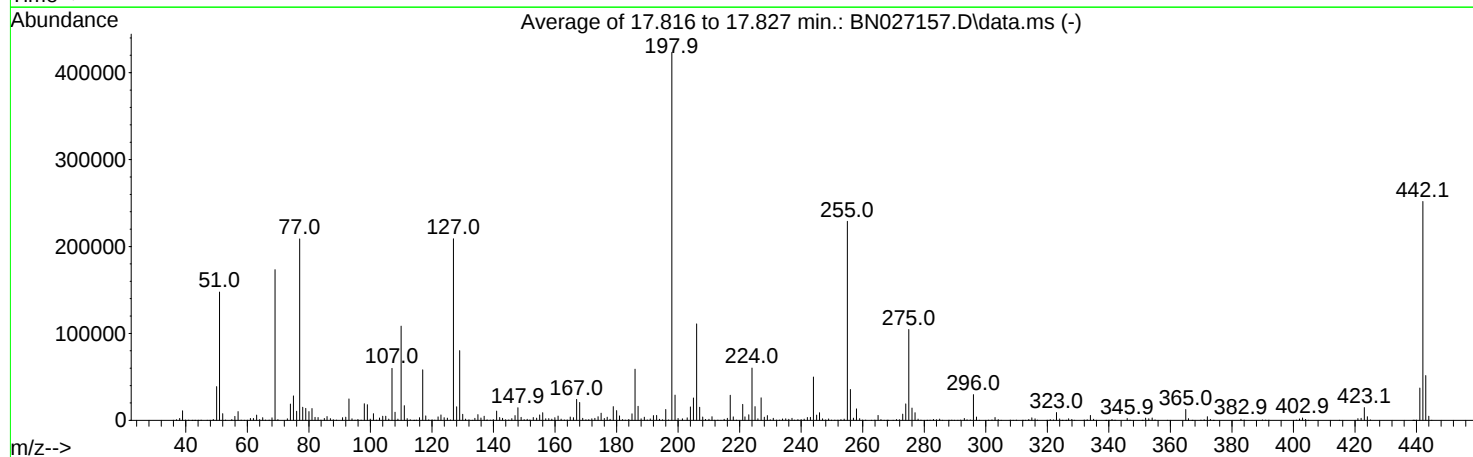


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
 Data File : BN027157.D
 Acq On : 26 Aug 2023 16:36
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 26 02:13:59 2023

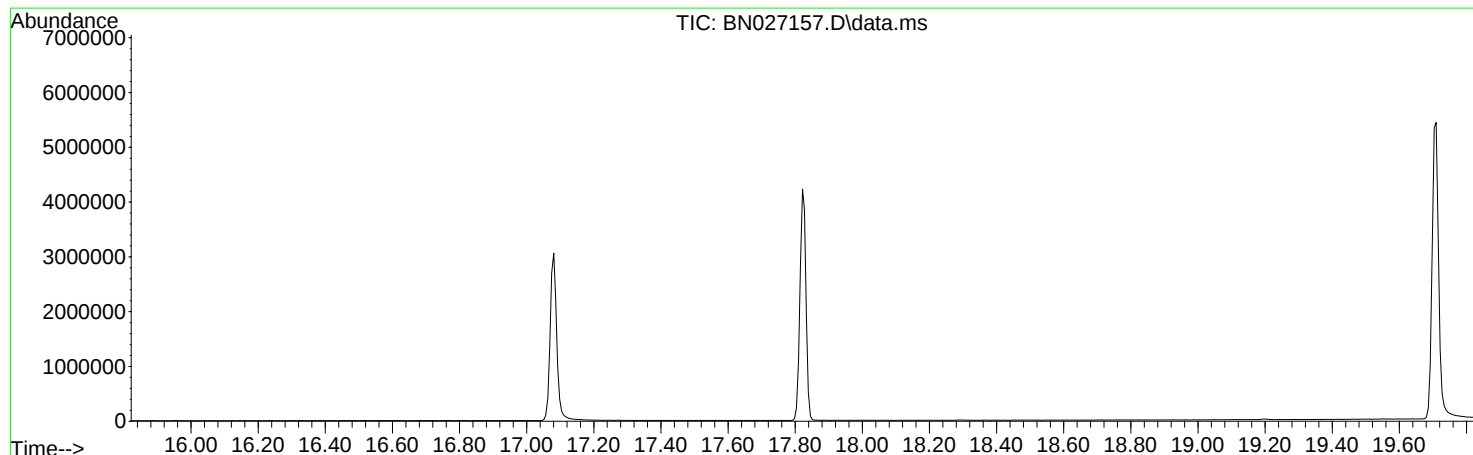




AutoFind: Scans 2538, 2539, 2540; Background Corrected with Scan 2531

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	147608	PASS
68	69	0.00	2	1.7	2940	PASS
69	198	0.00	100	41.0	173440	PASS
70	69	0.00	2	0.5	952	PASS
127	198	10	80	49.4	208875	PASS
197	198	0.00	2	0.1	534	PASS
198	198	100	100	100.0	423211	PASS
199	198	5	9	6.9	29032	PASS
275	198	10	60	24.7	104515	PASS
365	198	1	100	2.9	12441	PASS
441	198	0.01	100	8.8	37141	PASS
442	442	50	100	100.0	251883	PASS
443	442	15	24	20.5	51635	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
 Data File : BN027157.D
 Acq On : 26 Aug 2023 16:36
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 27 04:49:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Aug 27 04:48:19 2023
 Response via : Initial Calibration

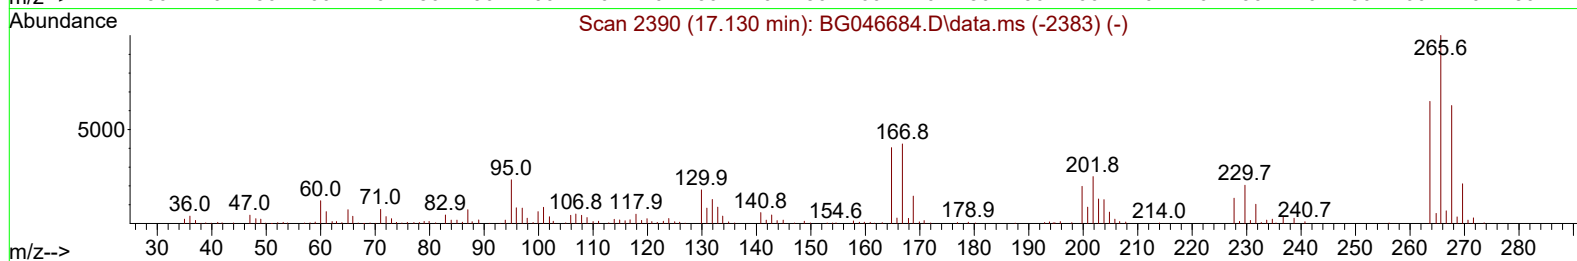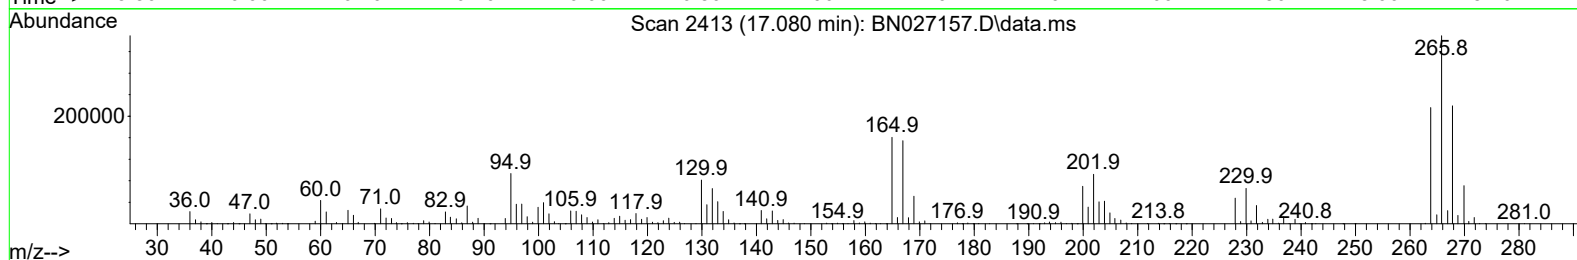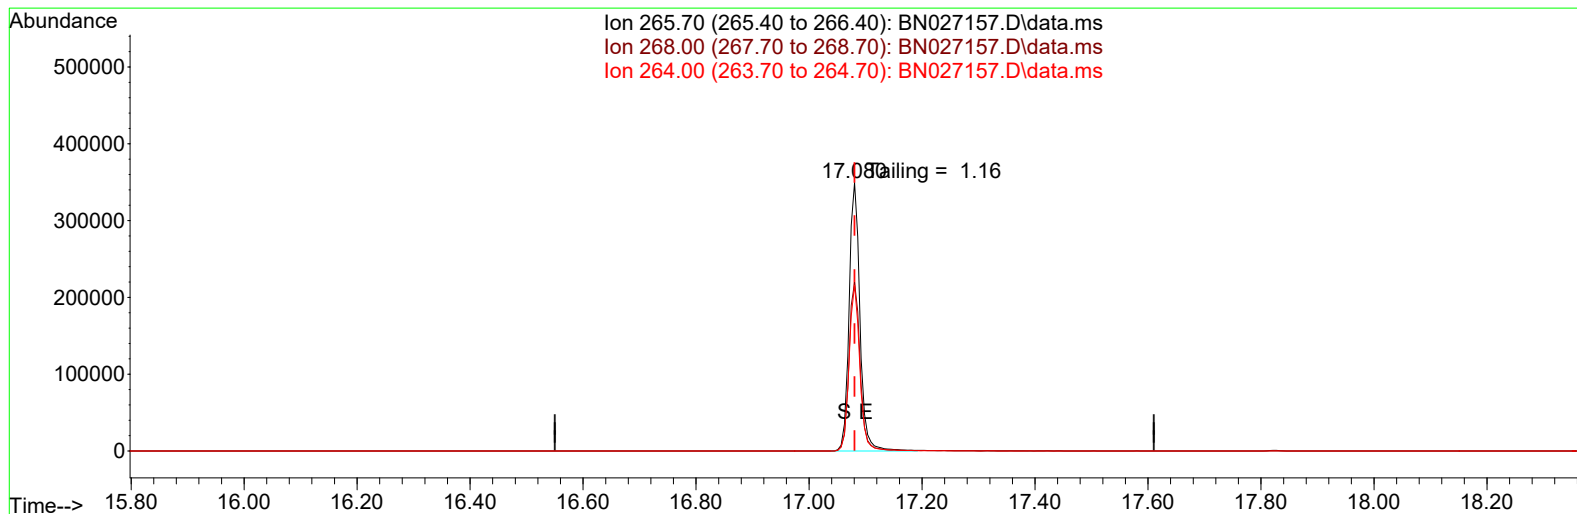

TIC: BN027157.D\data.ms

(70) Pentachlorophenol (C)

17.080min (-0.000) 22025.85 ng




response 468951

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.78
264.00	61.60	61.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
Data File : BN027157.D
Acq On : 26 Aug 2023 16:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 27 04:49:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 27 04:48:19 2023
Response via : Initial Calibration

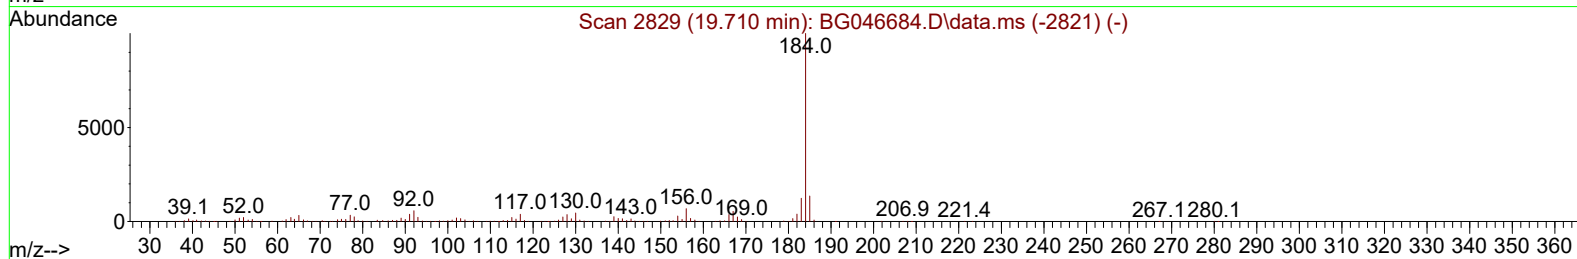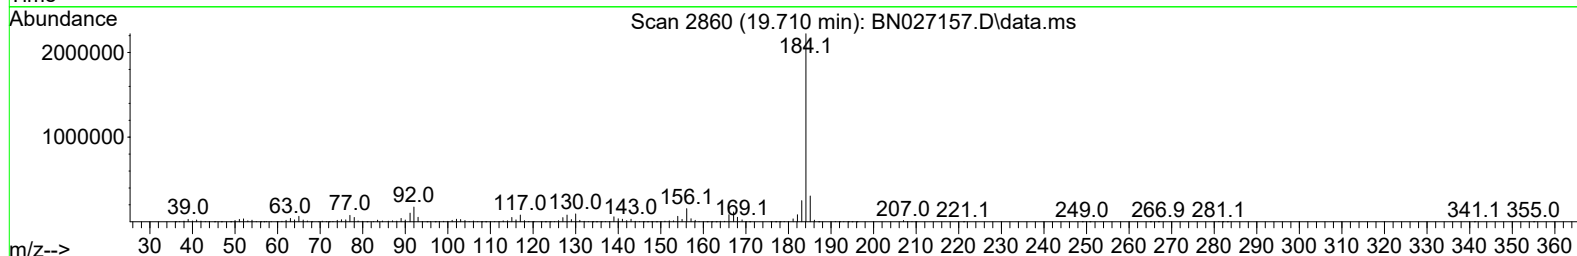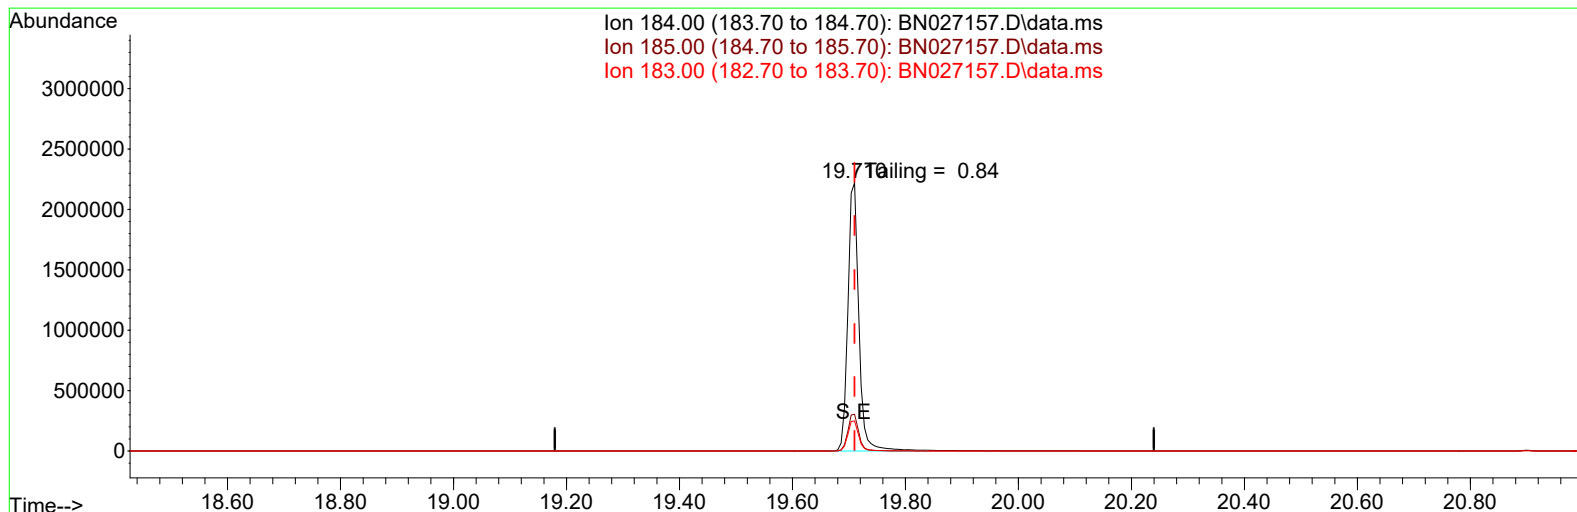

TIC: BN027157.D\data.ms

(77) Benzidine

19.710min (-0.000) 0.00 ng

response 3014282

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.73
183.00	13.20	11.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2023	BNA_N	<u>BN027157.D</u>
Compound Name	Response	Retention Time
DDT	1469122	20.904
DDD	19330	20.463
DDE	1006	19.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20336	1489458	1.37

Instrument :
BNA_N
ClientSampleId :
DFTPP