


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
 Data File : BN027175.D
 Acq On : 27 Aug 2023 04:54
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 26 02:13:59 2023

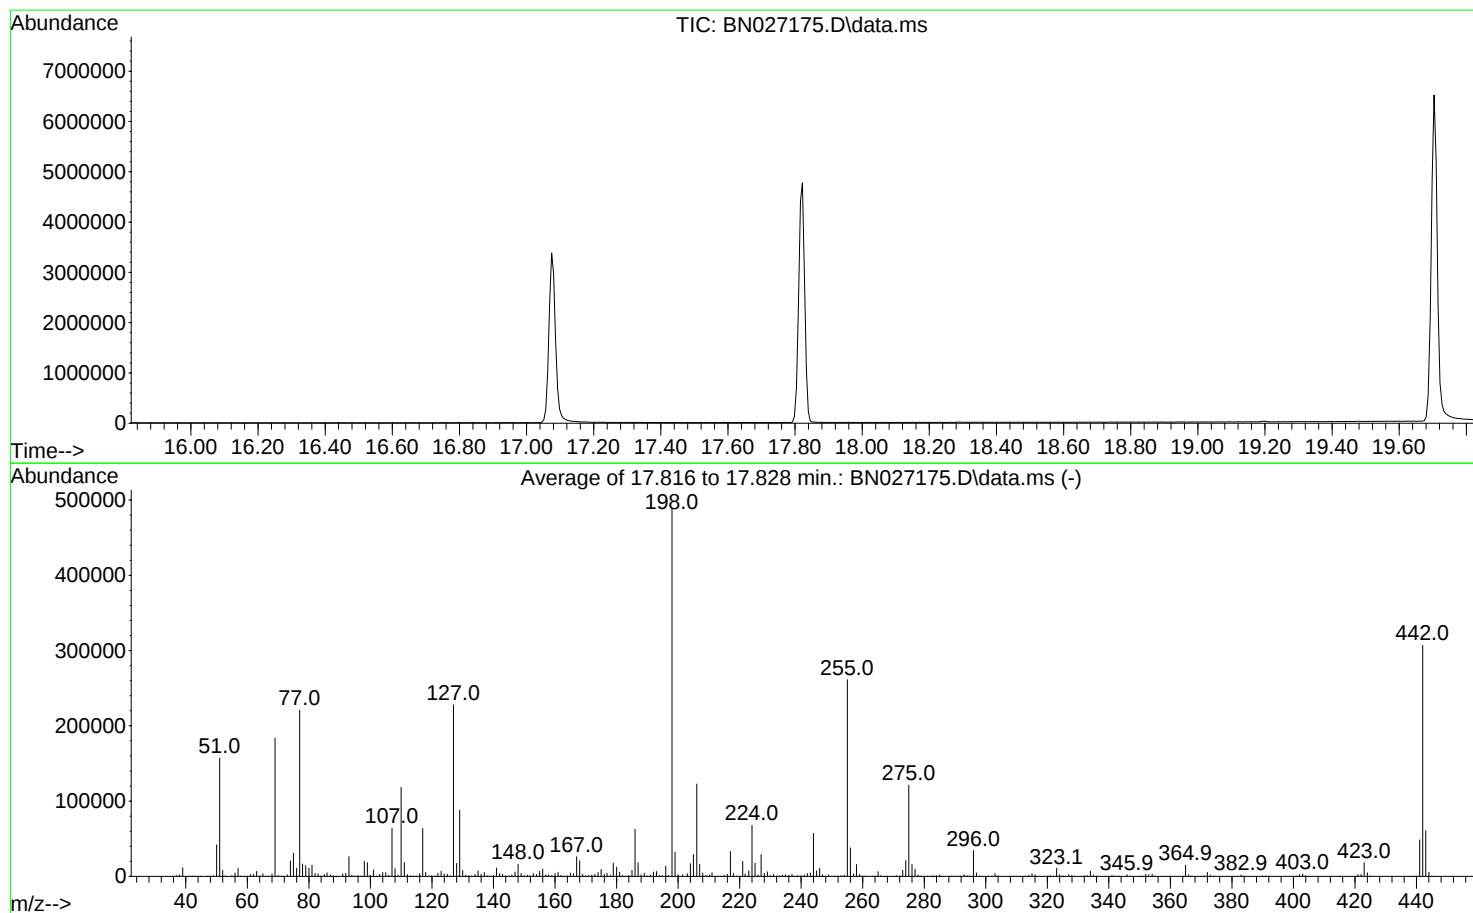




AutoFind: Scans 2538, 2539, 2540; Background Corrected with Scan 2531

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	157088	PASS
68	69	0.00	2	1.7	3119	PASS
69	198	0.00	100	37.6	183779	PASS
70	69	0.00	2	0.5	1001	PASS
127	198	10	80	46.6	228011	PASS
197	198	0.00	2	0.2	838	PASS
198	198	100	100	100.0	488811	PASS
199	198	5	9	6.6	32067	PASS
275	198	10	60	24.8	121280	PASS
365	198	1	100	3.0	14732	PASS
441	198	0.01	100	9.9	48424	PASS
442	442	50	100	100.0	307051	PASS
443	442	15	24	19.8	60701	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
Data File : BN027175.D
Acq On : 27 Aug 2023 04:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 27 05:28:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 27 05:28:54 2023
Response via : Initial Calibration

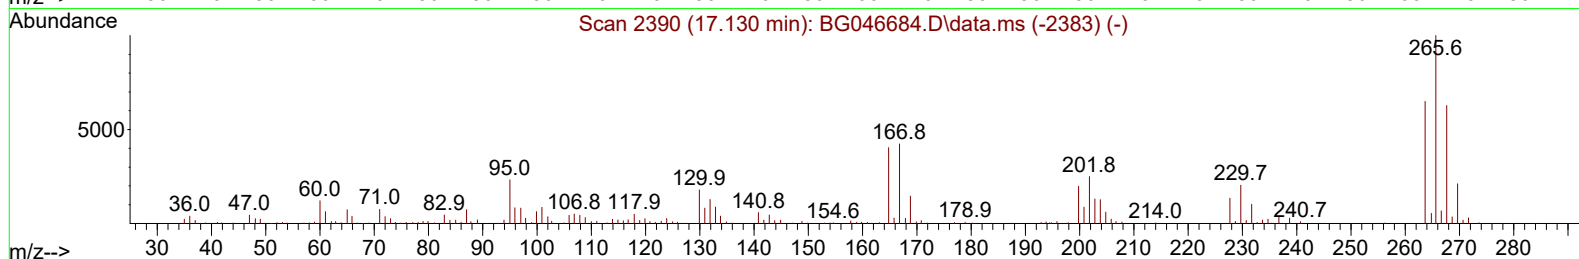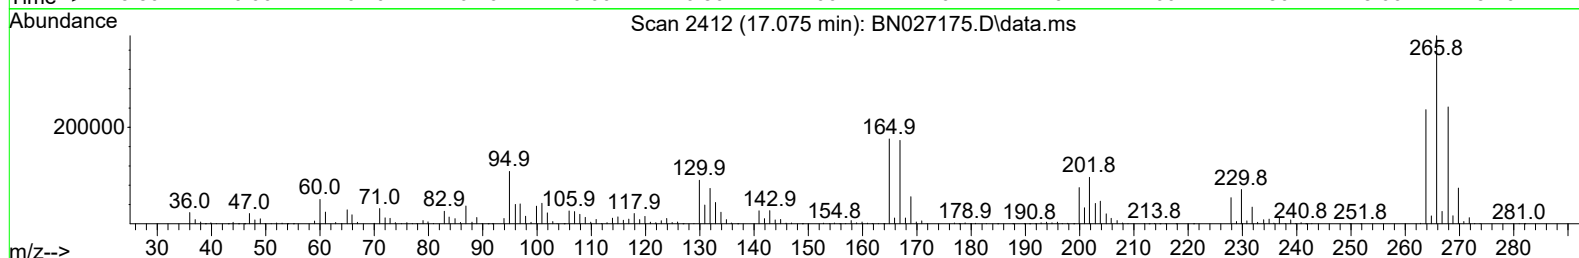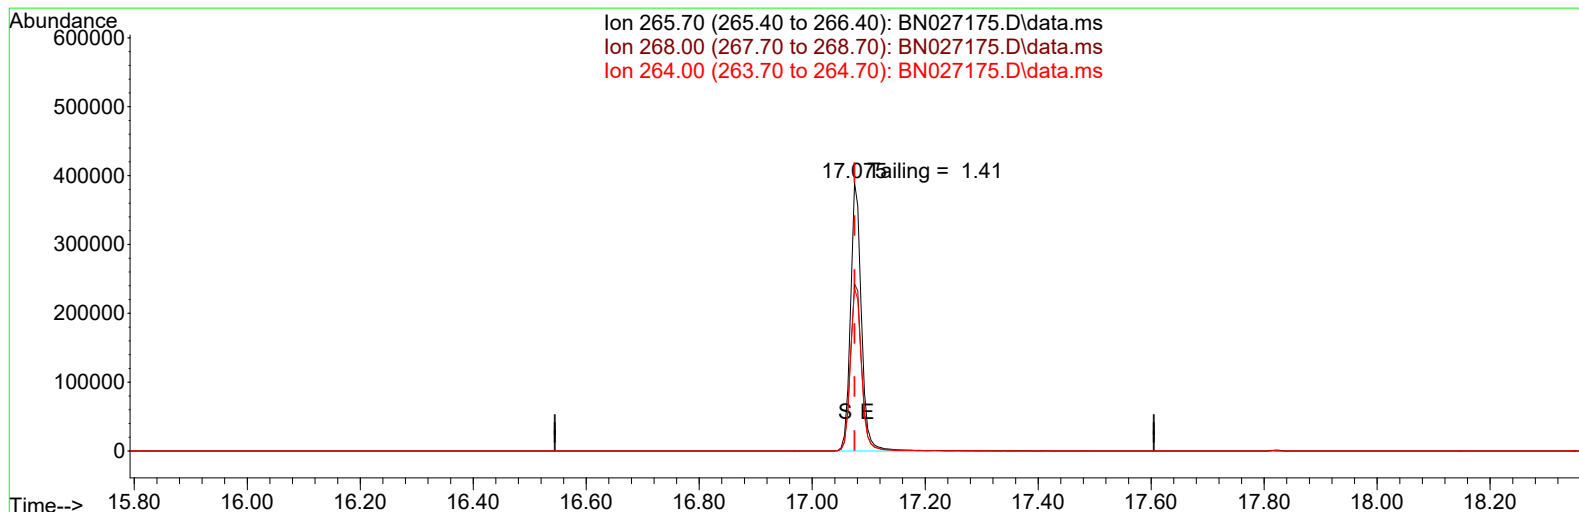

TIC: BN027175.D\data.ms

(70) Pentachlorophenol (C)

17.075min (0.000) 22288.92 ng




response 523879

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.18
264.00	61.60	60.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
Data File : BN027175.D
Acq On : 27 Aug 2023 04:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 27 05:28:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 27 05:28:54 2023
Response via : Initial Calibration

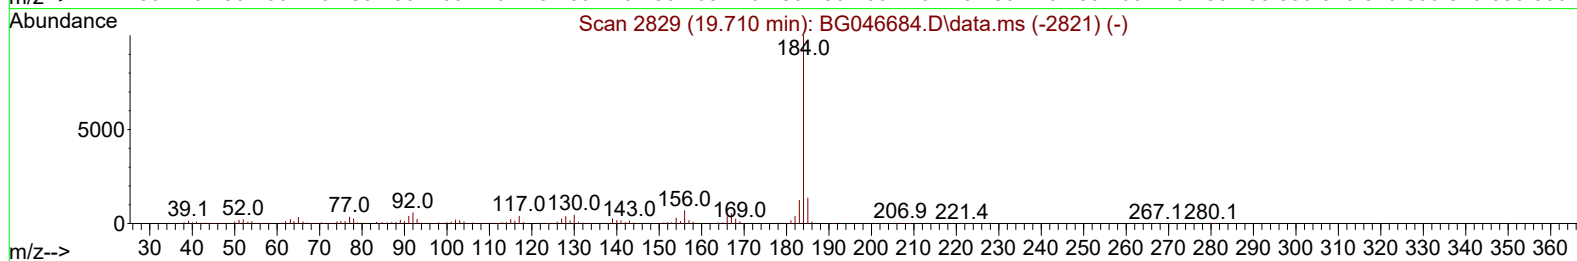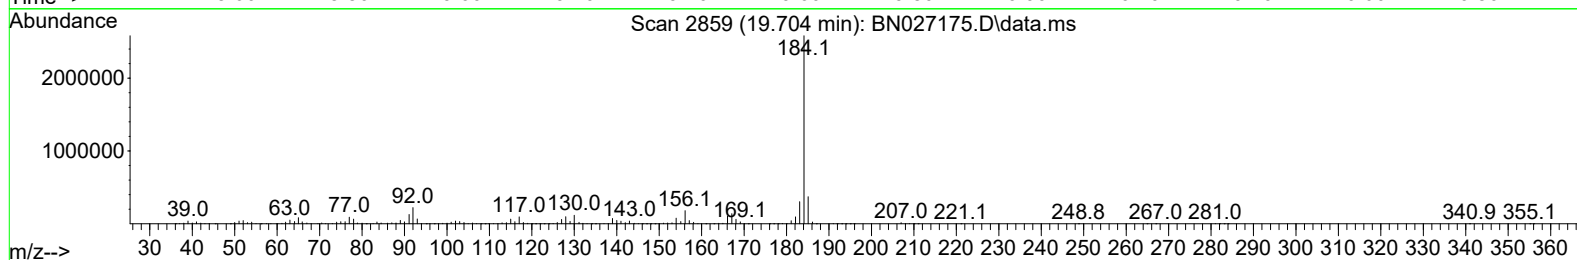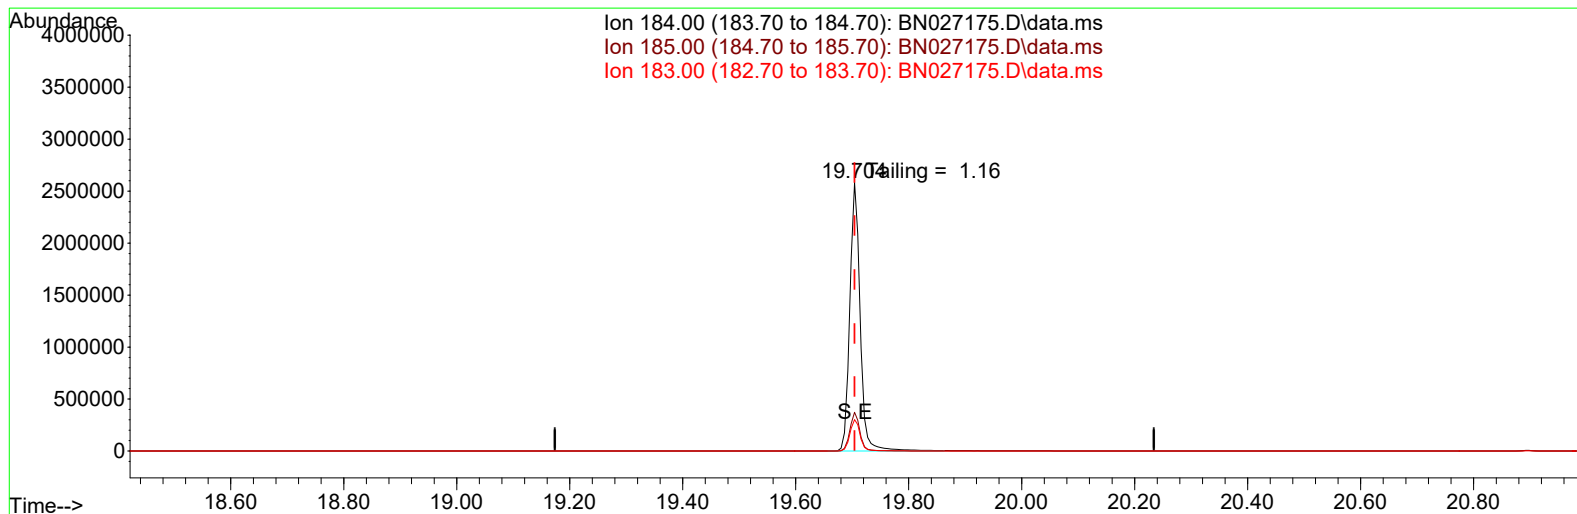

TIC: BN027175.D\data.ms

(77) Benzidine

19.704min (0.000) 0.00 ng

response 3320388

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.42
183.00	13.20	11.73
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2023	BNA_N	<u>BN027175.D</u>
Compound Name	Response	Retention Time
DDT	1657131	20.898
DDD	21046	20.457
DDE	910	19.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21956	1679087	1.31

Instrument :
BNA_N
ClientSampleId :
DFTPP