
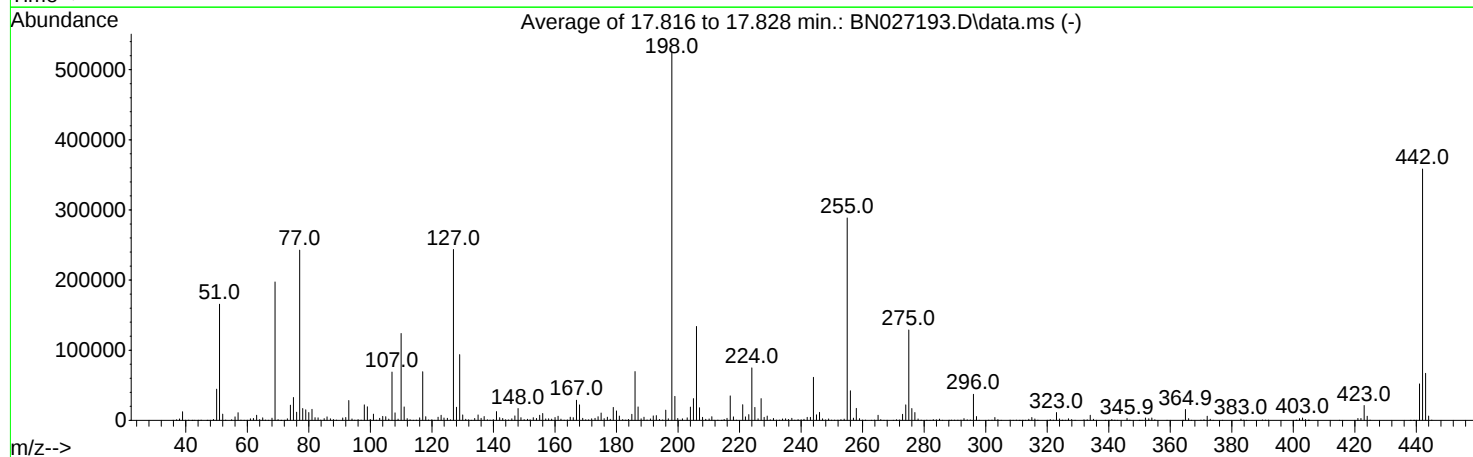


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
 Data File : BN027193.D
 Acq On : 27 Aug 2023 17:02
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 26 02:13:59 2023

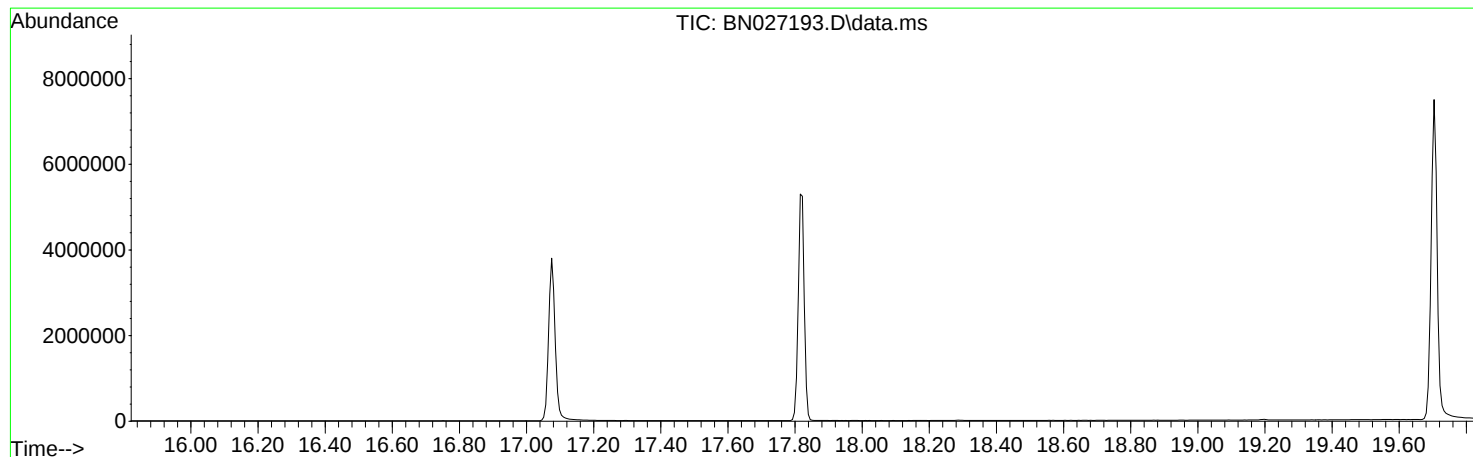




AutoFind: Scans 2538, 2539, 2540; Background Corrected with Scan 2530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	165610	PASS
68	69	0.00	2	1.7	3281	PASS
69	198	0.00	100	37.6	197264	PASS
70	69	0.00	2	0.6	1160	PASS
127	198	10	80	46.5	243691	PASS
197	198	0.00	2	0.5	2388	PASS
198	198	100	100	100.0	524480	PASS
199	198	5	9	6.5	34347	PASS
275	198	10	60	24.6	128904	PASS
365	198	1	100	3.0	15478	PASS
441	198	0.01	100	9.9	52117	PASS
442	442	50	100	100.0	358443	PASS
443	442	15	24	18.7	66984	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
 Data File : BN027193.D
 Acq On : 27 Aug 2023 17:02
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 28 01:21:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 28 01:21:07 2023
 Response via : Initial Calibration

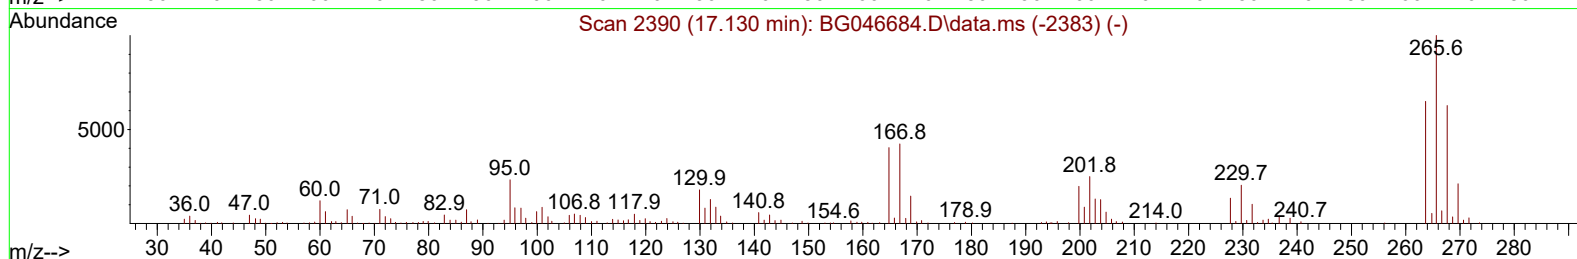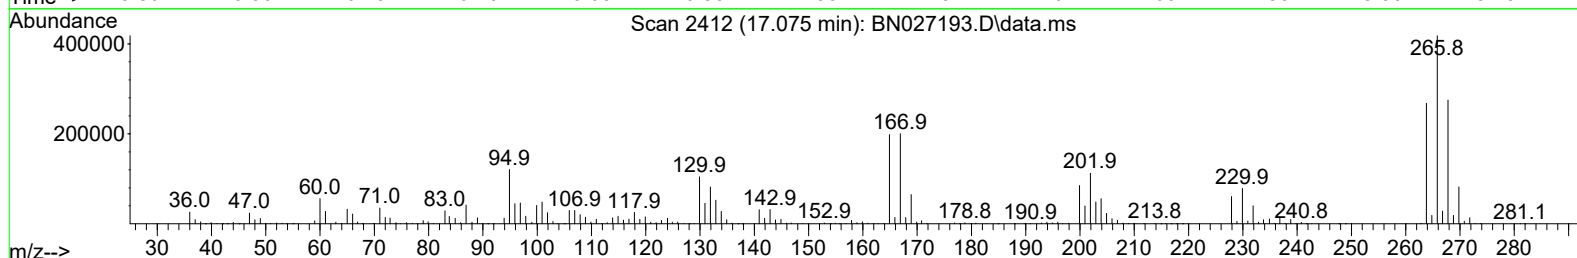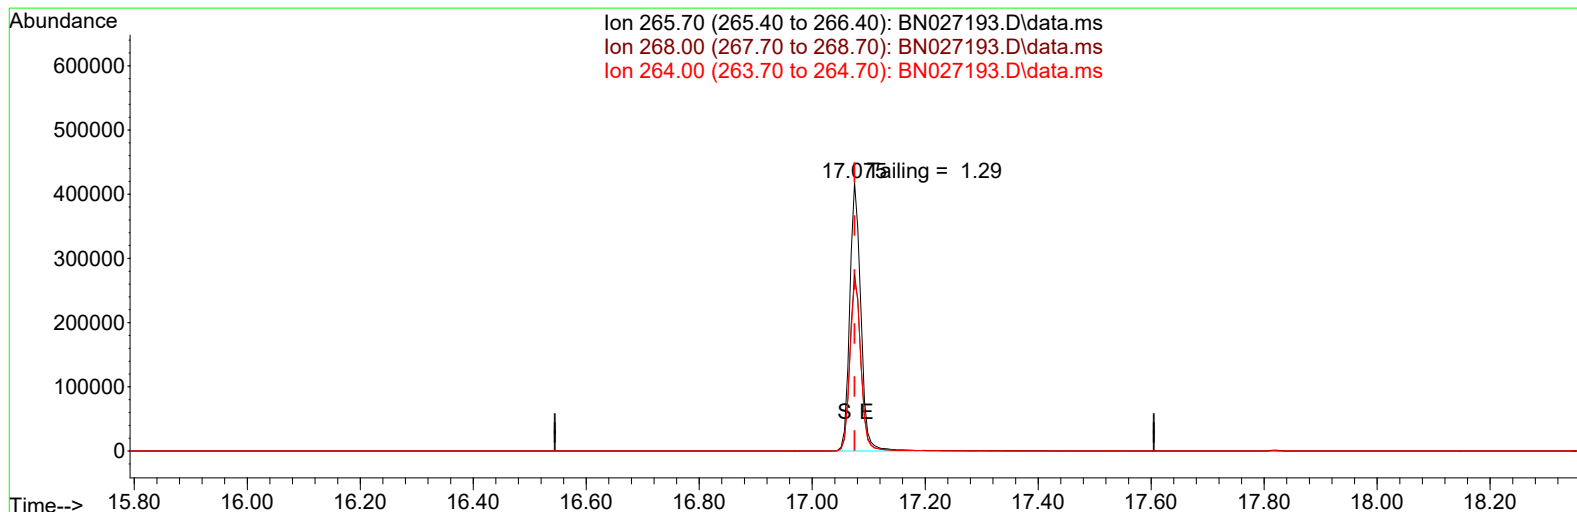

TIC: BN027193.D\data.ms

(70) Pentachlorophenol (C)

17.075min (0.000) 20760.76 ng




response 570727

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.80
264.00	61.60	64.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082523\
Data File : BN027193.D
Acq On : 27 Aug 2023 17:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 28 01:21:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 01:21:07 2023
Response via : Initial Calibration

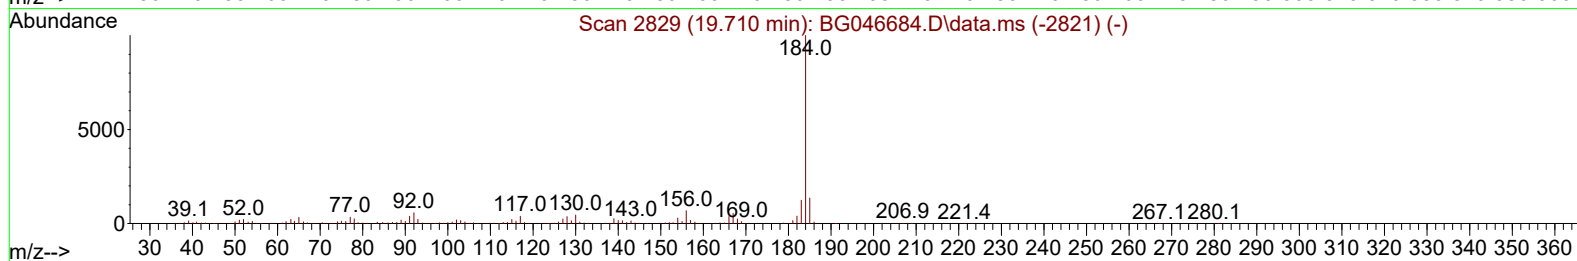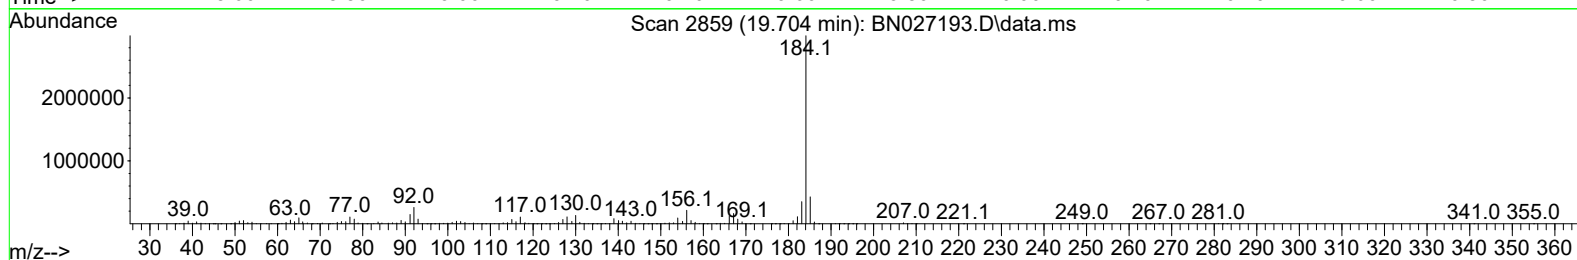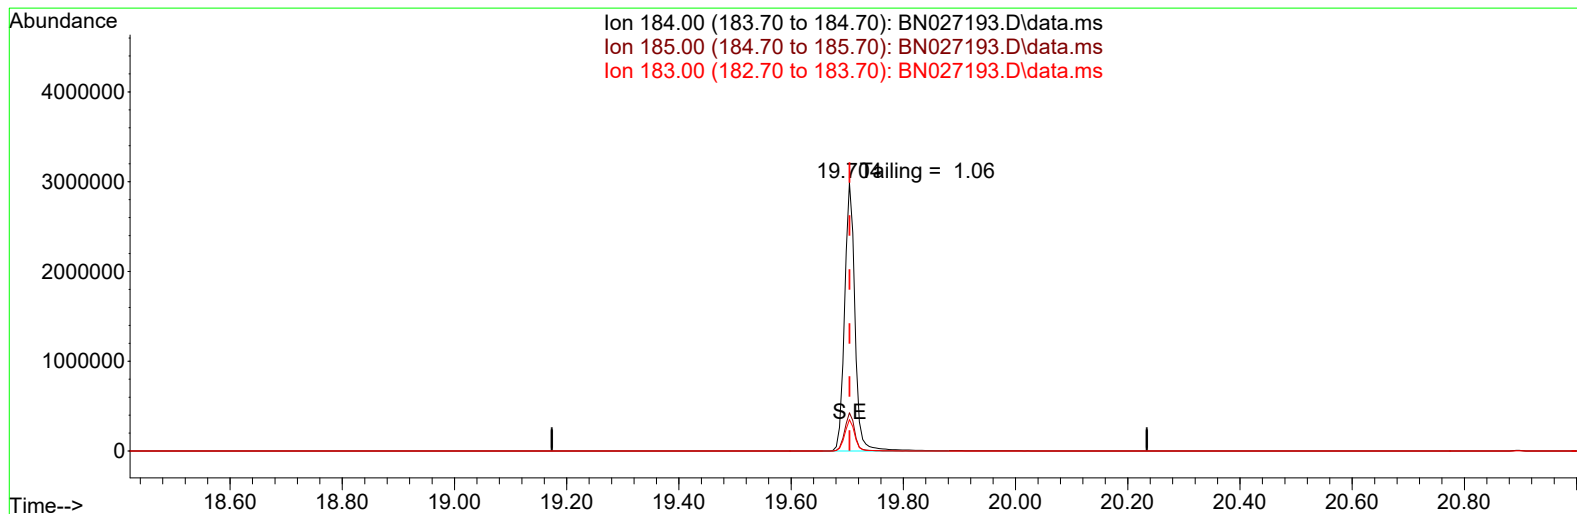

TIC: BN027193.D\data.ms

(77) Benzidine

19.704min (0.000) 0.00 ng

response 3850520

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	11.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2023	BNA_N	<u>BN027193.D</u>
Compound Name	Response	Retention Time
DDT	1851682	20.898
DDD	25829	20.457
DDE	1231	19.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27060	1878742	1.44

Instrument :
BNA_N
ClientSampleId :
DFTPP