


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082619\
 Data File : BN007411.D
 Acq On : 26 Aug 2019 16:01
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 24 00:38:17 2019

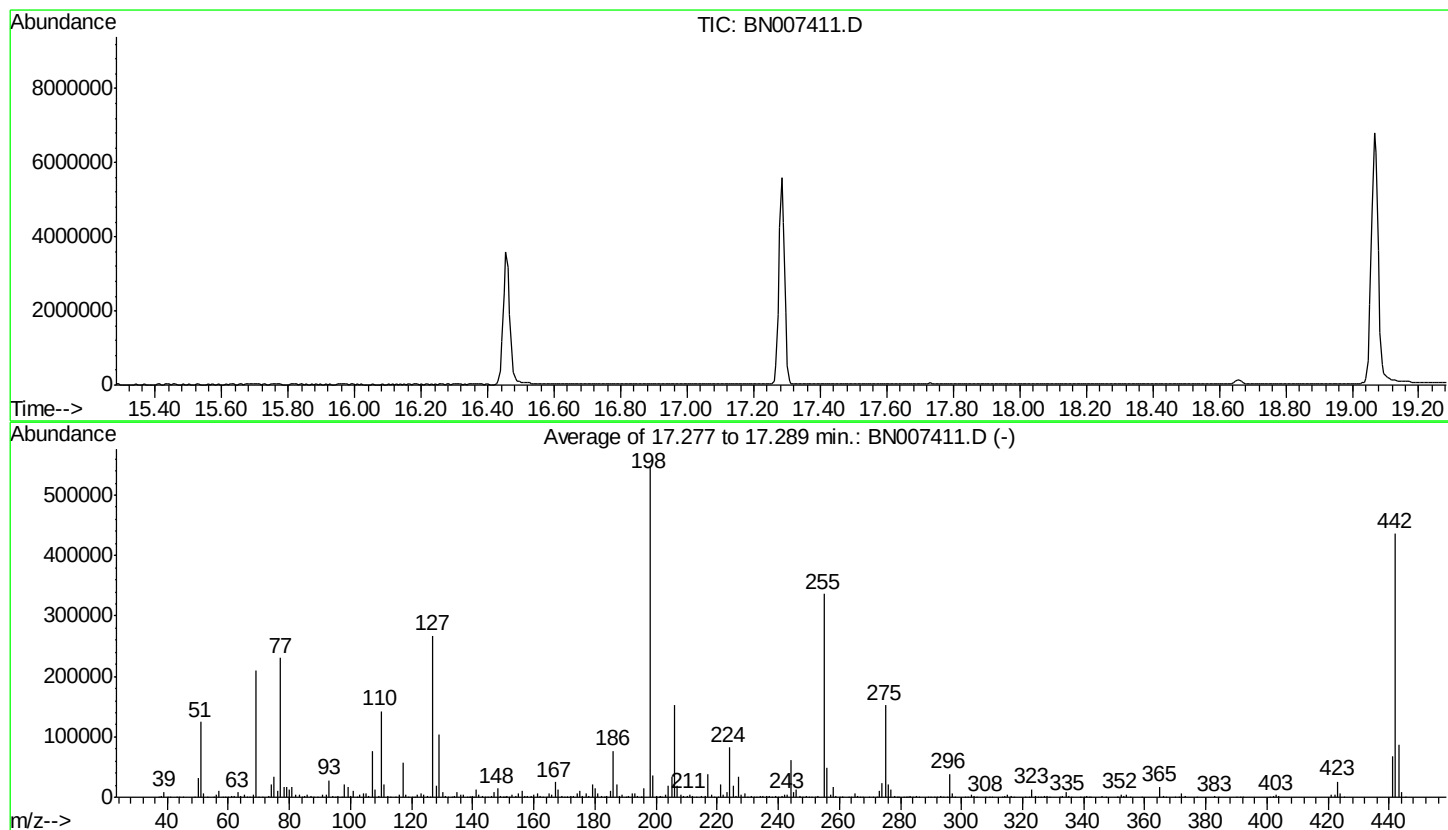

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.6	124192	PASS
68	69	0.00	2	1.7	3473	PASS
69	198	0.00	100	38.2	209752	PASS
70	69	0.00	2	0.5	1008	PASS
127	198	10	80	48.8	267776	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	548821	PASS
199	198	5	9	6.7	37021	PASS
275	198	10	60	27.8	152440	PASS
365	198	1	100	3.2	17731	PASS
441	198	0.01	100	12.3	67637	PASS
442	198	50	100	79.4	435690	PASS
443	442	15	24	19.7	85989	PASS