
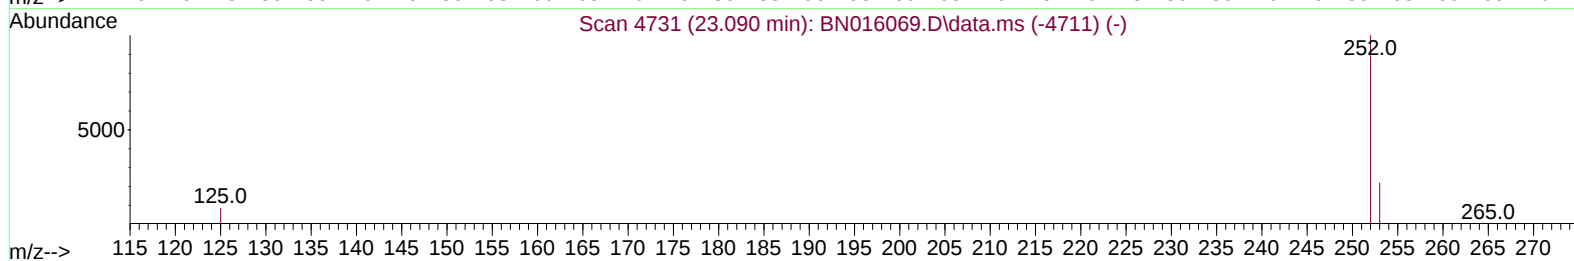
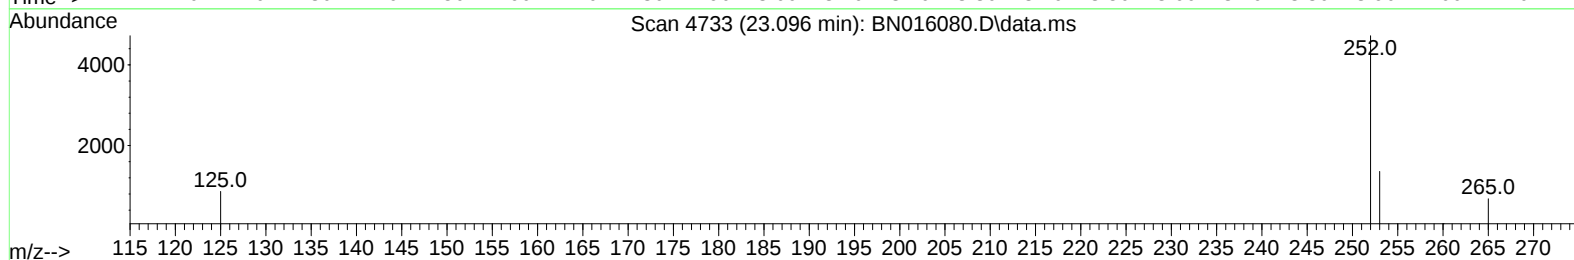


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082621\
Data File : BN016080.D
Acq On : 26 Aug 2021 21:31
Operator : CG/JU
Sample : M3458-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Sep 03 09:27:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 27 10:53:37 2021
Response via : Initial Calibration

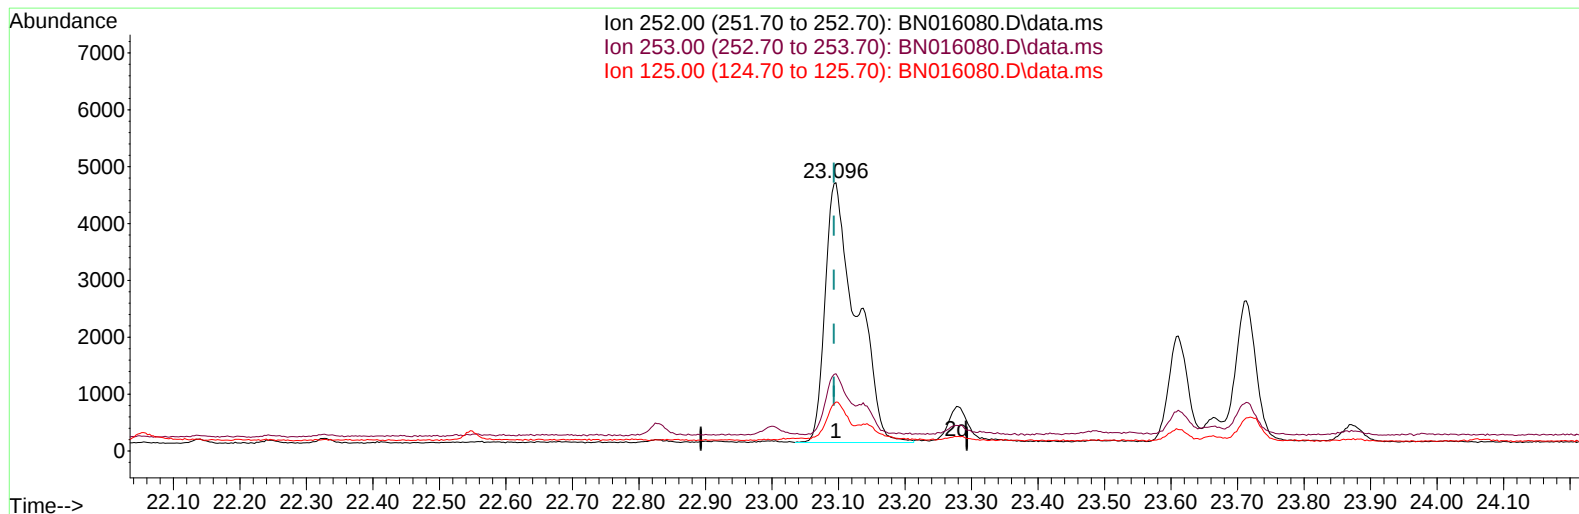

TIC: BN016080.D\data.ms

(24) Benzo(b)fluoranthene

23.096min (+ 0.003) 0.58 ng/u1

response 14841

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.30	28.83
125.00	10.80	18.26
0.00	0.00	0.00