
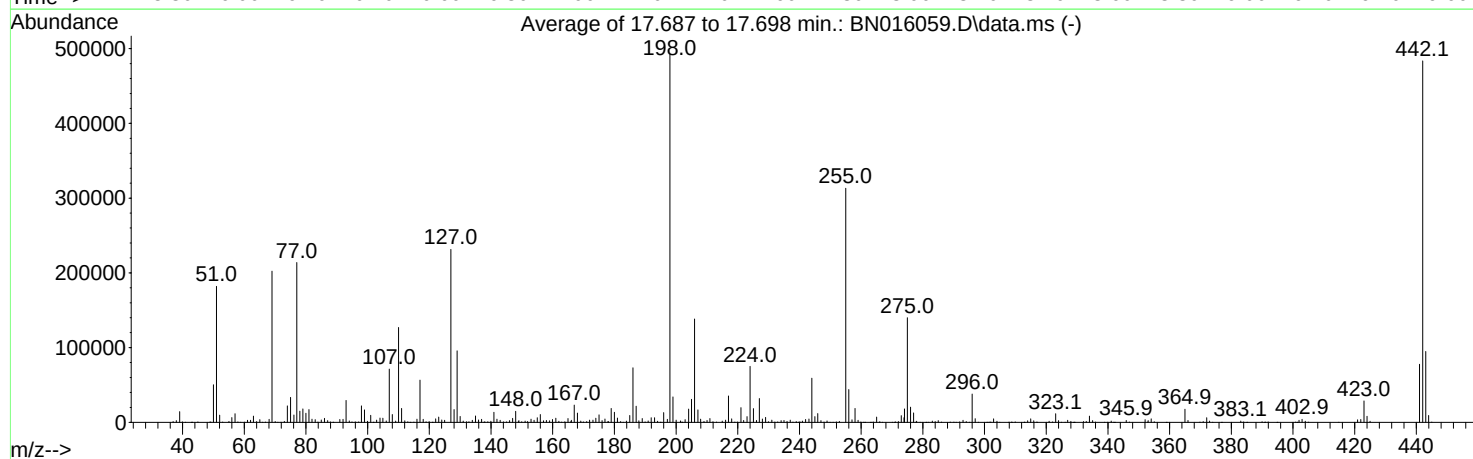


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082621\
 Data File : BN016059.D
 Acq On : 25 Aug 2021 15:29
 Operator : CG/JU
 Sample : DFTPP201
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 27 10:53:37 2021

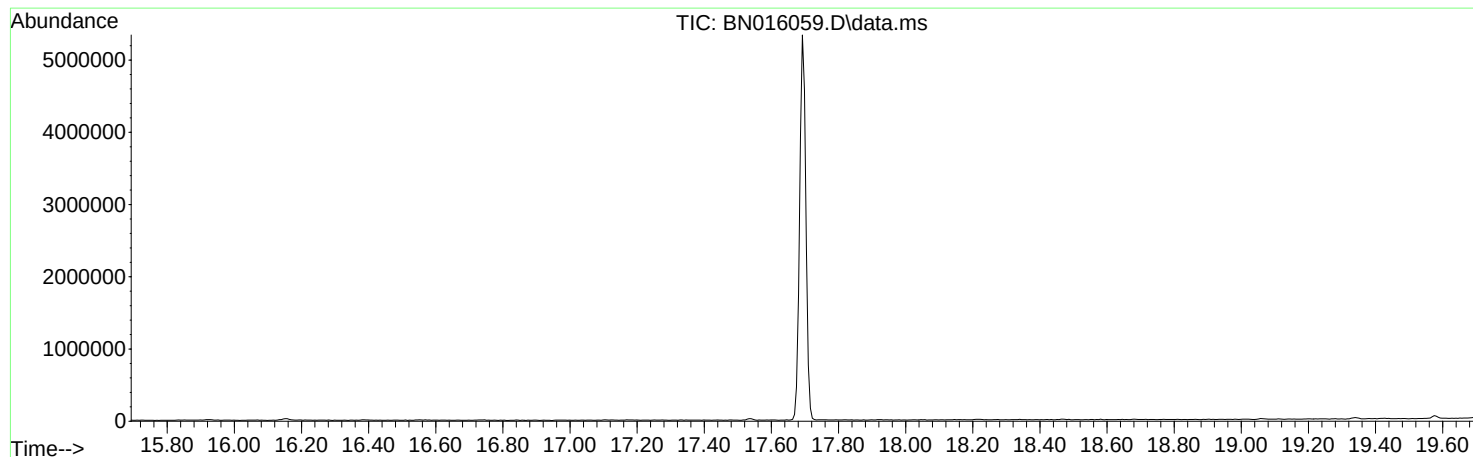

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	182016	PASS
68	69	0.00	2	2.0	4005	PASS
69	198	0.00	100	41.1	202315	PASS
70	69	0.00	2	0.5	1076	PASS
127	198	10	80	47.0	231424	PASS
197	198	0.00	2	0.8	3968	PASS
198	198	100	100	100.0	492160	PASS
199	198	5	9	6.9	34149	PASS
275	198	10	60	28.5	140048	PASS
365	198	1	100	3.6	17656	PASS
441	198	0.01	100	15.8	77643	PASS
442	198	50	100	98.3	483563	PASS
443	442	15	24	19.6	94832	PASS