
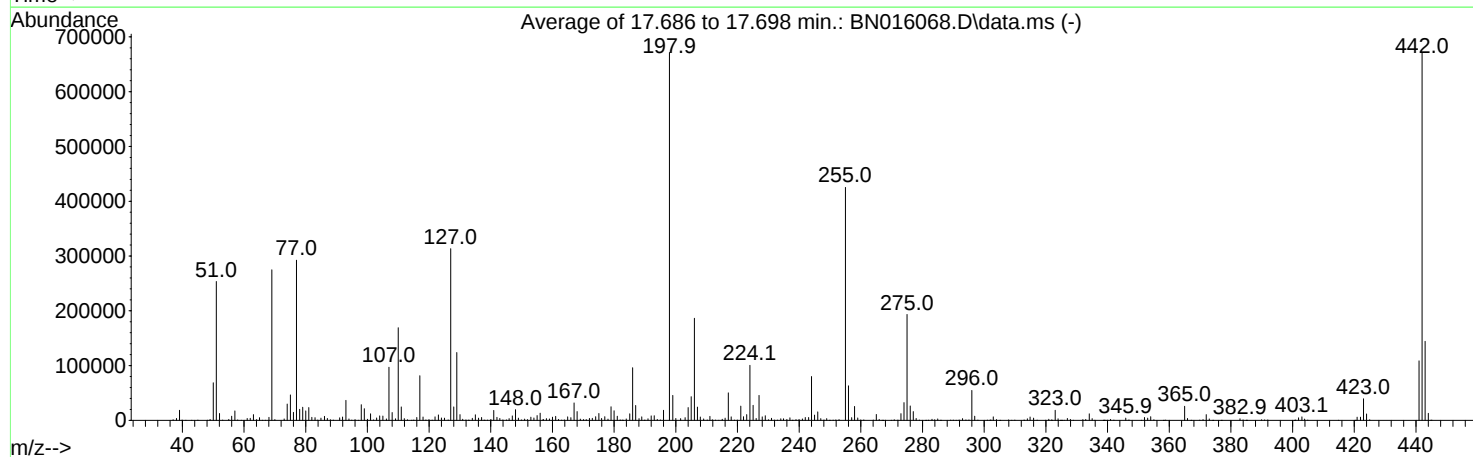


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082621\
 Data File : BN016068.D
 Acq On : 26 Aug 2021 09:04
 Operator : CG/JU
 Sample : DFTPP202
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 27 10:53:37 2021

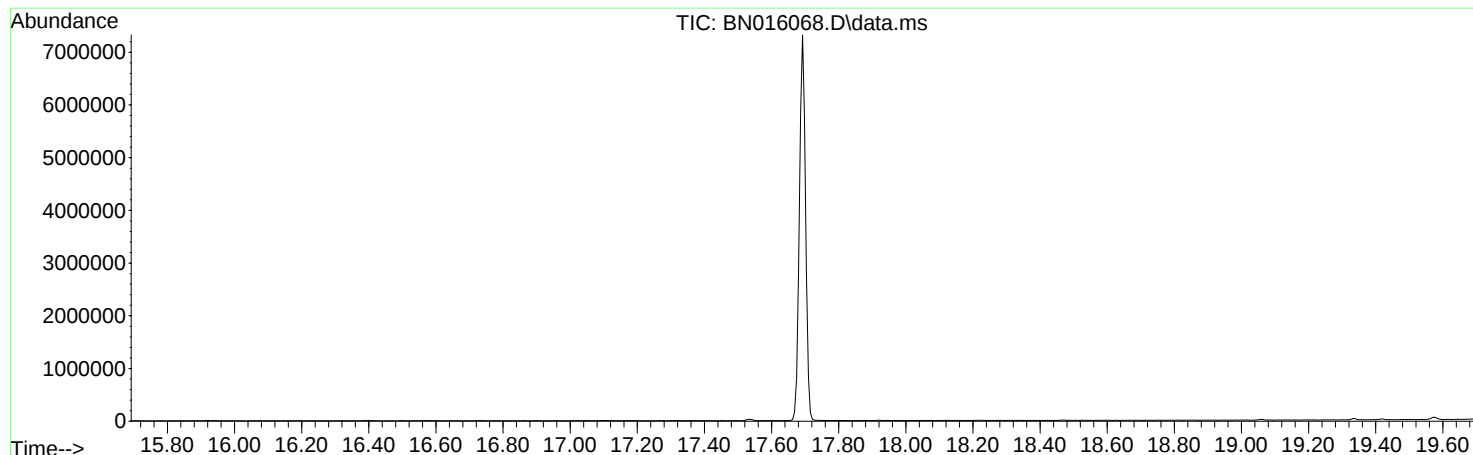

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	253560	PASS
68	69	0.00	2	2.0	5470	PASS
69	198	0.00	100	40.9	274731	PASS
70	69	0.00	2	0.6	1583	PASS
127	198	10	80	46.7	313323	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	671531	PASS
199	198	5	9	6.8	45672	PASS
275	198	10	60	28.8	193280	PASS
365	198	1	100	3.8	25789	PASS
441	198	0.01	100	16.2	108608	PASS
442	198	50	100	99.9	670677	PASS
443	442	15	24	21.5	144421	PASS