


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082621\
Data File : BN016079.D
Acq On : 26 Aug 2021 20:54
Operator : CG/JU
Sample : M3458-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AT7

Manual Integrations
APPROVED

mohammad
8/27/2021 5:09:56 PM

Quant Time: Aug 27 03:30:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Thu Aug 26 11:35:43 2021
Response via : Initial Calibration

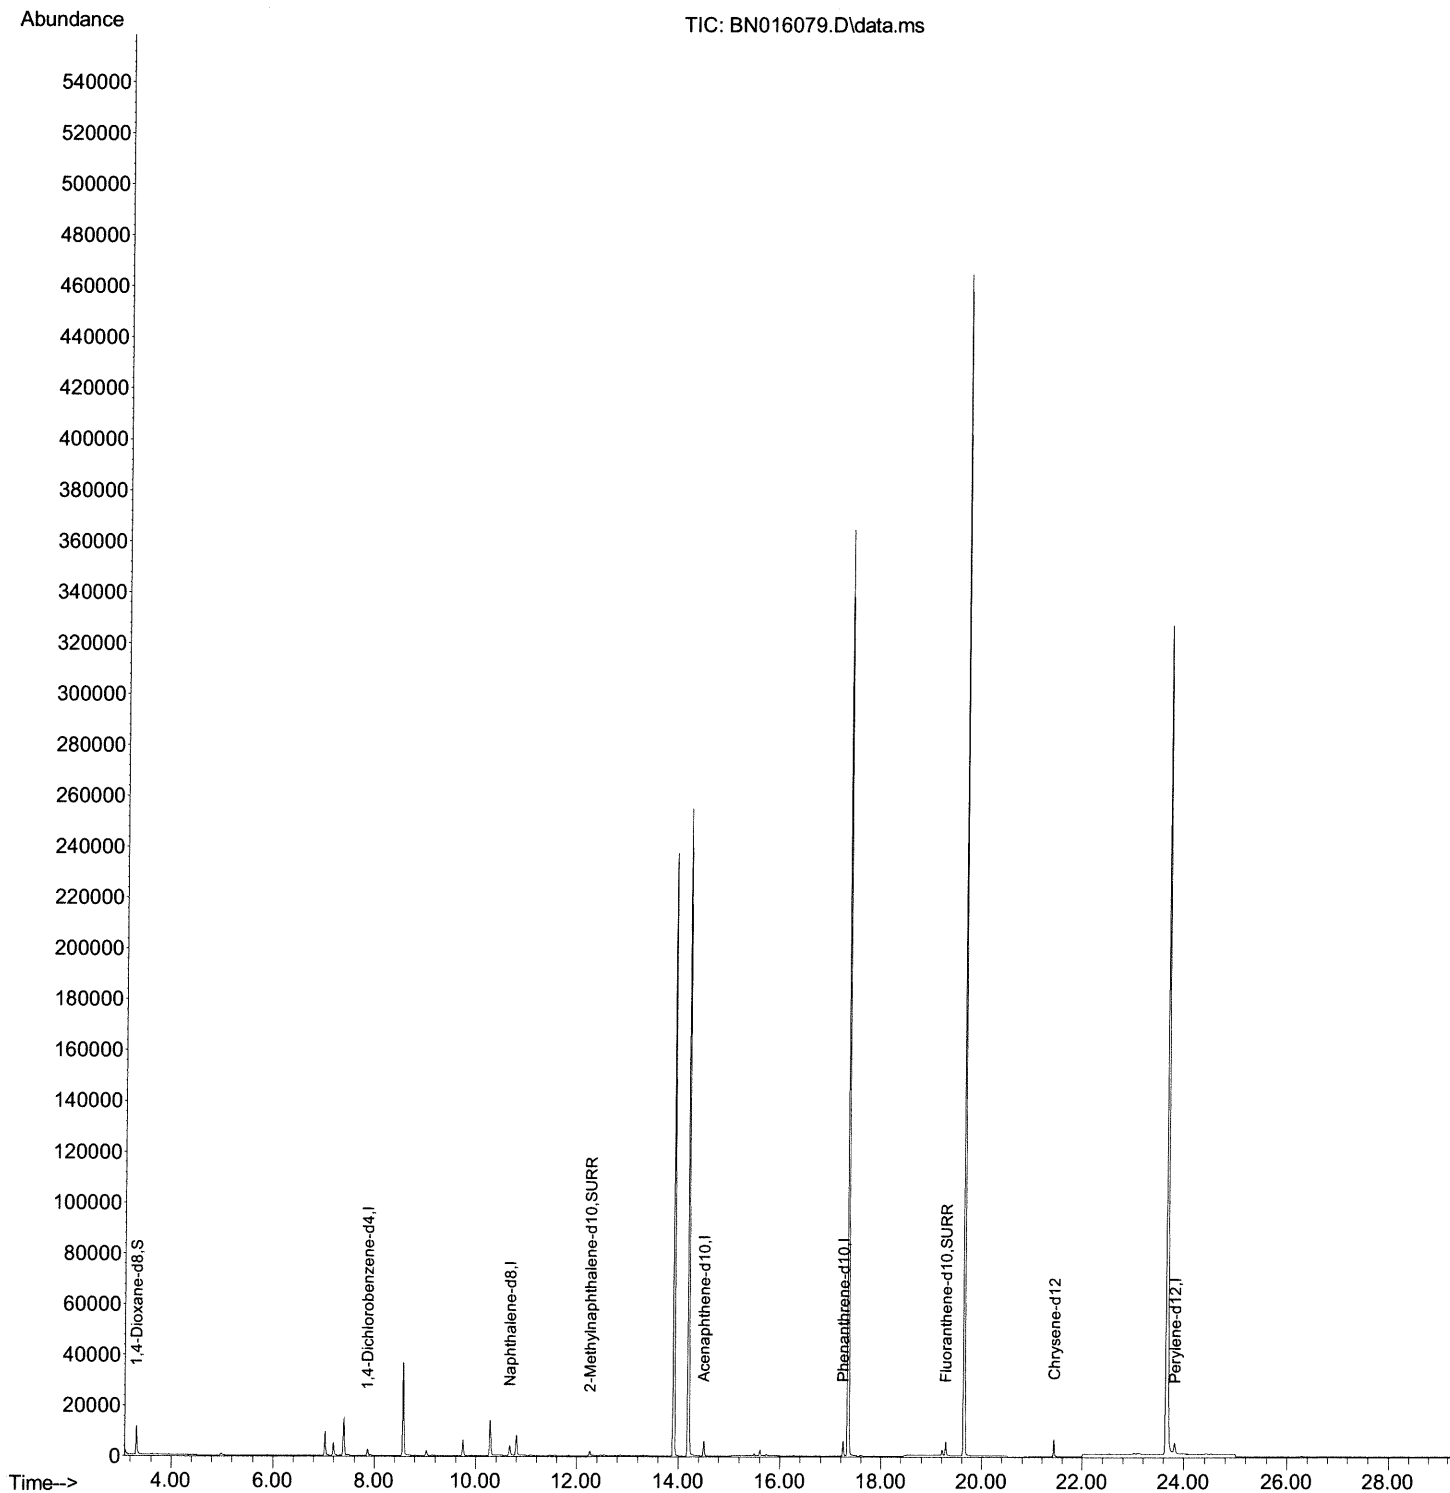

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082621\
 Data File : BN016079.D
 Acq On : 26 Aug 2021 20:54
 Operator : CG/JU
 Sample : M3458-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AT7

Manual Integrations
 APPROVED

mohammad
 8/27/2021 5:09:56 PM

Quant Time: Aug 27 03:30:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 26 11:35:43 2021
 Response via : Initial Calibration

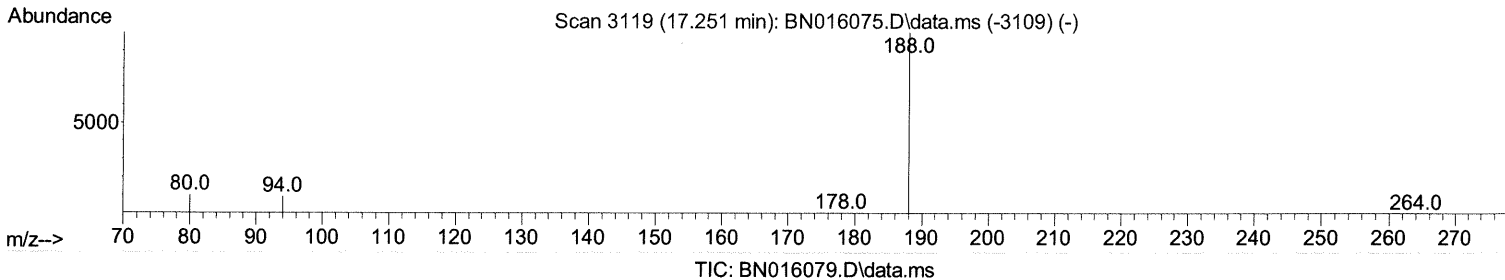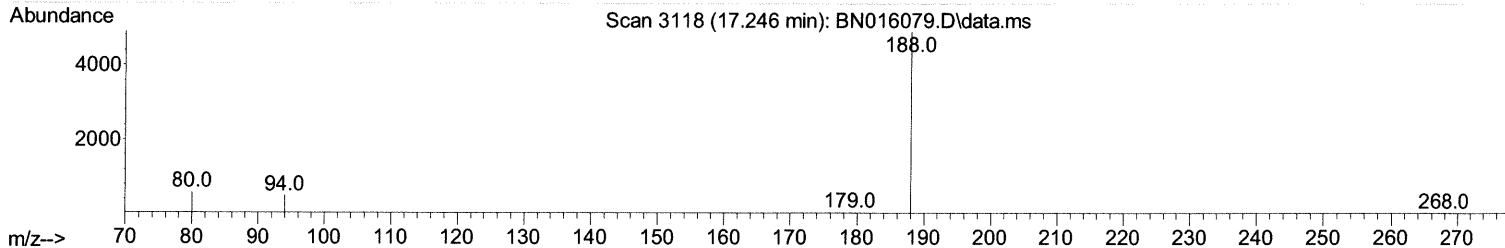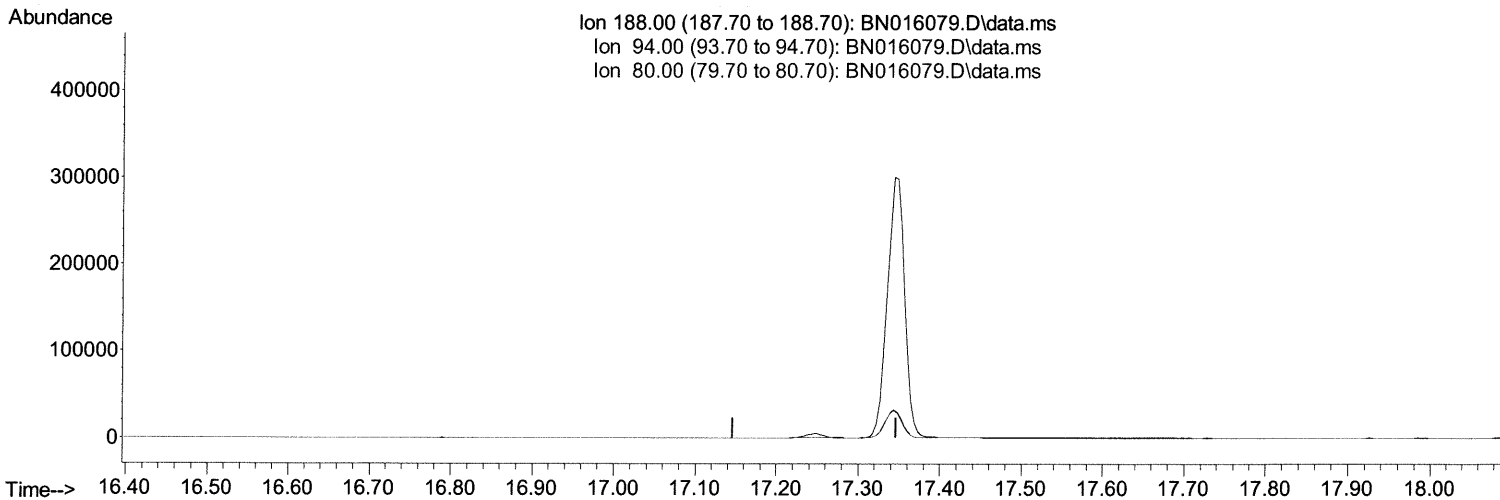

(13) Phenanthrene-d10 (I)

17.246min (-17.246) 0.00 ng/ul

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	10.20	0.00#
80.00	12.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082621\
Data File : BN016079.D
Acq On : 26 Aug 2021 20:54
Operator : CG/JU
Sample : M3458-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AT7

Manual Integrations
APPROVED

mohammad
8/27/2021 5:09:56 PM

Quant Time: Aug 27 03:30:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 26 11:35:43 2021
Response via : Initial Calibration

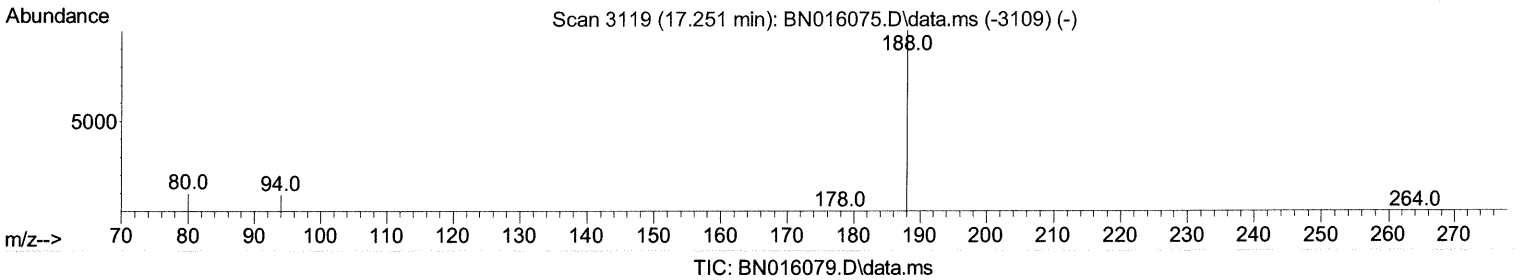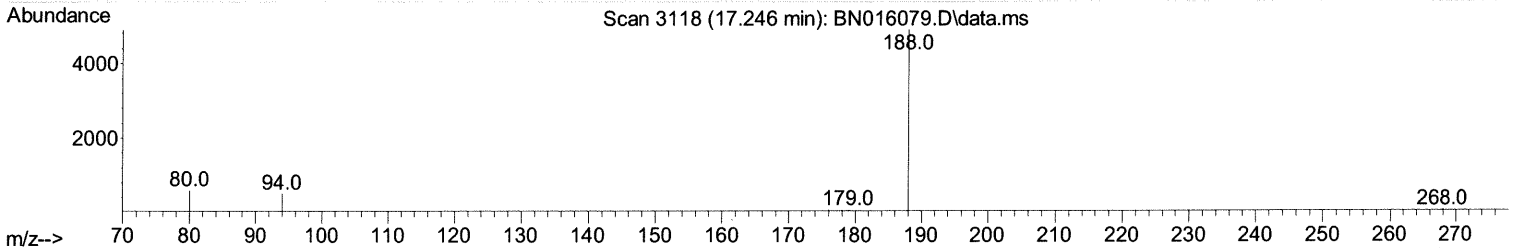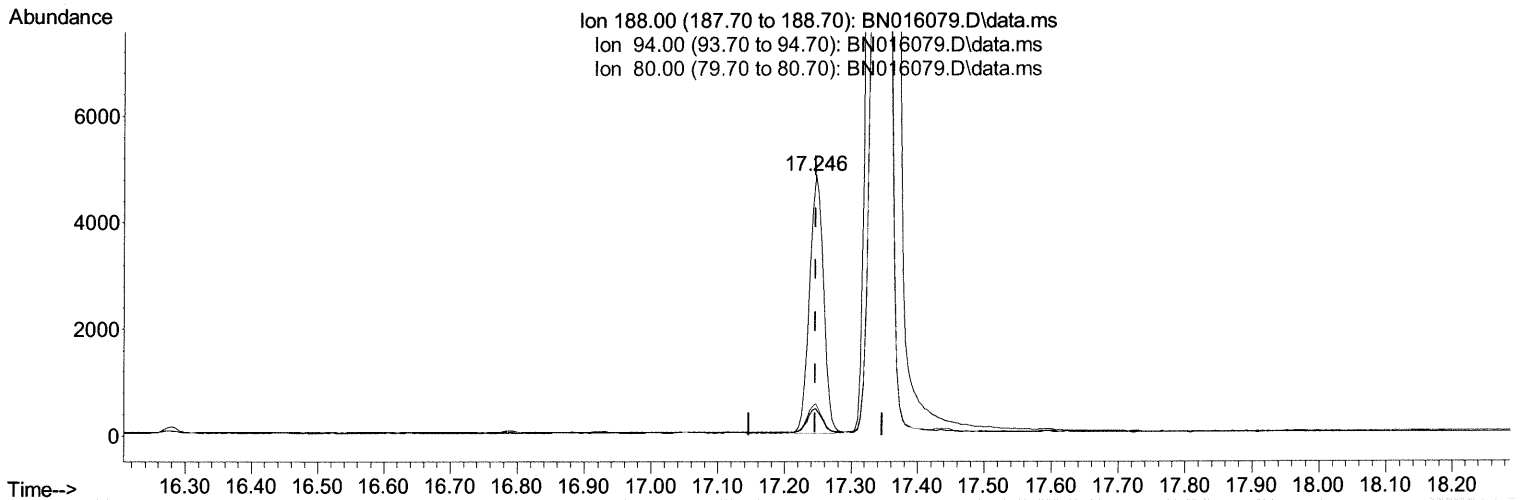

(13) Phenanthrene-d10 (I)

17.246min (-0.000) 0.40 ng/ul m 08/30/21 JU

response 7084

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	10.21
80.00	12.10	12.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082621\
 Data File : BN016079.D
 Acq On : 26 Aug 2021 20:54
 Operator : CG/JU
 Sample : M3458-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AT7

Manual Integrations
 APPROVED

mohammad
 8/27/2021 5:09:56 PM

Quant Time: Aug 27 03:30:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 26 11:35:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.867	152	1209	0.400	ng/ul	0.00
4) Naphthalene-d8	10.666	136	5180	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.501	164	3265	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.246	188	7084m >	0.400	ng/ul >	0.00 08/30/21 JU
17) Chrysene-d12	21.433	240	6714	0.400	ng/ul	0.00
23) Perylene-d12	23.815	264	6454	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	7974	4.868	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.255	152	2271	0.291	ng/ul	0.00
18) Fluoranthene-d10	19.280	212	5815	0.322	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed