


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082621\
Data File : BN016084.D
Acq On : 27 Aug 2021 00:35
Operator : CG/JU
Sample : PB138647BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK647

Manual Integrations
APPROVED

mohammad
8/27/2021 5:10:06 PM

Quant Time: Aug 27 03:31:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 26 11:35:43 2021
Response via : Initial Calibration

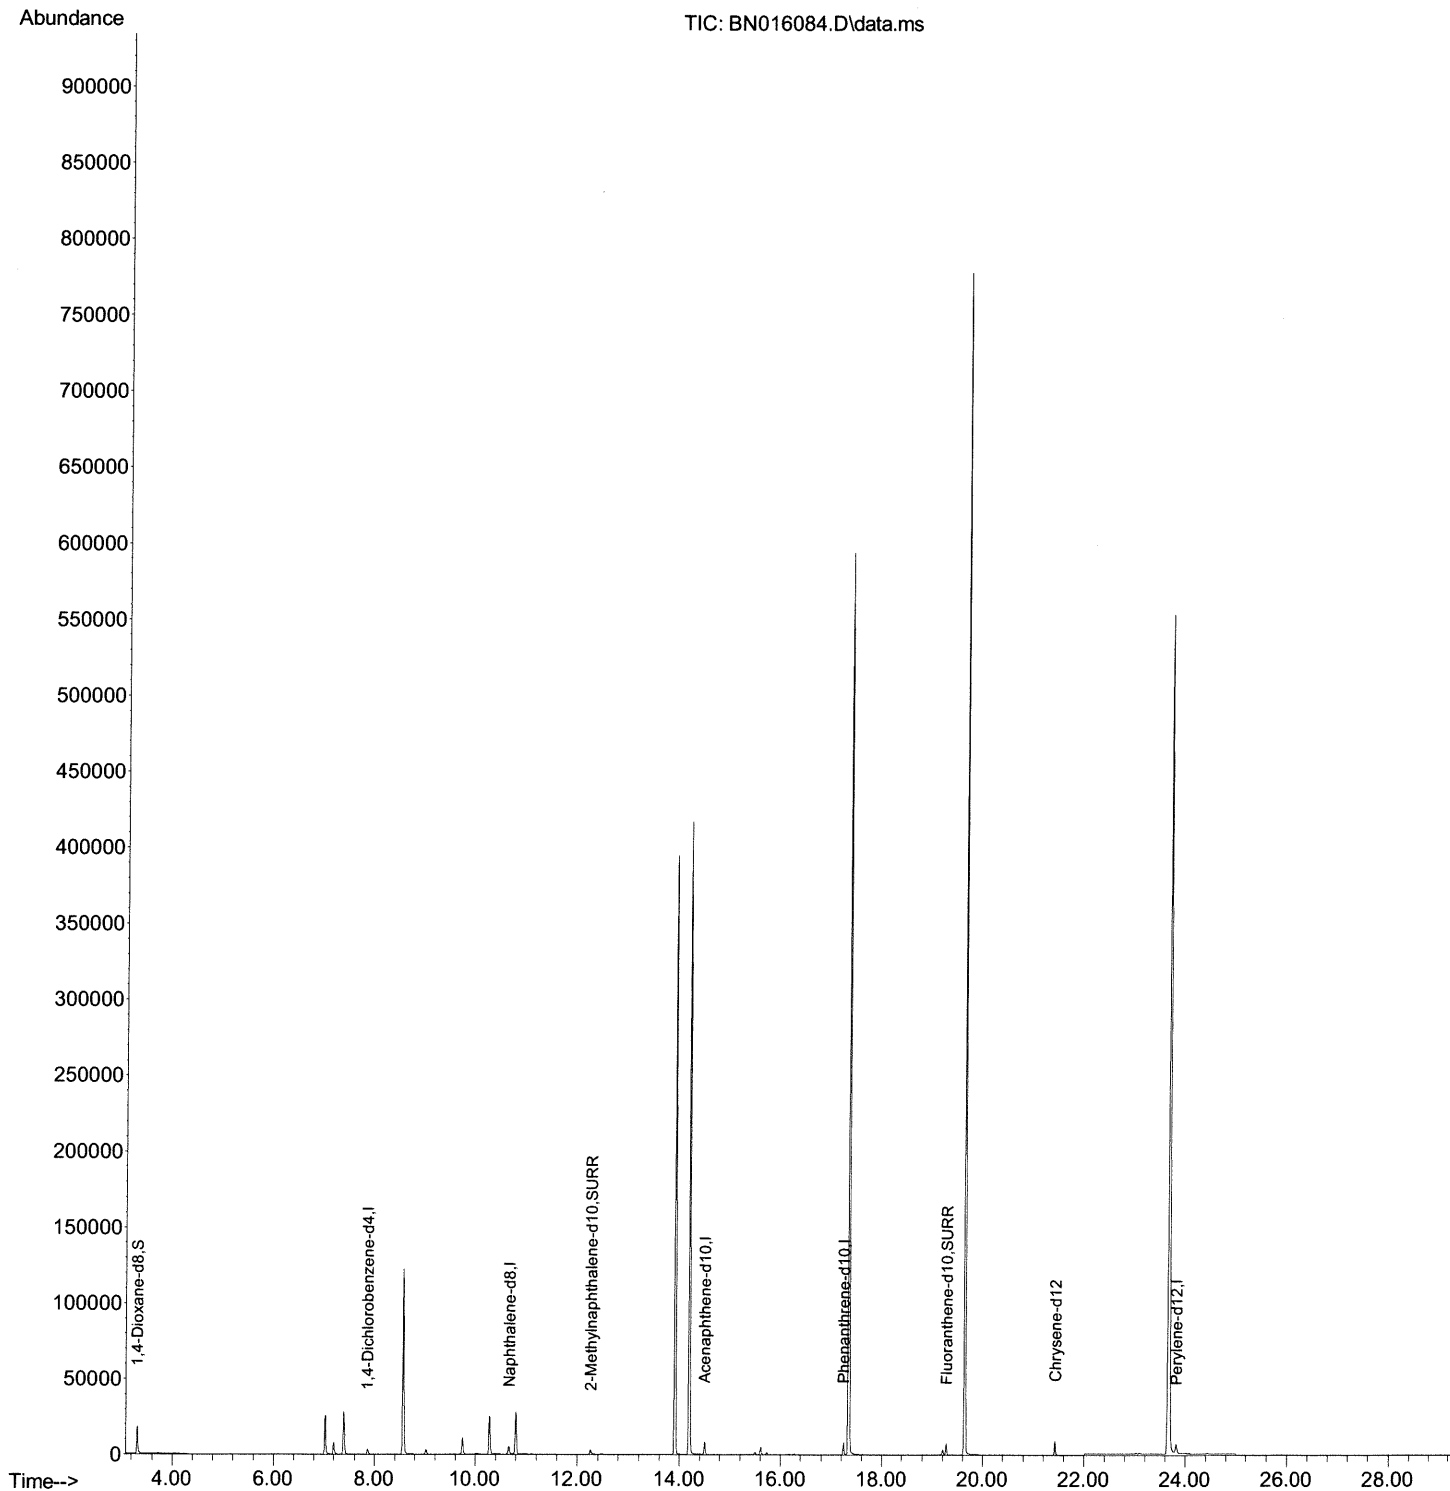

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082621\
Data File : BN016084.D
Acq On : 27 Aug 2021 00:35
Operator : CG/JU
Sample : PB138647BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK647

Manual Integrations
APPROVED

mohammad
8/27/2021 5:10:06 PM

Quant Time: Aug 27 03:31:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 26 11:35:43 2021
Response via : Initial Calibration

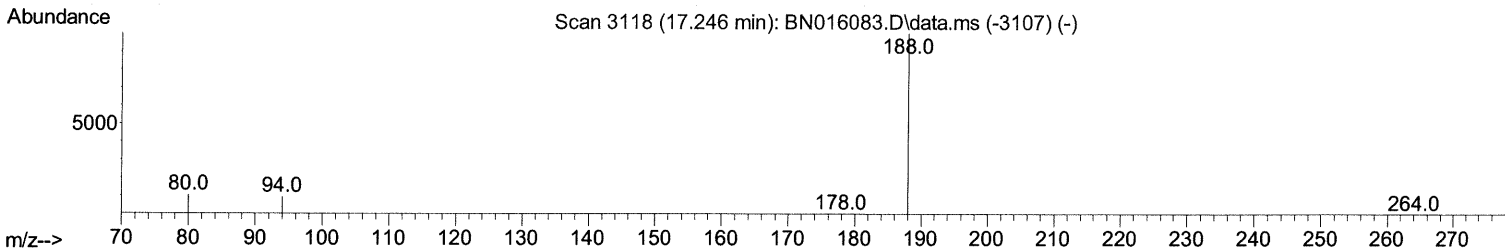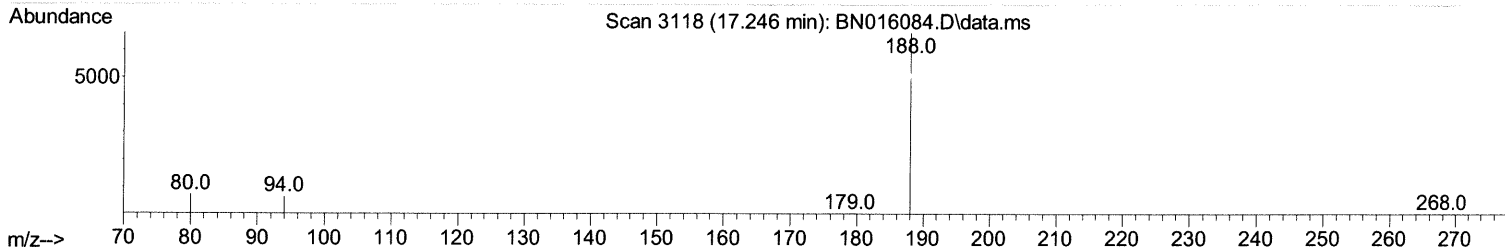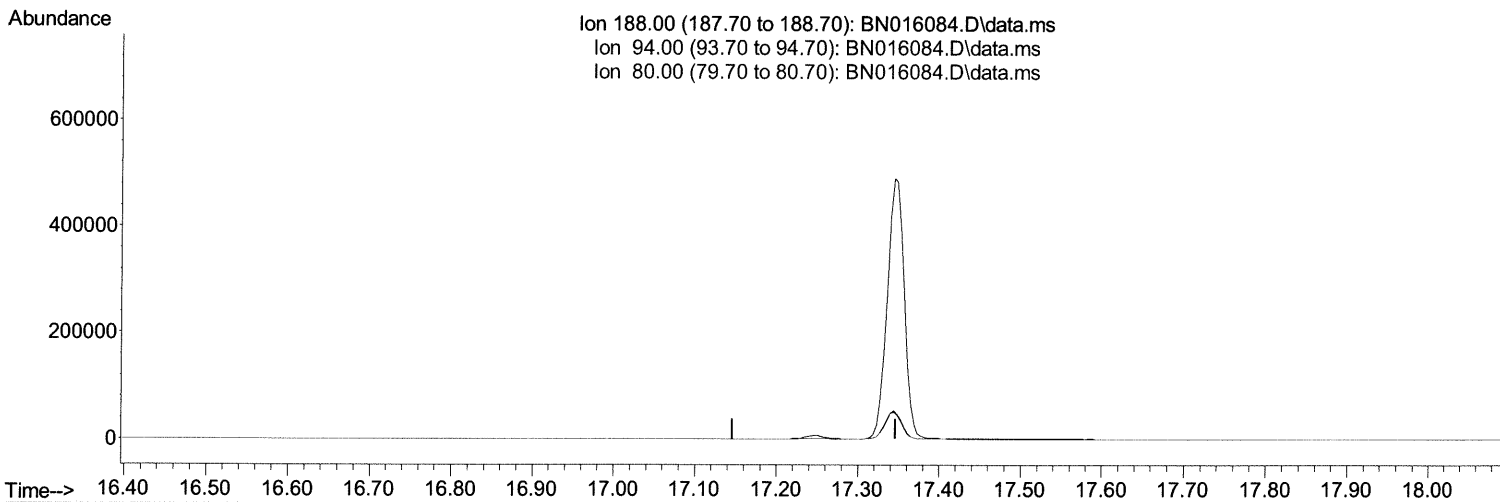

TIC: BN016084.D\data.ms

(13) Phenanthrene-d10 (I)

17.246min (-17.246) 0.00 ng/ul

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	10.20	0.00#
80.00	12.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082621\
 Data File : BN016084.D
 Acq On : 27 Aug 2021 00:35
 Operator : CG/JU
 Sample : PB138647BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK647

Manual Integrations
 APPROVED

mohammad
 8/27/2021 5:10:06 PM

Quant Time: Aug 27 03:31:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 26 11:35:43 2021
 Response via : Initial Calibration

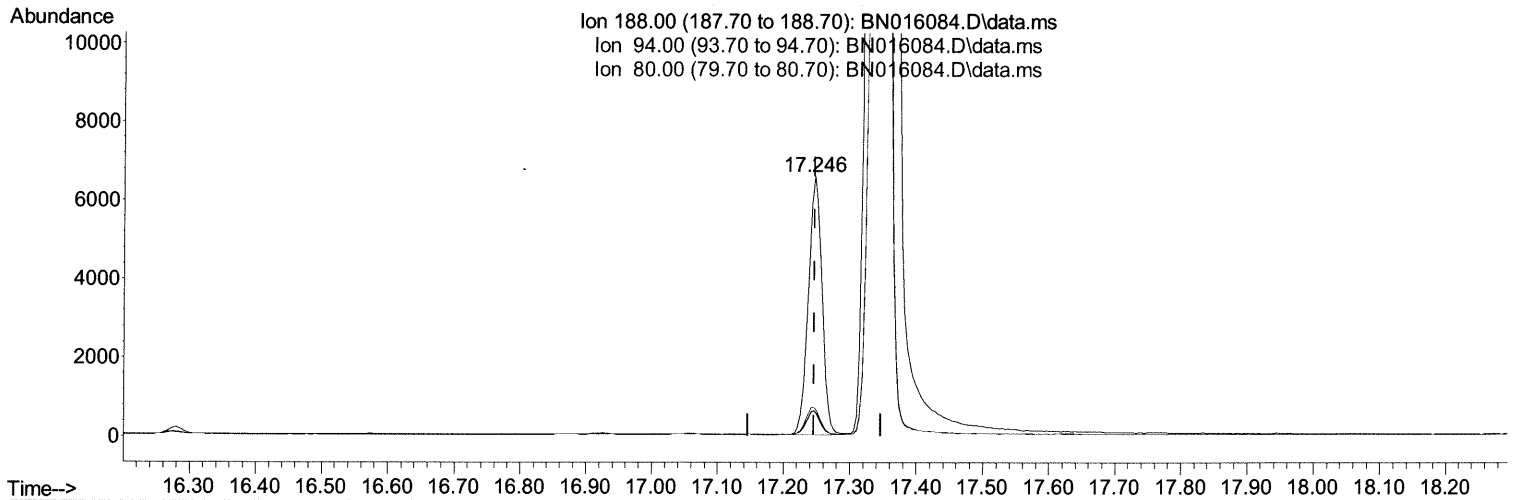

(13) Phenanthrene-d10 (I)

17.246min (+ 0.000) 0.40 ng/ul m 0 8/30/21 JU

response 9414

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	9.79
80.00	12.10	11.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082621\
 Data File : BN016084.D
 Acq On : 27 Aug 2021 00:35
 Operator : CG/JU
 Sample : PB138647BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK647

Manual Integrations
 APPROVED

mohammad
 8/27/2021 5:10:06 PM

Quant Time: Aug 27 03:31:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 26 11:35:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	1629	0.400	ng/ul	0.00
4) Naphthalene-d8	10.667	136	7069	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.502	164	4532	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.246	188	9414m >	0.400	ng/ul >	0.00
17) Chrysene-d12	21.433	240	9051	0.400	ng/ul	0.00
23) Perylene-d12	23.816	264	9089	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	12563	5.692	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.256	152	3461	0.325	ng/ul	0.00
18) Fluoranthene-d10	19.276	212	8334	0.342	ng/ul	0.00

Target Compounds Qvalue

 (#) = qualifier out of range (m) = manual integration (+) = signals summed