


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082621\
Data File : BN016085.D
Acq On : 27 Aug 2021 01:12
Operator : CG/JU
Sample : PB138654BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK654

Manual Integrations
APPROVED

mohammad
8/27/2021 5:10:08 PM

Quant Time: Aug 27 03:31:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 26 11:35:43 2021
Response via : Initial Calibration

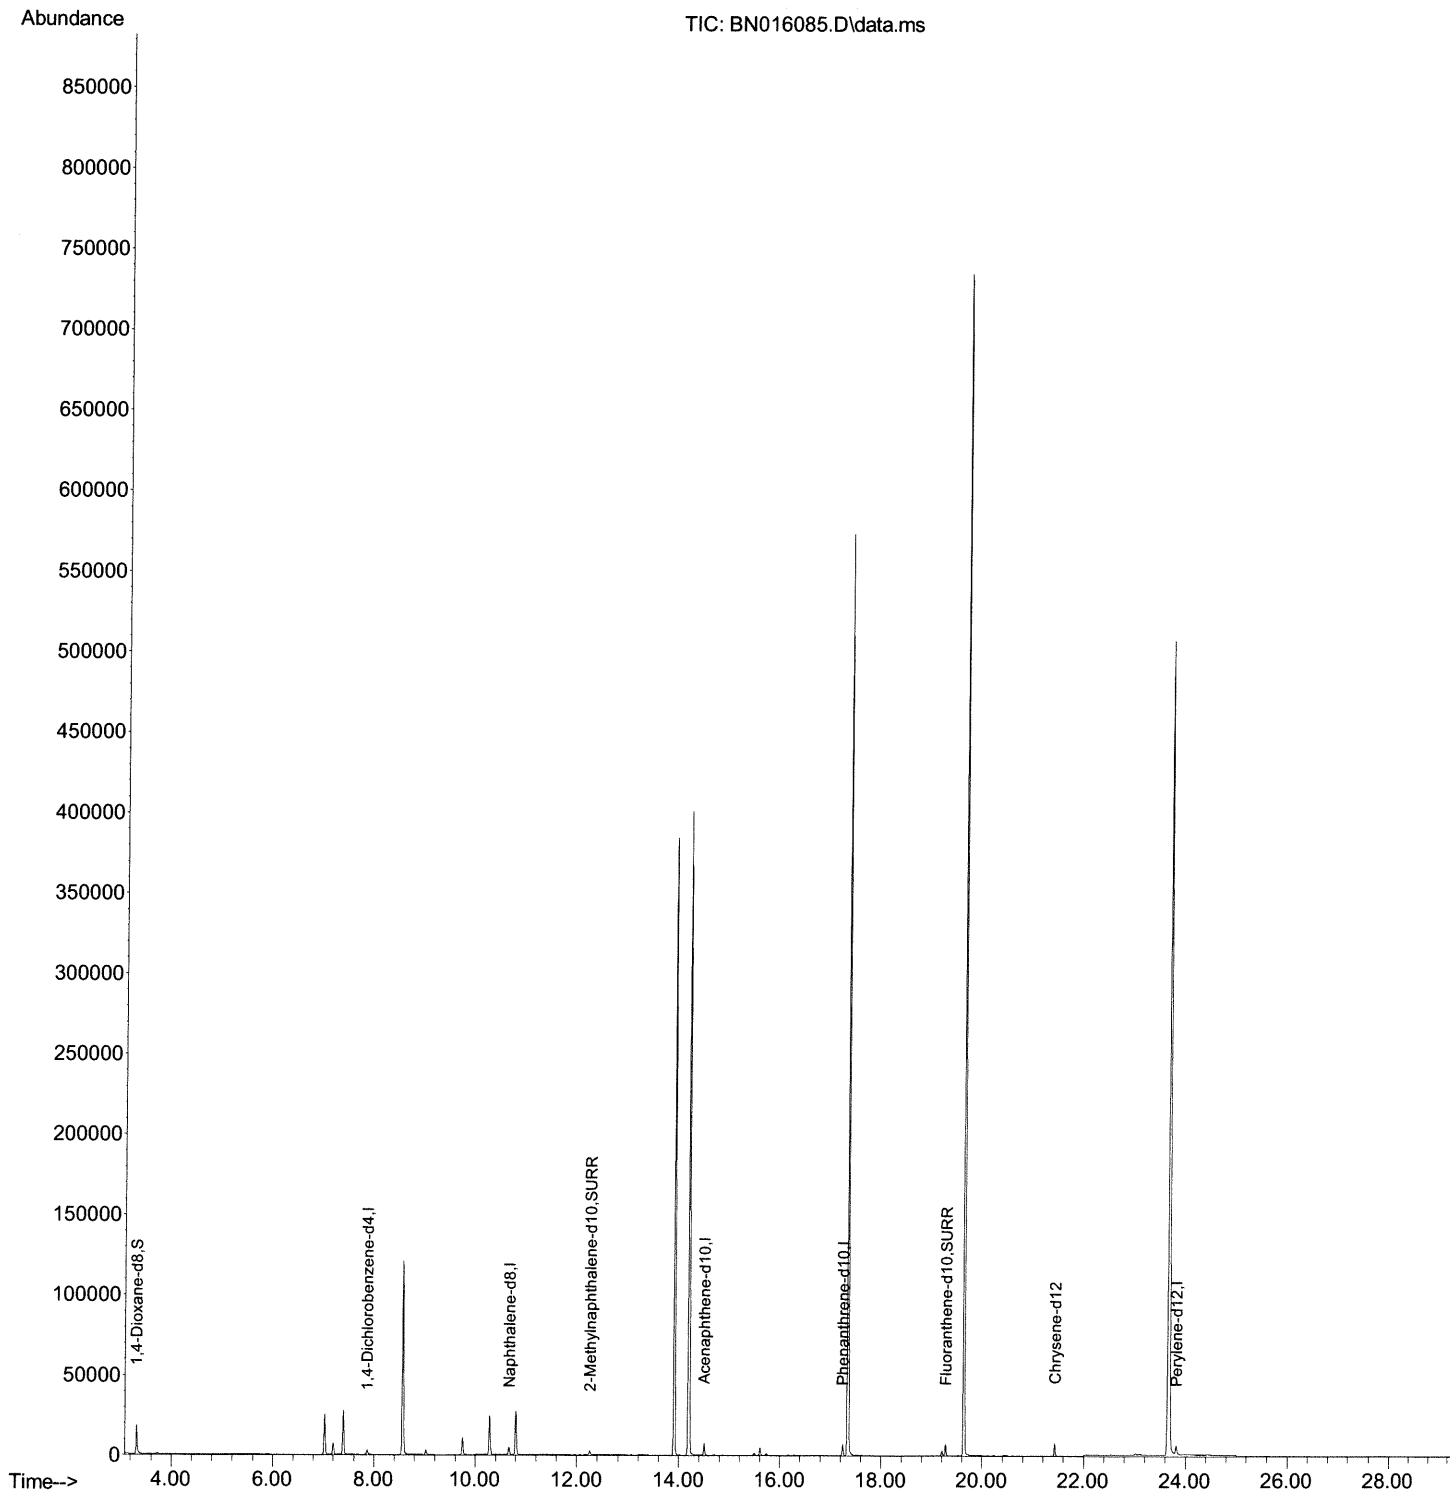

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082621\
 Data File : BN016085.D
 Acq On : 27 Aug 2021 01:12
 Operator : CG/JU
 Sample : PB138654BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK654

Manual Integrations
 APPROVED

mohammad
 8/27/2021 5:10:08 PM

Quant Time: Aug 27 03:31:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 26 11:35:43 2021
 Response via : Initial Calibration

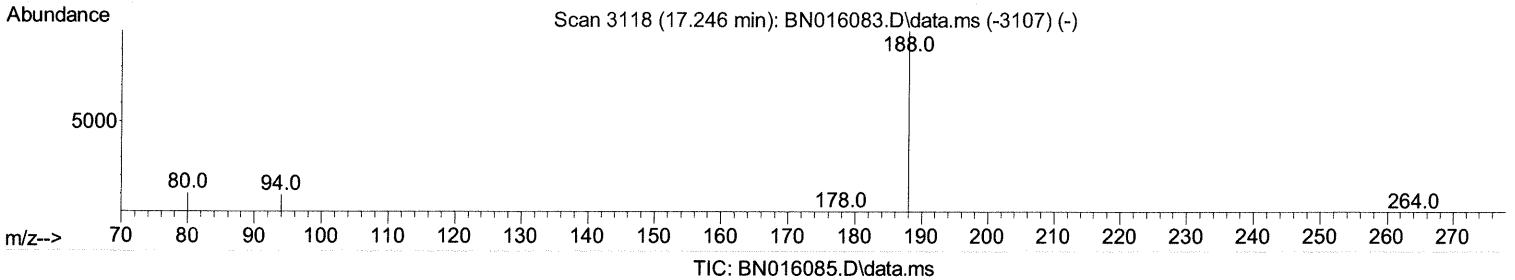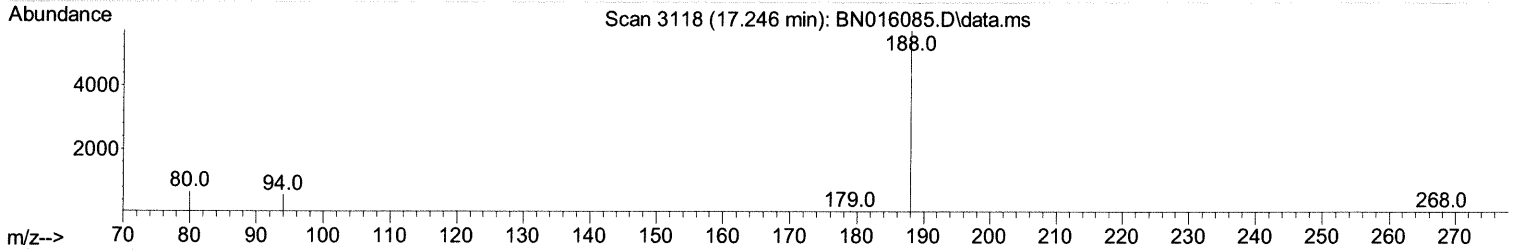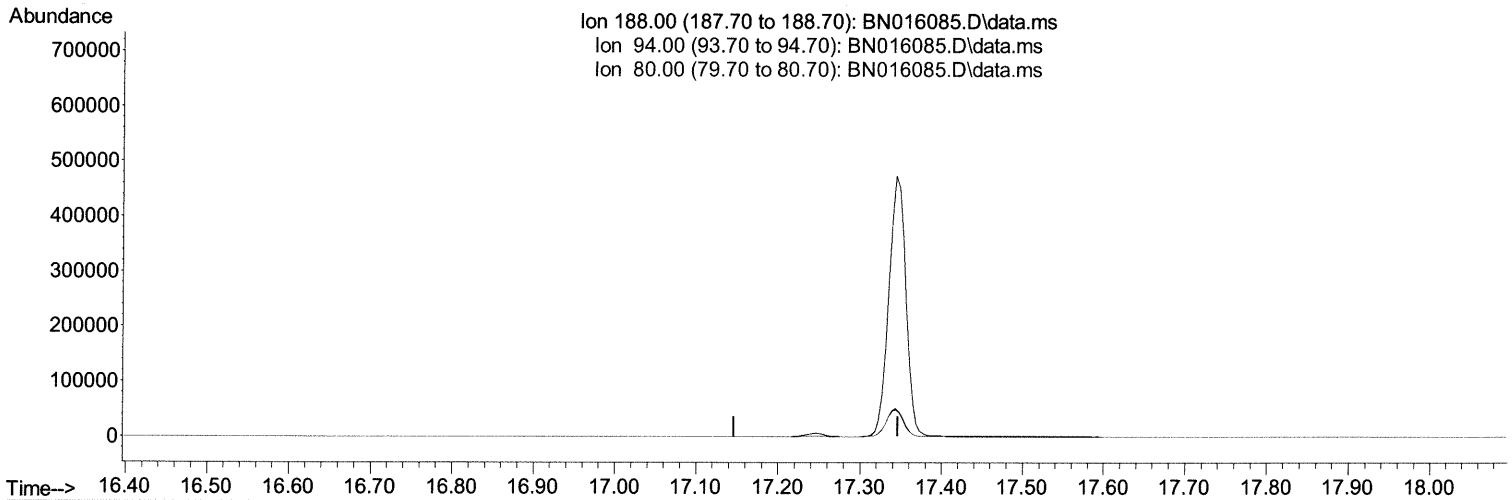

(13) Phenanthrene-d10 (I)

17.246min (-17.246) 0.00 ng/ul

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	10.20	0.00#
80.00	12.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082621\
 Data File : BN016085.D
 Acq On : 27 Aug 2021 01:12
 Operator : CG/JU
 Sample : PB138654BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK654

Manual Integrations
 APPROVED

mohammad
 8/27/2021 5:10:08 PM

Quant Time: Aug 27 03:31:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Thu Aug 26 11:35:43 2021
 Response via : Initial Calibration

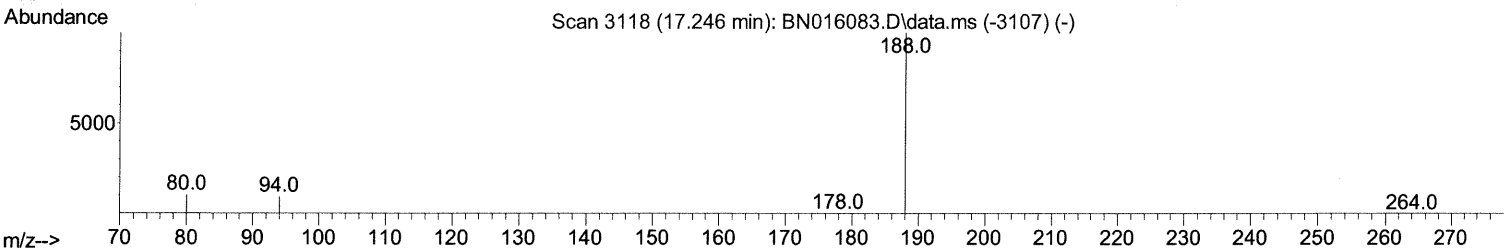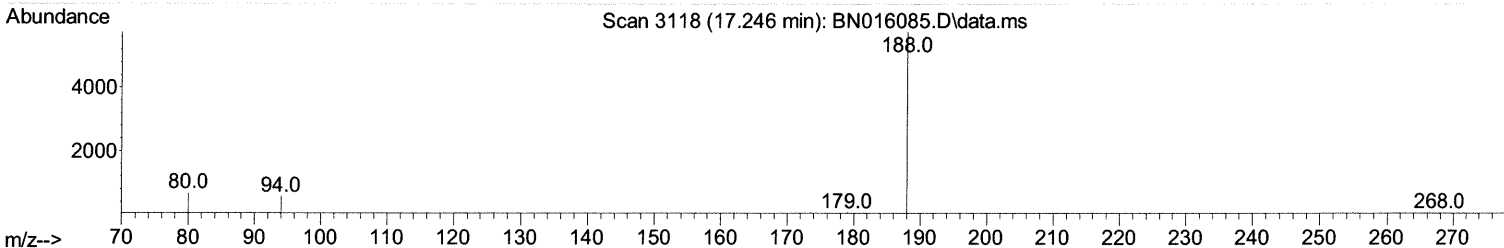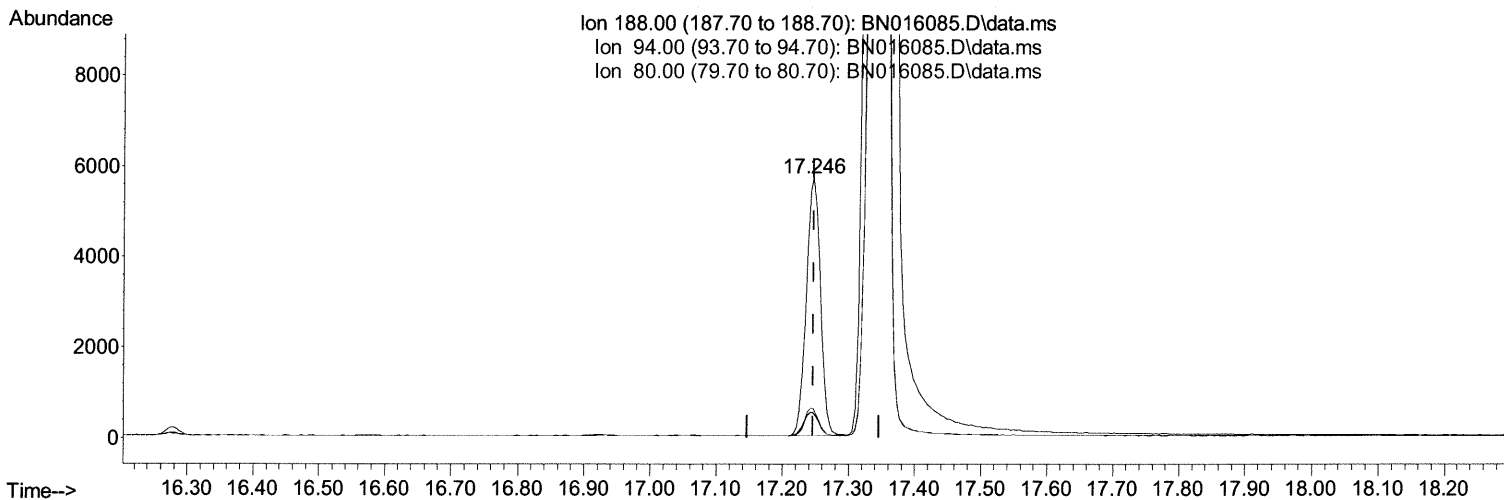

TIC: BN016085.D\data.ms

(13) Phenanthrene-d10 (I)

17.246min (-0.000) 0.40 ng/ul m 08/30/21 JU

response 8452

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	9.71
80.00	12.10	11.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082621\
 Data File : BN016085.D
 Acq On : 27 Aug 2021 01:12
 Operator : CG/JU
 Sample : PB138654BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK654

Manual Integrations
 APPROVED

mohammad
 8/27/2021 5:10:08 PM

Quant Time: Aug 27 03:31:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 26 11:35:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.867	152	1506	0.400	ng/ul	0.00
4) Naphthalene-d8	10.666	136	6499	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.501	164	4124	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.246	188	8452m >	0.400	ng/ul >	0.00
17) Chrysene-d12	21.430	240	7851	0.400	ng/ul	0.00
23) Perylene-d12	23.815	264	7820	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	12681	6.215	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.256	152	3436	0.351	ng/ul	0.00
18) Fluoranthene-d10	19.276	212	7955	0.376	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed