

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082718\
 Data File : BN002536.D
 Acq On : 27 Aug 2018 20:32
 Operator : JU/SJ
 Sample : J4598-21
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ETBN1

Quant Time: Aug 28 11:49:03 2018
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 25 04:34:18 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	81734	20.00	ng/ul	0.00
18) Naphthalene-d8	10.44	136	323210	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	189703	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	584680	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	742338	20.00	ng/ul	0.00
85) Perylene-d12	23.46	264	805474	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL
5) Phenol-d5	0.00	99	0	0.00	ng/ul
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul
43) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul
46) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
57) Fluorene-d10	0.00	176	0	0.00	ng/ul
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul
70) Anthracene-d10	0.00	188	0d	0.00	ng/ul
78) Pyrene-d10	0.00	212	0	0.00	ng/ul
89) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul


Target Compounds				Qvalue
28) Naphthalene	10.49	128	73900	4.444 ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082718\
Data File : BN002536.D
Acq On : 27 Aug 2018 20:32
Operator : JU/SJ
Sample : J4598-21
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ETBN1

Quant Time: Aug 28 11:49:03 2018
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 25 04:34:18 2018
Response via : Initial Calibration

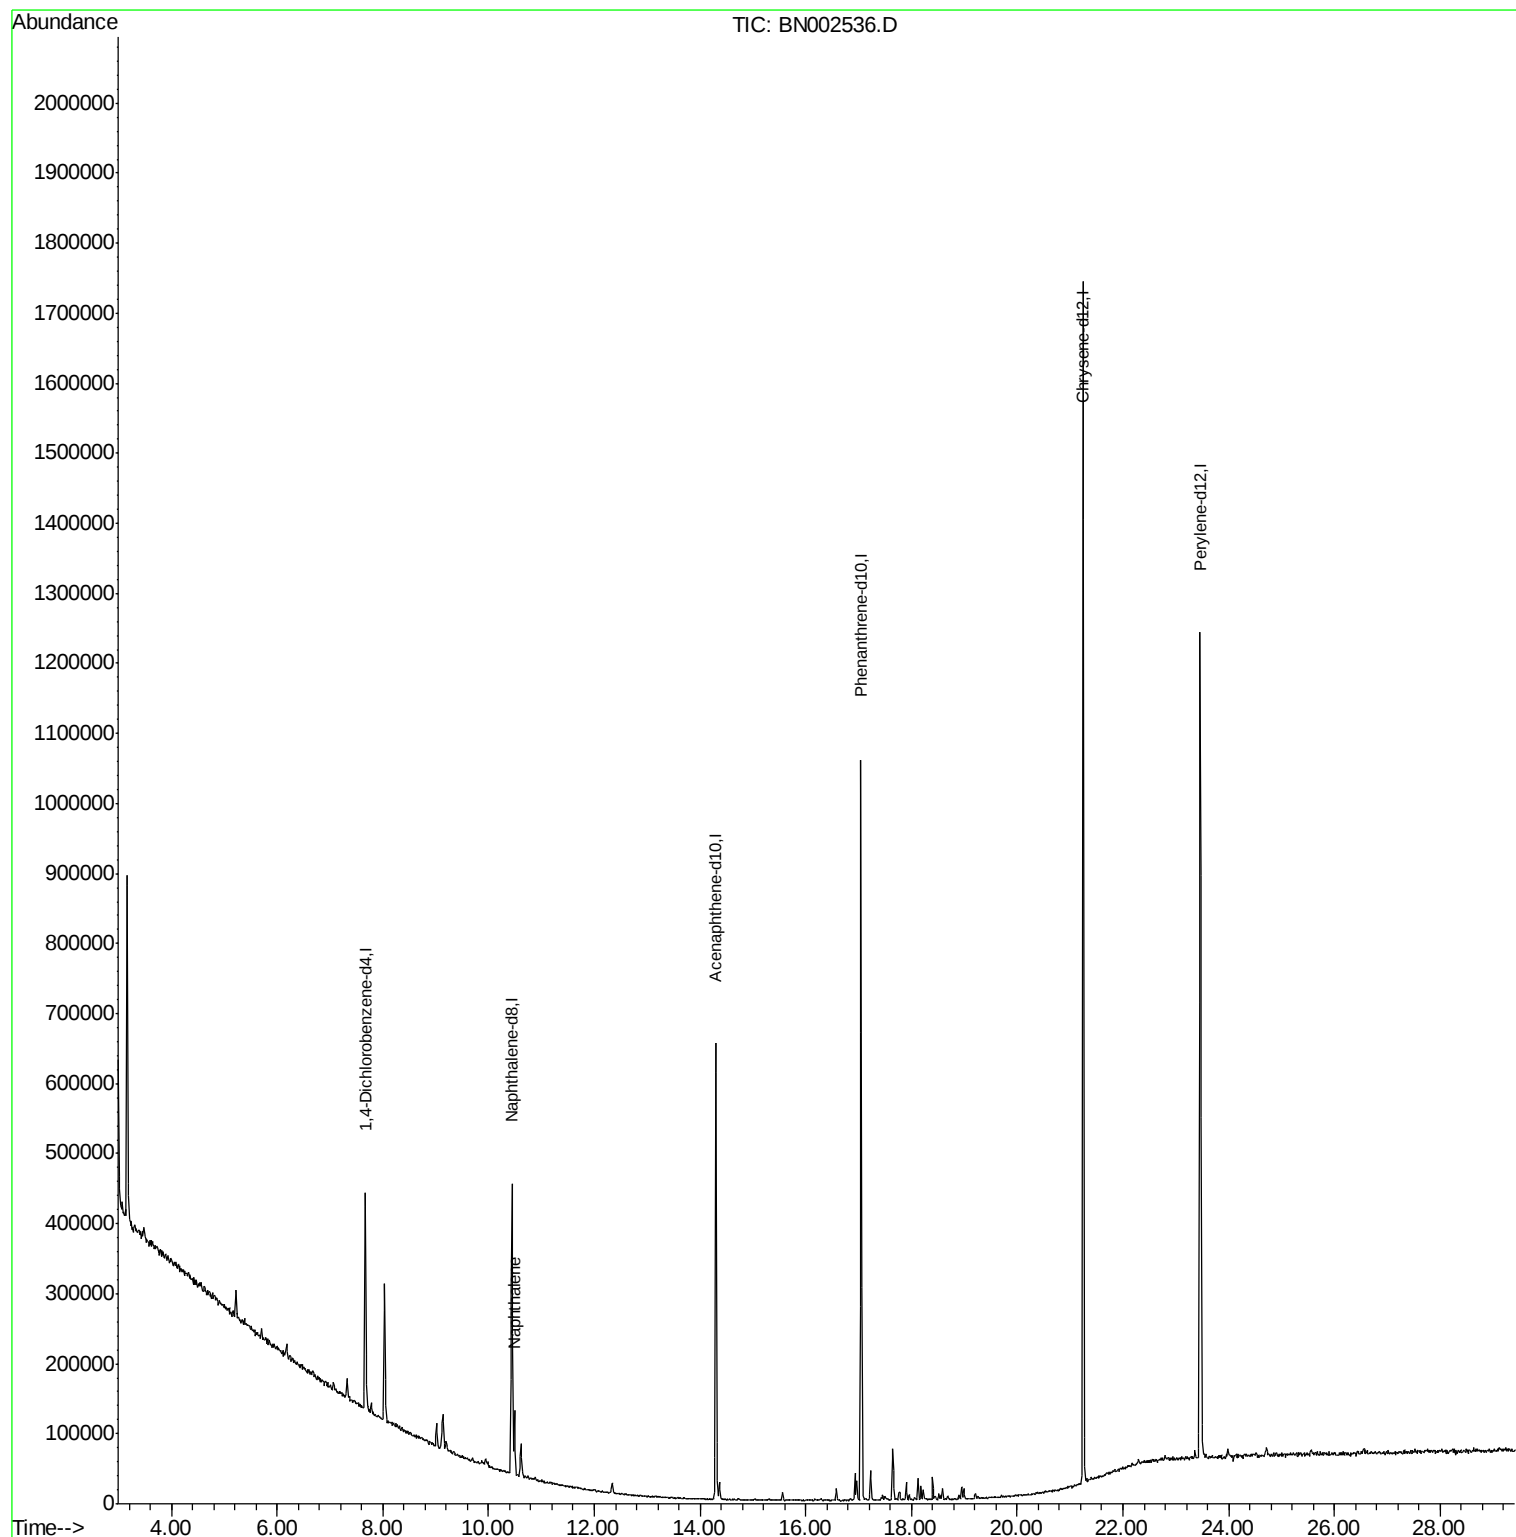

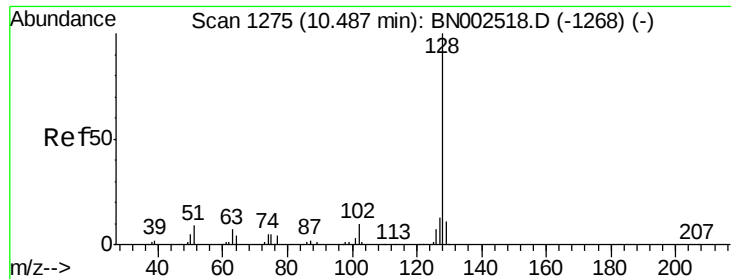

#28

Naphthalene

Concen: 4.444 ng/ul

RT: 10.49 min Scan# 1275

Delta R.T. 0.00 min

Lab File: BN002536.D

Acq: 27 Aug 2018 20:32

Instrument :

BNA_N

ClientSampleId :

ETBN1


Tgt Ion:128 Resp: 73900

Ion Ratio Lower Upper

128 100

129 11.4 8.8 13.2

127 14.4 10.5 15.7

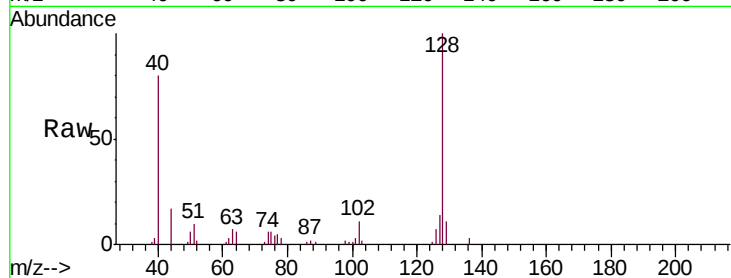

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

