
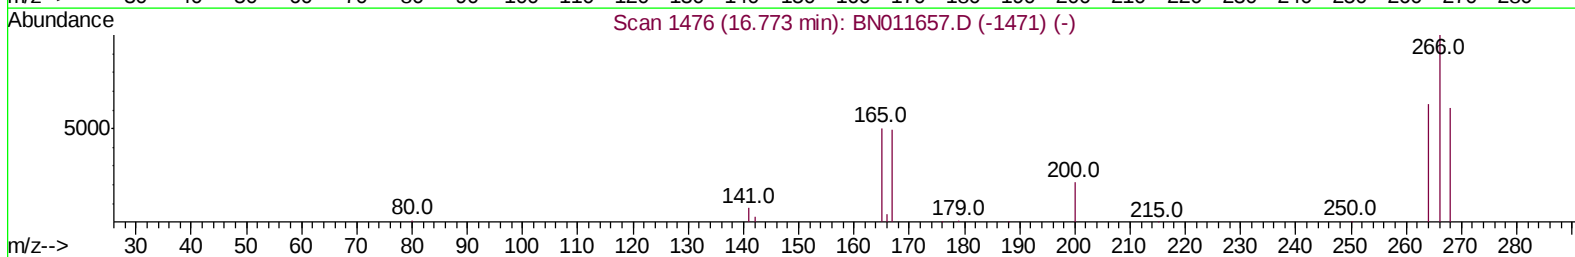
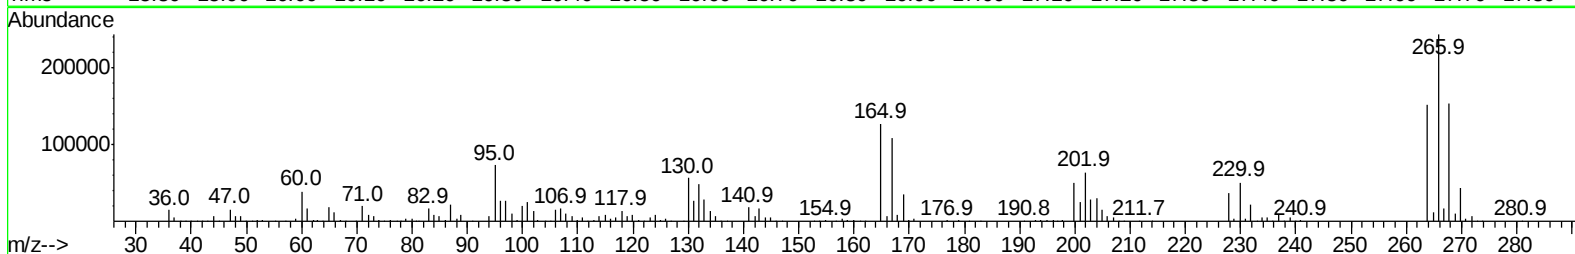


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082720\
Data File : BN011654.D
Acq On : 27 Aug 2020 09:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 01:37:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 27 14:34:48 2020
Response via : Initial Calibration

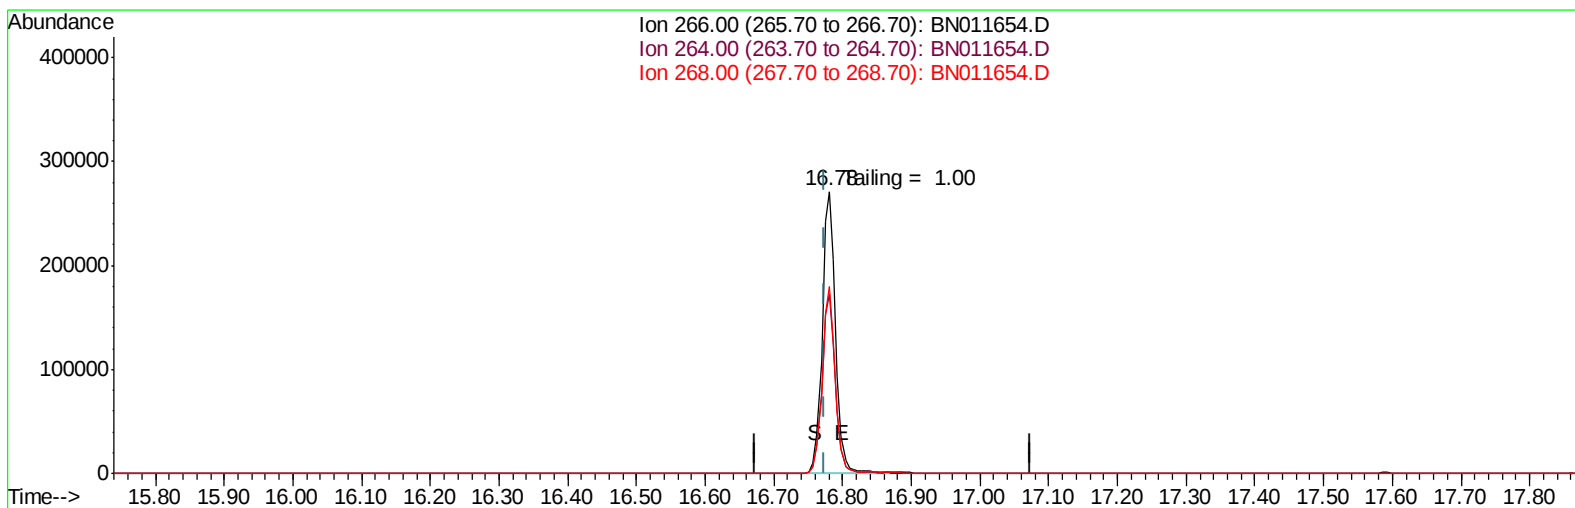

TIC: BN011654.D

(24) Pentachlorophenol

16.780min (+0.007) 0.00ng

response 367498

Ion	Exp%	Act%
266.00	100	100
264.00	61.90	63.63
268.00	66.20	64.26
0.00	0.00	0.00