
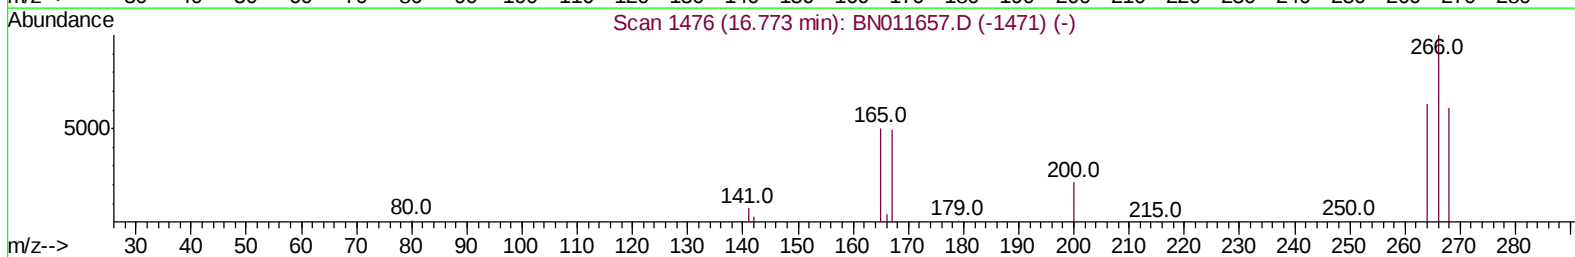
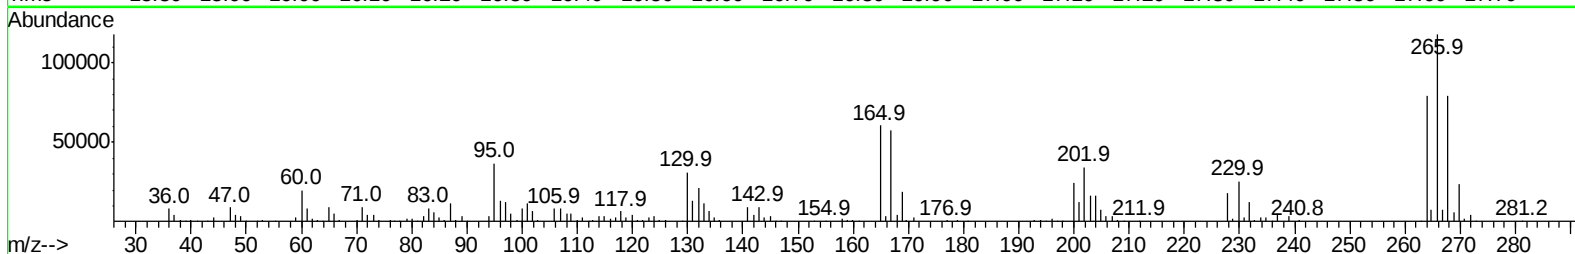


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082720\
Data File : BN011673.D
Acq On : 27 Aug 2020 21:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 00:55:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 27 14:34:48 2020
Response via : Initial Calibration

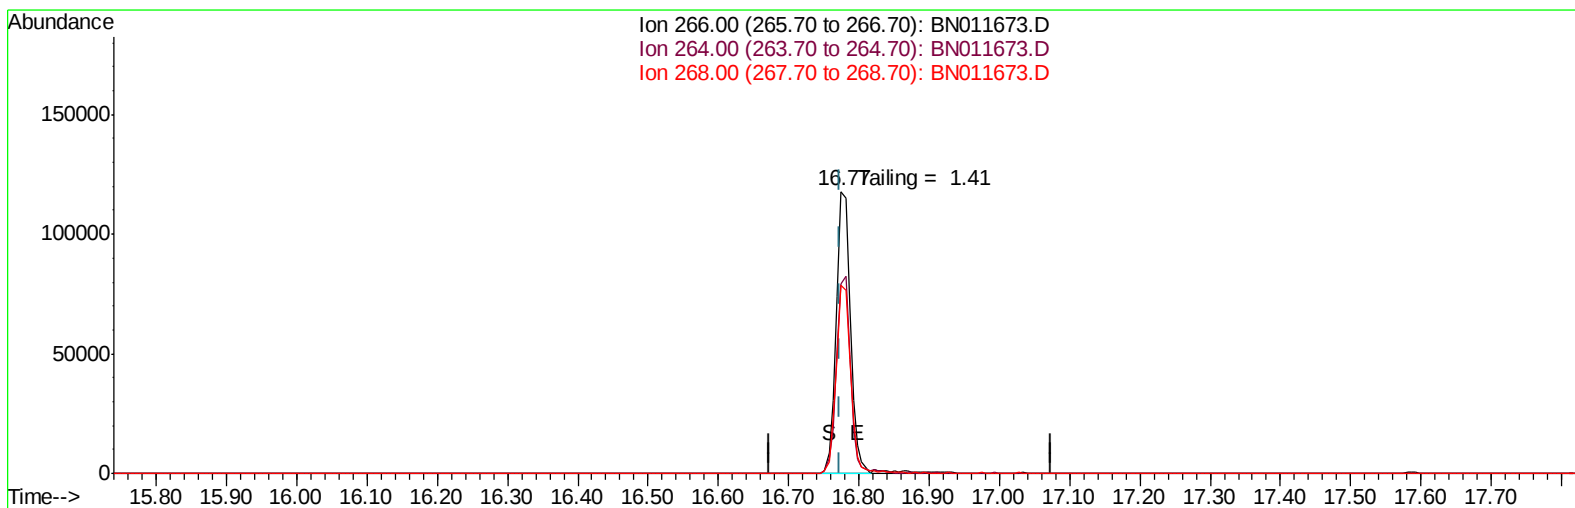

TIC: BN011673.D

(24) Pentachlorophenol

16.775min (+0.001) 0.00ng

response 164542

Ion	Exp%	Act%
266.00	100	100
264.00	61.90	69.55
268.00	66.20	68.85
0.00	0.00	0.00