

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082720\
 Data File : BN011668.D
 Acq On : 27 Aug 2020 17:30
 Operator : CG/JU
 Sample : L3737-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 KY038PS037-200818

Quant Time: Aug 27 18:33:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN082720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 27 14:34:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	1971	0.40	ng	0.00
7) Naphthalene-d8	10.53	136	7397	0.40	ng	0.00
13) Acenaphthene-d10	14.38	164	4283	0.40	ng	0.00
19) Phenanthrene-d10	17.13	188	10092	0.40	ng	0.00
29) Chrysene-d12	21.32	240	10370	0.40	ng	0.00
36) Perylene-d12	23.59	264	8455	0.40	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.34	112	337	0.06	ng	0.00
5) Phenol-d6	6.91	99	375	0.05	ng	0.00
8) Nitrobenzene-d5	8.88	82	3591	0.50	ng	0.00
11) 2-Methylnaphthalene-d10	12.12	152	3747	0.28	ng	0.00
14) 2,4,6-Tribromophenol	15.88	330	185	0.09	ng	0.00
15) 2-Fluorobiphenyl	13.00	172	9581	0.53	ng	0.00
27) Fluoranthene-d10	19.16	212	11049	0.34	ng	0.00
31) Terphenyl-d14	19.77	244	19827	0.77	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082720\
Data File : BN011668.D
Acq On : 27 Aug 2020 17:30
Operator : CG/JU
Sample : L3737-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
KY038PS037-200818

Quant Time: Aug 27 18:33:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 27 14:34:48 2020
Response via : Initial Calibration

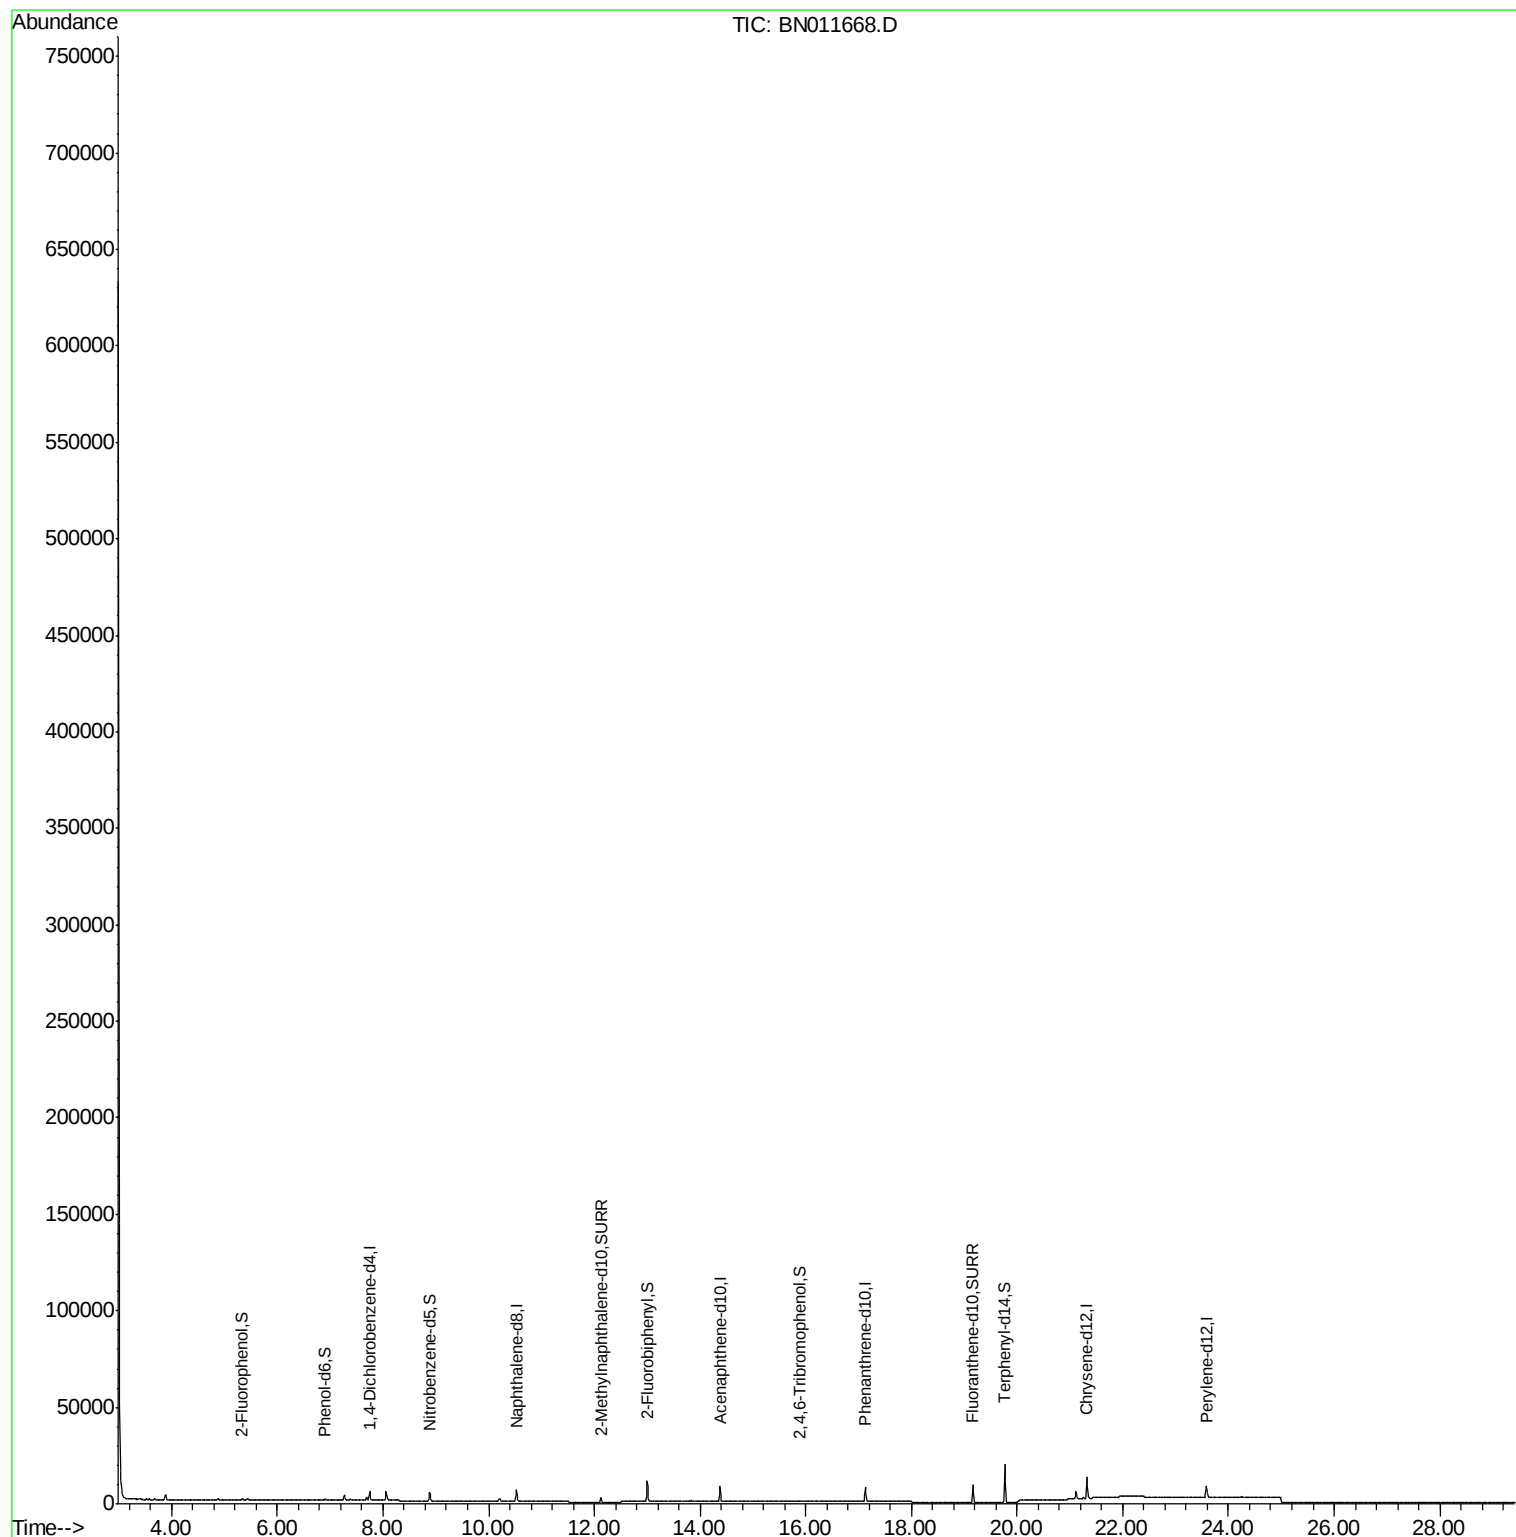

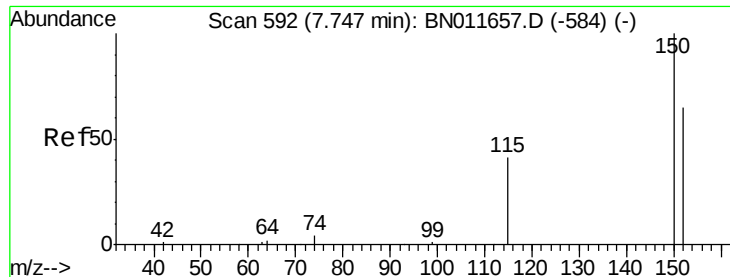


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.75 min Scan# 592
Delta R.T. -0.00 min
Lab File: BN011668.D
Acq: 27 Aug 2020 17:30

Instrument :
BNA_N
ClientSampleId :
KY038PS037-200818

Tot Ion:152 Resp: 1971
Ion Ratio Lower Upper
152 100
150 152.5 121.0 181.6
115 68.0 52.6 78.8

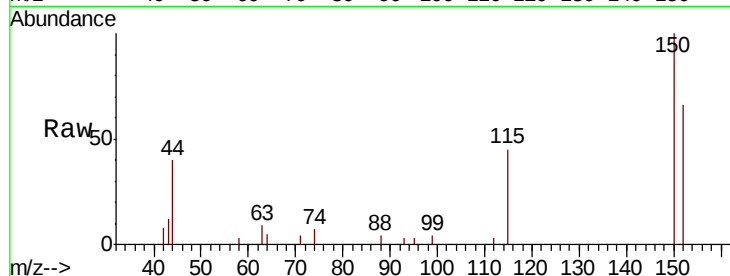


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

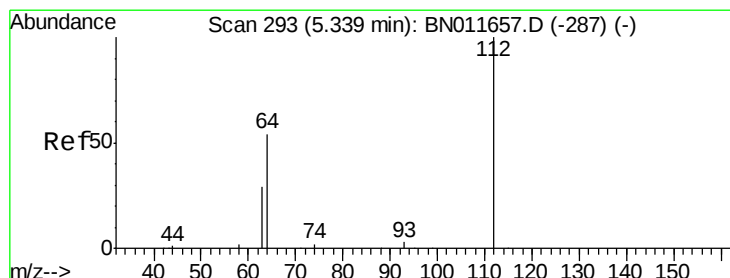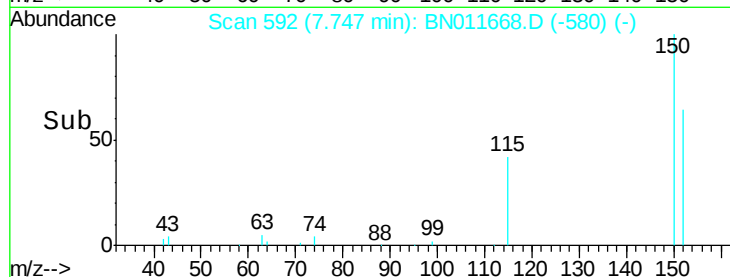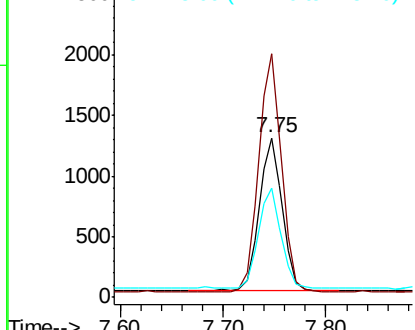



#4


2-Fluorophenol
Concen: 0.060 ng
RT: 5.34 min Scan# 293
Delta R.T. -0.00 min
Lab File: BN011668.D
Acq: 27 Aug 2020 17:30

Tgt Ion:112 Resp: 337
Ion Ratio Lower Upper
112 100
64 60.2 49.7 74.5
63 40.9 29.4 44.0

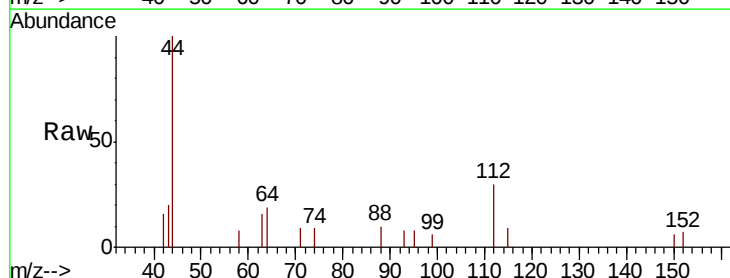

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

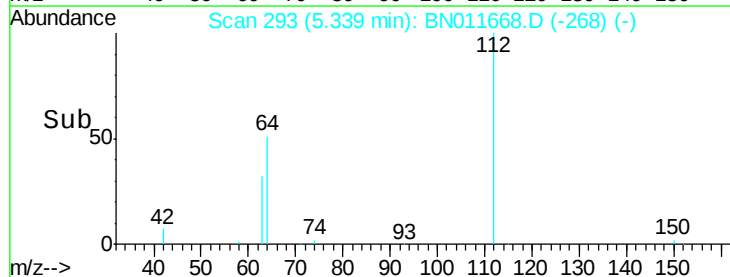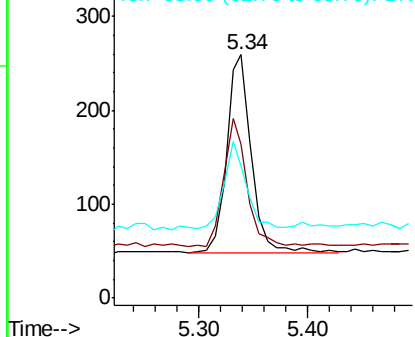

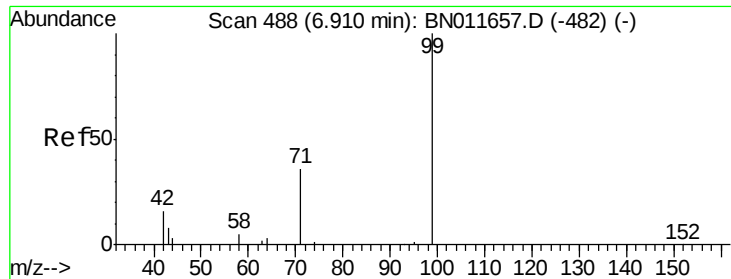

#5

Phenol-d6

Concen: 0.050 ng

RT: 6.91 min Scan# 488

Delta R.T. -0.00 min

Lab File: BN011668.D

Acq: 27 Aug 2020 17:30

Instrument :

BNA_N

ClientSampleId :

KY038PS037-200818


Tot Ion: 99 Resp: 375

Ion Ratio Lower Upper

99 100

42 29.1 20.2 30.2

71 54.9 33.3 49.9#



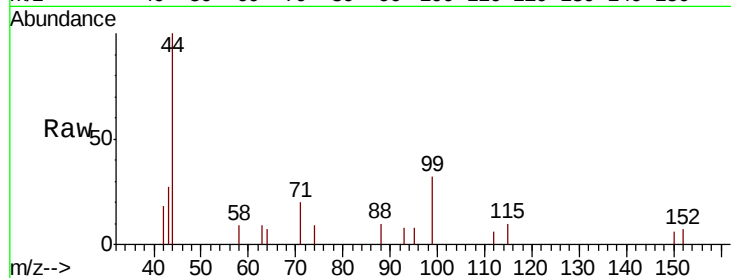


Abundance Ion 99.00 (98.70 to 99.70): BN011657.D (-482) (-)

Ion 42.00 (41.70 to 42.70): BN011657.D (-482) (-)

Ion 71.00 (70.70 to 71.70): BN011657.D (-482) (-)

Time-->

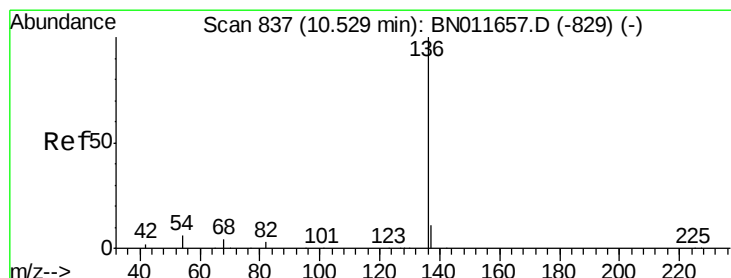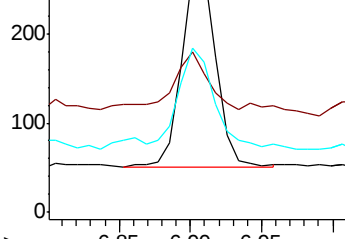

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.53 min Scan# 837

Delta R.T. -0.00 min

Lab File: BN011668.D

Acq: 27 Aug 2020 17:30

Tgt Ion: 136 Resp: 7397


Ion Ratio Lower Upper

136 100

137 12.0 9.3 13.9

54 7.5 5.8 8.8

68 5.1 4.1 6.1

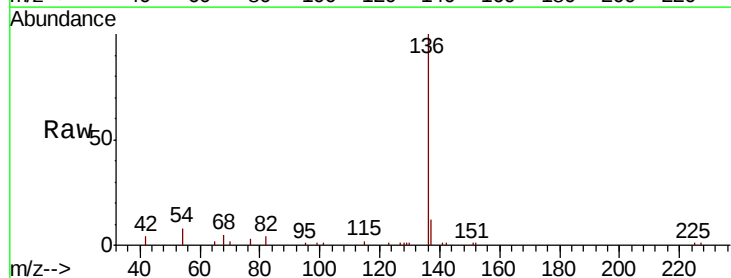



Abundance Ion 136.00 (135.70 to 136.70): BN011657.D (-829) (-)


Ion 137.00 (136.70 to 137.70): BN011657.D (-829) (-)

Ion 54.00 (53.70 to 54.70): BN011657.D (-829) (-)

Ion 68.00 (67.70 to 68.70): BN011657.D (-829) (-)

Time-->




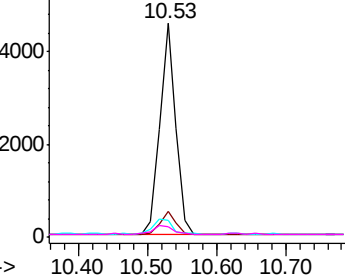




#8
 Nitrobenzene-d5
 Concen: 0.501 ng
 RT: 8.88 min Scan# 707
 Delta R.T. -0.00 min
 Lab File: BN011668.D
 Acq: 27 Aug 2020 17:30




Instrument :
 BNA_N
 ClientSampleId :
 KY038PS037-200818


Tot Ion	82	Resp	3591
Ion Ratio	Lower	Upper	
82	100		
128	33.1	26.2	39.2
54	61.5	48.2	72.4

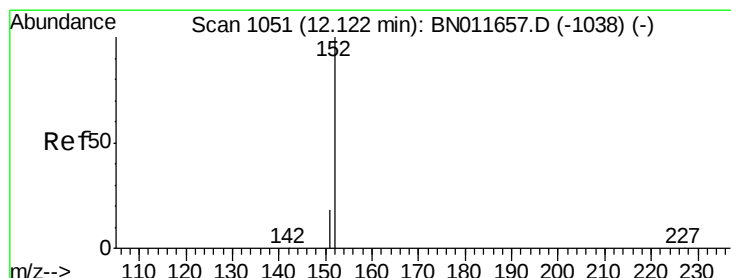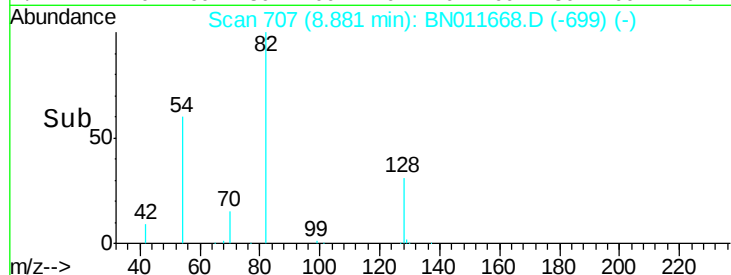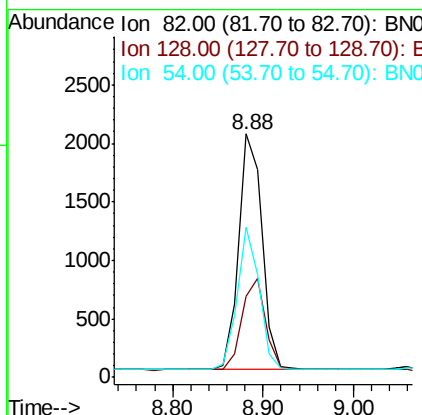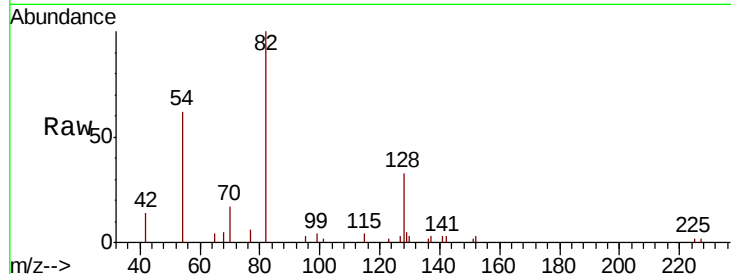

#11
 2-Methylnaphthalene-d10
 Concen: 0.281 ng
 RT: 12.12 min Scan# 1051
 Delta R.T. -0.00 min
 Lab File: BN011668.D
 Acq: 27 Aug 2020 17:30

Tgt Ion	152	Resp	3747
Ion Ratio	Lower	Upper	
152	100		
151	19.7	16.7	25.1

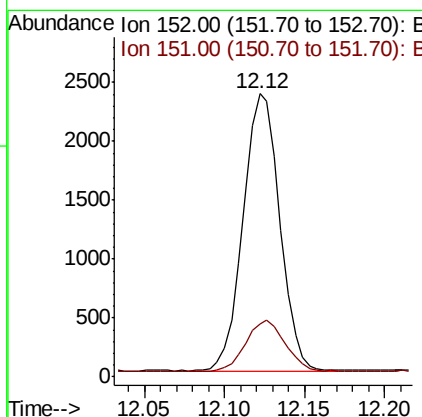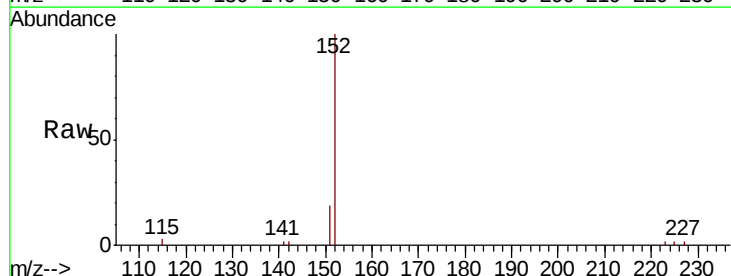



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.38 min Scan# 1285

Delta R.T. -0.00 min

Lab File: BN011668.D

Acq: 27 Aug 2020 17:30

Instrument :

BNA_N

ClientSampleId :

KY038PS037-200818


Tot Ion:164 Resp: 4283

Ion Ratio Lower Upper

164 100

162 102.4 81.4 122.0




160 48.2 38.5 57.7

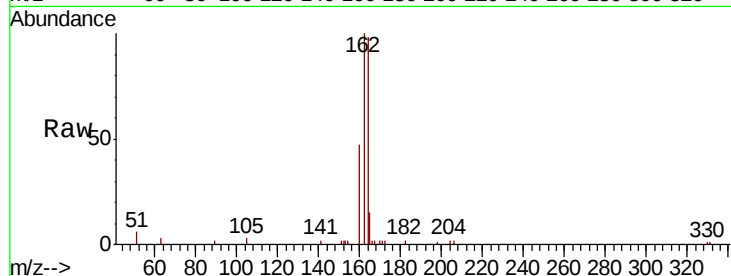

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

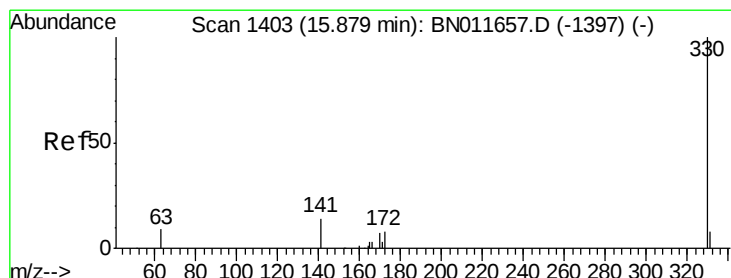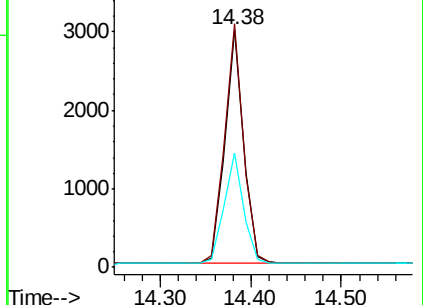

#14

2,4,6-Tribromophenol

Concen: 0.089 ng

RT: 15.88 min Scan# 1403

Delta R.T. -0.00 min

Lab File: BN011668.D

Acq: 27 Aug 2020 17:30


Tgt Ion:330 Resp: 185

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0



141 37.3 30.0 45.0

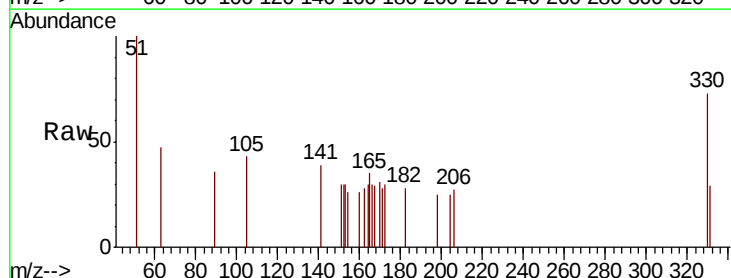


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



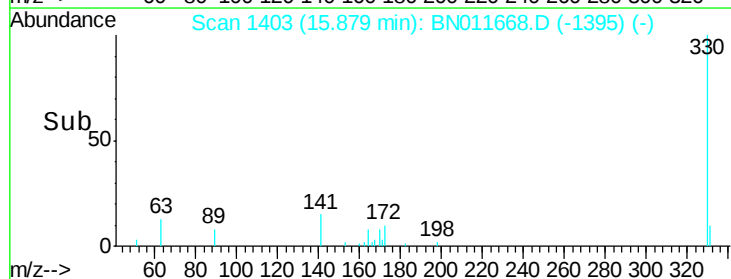
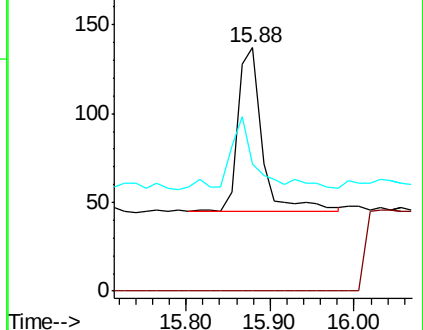




#15
2-Fluorobiphenyl
Concen: 0.529 ng
RT: 13.00 min Scan# 1176
Delta R.T. -0.00 min
Lab File: BN011668.D
Acq: 27 Aug 2020 17:30




Instrument :
BNA_N
ClientSampleId :
KY038PS037-200818


Tot Ion:172 Resp: 9581
Ion Ratio Lower Upper
172 100
171 35.9 30.0 45.0
170 25.5 20.1 30.1

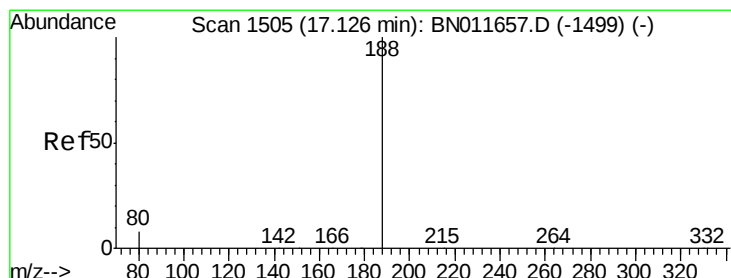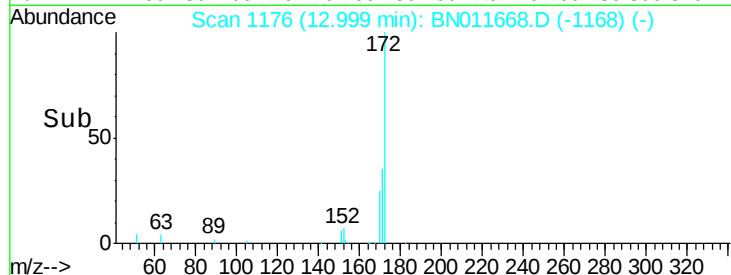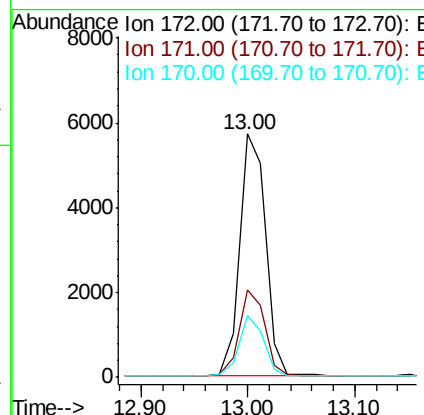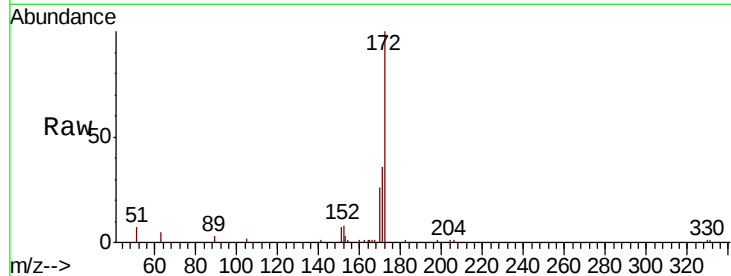

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.13 min Scan# 1505
Delta R.T. -0.00 min
Lab File: BN011668.D
Acq: 27 Aug 2020 17:30

Tgt Ion:188 Resp: 10092
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.6 6.6 9.8

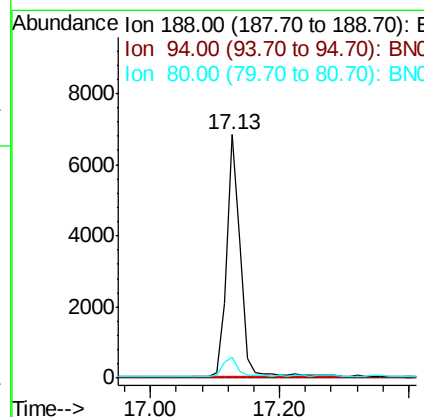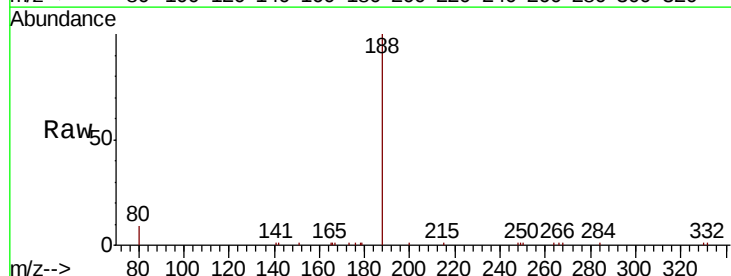


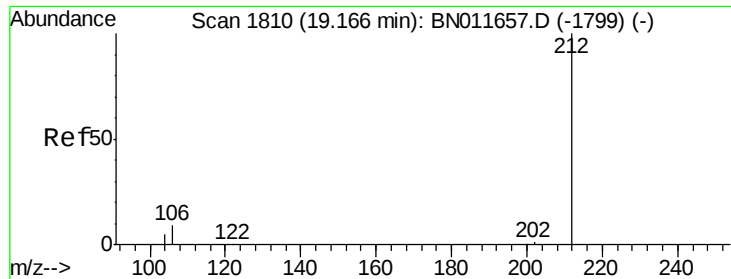




#27
 Fluoranthene-d10
 Concen: 0.341 ng
 RT: 19.16 min Scan# 1809
 Delta R.T. -0.01 min
 Lab File: BN011668.D
 Acq: 27 Aug 2020 17:30

Instrument :
 BNA_N
 ClientSampleId :
 KY038PS037-200818

Tot Ion:212 Resp: 11049
 Ion Ratio Lower Upper
 212 100
 106 9.5 7.6 11.4
 104 5.5 4.6 6.8

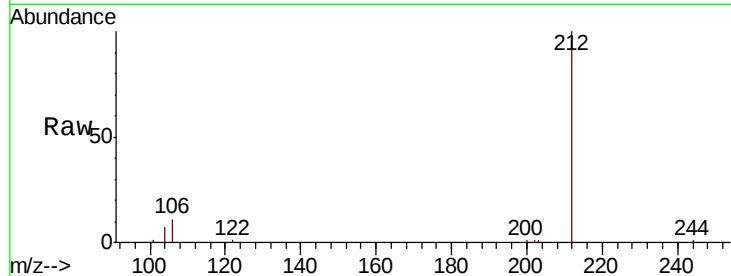


Abundance Ion 212.00 (211.70 to 212.70): E
 Ion 106.00 (105.70 to 106.70): E
 Ion 104.00 (103.70 to 104.70): E

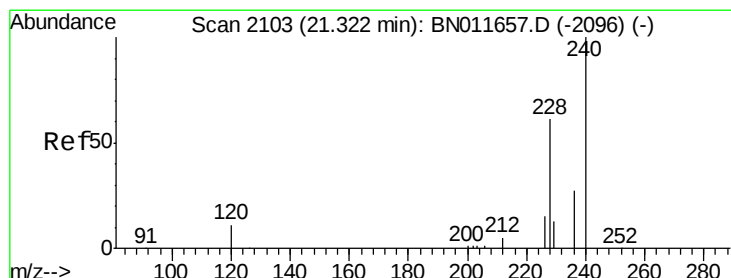
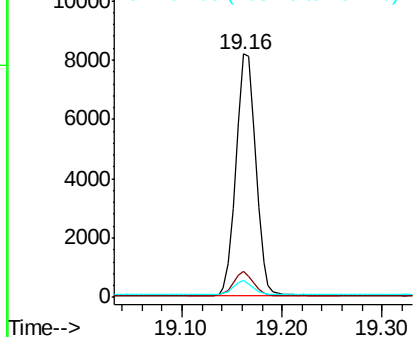



#29
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.32 min Scan# 2103
 Delta R.T. -0.00 min
 Lab File: BN011668.D
 Acq: 27 Aug 2020 17:30

Tgt Ion:240 Resp: 10370
 Ion Ratio Lower Upper
 240 100
 120 10.7 9.9 14.9
 236 28.0 22.2 33.4

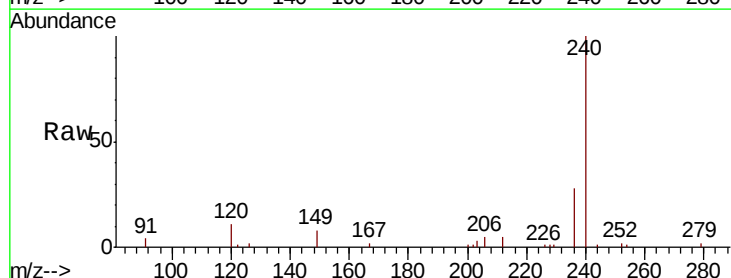

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

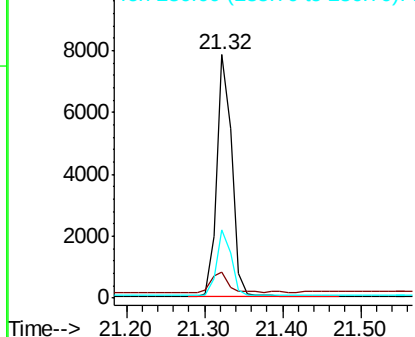

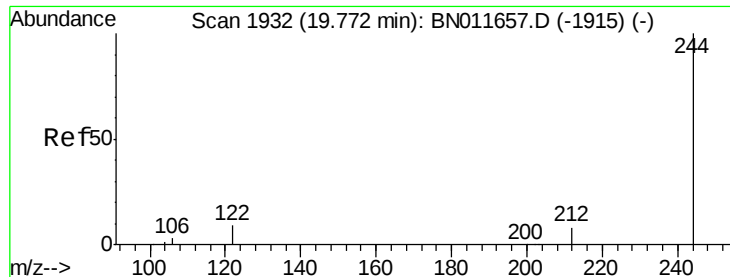

#31

Terphenyl-d14

Concen: 0.770 ng

RT: 19.77 min Scan# 1931

Delta R.T. -0.01 min

Lab File: BN011668.D

Acq: 27 Aug 2020 17:30

Instrument :

BNA_N

ClientSampleId :

KY038PS037-200818


Tot Ion:244 Resp: 19827

Ion Ratio Lower Upper

244 100

212 8.5 6.5 9.7

122 10.2 7.4 11.2

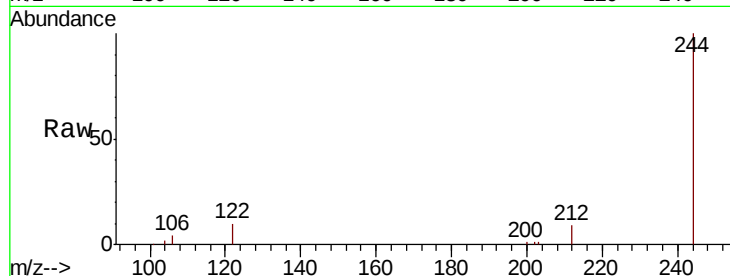


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

Time-->

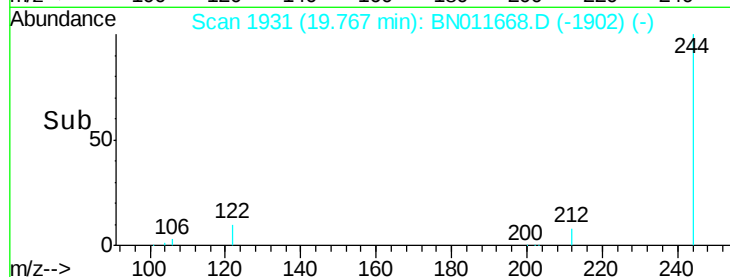


Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

Time-->

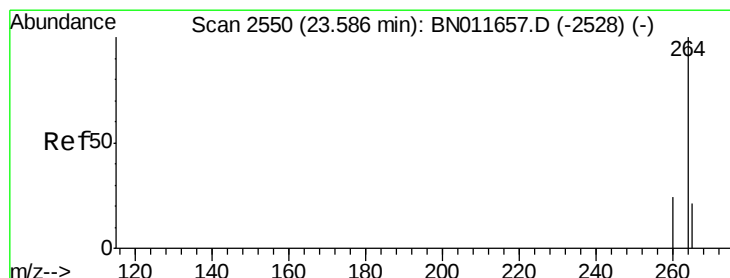

#36

Perylene-d12

Concen: 0.400 ng

RT: 23.59 min Scan# 2550

Delta R.T. -0.00 min

Lab File: BN011668.D

Acq: 27 Aug 2020 17:30


Tgt Ion:264 Resp: 8455

Ion Ratio Lower Upper

264 100

260 25.0 19.8 29.6

265 67.3 38.9 58.3#

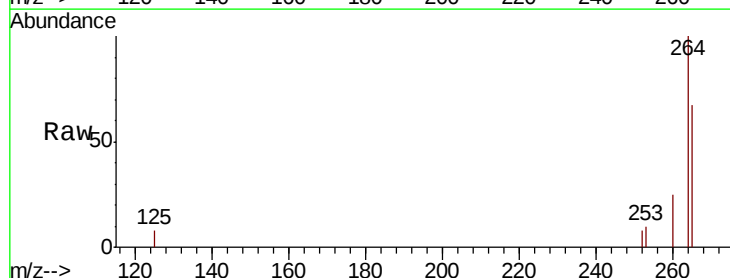


Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

Time-->

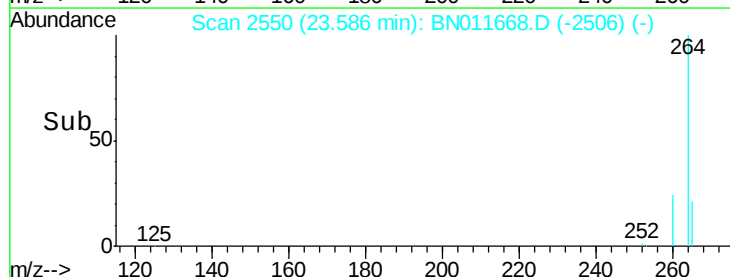

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

Time-->