

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082720\
 Data File : BN011669.D
 Acq On : 27 Aug 2020 18:06
 Operator : CG/JU
 Sample : L3737-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 KY038PS038-200818

Quant Time: Aug 28 00:45:13 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN082720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 27 14:34:48 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	1902	0.40	ng	0.00
7) Naphthalene-d8	10.53	136	7096	0.40	ng	0.00
13) Acenaphthene-d10	14.38	164	4177	0.40	ng	0.00
19) Phenanthrene-d10	17.13	188	9392	0.40	ng	0.00
29) Chrysene-d12	21.32	240	9586	0.40	ng	0.00
36) Perylene-d12	23.58	264	10167	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.34	112	922	0.17	ng	0.00
5) Phenol-d6	6.90	99	664	0.09	ng	0.00
8) Nitrobenzene-d5	8.88	82	3486	0.51	ng	0.00
11) 2-Methylnaphthalene-d10	12.12	152	3636	0.28	ng	0.00
14) 2,4,6-Tribromophenol	15.88	330	764	0.38	ng	0.00
15) 2-Fluorobiphenyl	13.00	172	9227	0.52	ng	0.00
27) Fluoranthene-d10	19.16	212	10101	0.34	ng	0.00
31) Terphenyl-d14	19.77	244	17990	0.76	ng	0.00
Target Compounds						
30) Pyrene	19.55	202	755	0.023	ng	# 93
34) Bis(2-ethylhexyl)phthalate	21.25	149	462	0.033	ng	# 99
37) Benzo(b)fluoranthene	22.90	252	800	0.021	ng	# 8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082720\
Data File : BN011669.D
Acq On : 27 Aug 2020 18:06
Operator : CG/JU
Sample : L3737-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
KY038PS038-200818

Quant Time: Aug 28 00:45:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 27 14:34:48 2020
Response via : Initial Calibration

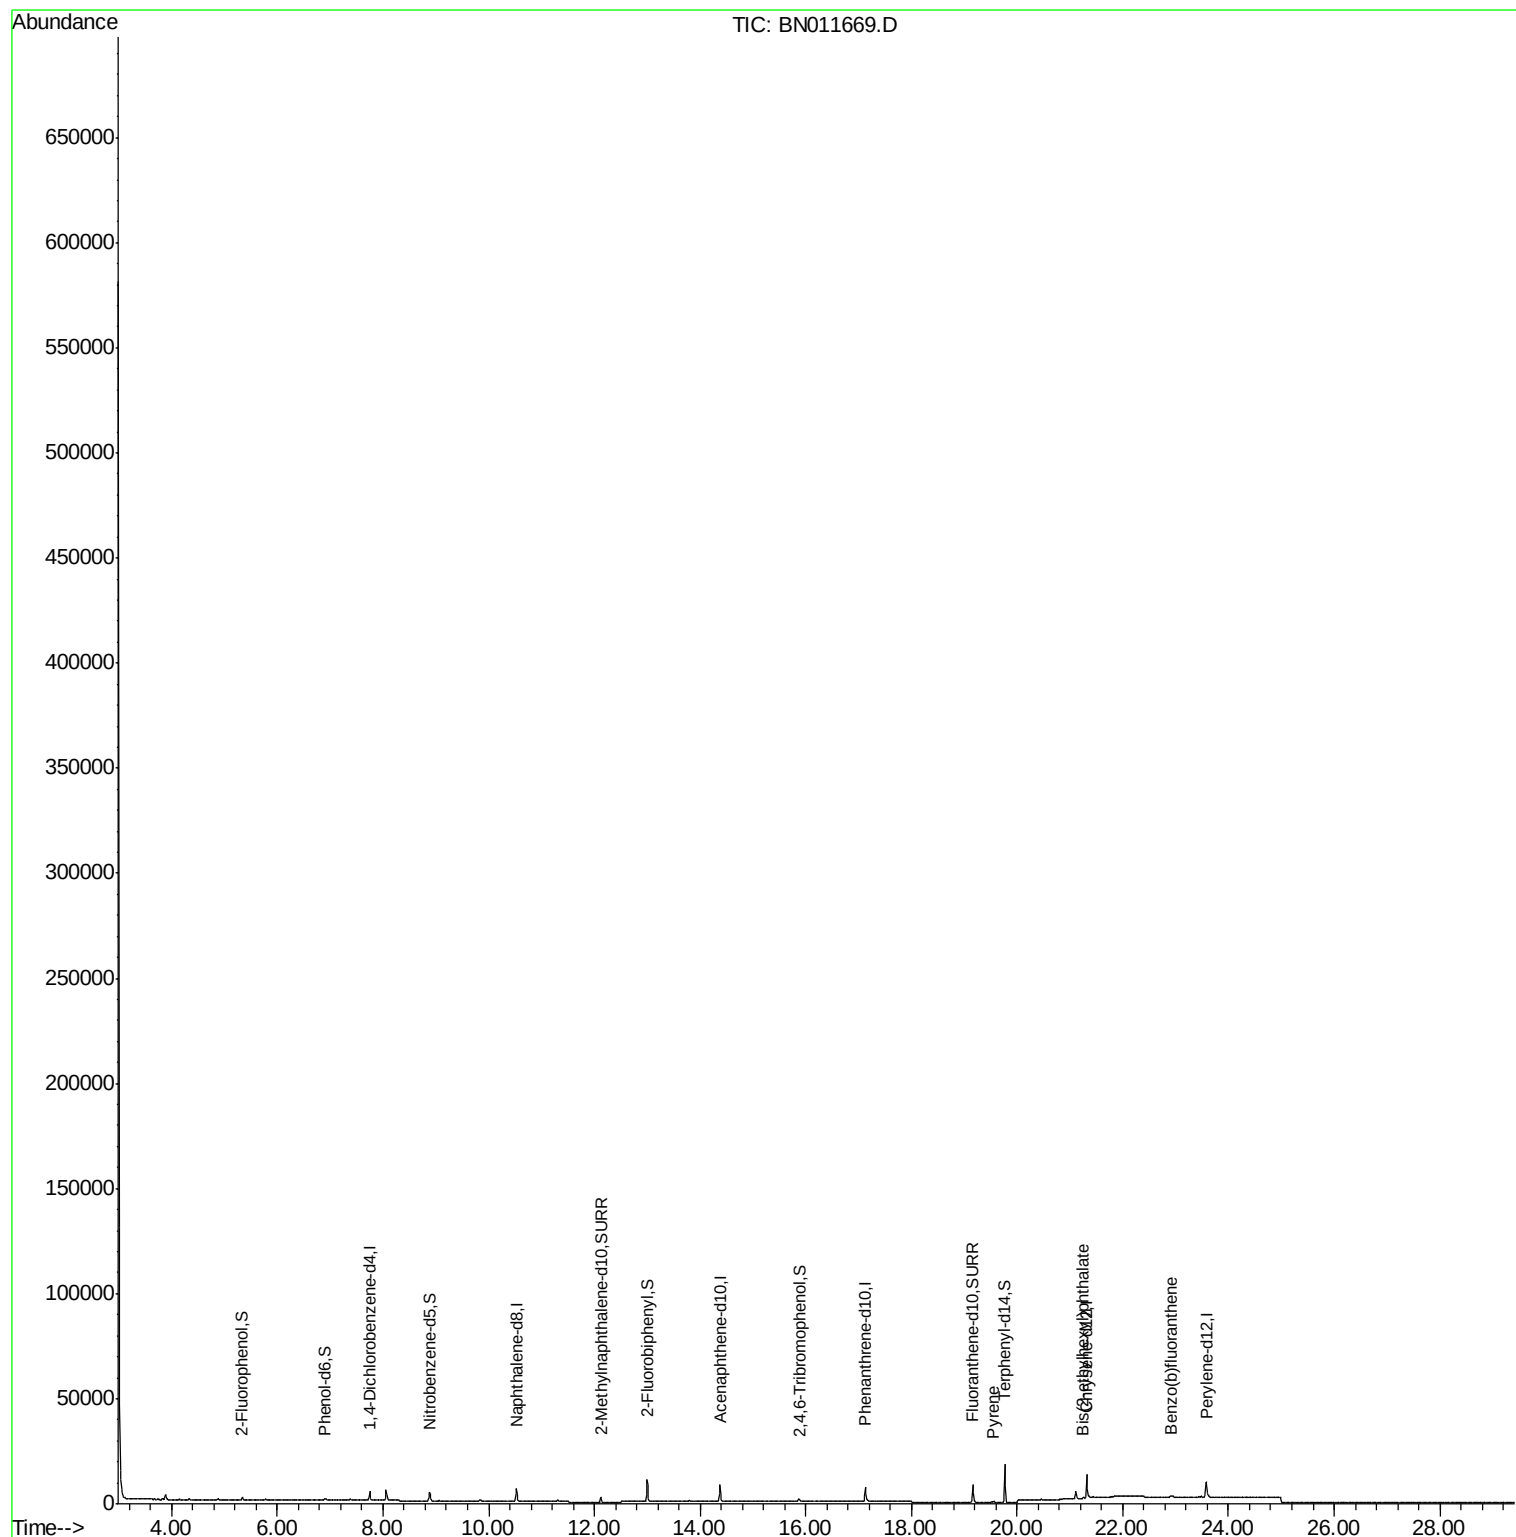

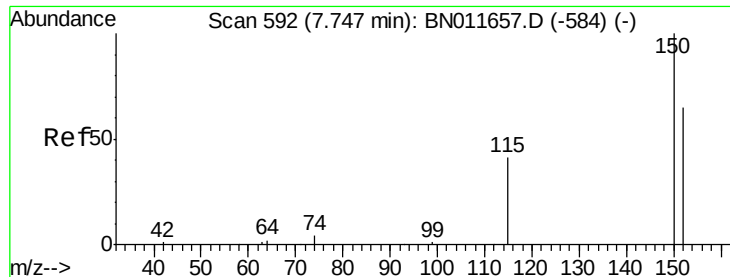


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.75 min Scan# 592
Delta R.T. -0.00 min
Lab File: BN011669.D
Acq: 27 Aug 2020 18:06

Instrument :
BNA_N
ClientSampleId :
KY038PS038-200818

Tot Ion:152 Resp: 1902
Ion Ratio Lower Upper
152 100
150 149.7 121.0 181.6
115 64.8 52.6 78.8

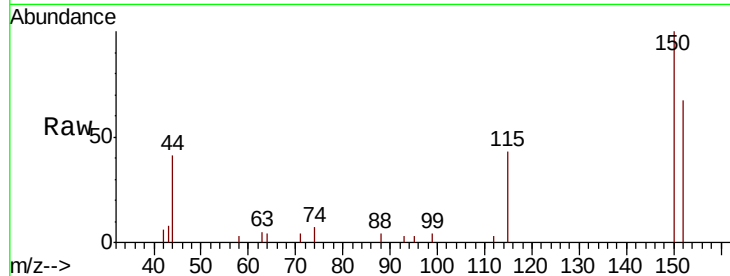


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

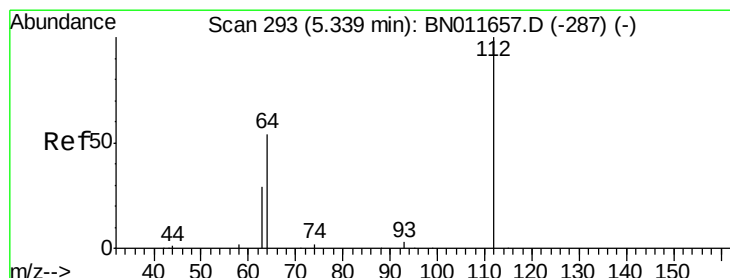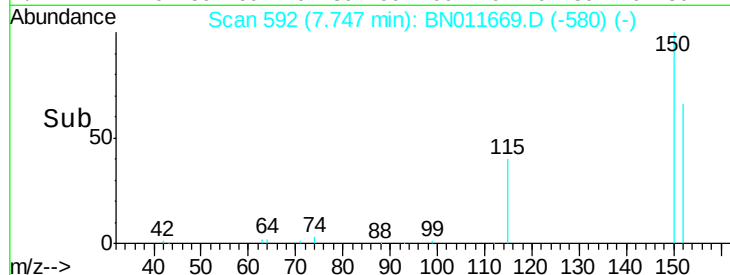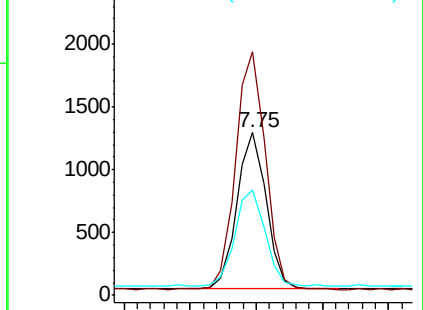



#4


2-Fluorophenol
Concen: 0.172 ng
RT: 5.34 min Scan# 293
Delta R.T. -0.00 min
Lab File: BN011669.D
Acq: 27 Aug 2020 18:06

Tgt Ion:112 Resp: 922
Ion Ratio Lower Upper
112 100
64 62.9 49.7 74.5
63 37.6 29.4 44.0

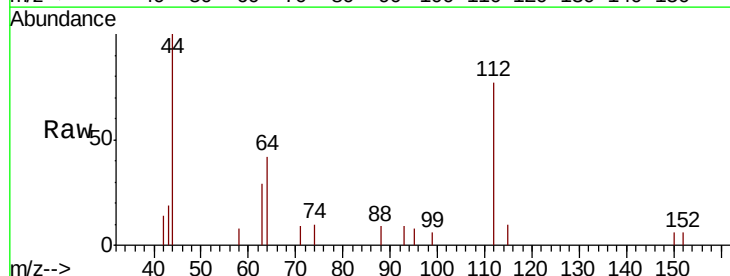

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

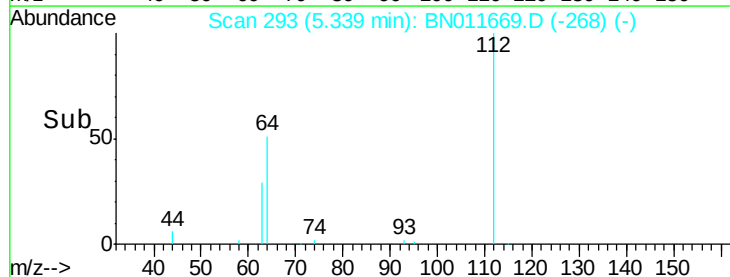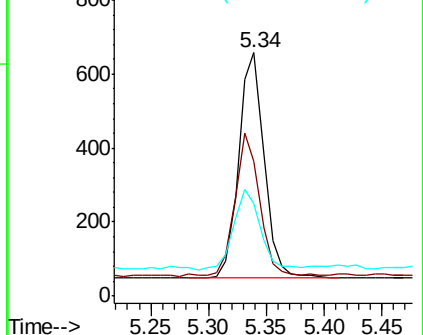

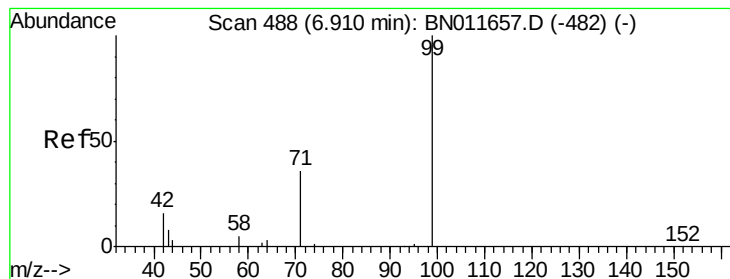

#5

Phenol-d6

Concen: 0.091 ng

RT: 6.90 min Scan# 487

Delta R.T. -0.01 min

Lab File: BN011669.D

Acq: 27 Aug 2020 18:06

Instrument :

BNA_N

ClientSampleId :

KY038PS038-200818


Tot Ion: 99 Resp: 664

Ion Ratio Lower Upper

99 100

42 30.3 20.2 30.2#

71 44.0 33.3 49.9



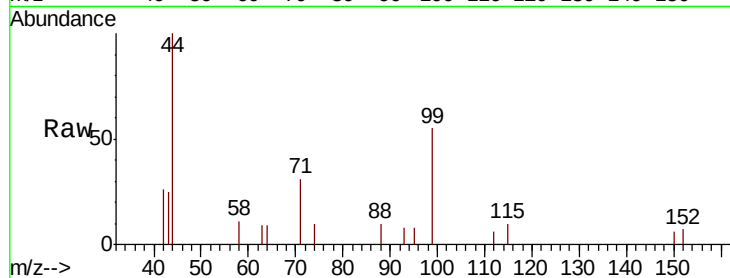


Abundance Ion 99.00 (98.70 to 99.70): BN011657.D (-482) (-)

Ion 42.00 (41.70 to 42.70): BN011657.D (-482) (-)

Ion 71.00 (70.70 to 71.70): BN011657.D (-482) (-)

Time-->

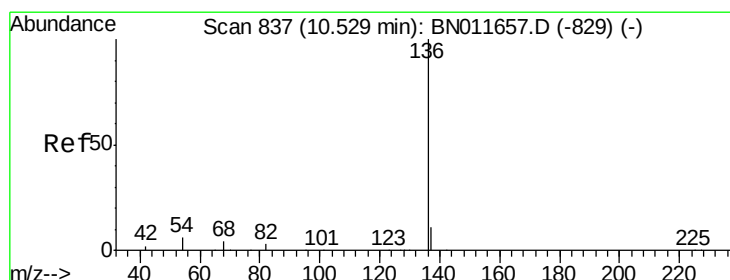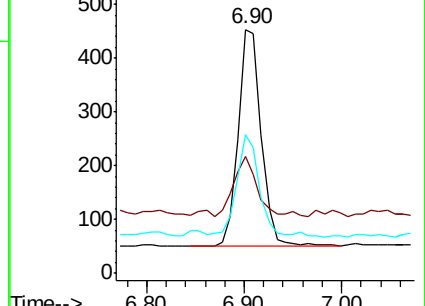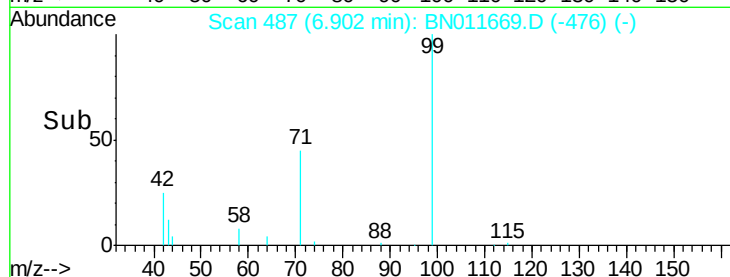

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.53 min Scan# 837

Delta R.T. -0.00 min

Lab File: BN011669.D

Acq: 27 Aug 2020 18:06

Tgt Ion: 136 Resp: 7096


Ion Ratio Lower Upper

136 100

137 12.4 9.3 13.9

54 7.4 5.8 8.8

68 5.0 4.1 6.1

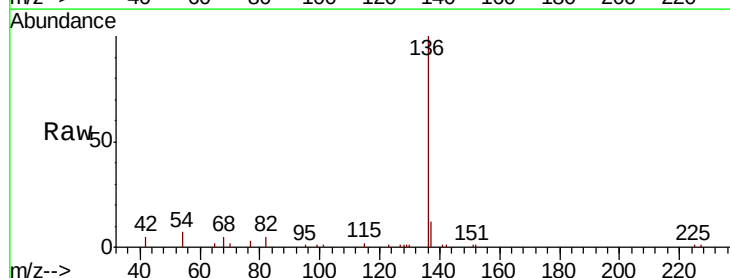



Abundance Ion 136.00 (135.70 to 136.70): BN011657.D (-829) (-)


Ion 137.00 (136.70 to 137.70): BN011657.D (-829) (-)

Ion 54.00 (53.70 to 54.70): BN011657.D (-829) (-)

Ion 68.00 (67.70 to 68.70): BN011657.D (-829) (-)

Time-->

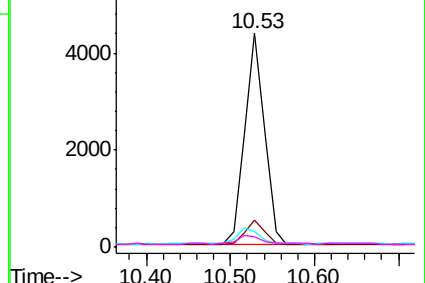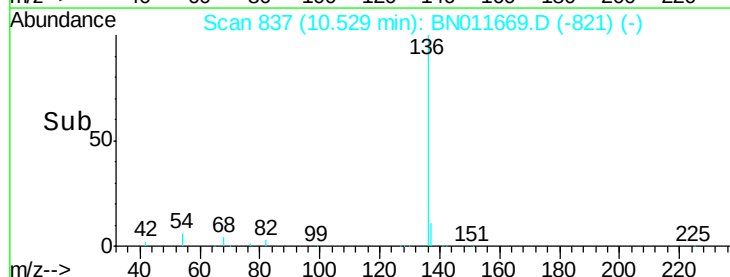



#8

Nitrobenzene-d5

Concen: 0.507 ng

RT: 8.88 min Scan# 707

Delta R.T. -0.00 min

Lab File: BN011669.D

Acq: 27 Aug 2020 18:06

Instrument :

BNA_N

ClientSampleId :

KY038PS038-200818


Tot Ion: 82 Resp: 3486

Ion Ratio Lower Upper

82 100

128 32.5 26.2 39.2




54 62.8 48.2 72.4

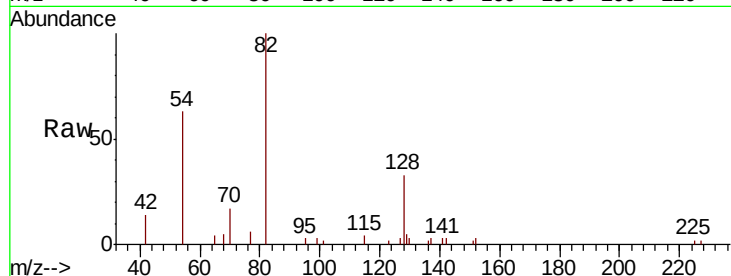

Abundance Ion 82.00 (81.70 to 82.70): BN011669.D (-699) (-)

Ion 128.00 (127.70 to 128.70): BN011669.D (-699) (-)

Ion 54.00 (53.70 to 54.70): BN011669.D (-699) (-)

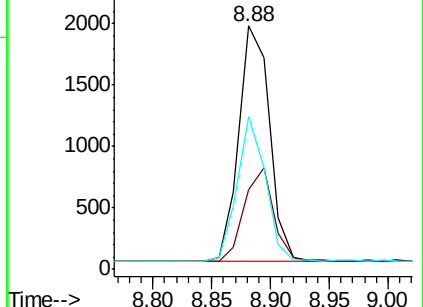

#11

2-Methylnaphthalene-d10

Concen: 0.284 ng

RT: 12.12 min Scan# 1051

Delta R.T. -0.00 min

Lab File: BN011669.D


Acq: 27 Aug 2020 18:06

Tgt Ion: 152 Resp: 3636

Ion Ratio Lower Upper



152 100


151 19.0 16.7 25.1



Abundance Ion 152.00 (151.70 to 152.70): BN011669.D (-1006) (-)

Ion 151.00 (150.70 to 151.70): BN011669.D (-1006) (-)

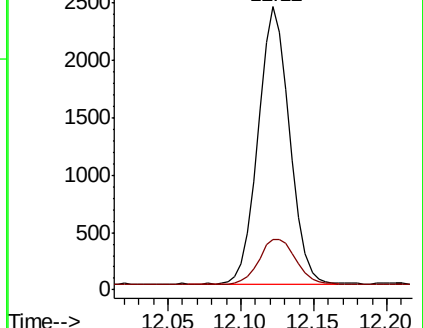



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.38 min Scan# 1285

Delta R.T. -0.00 min

Lab File: BN011669.D

Acq: 27 Aug 2020 18:06

Instrument :

BNA_N

ClientSampleId :

KY038PS038-200818


Tot Ion:164 Resp: 4177

Ion Ratio Lower Upper

164 100

162 103.4 81.4 122.0




160 49.8 38.5 57.7

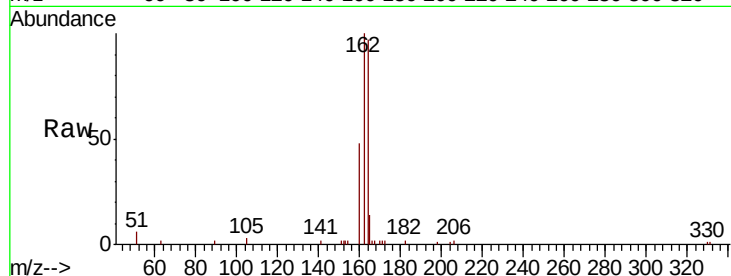

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

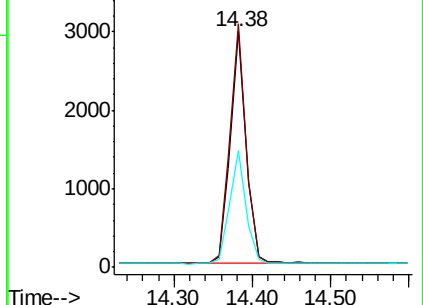

#14

2,4,6-Tribromophenol

Concen: 0.377 ng

RT: 15.88 min Scan# 1403

Delta R.T. -0.00 min

Lab File: BN011669.D

Acq: 27 Aug 2020 18:06


Tgt Ion:330 Resp: 764

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0



141 33.5 30.0 45.0




Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

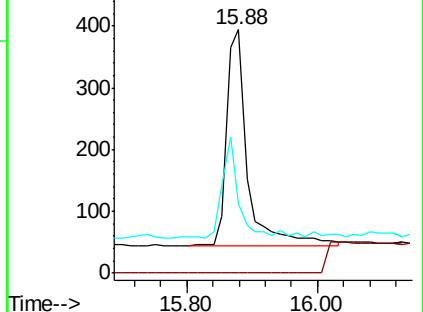

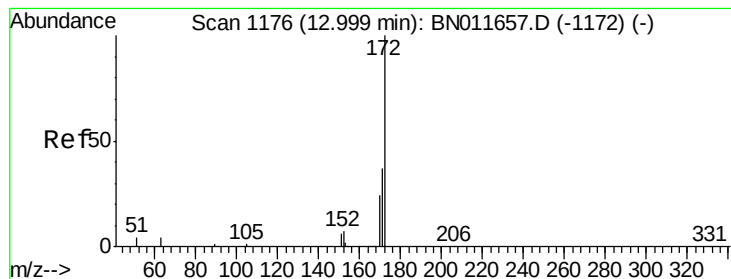

#15

2-Fluorobiphenyl

Concen: 0.522 ng

RT: 13.00 min Scan# 1176

Delta R.T. -0.00 min

Lab File: BN011669.D

Acq: 27 Aug 2020 18:06

Instrument :

BNA_N

ClientSampleId :

KY038PS038-200818


Tot Ion:172 Resp: 9227

Ion Ratio Lower Upper

172 100

171 36.2 30.0 45.0




170 25.3 20.1 30.1



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

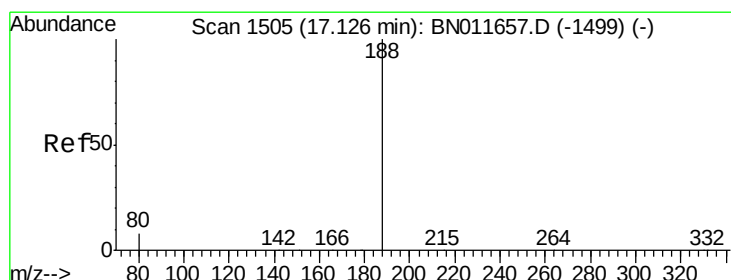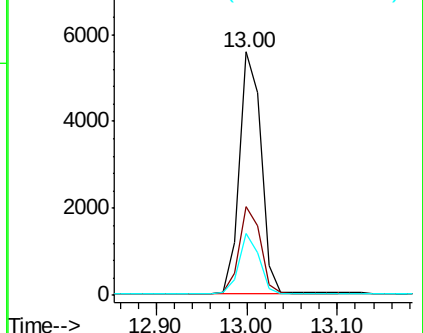

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.13 min Scan# 1505

Delta R.T. -0.00 min

Lab File: BN011669.D

Acq: 27 Aug 2020 18:06


Tgt Ion:188 Resp: 9392

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0



80 8.1 6.6 9.8

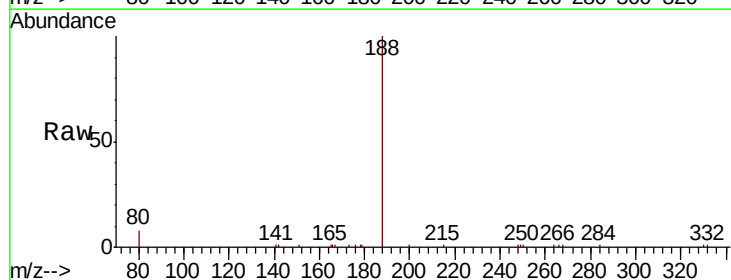


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

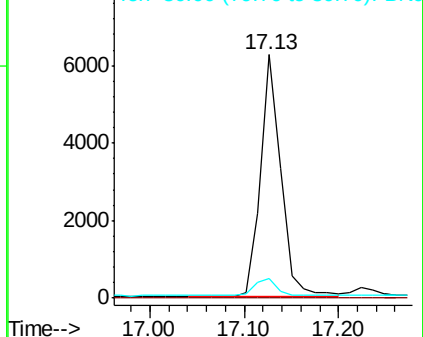

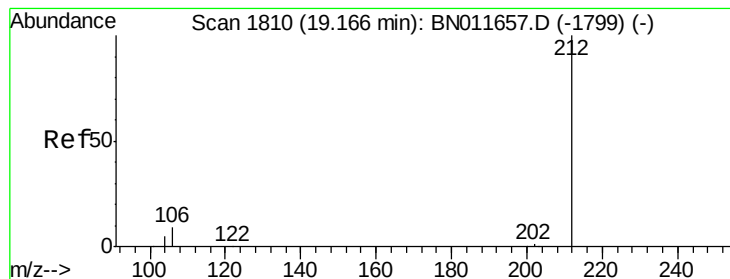

#27

Fluoranthene-d10

Concen: 0.335 ng

RT: 19.16 min Scan# 1809

Delta R.T. -0.01 min

Lab File: BN011669.D

Acq: 27 Aug 2020 18:06

Instrument :

BNA_N

ClientSampleId :

KY038PS038-200818



Tot Ion:212 Resp: 10101

Ion Ratio Lower Upper

212 100

106 9.3 7.6 11.4



104 5.5 4.6 6.8

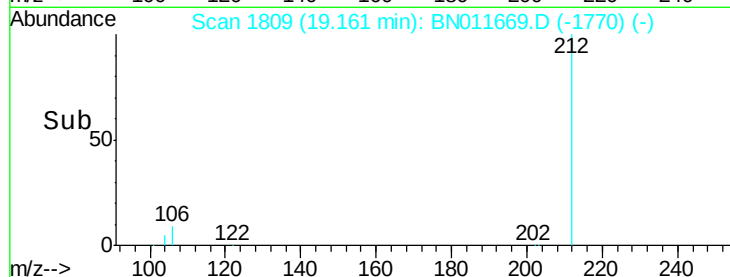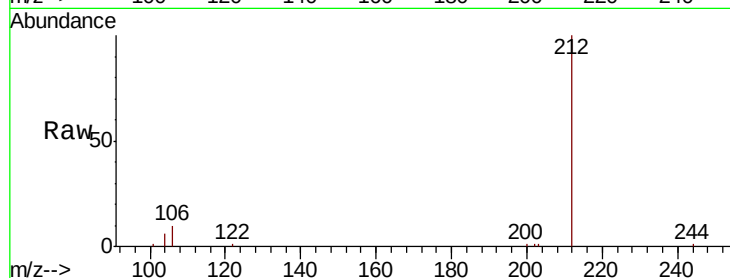

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

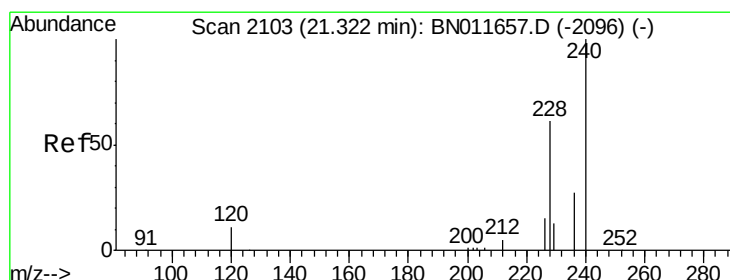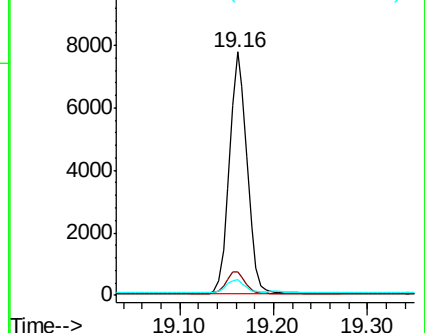

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.32 min Scan# 2103

Delta R.T. -0.00 min

Lab File: BN011669.D

Acq: 27 Aug 2020 18:06



Tgt Ion:240 Resp: 9586

Ion Ratio Lower Upper

240 100

120 8.2 9.9 14.9#


236 28.1 22.2 33.4

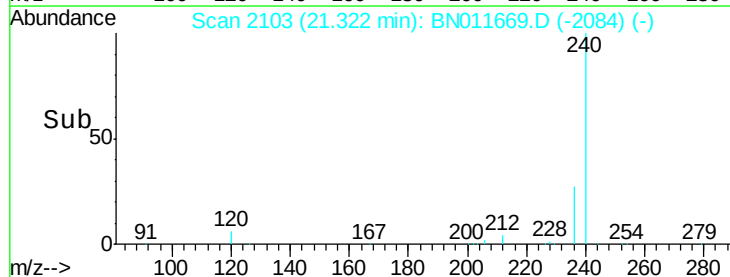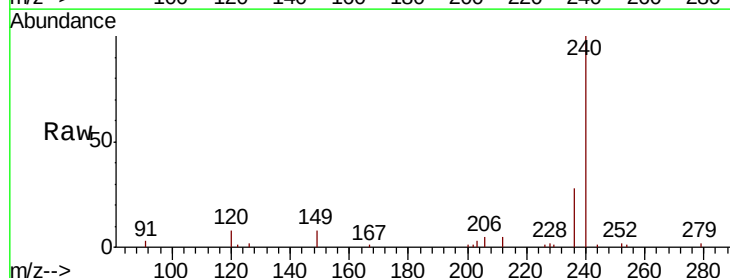


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

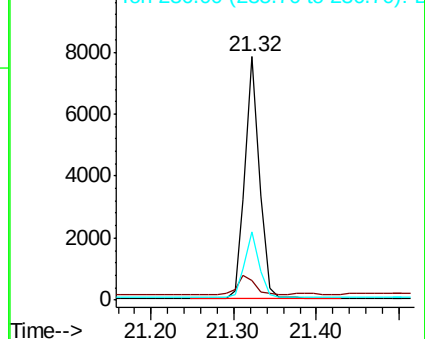


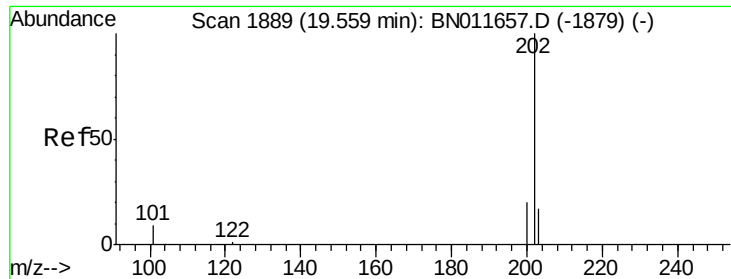




#30
Pvrene
Concen: 0.023 ng
RT: 19.55 min Scan# 1888
Delta R.T. -0.01 min
Lab File: BN011669.D
Acq: 27 Aug 2020 18:06

Instrument :
BNA_N
ClientSampleId :
KY038PS038-200818

Tot Ion:202 Resp: 755
Ion Ratio Lower Upper
202 100
200 21.3 16.3 24.5
203 22.8 14.1 21.1#

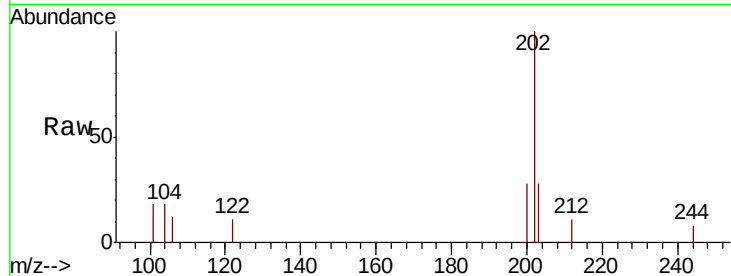


Abundance Ion 202.00 (201.70 to 202.70): E
800 Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E


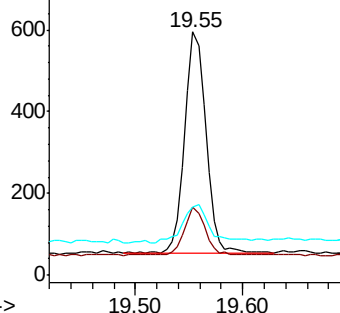



#31
Terphenyl-d14
Concen: 0.756 ng
RT: 19.77 min Scan# 1931
Delta R.T. -0.01 min
Lab File: BN011669.D
Acq: 27 Aug 2020 18:06

Tgt Ion:244 Resp: 17990
Ion Ratio Lower Upper
244 100
212 8.2 6.5 9.7
122 9.3 7.4 11.2



Abundance Ion 244.00 (243.70 to 244.70): E
20000 Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

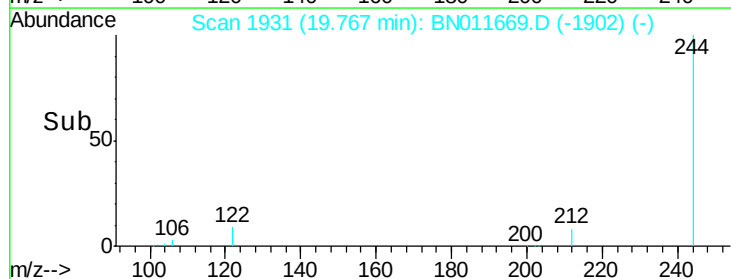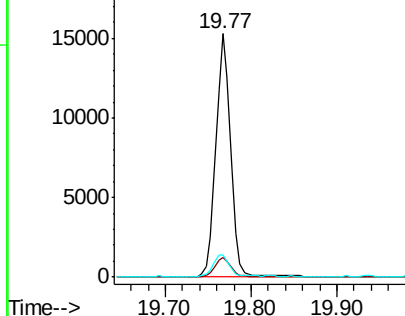



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.033 ng

RT: 21.25 min Scan# 2096

Delta R.T. -0.01 min

Lab File: BN011669.D

Acq: 27 Aug 2020 18:06

Instrument :

BNA_N

ClientSampleId :

KY038PS038-200818


Tot Ion:149 Resp: 462

Ion Ratio Lower Upper

149 100

167 28.8 23.2 34.8




279 6.7 4.0 6.0#



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

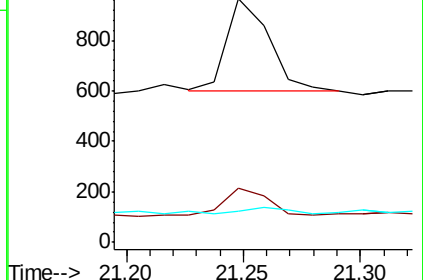

#36

Perylene-d12

Concen: 0.400 ng

RT: 23.58 min Scan# 2548

Delta R.T. -0.01 min

Lab File: BN011669.D

Acq: 27 Aug 2020 18:06


Tgt Ion:264 Resp: 10167

Ion Ratio Lower Upper

264 100

260 25.1 19.8 29.6



265 59.6 38.9 58.3#




Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

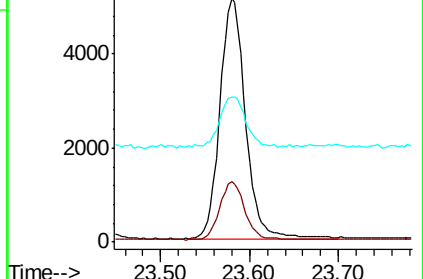

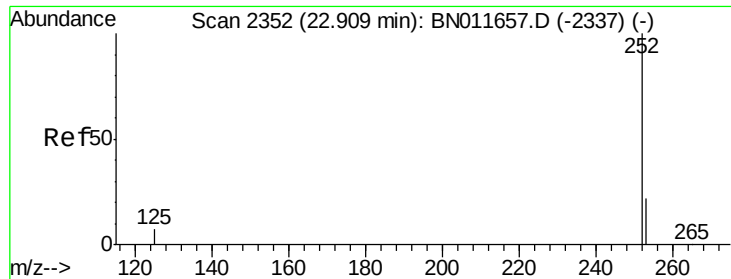

#37

Benzo(b)fluoranthene

Concen: 0.021 ng

RT: 22.90 min Scan# 2350

Delta R.T. -0.01 min

Lab File: BN011669.D


Acq: 27 Aug 2020 18:06

Instrument :

BNA_N

ClientSampleId :

KY038PS038-200818



Tot Ion: 252 Resp: 800

Ion Ratio Lower Upper

252 100

253 67.8 19.7 29.5#

125 49.2 7.8 11.8#

