


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082720\
 Data File : BN011654.D
 Acq On : 27 Aug 2020 09:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 27 14:34:48 2020

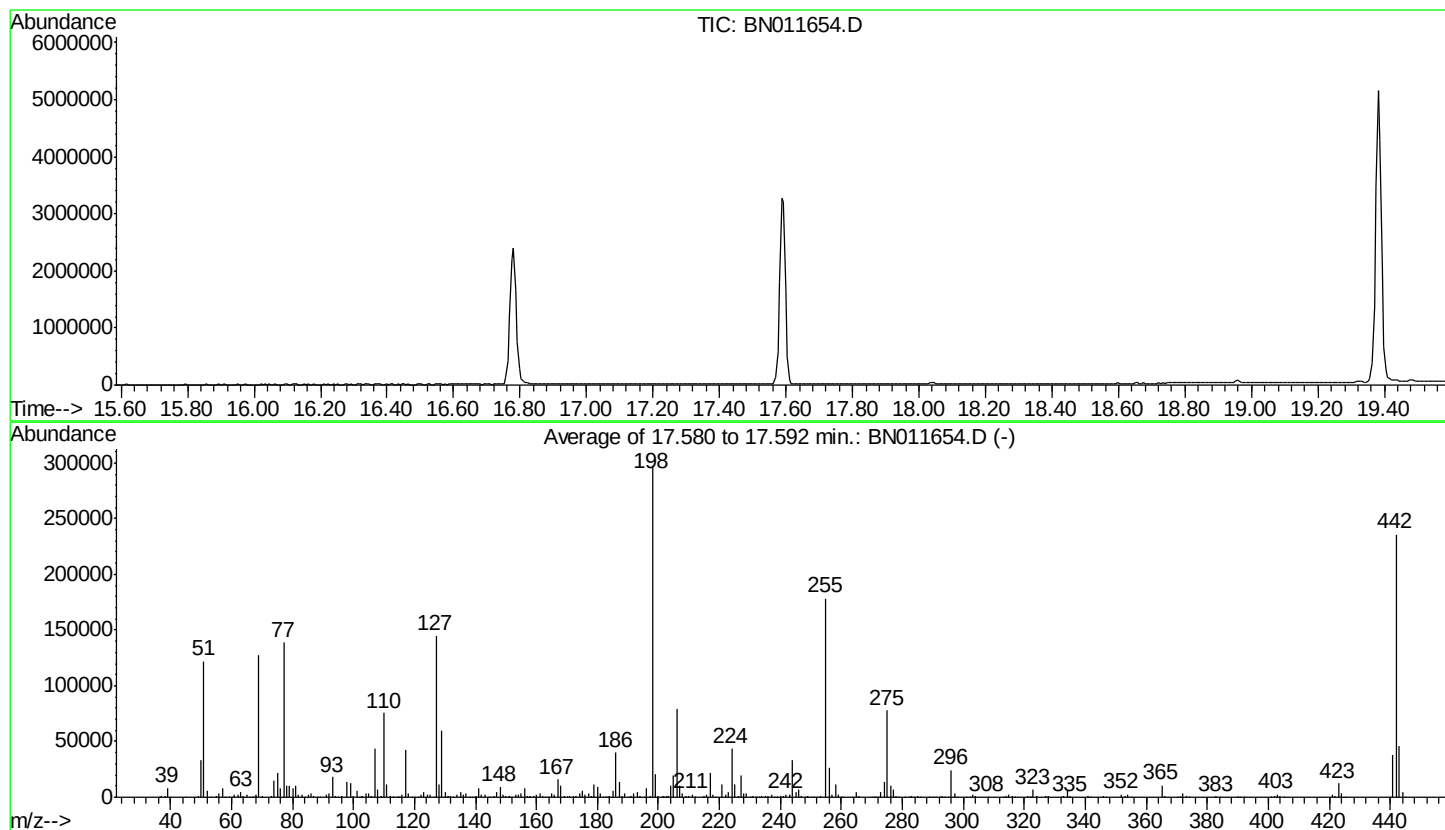

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	122202	PASS
68	69	0.00	2	1.7	2221	PASS
69	198	0.00	100	42.7	127096	PASS
70	69	0.00	2	0.6	823	PASS
127	198	10	80	48.7	144864	PASS
197	198	0.00	2	0.3	820	PASS
198	198	100	100	100.0	297514	PASS
199	198	5	9	6.8	20319	PASS
275	198	10	60	26.2	77946	PASS
365	198	1	100	3.6	10855	PASS
441	198	0.01	100	12.9	38282	PASS
442	198	50	100	79.2	235717	PASS
443	442	15	24	19.4	45648	PASS